

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN032125\  
 Data File : VN086058.D  
 Acq On : 21 Mar 2025 22:31  
 Operator : JC\MD  
 Sample : Q1606-06  
 Misc : 5.0mL/MSVOA\_N/WATER  
 ALS Vial : 25 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 RT4534


Quant Time: Mar 21 23:59:16 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N031825W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Mar 19 03:20:56 2025  
 Response via : Initial Calibration

| Compound                      | R.T.           | QIon | Response            | Conc   | Units  | Dev(Min) |
|-------------------------------|----------------|------|---------------------|--------|--------|----------|
| -----                         |                |      |                     |        |        |          |
| Internal Standards            |                |      |                     |        |        |          |
| 1) Pentafluorobenzene         | 8.224          | 168  | 142558              | 50.000 | ug/l   | 0.00     |
| 34) 1,4-Difluorobenzene       | 9.100          | 114  | 274594              | 50.000 | ug/l   | 0.00     |
| 63) Chlorobenzene-d5          | 11.865         | 117  | 264941              | 50.000 | ug/l   | 0.00     |
| 72) 1,4-Dichlorobenzene-d4    | 13.788         | 152  | 101760              | 50.000 | ug/l   | 0.00     |
| System Monitoring Compounds   |                |      |                     |        |        |          |
| 33) 1,2-Dichloroethane-d4     | 8.577          | 65   | 114028              | 58.413 | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 74 - 125 |      | Recovery = 116.820% |        |        |          |
| 35) Dibromofluoromethane      | 8.165          | 113  | 97734               | 50.993 | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 75 - 124 |      | Recovery = 101.980% |        |        |          |
| 50) Toluene-d8                | 10.565         | 98   | 350213              | 50.347 | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 86 - 113 |      | Recovery = 100.700% |        |        |          |
| 62) 4-Bromofluorobenzene      | 12.847         | 95   | 105995              | 42.727 | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 77 - 121 |      | Recovery = 85.460%  |        |        |          |
| Target Compounds              |                |      |                     |        |        |          |
|                               |                |      |                     |        | Qvalue |          |
| 11) Tert butyl alcohol        | 5.536          | 59   | 193                 | 0.698  | ug/l # | 73       |
| 16) Acetone                   | 4.430          | 43   | 25576               | 42.885 | ug/l   | 99       |
| 18) Methyl Acetate            | 5.030          | 43   | 2310                | 1.566  | ug/l # | 85       |
| 20) Methylene Chloride        | 5.277          | 84   | 9624                | 5.516  | ug/l   | 96       |
| 25) 2-Butanone                | 7.494          | 43   | 3497                | 4.064  | ug/l # | 85       |
| 29) Tetrahydrofuran           | 7.841          | 42   | 123                 | 0.232  | ug/l # | 24       |
| 30) Chloroform                | 7.965          | 83   | 658                 | 0.208  | ug/l # | 74       |
| 31) Cyclohexane               | 8.230          | 56   | 3171                | 1.304  | ug/l # | 1        |
| 36) 1,1-Dichloropropene       | 8.224          | 75   | 11963               | 4.740  | ug/l # | 48       |
| 37) Ethyl Acetate             | 7.571          | 43   | 1945                | 0.914  | ug/l # | 64       |
| 38) Carbon Tetrachloride      | 8.218          | 117  | 15131               | 4.560  | ug/l # | 15       |
| 40) Benzene                   | 8.600          | 78   | 24237               | 3.059  | ug/l   | 97       |
| 42) 1,2-Dichloroethane        | 8.683          | 62   | 593                 | 0.215  | ug/l # | 74       |
| 43) Isopropyl Acetate         | 8.688          | 43   | 100243              | 21.727 | ug/l # | 80       |
| 45) 1,2-Dichloropropane       | 9.735          | 63   | 860                 | 0.477  | ug/l # | 44       |
| 48) Methyl methacrylate       | 9.659          | 41   | 2163                | 1.421  | ug/l # | 31       |
| 51) 4-Methyl-2-Pentanone      | 10.441         | 43   | 6943                | 3.412  | ug/l # | 63       |
| 52) Toluene                   | 10.629         | 92   | 2166                | 0.445  | ug/l   | 99       |
| 54) cis-1,3-Dichloropropene   | 10.353         | 75   | 26719               | 8.805  | ug/l # | 72       |
| 56) Ethyl methacrylate        | 10.982         | 69   | 1442                | 0.803  | ug/l # | 1        |
| 57) 1,3-Dichloropropane       | 11.200         | 76   | 3458                | 1.097  | ug/l # | 42       |
| 59) 2-Hexanone                | 11.165         | 43   | 53002               | 35.757 | ug/l # | 18       |
| 71) Bromoform                 | 12.847         | 173  | 983                 | 0.522  | ug/l # | 28       |
| 74) N-amyl acetate            | 12.482         | 43   | 715                 | 0.308  | ug/l # | 35       |
| 76) 1,2,3-Trichloropropane    | 12.847         | 75   | 52407               | 23.004 | ug/l # | 1        |
| 81) trans-1,4-Dichloro-2-b... | 12.847         | 75   | 52407               | 60.818 | ug/l # | 16       |
| -----                         |                |      |                     |        |        |          |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Mar 21 23:59:16 2025  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N031825W.M  
Quant Title : SW846 8260  
QLast Update : Wed Mar 19 03:20:56 2025  
Response via : Initial Calibration









#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 8.224 min Scan# 1066  
Delta R.T. -0.000 min  
Lab File: VN086058.D  
Acq: 21 Mar 2025 22:31




Instrument :  
MSVOA\_N  
ClientSampleId :  
RT4534


Tgt Ion:168 Resp: 142558  
Ion Ratio Lower Upper  
168 100  
99 60.3 49.4 74.2

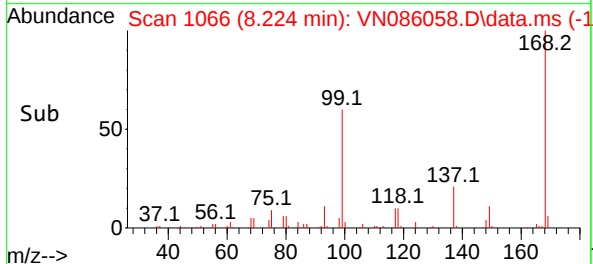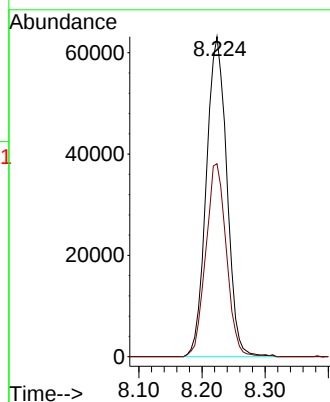

#11  
Tert butyl alcohol  
Concen: 0.698 ug/l  
RT: 5.536 min Scan# 609  
Delta R.T. 0.012 min  
Lab File: VN086058.D  
Acq: 21 Mar 2025 22:31

Tgt Ion: 59 Resp: 193  
Ion Ratio Lower Upper  
59 100  
57 0.0 7.9 11.9#

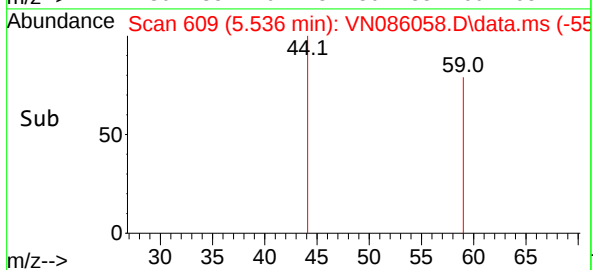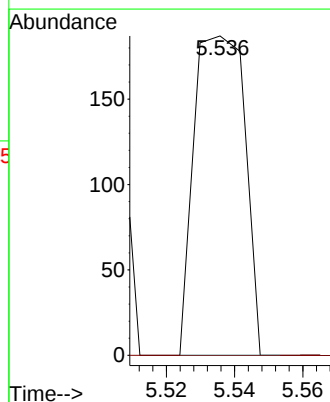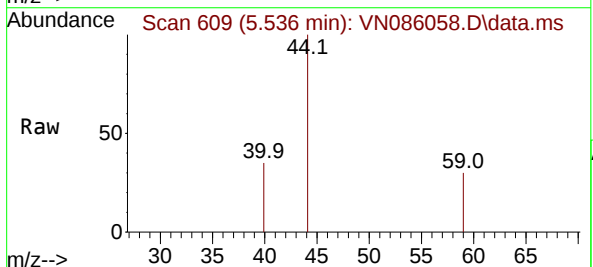



#16

Acetone

Concen: 42.885 ug/l

RT: 4.430 min Scan# 41

Delta R.T. 0.006 min

Lab File: VN086058.D

Acq: 21 Mar 2025 22:31

Instrument :

MSVOA\_N

ClientSampleId :





RT4534

Tgt Ion: 43 Resp: 25576

Ion Ratio Lower Upper

43 100

58 36.4 29.4 44.2

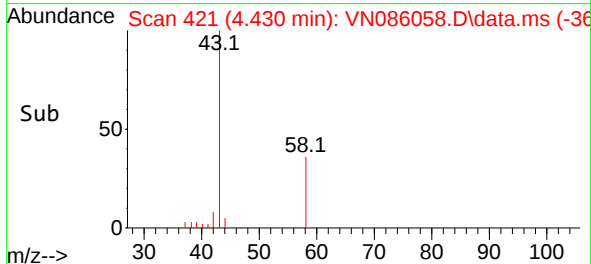

#18

Methyl Acetate

Concen: 1.566 ug/l

RT: 5.030 min Scan# 523

Delta R.T. 0.006 min

Lab File: VN086058.D




Acq: 21 Mar 2025 22:31


Tgt Ion: 43 Resp: 2310

Ion Ratio Lower Upper

43 100

74 21.5 23.9 35.9#


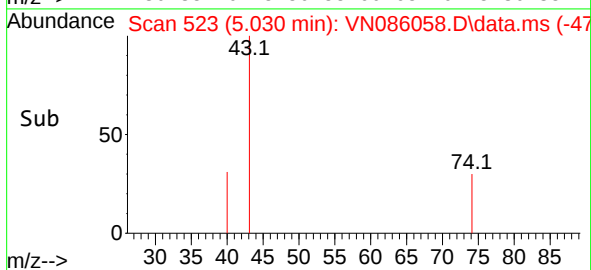

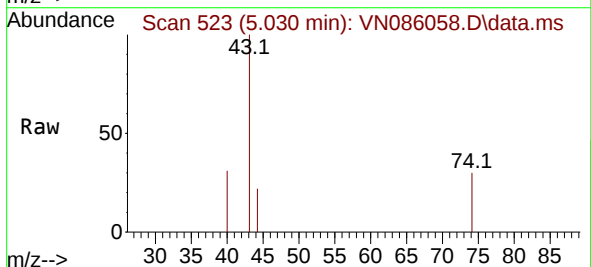


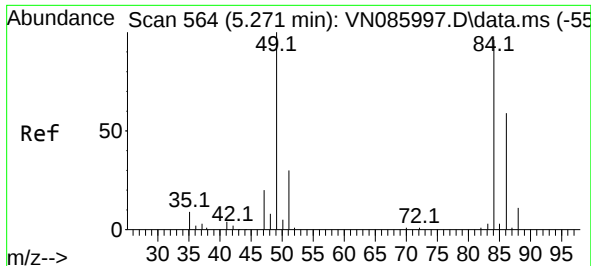

#20  
Methylene Chloride  
Concen: 5.516 ug/l  
RT: 5.277 min Scan# 51  
Delta R.T. 0.006 min  
Lab File: VN086058.D  
Acq: 21 Mar 2025 22:31




Instrument :  
MSVOA\_N  
ClientSampleId :  
RT4534


|             |             |
|-------------|-------------|
| Tgt Ion: 84 | Resp: 9624  |
| Ion Ratio   | Lower Upper |
| 84 100      |             |
| 49 110.6    | 83.3 124.9  |
| 51 32.1     | 24.8 37.2   |
| 86 59.7     | 48.7 73.1   |

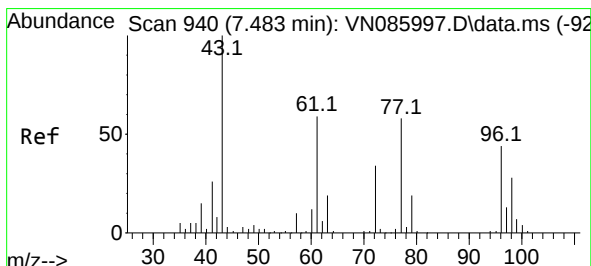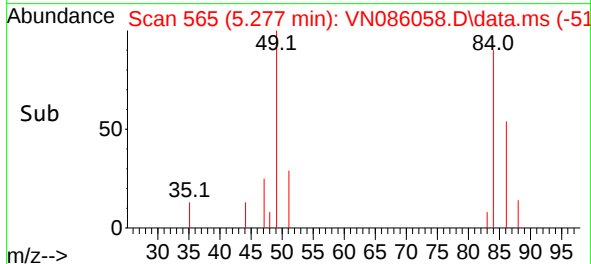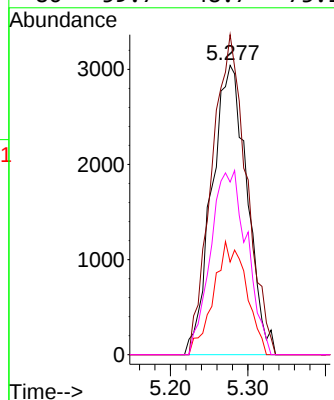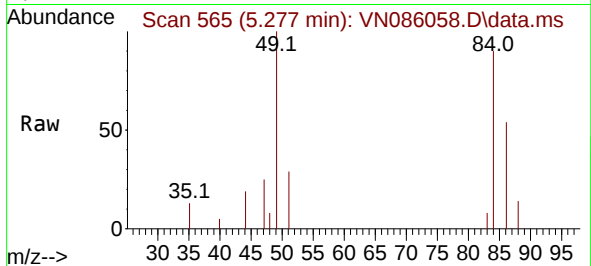

#25  
2-Butanone  
Concen: 4.064 ug/l  
RT: 7.494 min Scan# 942  
Delta R.T. 0.012 min  
Lab File: VN086058.D  
Acq: 21 Mar 2025 22:31

|             |            |       |  |
|-------------|------------|-------|--|
| Tgt Ion: 43 | Resp: 3497 |       |  |
| Ion Ratio   | Lower      | Upper |  |
| 43 100      |            |       |  |
| 72 25.5     | 27.4       | 41.0# |  |

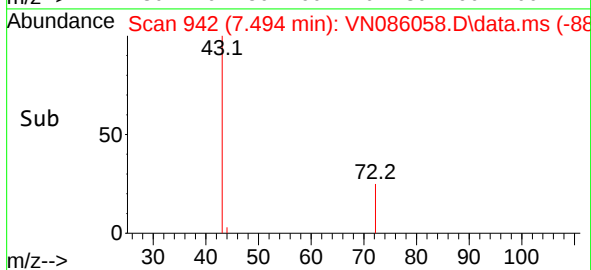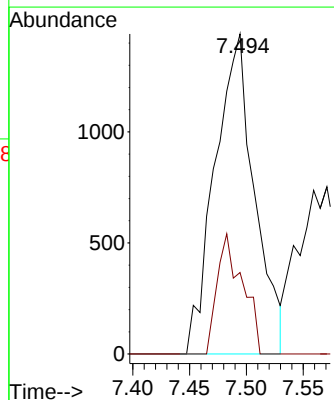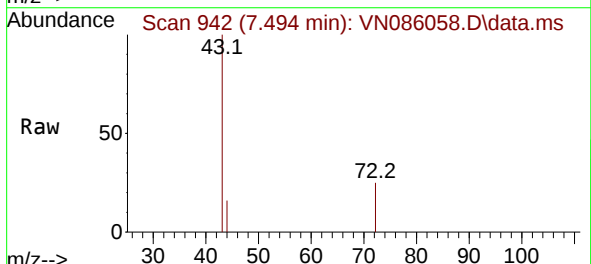



#29

Tetrahydrofuran

Concen: 0.232 ug/l

RT: 7.841 min Scan# 1001

Delta R.T. 0.006 min

Lab File: VN086058.D

Acq: 21 Mar 2025 22:31

Instrument :

MSVOA\_N

ClientSampleId :

RT4534





Tgt Ion: 42 Resp: 123

Ion Ratio Lower Upper

42 100

72 0.0 45.0 67.4#

71 0.0 41.9 62.9#

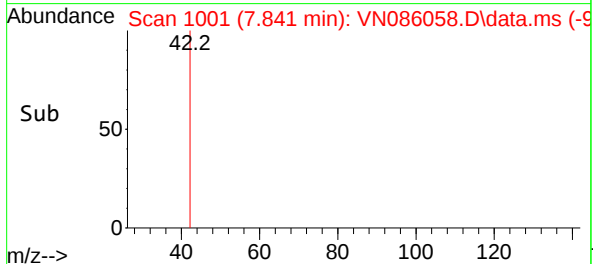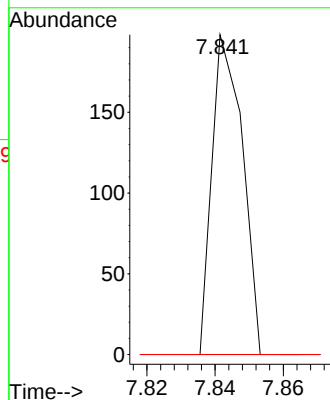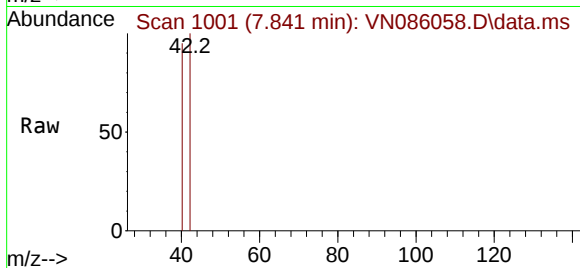

#30

Chloroform

Concen: 0.208 ug/l

RT: 7.965 min Scan# 1022

Delta R.T. -0.000 min

Lab File: VN086058.D




Acq: 21 Mar 2025 22:31


Tgt Ion: 83 Resp: 658

Ion Ratio Lower Upper

83 100


85 44.2 51.5 77.3#

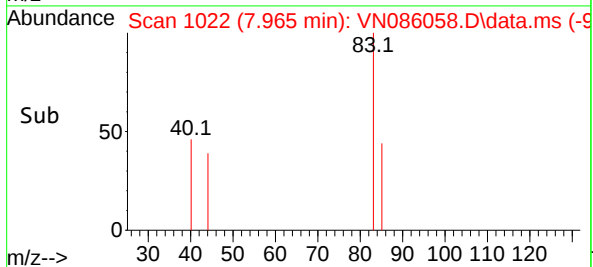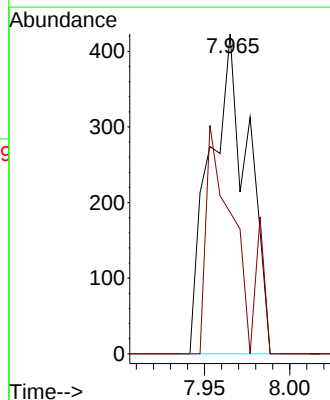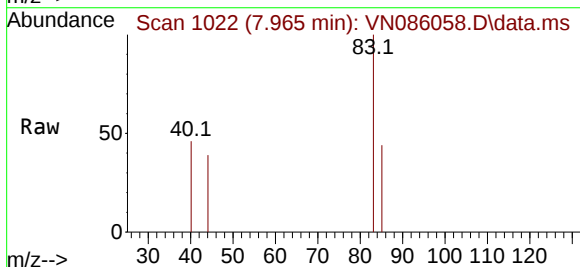






#31  
Cyclohexane  
Concen: 1.304 ug/l  
RT: 8.230 min Scan# 1071  
Delta R.T. -0.024 min  
Lab File: VN086058.D  
Acq: 21 Mar 2025 22:31

Instrument :  
MSVOA\_N  
ClientSampleId :  
RT4534



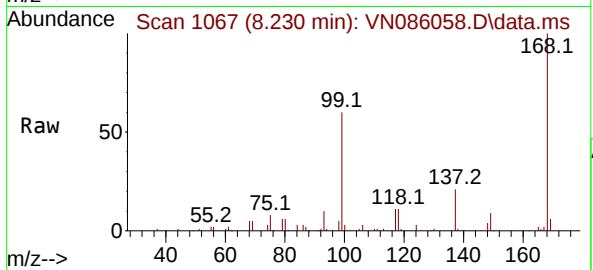



Tgt Ion: 56 Resp: 3171  
Ion Ratio Lower Upper  
56 100  
69 228.6 28.0 42.0#  
84 147.1 75.0 112.6#

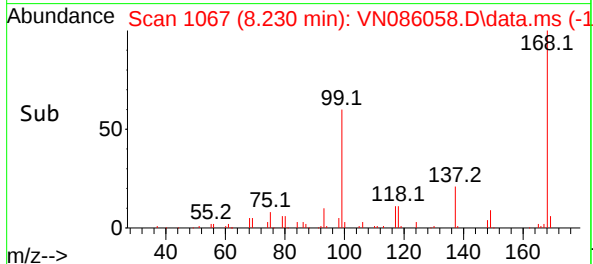

#33  
1,2-Dichloroethane-d4  
Concen: 58.413 ug/l  
RT: 8.577 min Scan# 1126  
Delta R.T. -0.000 min  
Lab File: VN086058.D  
Acq: 21 Mar 2025 22:31

Tgt Ion: 65 Resp: 114028  
Ion Ratio Lower Upper  
65 100  
67 52.4 0.0 102.2

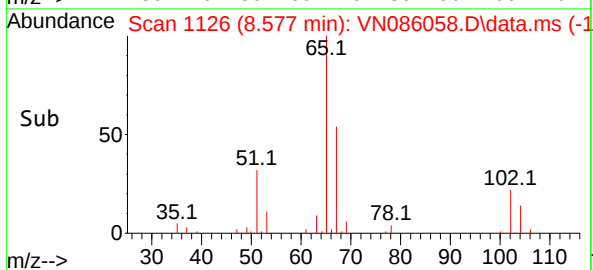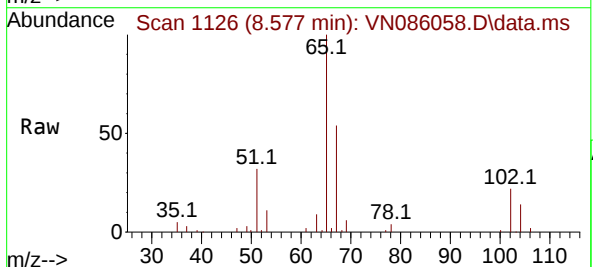



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN086058.D

Acq: 21 Mar 2025 22:31

Instrument :

MSVOA\_N

ClientSampleId :

RT4534





Tgt Ion:114 Resp: 274594

Ion Ratio Lower Upper

114 100

63 19.5 0.0 39.6

88 16.8 0.0 32.6

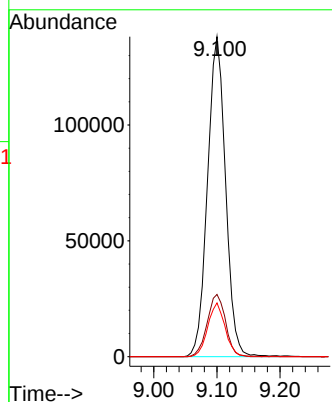

#35

Dibromofluoromethane

Concen: 50.993 ug/l

RT: 8.165 min Scan# 1056

Delta R.T. -0.000 min

Lab File: VN086058.D

Acq: 21 Mar 2025 22:31




Tgt Ion:113 Resp: 97734


Ion Ratio Lower Upper

113 100

111 101.1 81.8 122.8

192 19.1 15.9 23.9

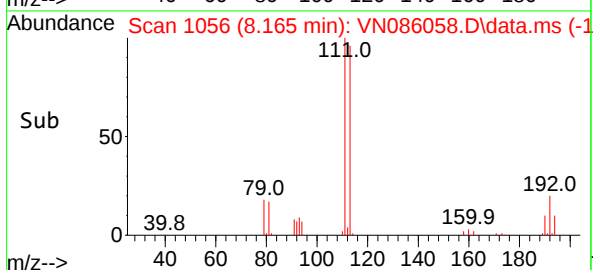



#36

1,1-Dichloropropene

Concen: 4.740 ug/l

RT: 8.224 min Scan# 1066

Delta R.T. -0.141 min

Lab File: VN086058.D

Acq: 21 Mar 2025 22:31

Instrument :

MSVOA\_N

ClientSampleId :

RT4534





Tgt Ion: 75 Resp: 11963

Ion Ratio Lower Upper

75 100

110 8.0 17.8 53.3#

77 0.0 25.0 37.4#

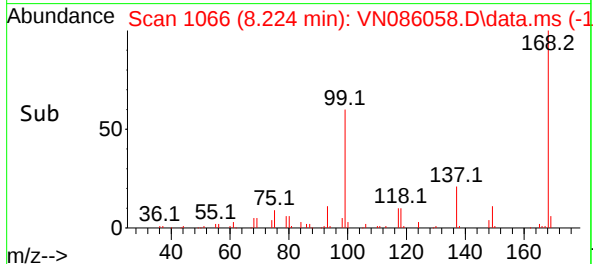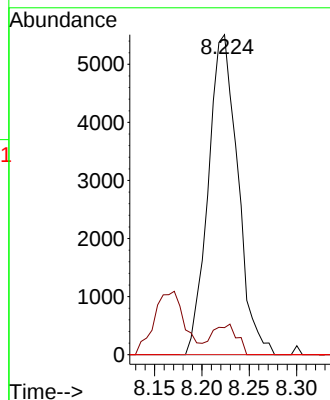

#37

Ethyl Acetate

Concen: 0.914 ug/l

RT: 7.571 min Scan# 955

Delta R.T. 0.012 min

Lab File: VN086058.D

Acq: 21 Mar 2025 22:31




Tgt Ion: 43 Resp: 1945


Ion Ratio Lower Upper

43 100

61 0.0 13.0 19.4#

70 0.0 11.0 16.6#


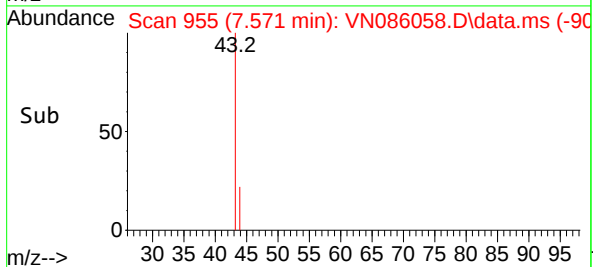
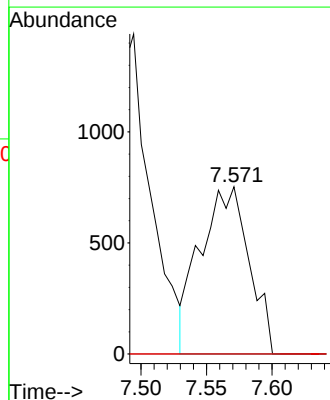
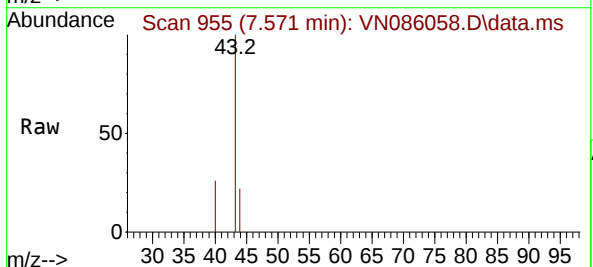




#38  
Carbon Tetrachloride  
Concen: 4.560 ug/l  
RT: 8.218 min Scan# 1065  
Delta R.T. -0.141 min  
Lab File: VN086058.D  
Acq: 21 Mar 2025 22:31




Instrument :  
MSVOA\_N  
ClientSampleId :  
RT4534


Tgt Ion:117 Resp: 15131  
Ion Ratio Lower Upper  
117 100  
119 4.1 77.0 115.4#  
121 0.0 25.6 38.4#

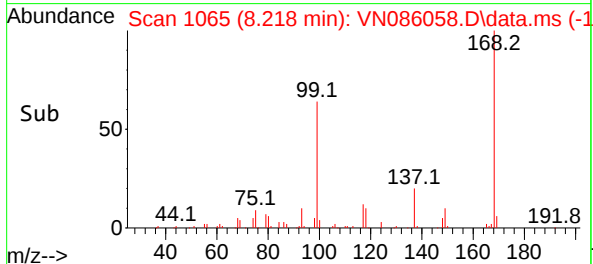

#40  
Benzene  
Concen: 3.059 ug/l  
RT: 8.600 min Scan# 1130  
Delta R.T. -0.006 min  
Lab File: VN086058.D  
Acq: 21 Mar 2025 22:31

Tgt Ion: 78 Resp: 24237  
Ion Ratio Lower Upper  
78 100  
77 21.9 18.9 28.3

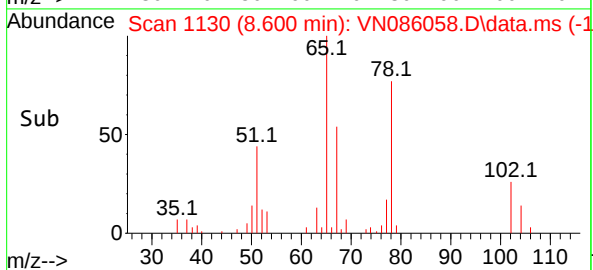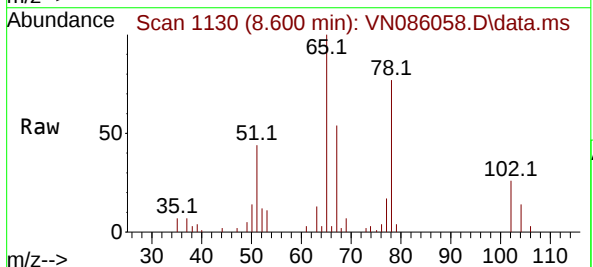



#42

1,2-Dichloroethane

Concen: 0.215 ug/l

RT: 8.683 min Scan# 1144

Delta R.T. 0.012 min

Lab File: VN086058.D

Acq: 21 Mar 2025 22:31

Instrument :

MSVOA\_N

ClientSampleId :





RT4534

Tgt Ion: 62 Resp: 593

Ion Ratio Lower Upper

62 100

98 0.0 0.0 18.6

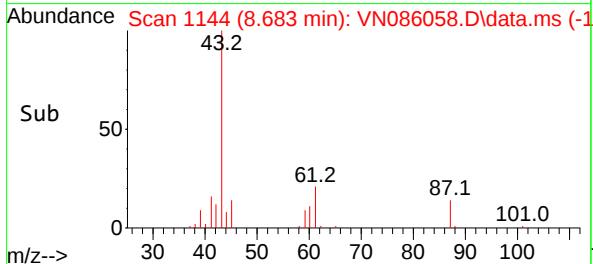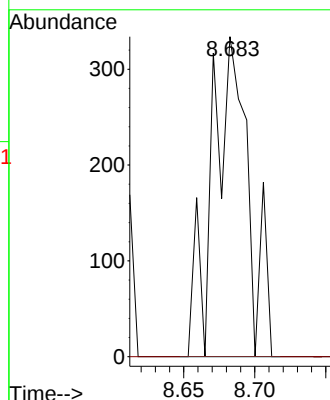

#43

Isopropyl Acetate

Concen: 21.727 ug/l

RT: 8.688 min Scan# 1145

Delta R.T. 0.006 min

Lab File: VN086058.D

Acq: 21 Mar 2025 22:31




Tgt Ion: 43 Resp: 100243


Ion Ratio Lower Upper

43 100

61 17.2 25.0 37.6#

87 11.9 13.0 19.4#

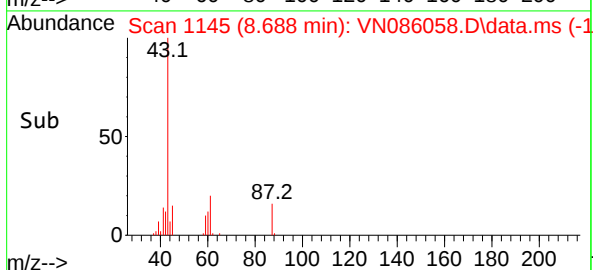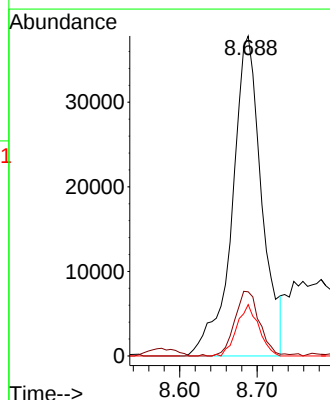



#45

1,2-Dichloropropane

Concen: 0.477 ug/l

RT: 9.735 min Scan# 11

Delta R.T. 0.118 min

Lab File: VN086058.D

Acq: 21 Mar 2025 22:31

Instrument :

MSVOA\_N

ClientSampleId :





RT4534

Tgt Ion: 63 Resp: 860

Ion Ratio Lower Upper

63 100

65 0.0 24.7 37.1#

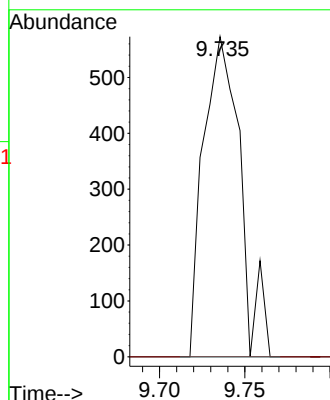

#48

Methyl methacrylate

Concen: 1.421 ug/l

RT: 9.659 min Scan# 1310

Delta R.T. -0.018 min

Lab File: VN086058.D

Acq: 21 Mar 2025 22:31




Tgt Ion: 41 Resp: 2163


Ion Ratio Lower Upper

41 100

69 0.0 83.1 124.7#

39 50.3 45.6 68.4


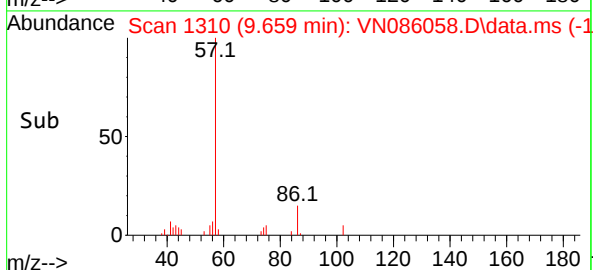
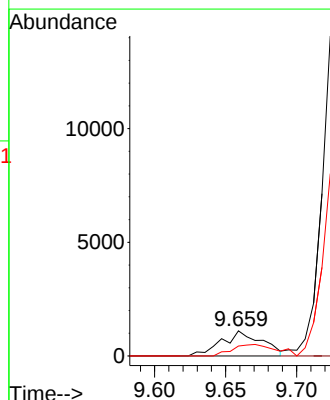





#50  
Toluene-d8  
Concen: 50.347 ug/l  
RT: 10.565 min Scan# 1464  
Delta R.T. -0.000 min  
Lab File: VN086058.D  
Acq: 21 Mar 2025 22:31




Instrument :  
MSVOA\_N  
ClientSampleId :  
RT4534


Tgt Ion: 98 Resp: 350213  
Ion Ratio Lower Upper  
98 100  
100 64.9 53.1 79.7

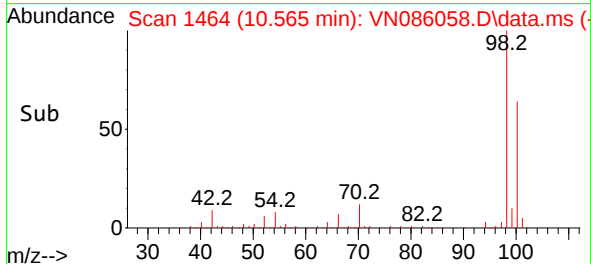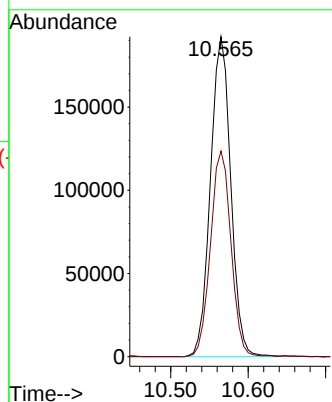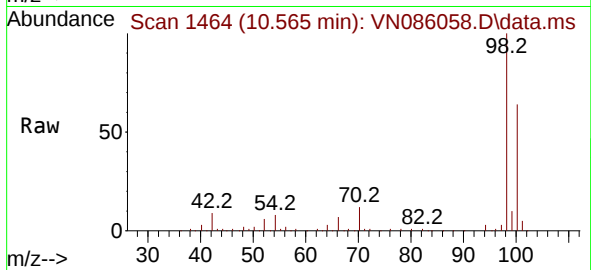

#51  
4-Methyl-2-Pentanone  
Concen: 3.412 ug/l  
RT: 10.441 min Scan# 1443  
Delta R.T. -0.000 min  
Lab File: VN086058.D  
Acq: 21 Mar 2025 22:31

Tgt Ion: 43 Resp: 6943  
Ion Ratio Lower Upper  
43 100  
58 22.2 37.4 56.0#

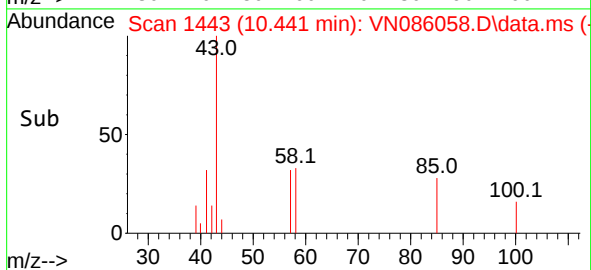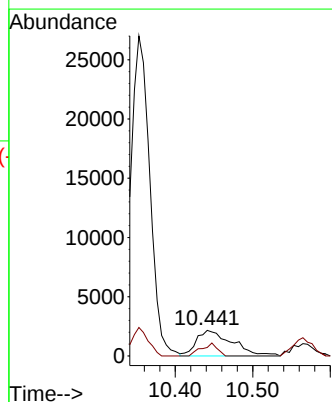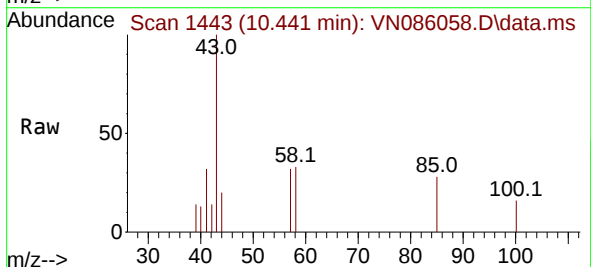

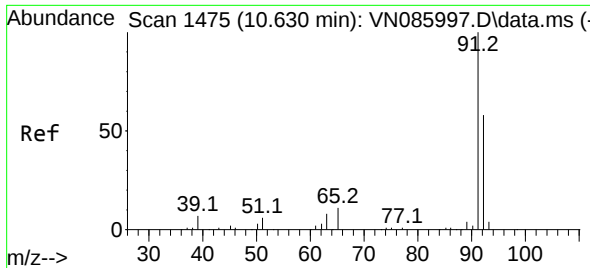

#52

Toluene

Concen: 0.445 ug/l

RT: 10.629 min Scan# 1475

Delta R.T. -0.000 min

Lab File: VN086058.D

Acq: 21 Mar 2025 22:31

Instrument :

MSVOA\_N

ClientSampleId :





RT4534

Tgt Ion: 92 Resp: 2166

Ion Ratio Lower Upper

92 100

91 169.3 136.2 204.4

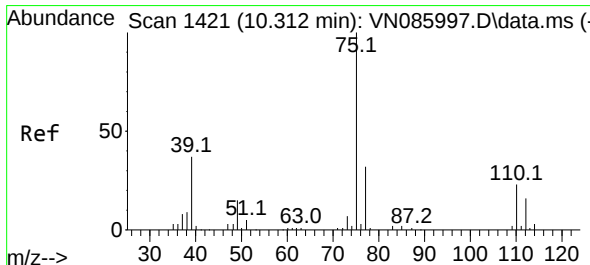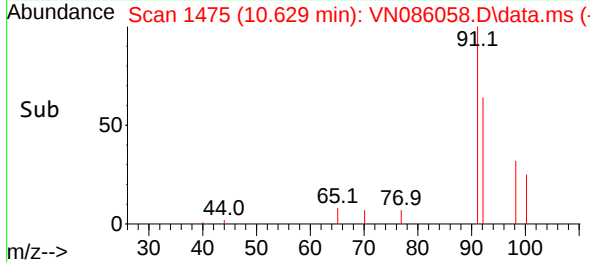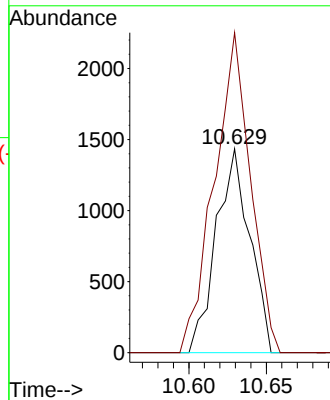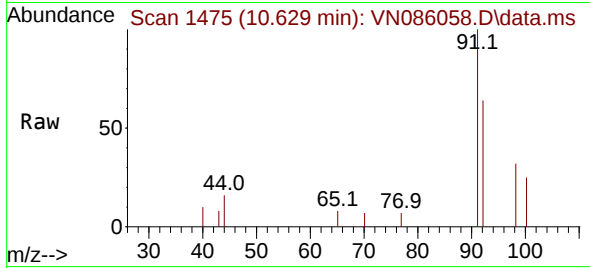

#54

cis-1,3-Dichloropropene

Concen: 8.805 ug/l

RT: 10.353 min Scan# 1428

Delta R.T. 0.041 min

Lab File: VN086058.D

Acq: 21 Mar 2025 22:31




Tgt Ion: 75 Resp: 26719


Ion Ratio Lower Upper

75 100

77 0.0 25.3 37.9#

39 35.0 29.6 44.4


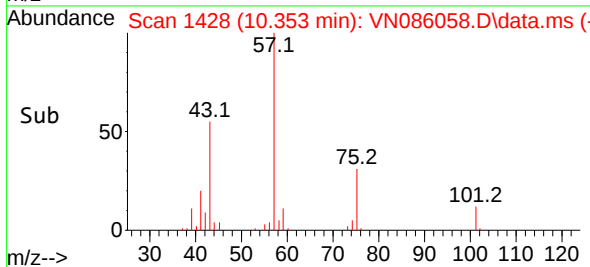
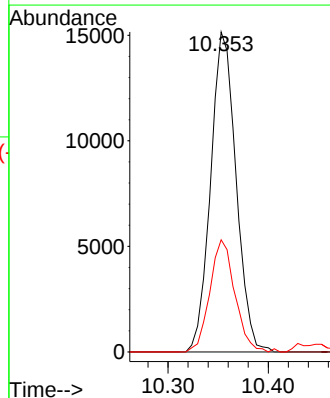
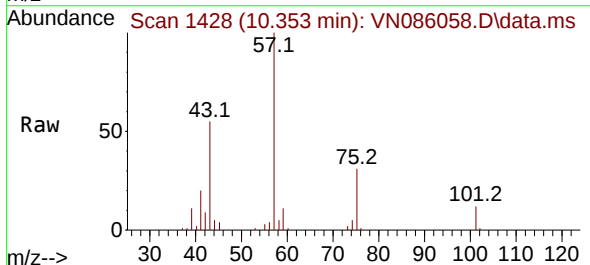


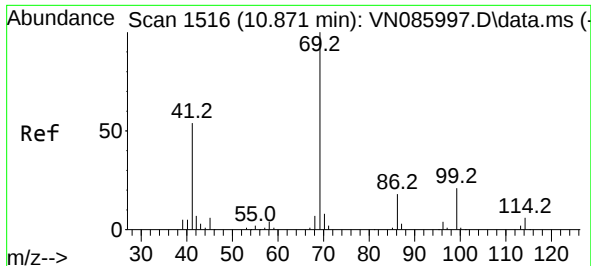

#56  
Ethyl methacrylate  
Concen: 0.803 ug/l  
RT: 10.982 min Scan# 1535  
Delta R.T. 0.111 min  
Lab File: VN086058.D  
Acq: 21 Mar 2025 22:31




Instrument :  
MSVOA\_N  
ClientSampleId :  
RT4534


Tgt Ion: 69 Resp: 1442  
Ion Ratio Lower Upper  
69 100  
41 2188.1 41.6 62.4#  
39 1073.2 21.8 32.8#

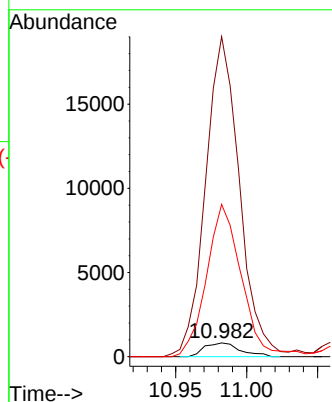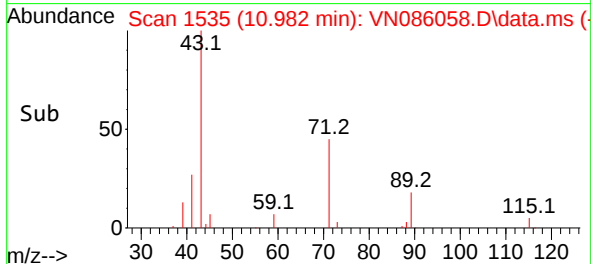

#57  
1,3-Dichloropropane  
Concen: 1.097 ug/l  
RT: 11.200 min Scan# 1572  
Delta R.T. 0.041 min  
Lab File: VN086058.D  
Acq: 21 Mar 2025 22:31

Tgt Ion: 76 Resp: 3458  
Ion Ratio Lower Upper  
76 100  
78 0.0 25.8 38.6#




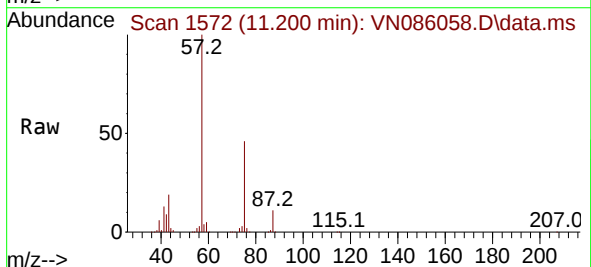


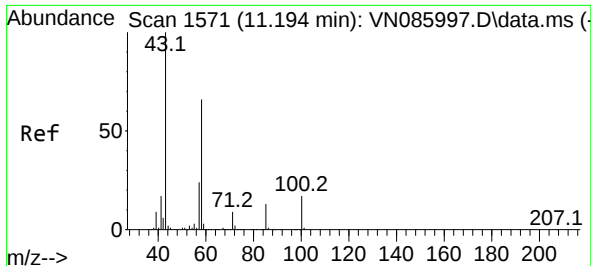

#59  
2-Hexanone  
Concen: 35.757 ug/l  
RT: 11.165 min Scan# 111  
Delta R.T. -0.030 min  
Lab File: VN086058.D  
Acq: 21 Mar 2025 22:31




Instrument :  
MSVOA\_N  
ClientSampleId :  
RT4534


Tgt Ion: 43 Resp: 53002  
Ion Ratio Lower Upper  
43 100  
58 0.0 32.4 97.2#

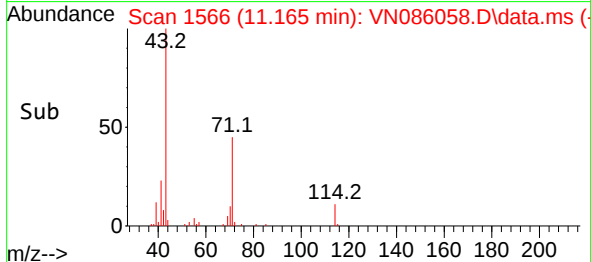

#62  
4-Bromofluorobenzene  
Concen: 42.727 ug/l  
RT: 12.847 min Scan# 1852  
Delta R.T. -0.000 min  
Lab File: VN086058.D  
Acq: 21 Mar 2025 22:31

Tgt Ion: 95 Resp: 105995  
Ion Ratio Lower Upper  
95 100  
174 80.3 0.0 156.8  
176 76.1 0.0 152.2


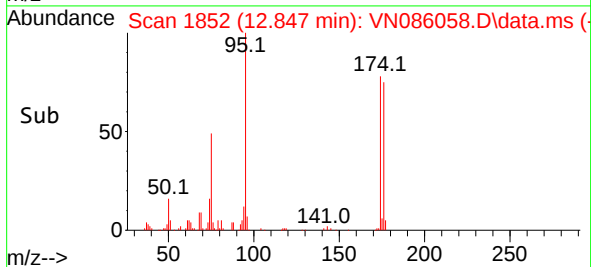

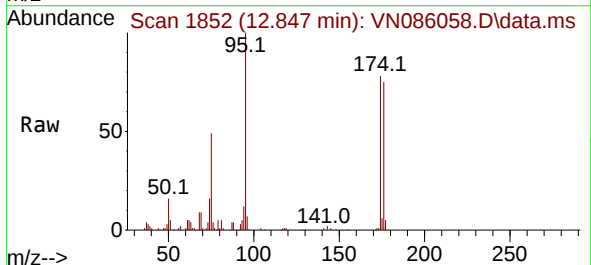




#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 11.865 min Scan# 117  
Delta R.T. -0.000 min  
Lab File: VN086058.D  
Acq: 21 Mar 2025 22:31




Instrument :  
MSVOA\_N  
ClientSampleId :  
RT4534


Tgt Ion:117 Resp: 264941  
Ion Ratio Lower Upper  
117 100  
82 56.0 46.7 70.1  
119 31.5 26.5 39.7

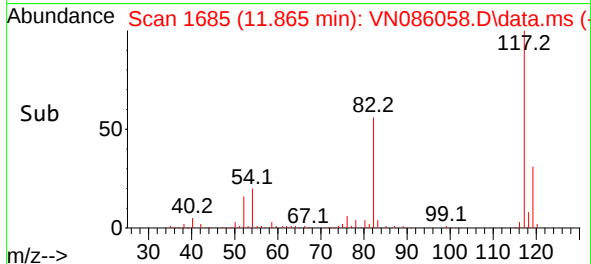

#71  
Bromoform  
Concen: 0.522 ug/l  
RT: 12.847 min Scan# 1852  
Delta R.T. 0.270 min  
Lab File: VN086058.D  
Acq: 21 Mar 2025 22:31

Tgt Ion:173 Resp: 983  
Ion Ratio Lower Upper  
173 100  
175 0.0 24.3 73.0#  
254 0.0 0.0 0.0


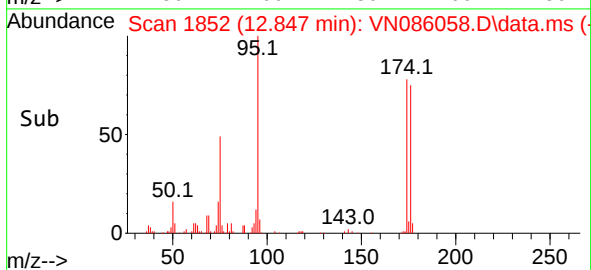

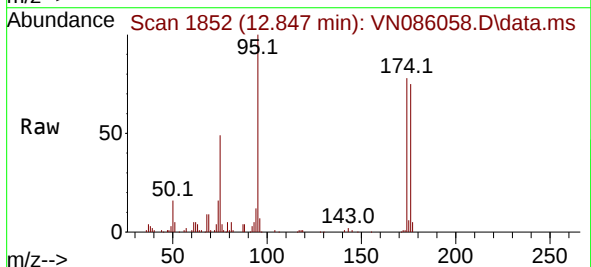


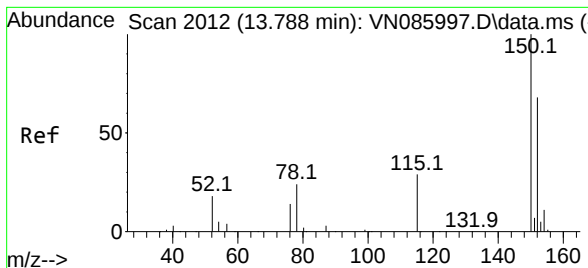

#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 13.788 min Scan# 20  
Delta R.T. -0.000 min  
Lab File: VN086058.D  
Acq: 21 Mar 2025 22:31




Instrument :  
MSVOA\_N  
ClientSampleId :  
RT4534


Tgt Ion:152 Resp: 101760  
Ion Ratio Lower Upper  
152 100  
115 60.4 31.1 93.2  
150 156.9 0.0 359.6

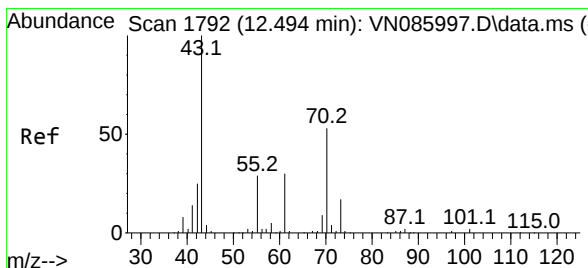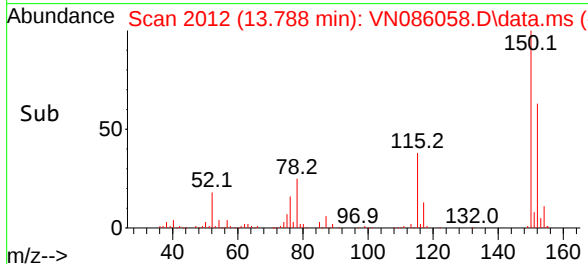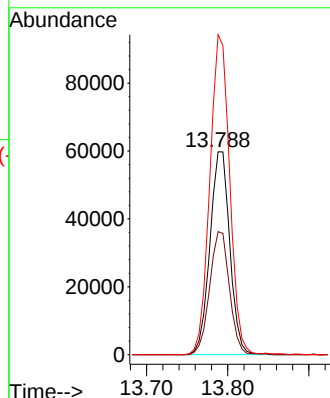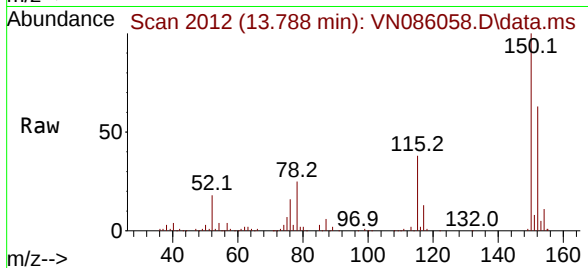

#74  
N-ethyl acetate  
Concen: 0.308 ug/l  
RT: 12.482 min Scan# 1790  
Delta R.T. -0.012 min  
Lab File: VN086058.D  
Acq: 21 Mar 2025 22:31

Tgt Ion: 43 Resp: 715  
Ion Ratio Lower Upper  
43 100  
70 0.0 43.0 64.4#  
55 0.0 23.8 35.8#  
61 0.0 23.4 35.0#


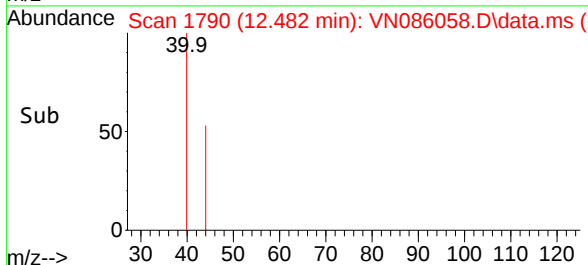
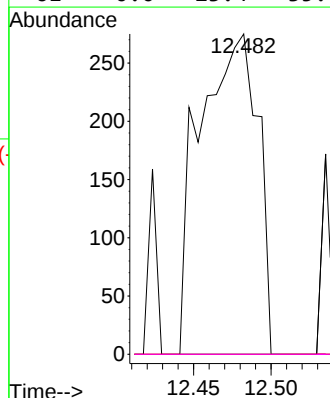
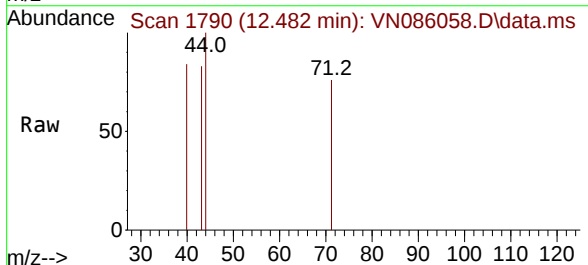


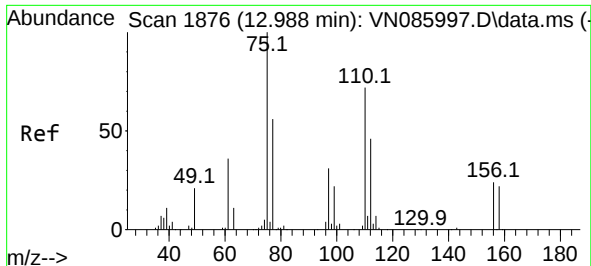

#76  
1,2,3-Trichloropropane  
Concen: 23.004 ug/l  
RT: 12.847 min Scan# 1852  
Delta R.T. -0.141 min  
Lab File: VN086058.D  
Acq: 21 Mar 2025 22:31

Instrument :  
MSVOA\_N  
ClientSampleId :  
RT4534

Tgt Ion: 75 Resp: 52407  
Ion Ratio Lower Upper  
75 100  
77 1.0 83.7 251.0#

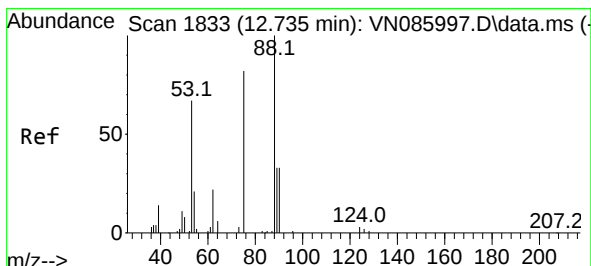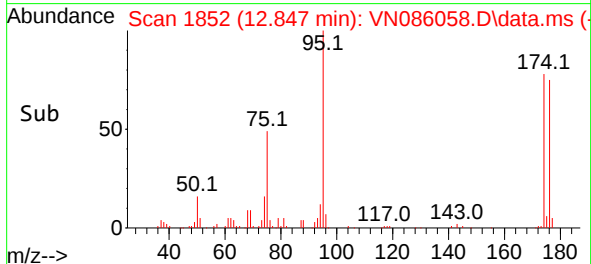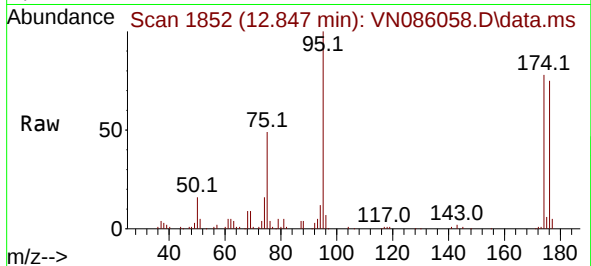

#81  
trans-1,4-Dichloro-2-butene  
Concen: 60.818 ug/l  
RT: 12.847 min Scan# 1852  
Delta R.T. 0.112 min  
Lab File: VN086058.D  
Acq: 21 Mar 2025 22:31

Tgt Ion: 75 Resp: 52407  
Ion Ratio Lower Upper  
75 100  
53 0.3 66.0 99.0#  
89 0.0 36.9 55.3#

