


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032125\
Data File : VN086035.D
Acq On : 21 Mar 2025 12:44
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031825W.M
Title : SW846 8260
Last Update : Wed Mar 19 03:20:56 2025

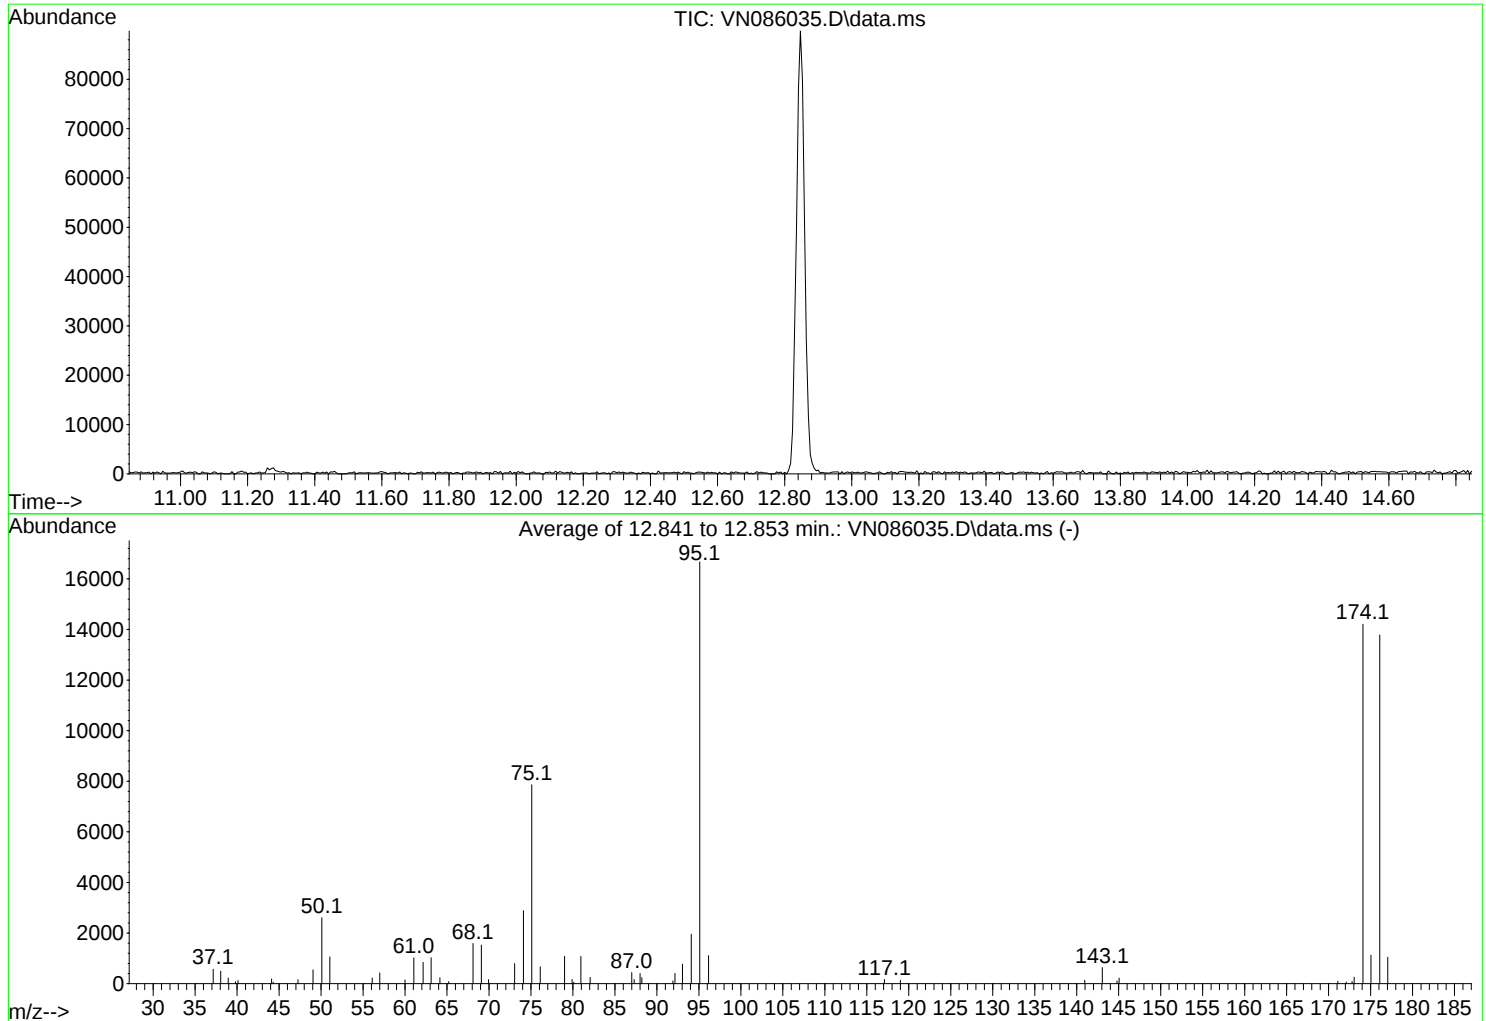

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.6	2609	PASS
75	95	30	60	47.2	7862	PASS
95	95	100	100	100.0	16672	PASS
96	95	5	9	6.6	1105	PASS
173	174	0.00	2	1.8	253	PASS
174	95	50	100	85.2	14208	PASS
175	174	5	9	7.9	1123	PASS
176	174	95	101	97.0	13780	PASS
177	176	5	9	7.6	1044	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
37.15	569	56.10	223	73.05	791	88.00	391
38.05	496	57.00	426	74.10	2885	88.20	234
38.95	221	60.00	144	75.10	7862	91.90	111
39.80	79	61.05	1017	76.10	663	92.15	401
40.10	127	62.15	844	79.00	1082	93.05	773
44.10	181	63.10	1027	79.90	162	94.10	1954
44.30	58	64.15	236	80.10	58	95.10	16672
47.25	160	65.20	83	80.95	1075	96.15	1105
49.05	543	68.10	1589	82.05	248	117.10	164
50.10	2609	69.10	1524	87.00	434	119.00	135
51.05	1057	69.95	161	87.30	164	140.95	136

Average of 12.841 to 12.853 min.: VN086035.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
143.05	632						
144.80	108						
145.05	224						
171.10	98						
172.10	63						
172.80	91						
173.05	253						
174.10	14208						
175.05	1123						
176.10	13780						
177.05	1044						

Instrument :

MSVOA_N

ClientSampleId :

BFB