


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN032219\
 Data File : VN054546.D
 Acq On : 22 Mar 2019 9:00
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N032019W.M
 Title : SW846 8260
 Last Update : Fri Mar 22 02:09:07 2019

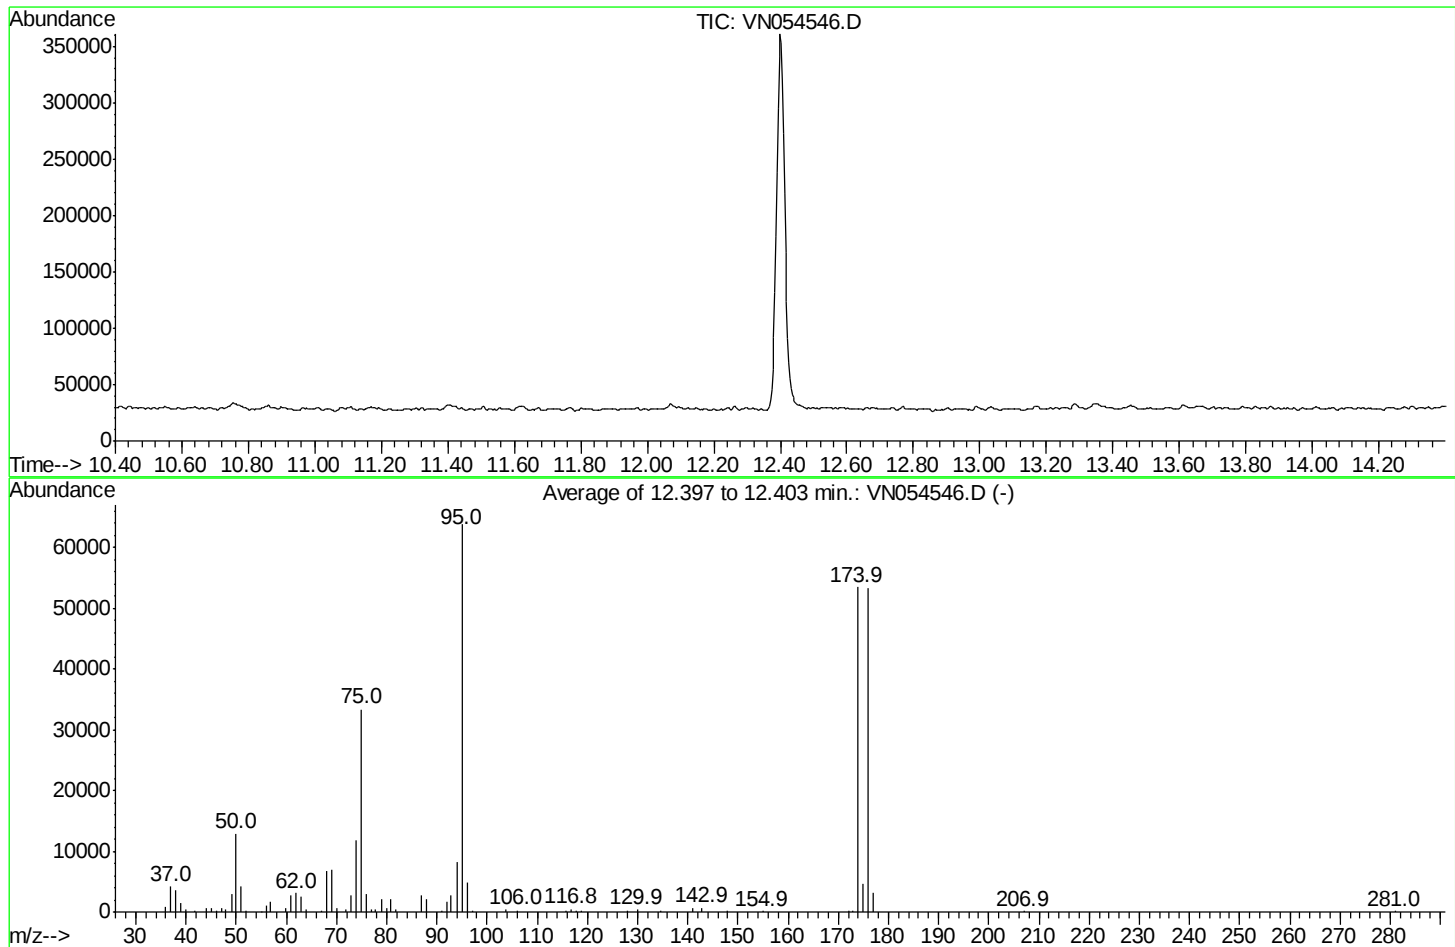

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	12954	PASS
75	95	30	60	52.2	33360	PASS
95	95	100	100	100.0	63856	PASS
96	95	5	9	7.6	4855	PASS
173	174	0.00	2	0.5	282	PASS
174	95	50	100	83.8	53520	PASS
175	174	5	9	8.6	4625	PASS
176	174	95	101	99.6	53298	PASS
177	176	5	9	5.9	3127	PASS