

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032222\
 Data File : VN071458.D
 Acq On : 22 Mar 2022 11:06
 Operator : JC\MD
 Sample : VN0322MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0322MBL01

Quant Time: Mar 23 07:05:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030722W.M
 Quant Title : SW846 8260
 QLast Update : Tue Mar 08 06:52:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.081	168	682104	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.963	114	1156578	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.739	117	1097137	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.674	152	393311	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.434	65	448142	47.937	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	95.880%
35) Dibromofluoromethane	8.016	113	339781	46.555	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	93.120%
50) Toluene-d8	10.439	98	1426487	48.544	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	97.080%
62) 4-Bromofluorobenzene	12.727	95	474332	47.668	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	95.340%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032222\
Data File : VN071458.D
Acq On : 22 Mar 2022 11:06
Operator : JC\MD
Sample : VN0322MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0322MBL01

Quant Time: Mar 23 07:05:52 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030722W.M
Quant Title : SW846 8260
QLast Update : Tue Mar 08 06:52:46 2022
Response via : Initial Calibration

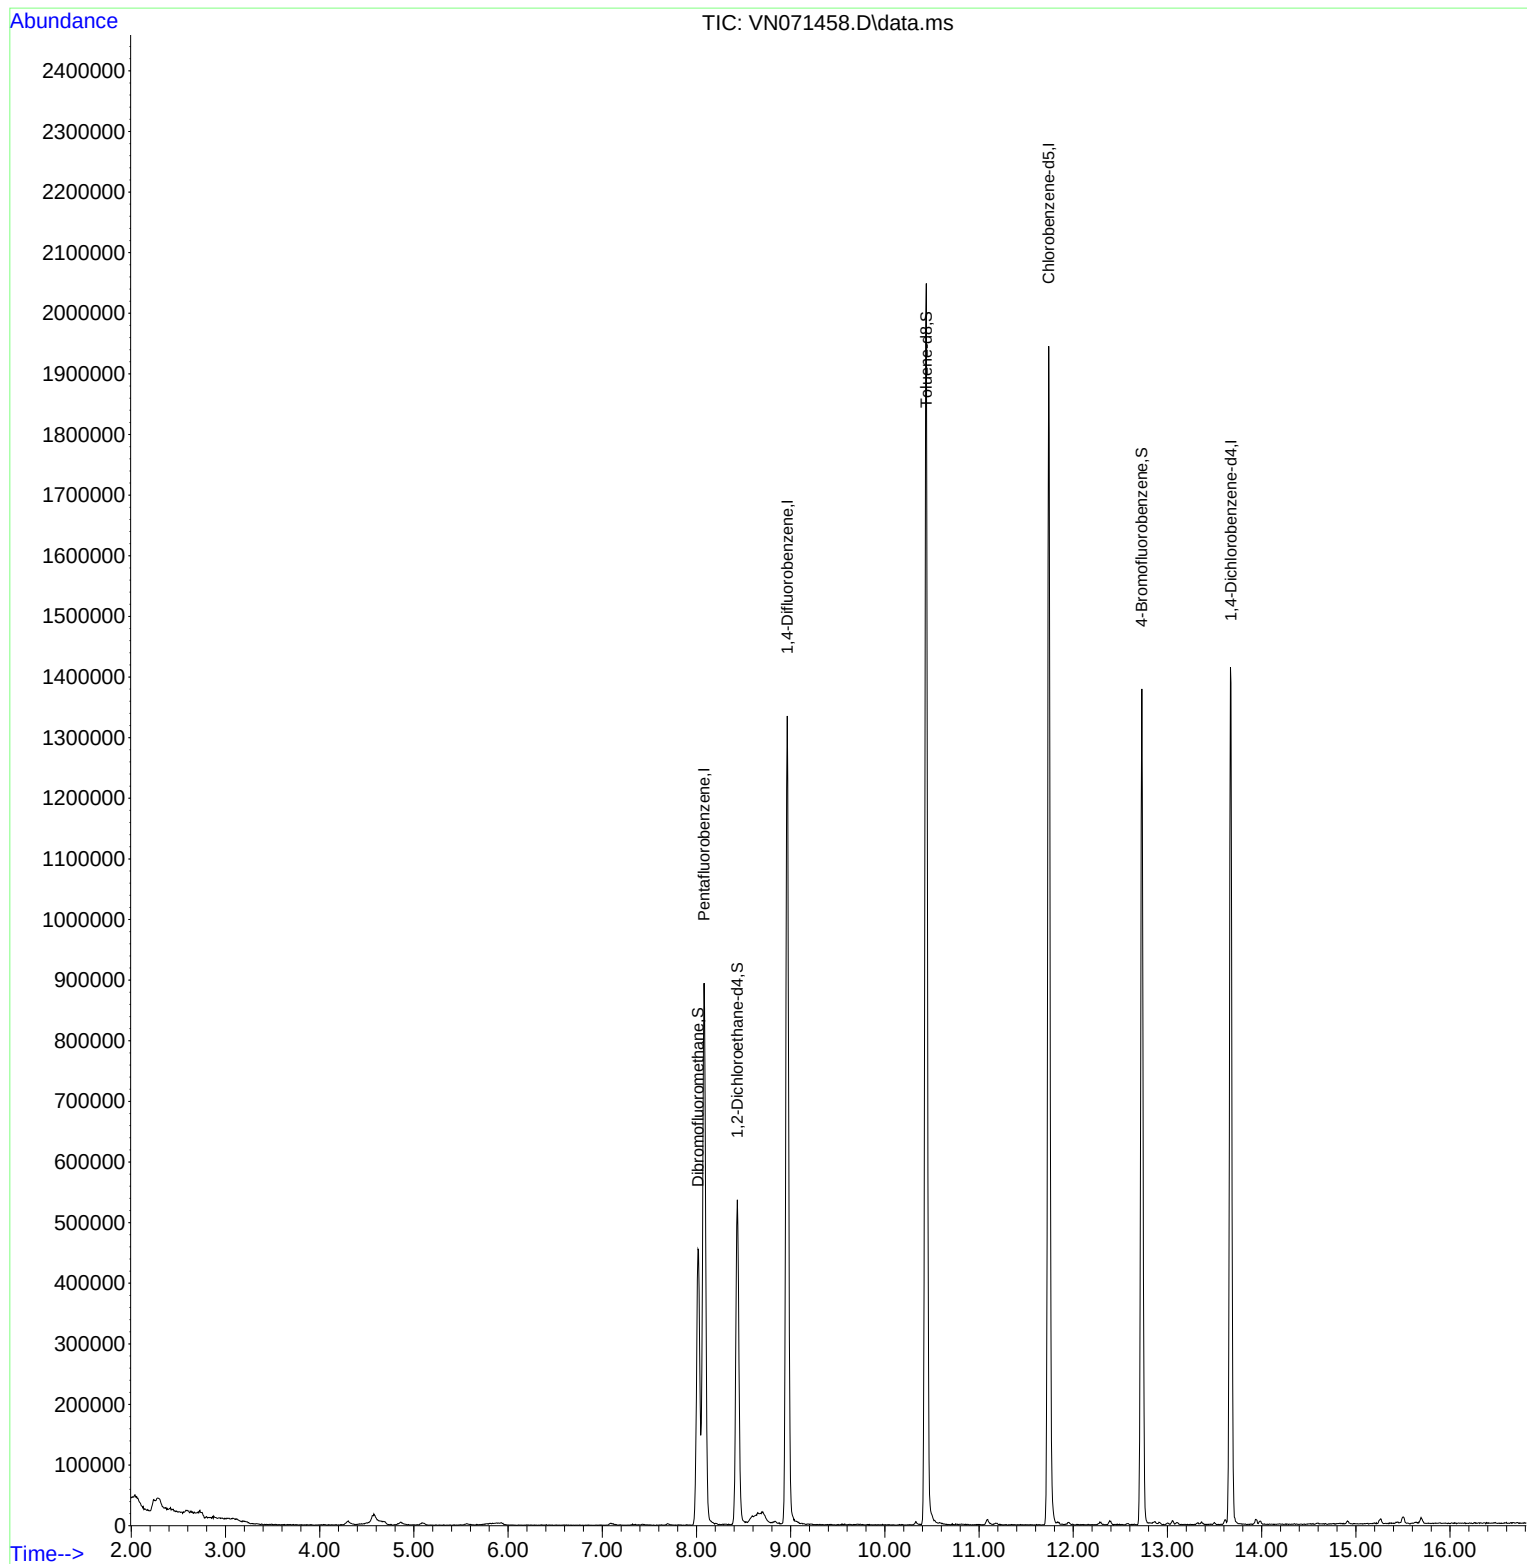

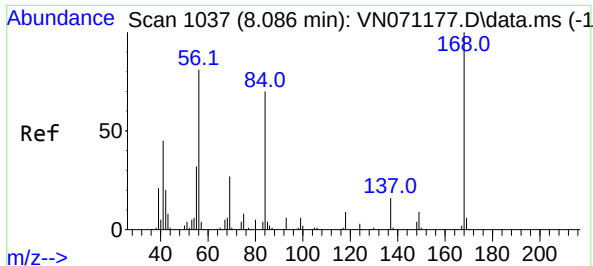

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.081 min Scan# 1

Delta R.T. -0.005 min

Lab File: VN071458.D

Acq: 22 Mar 2022 11:06

Instrument :

MSVOA_N

ClientSampleId :





VN0322MBL01

Tgt Ion:168 Resp: 682104

Ion Ratio Lower Upper

168 100

99 59.5 41.3 61.9

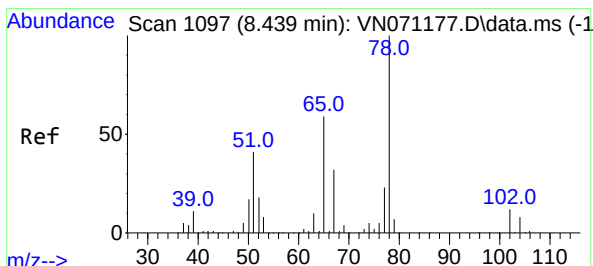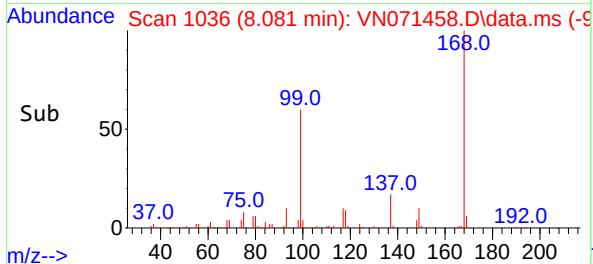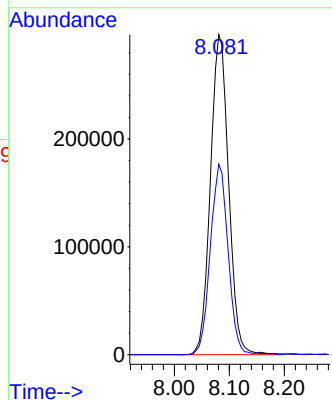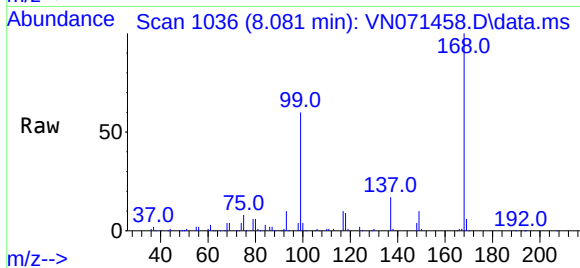

1,2-Dichloroethane-d4

Concen: 47.937 ug/l

RT: 8.434 min Scan# 1096

Delta R.T. -0.006 min

Lab File: VN071458.D




Acq: 22 Mar 2022 11:06


Tgt Ion: 65 Resp: 448142

Ion Ratio Lower Upper

65 100

67 51.9 0.0 103.0


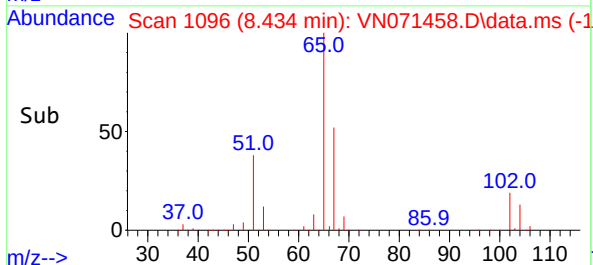
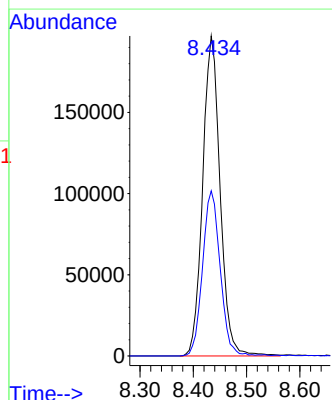
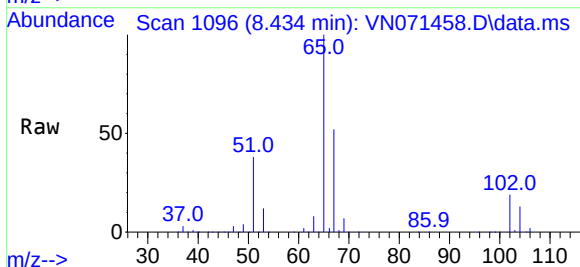


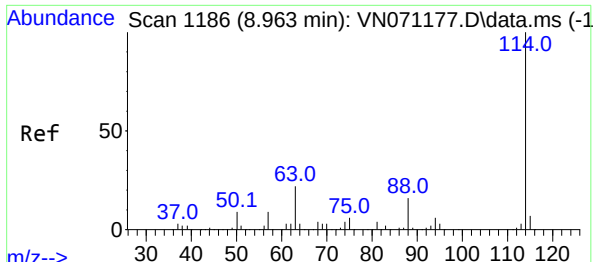

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.963 min Scan# 1186
Delta R.T. -0.000 min
Lab File: VN071458.D
Acq: 22 Mar 2022 11:06




Instrument :
MSVOA_N
ClientSampleId :
VN0322MBL01


Tgt Ion:114 Resp: 1156578
Ion Ratio Lower Upper
114 100
63 21.8 0.0 37.8
88 16.2 0.0 27.4

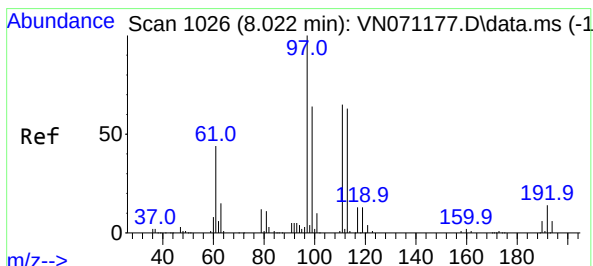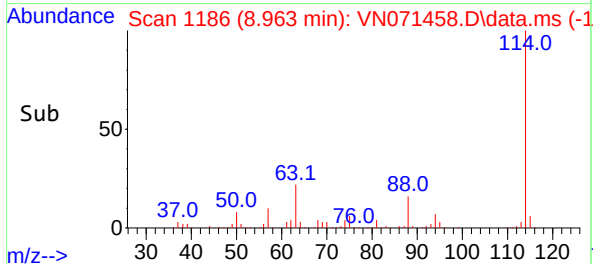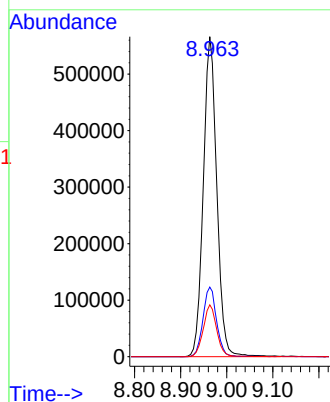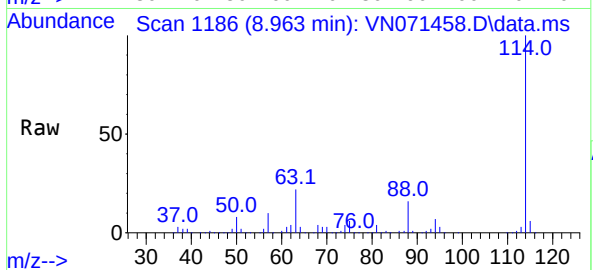

#35
Dibromofluoromethane
Concen: 46.555 ug/l
RT: 8.016 min Scan# 1025
Delta R.T. -0.006 min
Lab File: VN071458.D
Acq: 22 Mar 2022 11:06

Tgt Ion:113 Resp: 339781
Ion Ratio Lower Upper
113 100
111 103.8 82.2 123.2
192 20.5 16.9 25.3


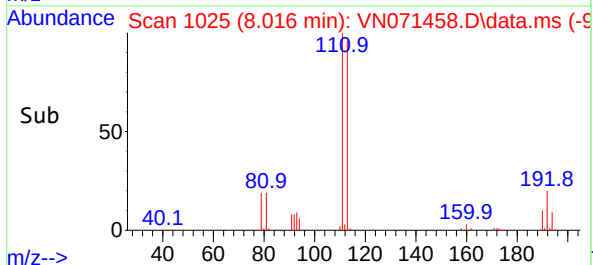
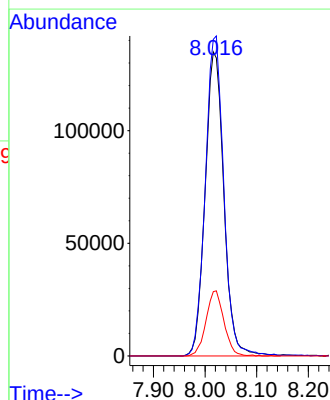
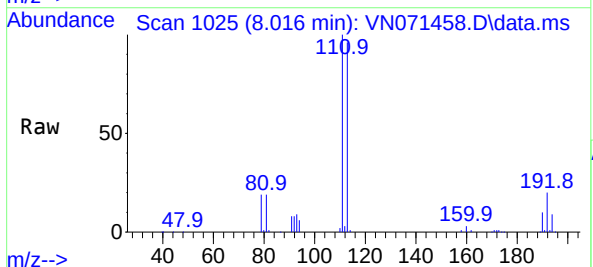


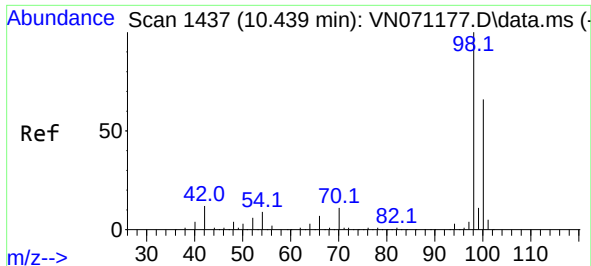

#50
Toluene-d8
Concen: 48.544 ug/l
RT: 10.439 min Scan# 1437
Delta R.T. 0.000 min
Lab File: VN071458.D
Acq: 22 Mar 2022 11:06




Instrument :
MSVOA_N
ClientSampleId :
VN0322MBL01


Tgt Ion: 98 Resp: 1426487
Ion Ratio Lower Upper
98 100
100 65.1 50.4 75.6

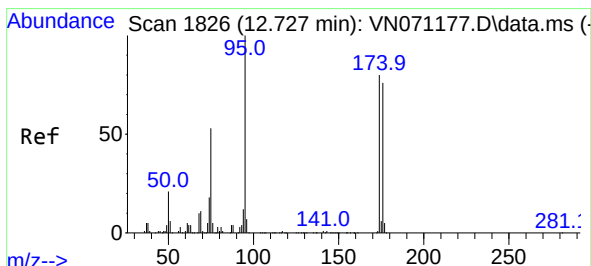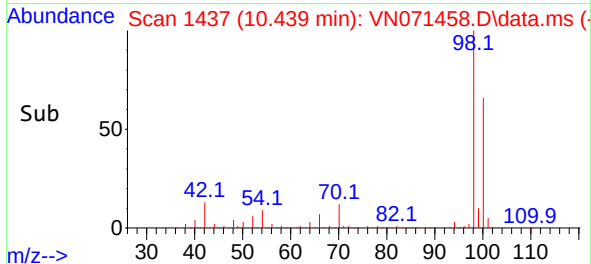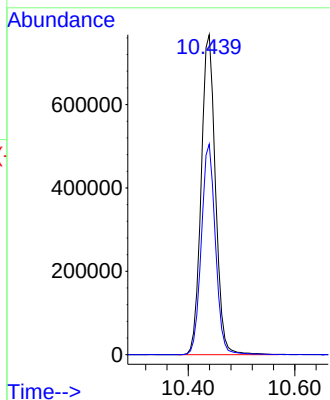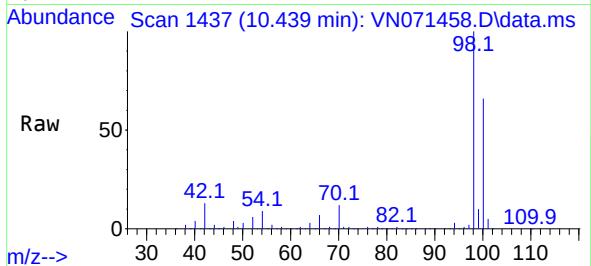

#62
4-Bromofluorobenzene
Concen: 47.668 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.000 min
Lab File: VN071458.D
Acq: 22 Mar 2022 11:06

Tgt Ion: 95 Resp: 474332
Ion Ratio Lower Upper
95 100
174 78.7 0.0 187.2
176 75.7 0.0 181.4


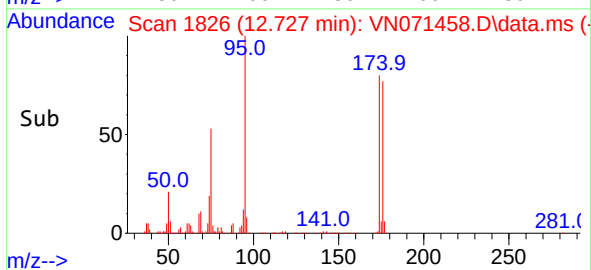
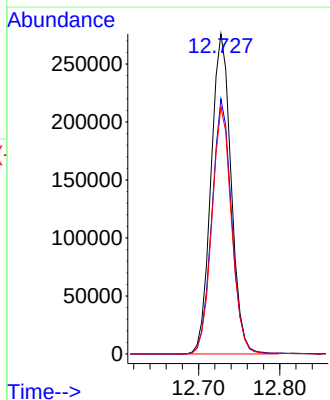
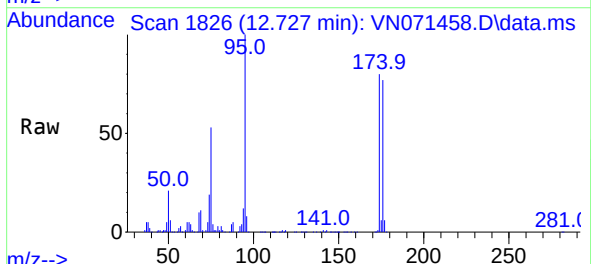


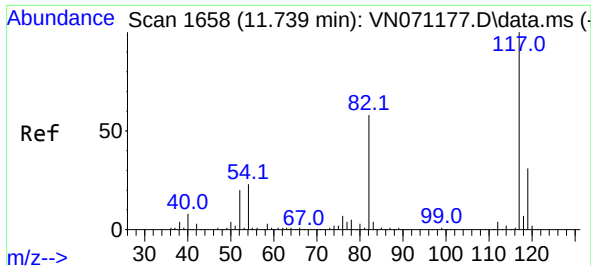

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.739 min Scan# 117
Delta R.T. 0.000 min
Lab File: VN071458.D
Acq: 22 Mar 2022 11:06

Instrument :
MSVOA_N
ClientSampleId :
VN0322MBL01

Tgt Ion:117 Resp: 1097137
Ion Ratio Lower Upper
117 100
82 58.5 42.4 63.6
119 32.3 25.4 38.2

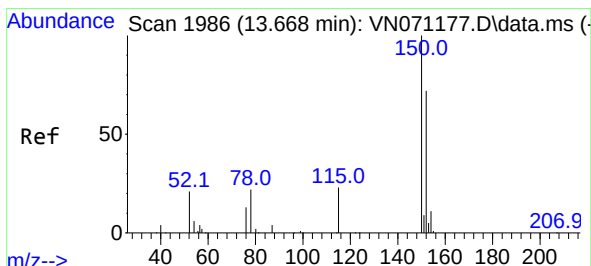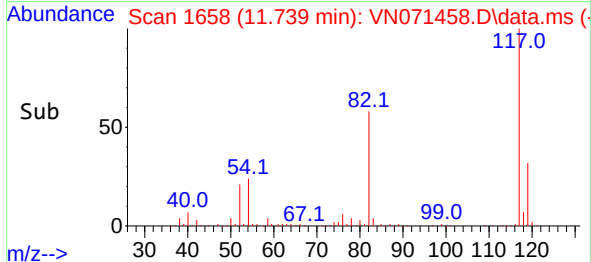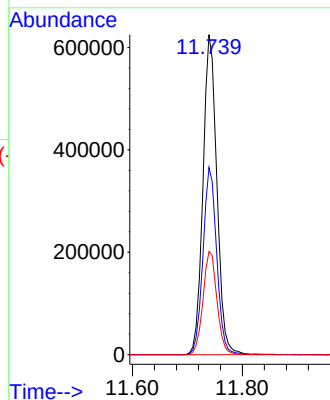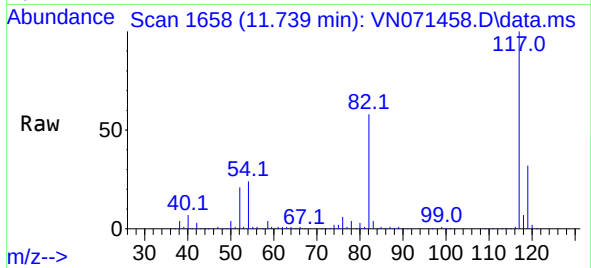

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.674 min Scan# 1987
Delta R.T. 0.006 min
Lab File: VN071458.D
Acq: 22 Mar 2022 11:06

Tgt Ion:152 Resp: 393311
Ion Ratio Lower Upper
152 100
115 58.0 27.5 82.5
150 155.8 0.0 344.4

