

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN032319\
 Data File : VN054599.D
 Acq On : 23 Mar 2019 12:47
 Operator : JC/SP
 Sample : K1912-16
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 TB-20190313

Quant Time: Mar 25 04:00:56 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N032019W.M
 Quant Title : SW846 8260
 QLast Update : Fri Mar 22 02:09:07 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.66	168	654743	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	985925	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	813478	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.34	152	278302	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.03	65	425582	52.26	ug/l	0.00
Spiked Amount	50.000		Recovery	=	104.52%	
35) Dibromofluoromethane	7.59	113	328370	51.70	ug/l	0.00
Spiked Amount	50.000		Recovery	=	103.40%	
50) Toluene-d8	10.09	98	1257437	52.66	ug/l	0.00
Spiked Amount	50.000		Recovery	=	105.32%	
62) 4-Bromofluorobenzene	12.40	95	378178	46.54	ug/l	0.00
Spiked Amount	50.000		Recovery	=	93.08%	


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN032319\
Data File : VN054599.D
Acq On : 23 Mar 2019 12:47
Operator : JC/SP
Sample : K1912-16
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
TB-20190313

Quant Time: Mar 25 04:00:56 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N032019W.M
Quant Title : SW846 8260
QLast Update : Fri Mar 22 02:09:07 2019
Response via : Initial Calibration

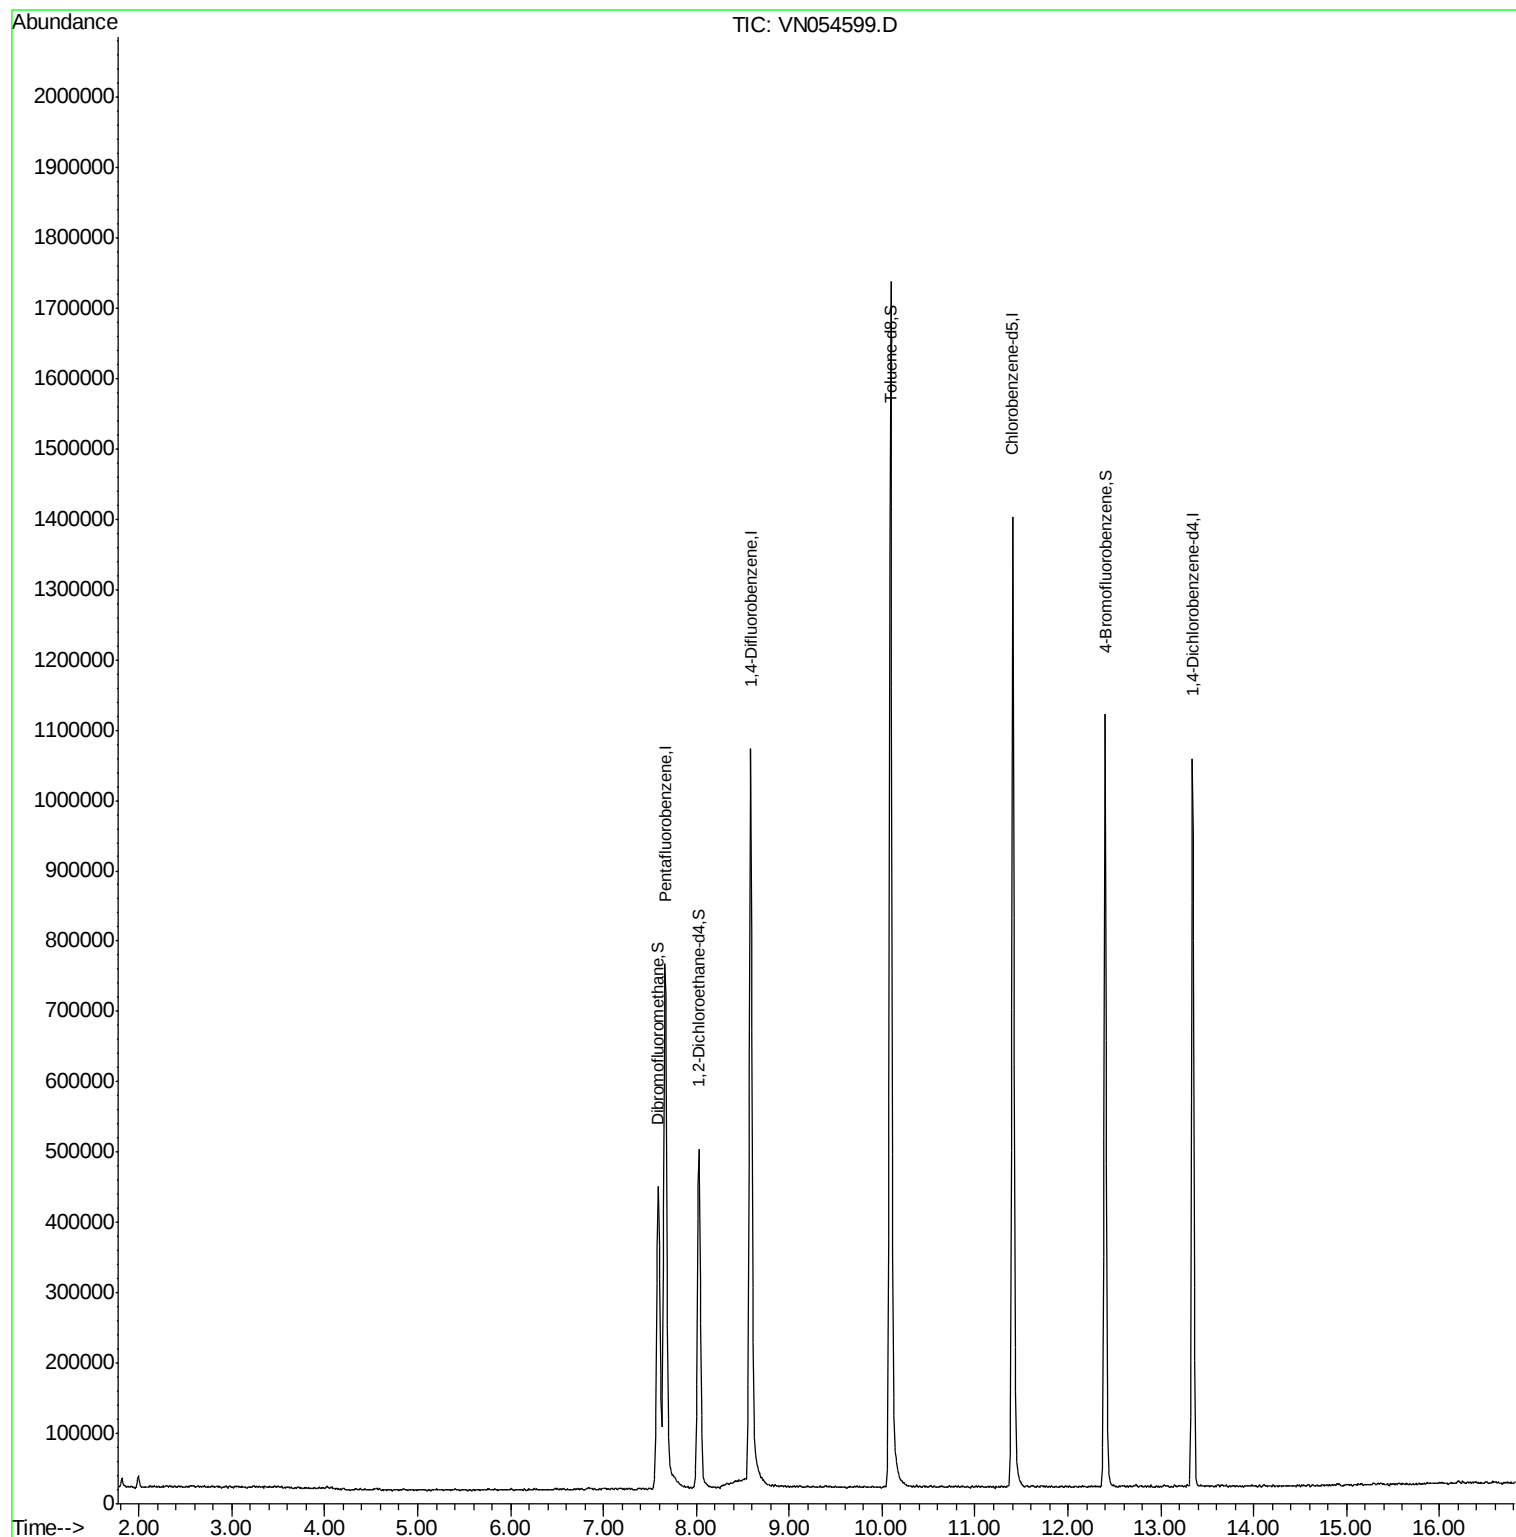



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.66 min Scan# 1832

Delta R.T. -0.00 min

Lab File: VN054599.D

Acq: 23 Mar 2019 12:47

Instrument :

MSVOA_N

ClientSampleId :


TB-20190313

Tot Ion:168 Resp: 654743

Ion Ratio Lower Upper

168 100

99 55.1 37.1 55.7

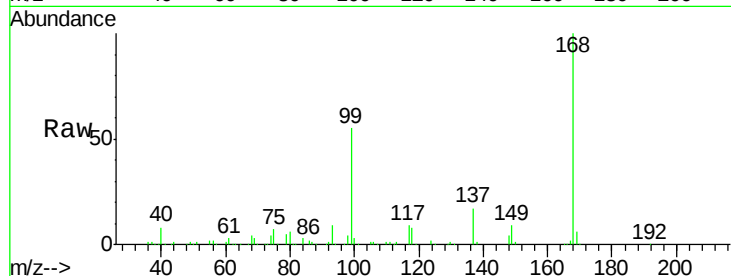

Abundance Ion 167.90 (167.60 to 168.60): VN054459.D (-1813) (-)

Ion 98.90 (98.60 to 99.60): VN054459.D (-1813) (-)

7.66

250000

200000



150000

100000

50000

0

Time--> 7.50 7.60 7.70 7.80 7.90

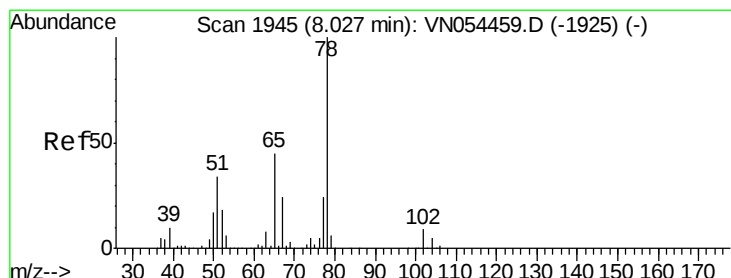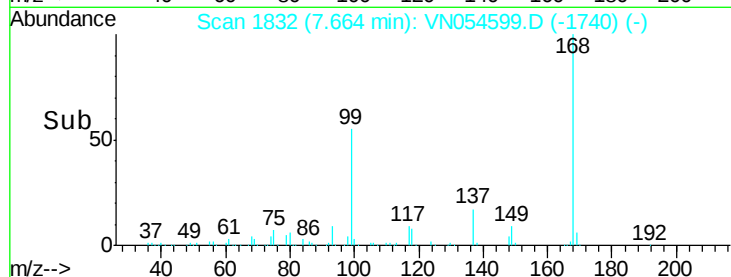

#33

1,2-Dichloroethane-d4

Concen: 52.257 ug/l

RT: 8.03 min Scan# 1945

Delta R.T. -0.00 min

Lab File: VN054599.D


Acq: 23 Mar 2019 12:47

Tgt Ion: 65 Resp: 425582

Ion Ratio Lower Upper

65 100

67 52.5 0.0 104.6

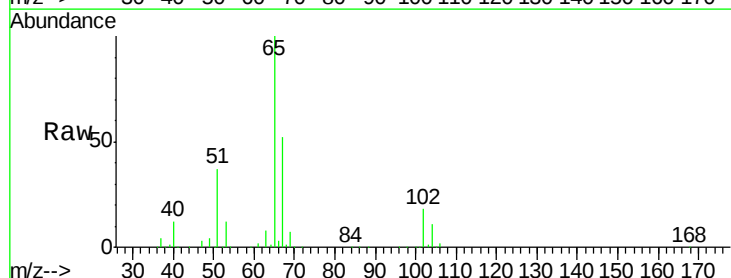

Abundance Ion 64.90 (64.60 to 65.60): VN054459.D (-1925) (-)

Ion 66.90 (66.60 to 67.60): VN054459.D (-1925) (-)

8.03

200000


150000


100000

50000

0

Time--> 7.90 8.00 8.10 8.20

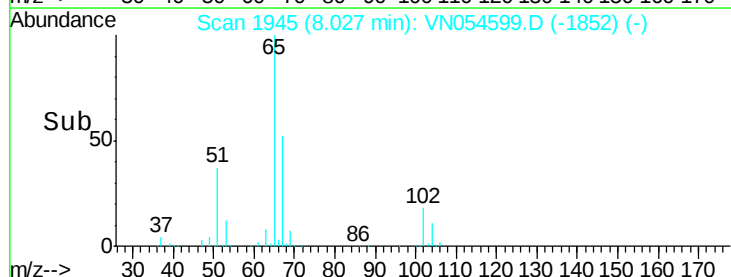

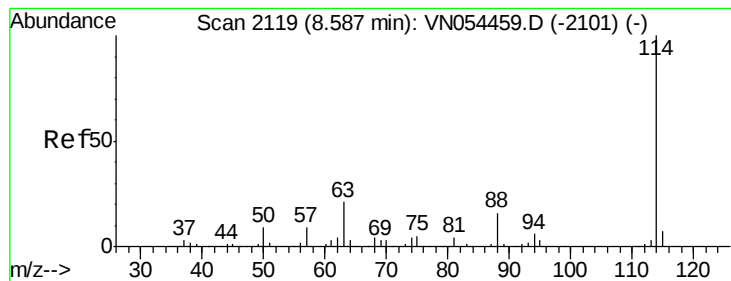

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.59 min Scan# 2119

Delta R.T. -0.00 min

Lab File: VN054599.D

Acq: 23 Mar 2019 12:47

Instrument :

MSVOA_N

ClientSampleId :

TB-20190313


Tot Ion:114 Resp: 985925

Ion Ratio Lower Upper

114 100

63 22.1 0.0 35.2




88 15.9 0.0 30.2

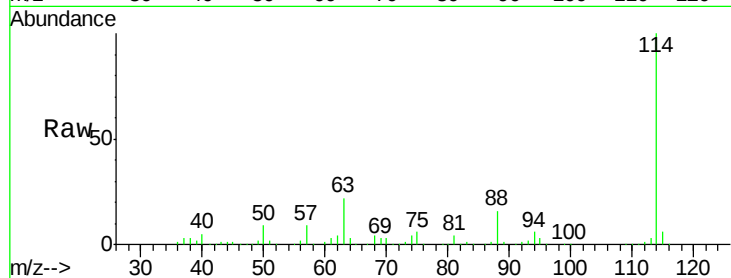

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VN0

Ion 87.90 (87.60 to 88.60): VN0

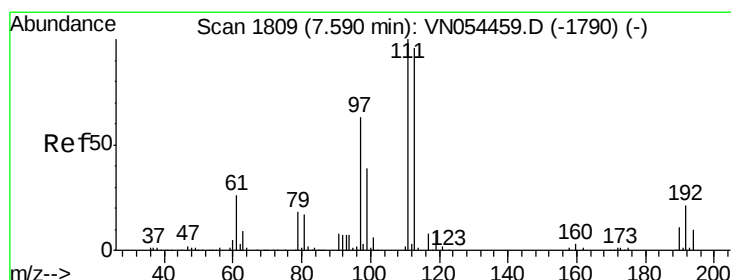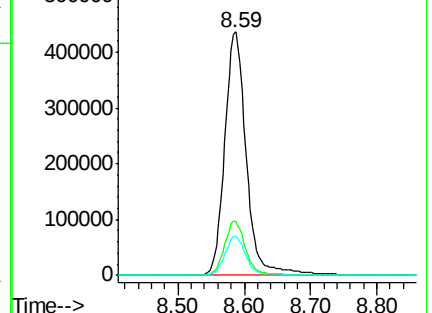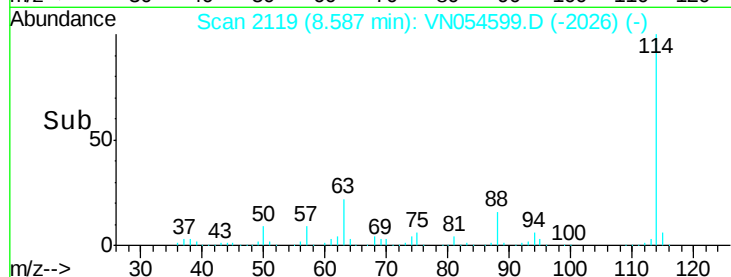

#35

Dibromofluoromethane

Concen: 51.697 ug/l

RT: 7.59 min Scan# 1809

Delta R.T. -0.00 min

Lab File: VN054599.D

Acq: 23 Mar 2019 12:47


Tgt Ion:113 Resp: 328370

Ion Ratio Lower Upper

113 100

111 102.7 82.2 123.4



192 20.5 19.2 28.8

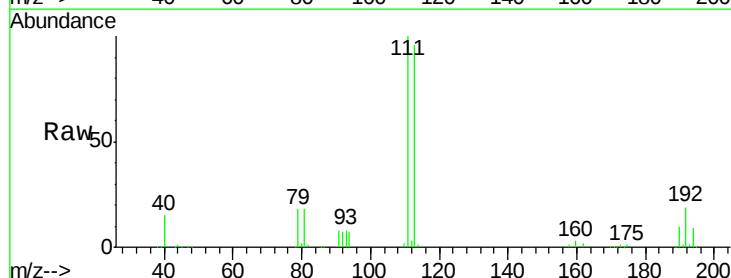


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

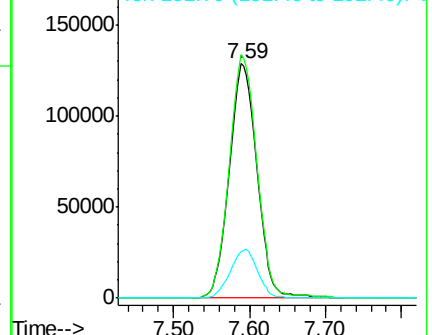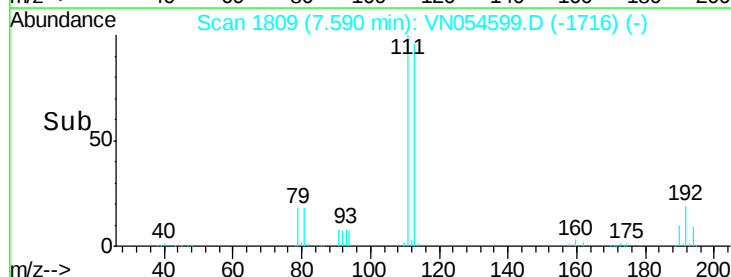

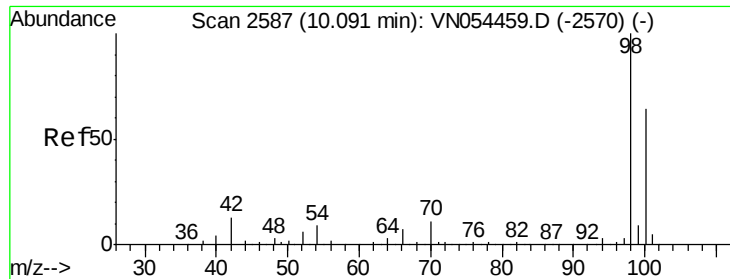

#50

Toluene-d8

Concen: 52.659 ug/l

RT: 10.09 min Scan# 2587

Delta R.T. -0.00 min

Lab File: VN054599.D

Acq: 23 Mar 2019 12:47

Instrument :

MSVOA_N

ClientSampleId :


TB-20190313

Tot Ion: 98 Resp: 1257437

Ion Ratio Lower Upper




98 100

100 63.7 51.2 76.8

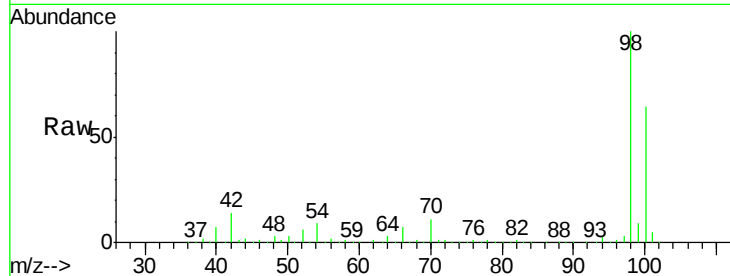

Abundance Ion 98.00 (97.70 to 98.70): VN054459.D (-2570) (-)

Ion 100.00 (99.70 to 100.70): VN054459.D (-2570) (-)

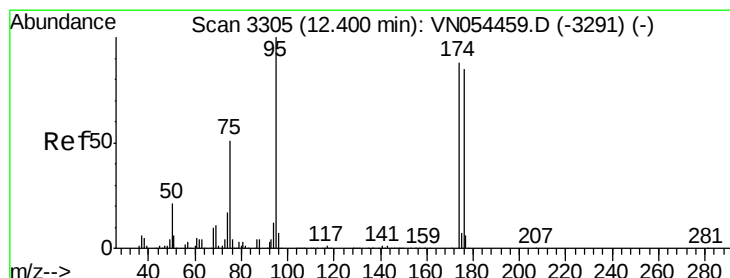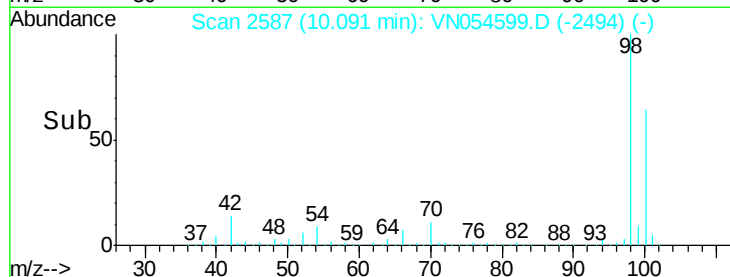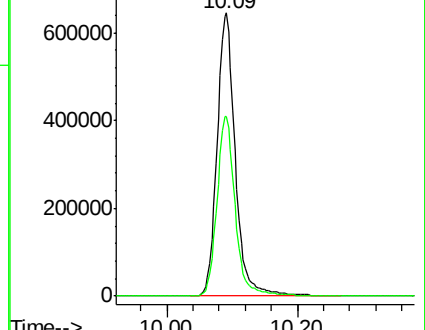

#62

4-Bromofluorobenzene

Concen: 46.542 ug/l

RT: 12.40 min Scan# 3305

Delta R.T. -0.00 min

Lab File: VN054599.D

Acq: 23 Mar 2019 12:47


Tgt Ion: 95 Resp: 378178

Ion Ratio Lower Upper

95 100

174 84.1 0.0 191.0



176 81.4 0.0 187.4

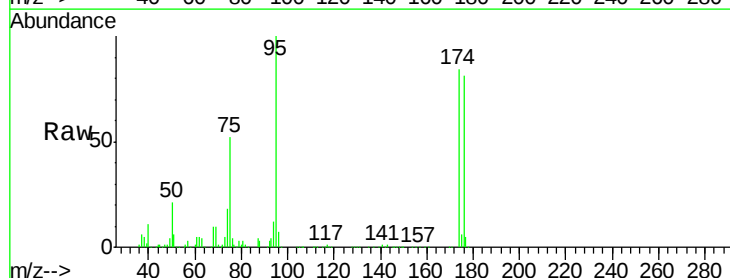


Abundance Ion 94.90 (94.60 to 95.60): VN054459.D (-3291) (-)

Ion 173.80 (173.50 to 174.50): VN054459.D (-3291) (-)

Ion 175.80 (175.50 to 176.50): VN054459.D (-3291) (-)

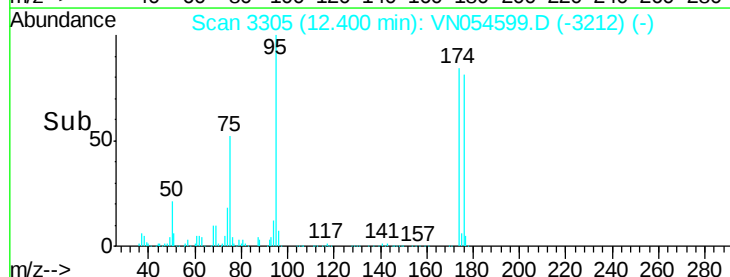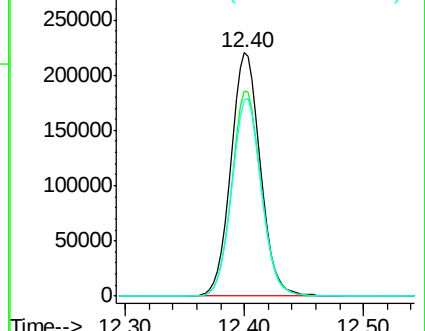


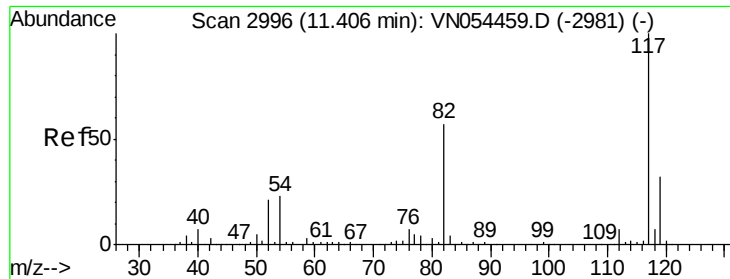




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.41 min Scan# 2996
Delta R.T. -0.00 min
Lab File: VN054599.D
Acq: 23 Mar 2019 12:47

Instrument :
MSVOA_N
ClientSampled :
TB-20190313

Tot Ion:117 Resp: 813478
Ion Ratio Lower Upper
117 100
82 56.5 40.0 60.0
119 32.1 25.8 38.6

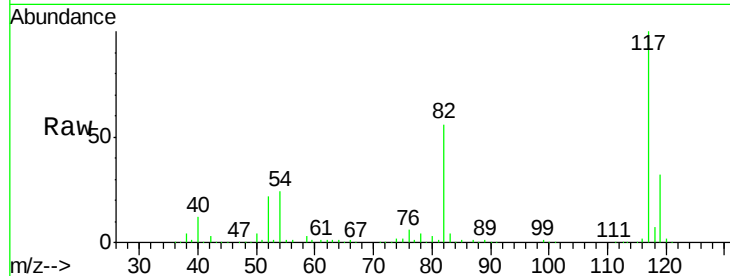


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V

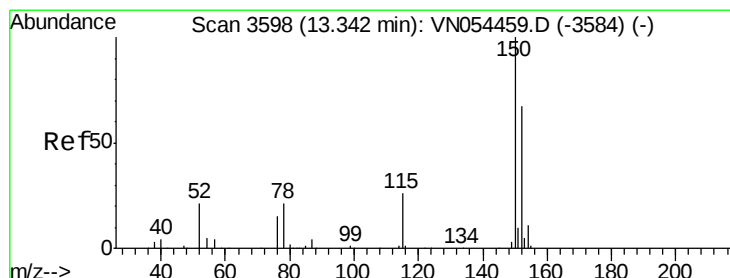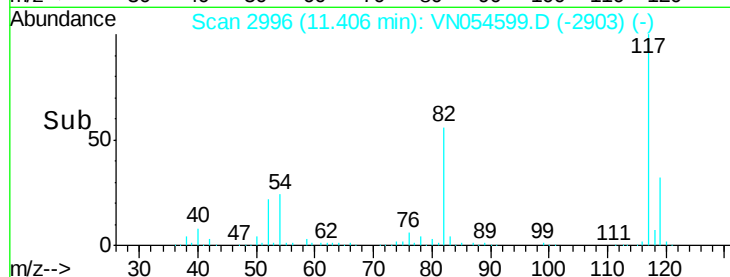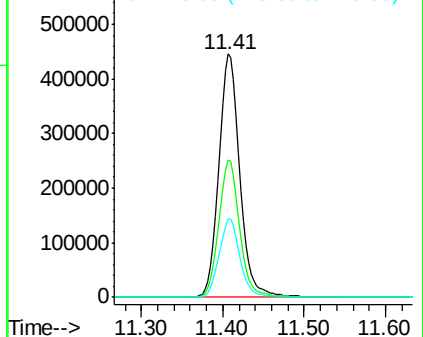

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.34 min Scan# 3598
Delta R.T. -0.00 min
Lab File: VN054599.D
Acq: 23 Mar 2019 12:47

Tgt Ion:152 Resp: 278302
Ion Ratio Lower Upper
152 100
115 58.3 27.2 81.6
150 158.1 0.0 349.2

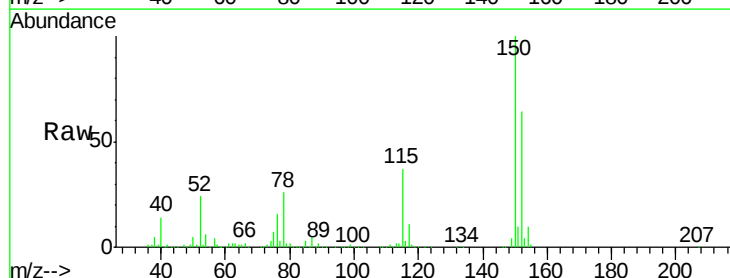

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

