


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN032319\
 Data File : VN054615.D
 Acq On : 23 Mar 2019 20:34
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N032019W.M
 Title : SW846 8260
 Last Update : Fri Mar 22 02:09:07 2019

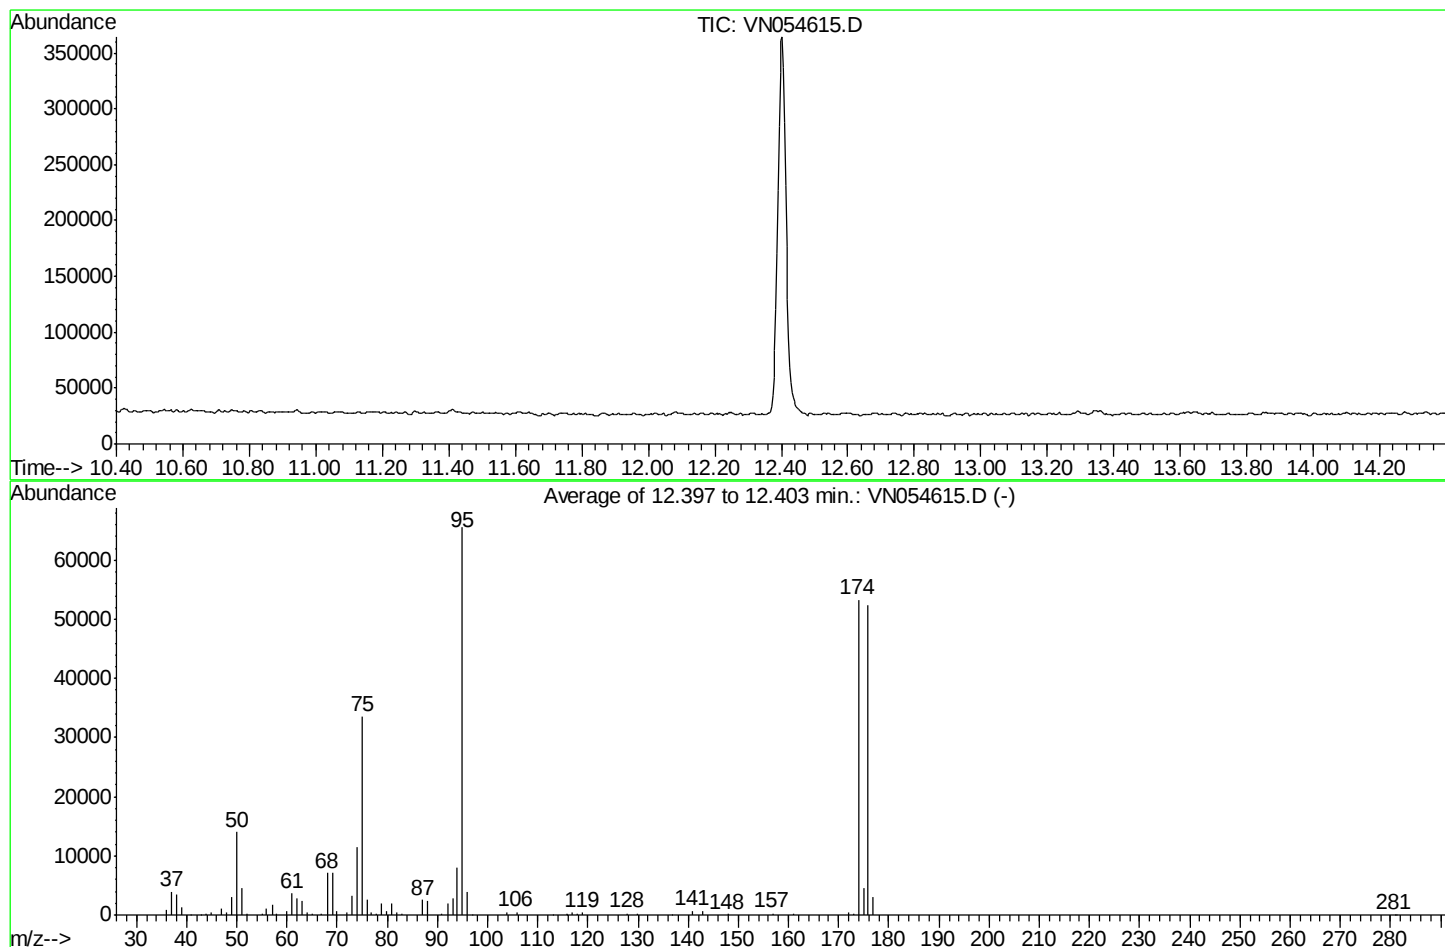

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.4	14041	PASS
75	95	30	60	51.2	33552	PASS
95	95	100	100	100.0	65562	PASS
96	95	5	9	6.0	3907	PASS
173	174	0.00	2	0.6	305	PASS
174	95	50	100	81.4	53341	PASS
175	174	5	9	8.5	4559	PASS
176	174	95	101	98.1	52328	PASS
177	176	5	9	5.9	3111	PASS