


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032322\
Data File : VN071503.D
Acq On : 23 Mar 2022 12:03
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N031722W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Thu Mar 17 06:37:08 2022

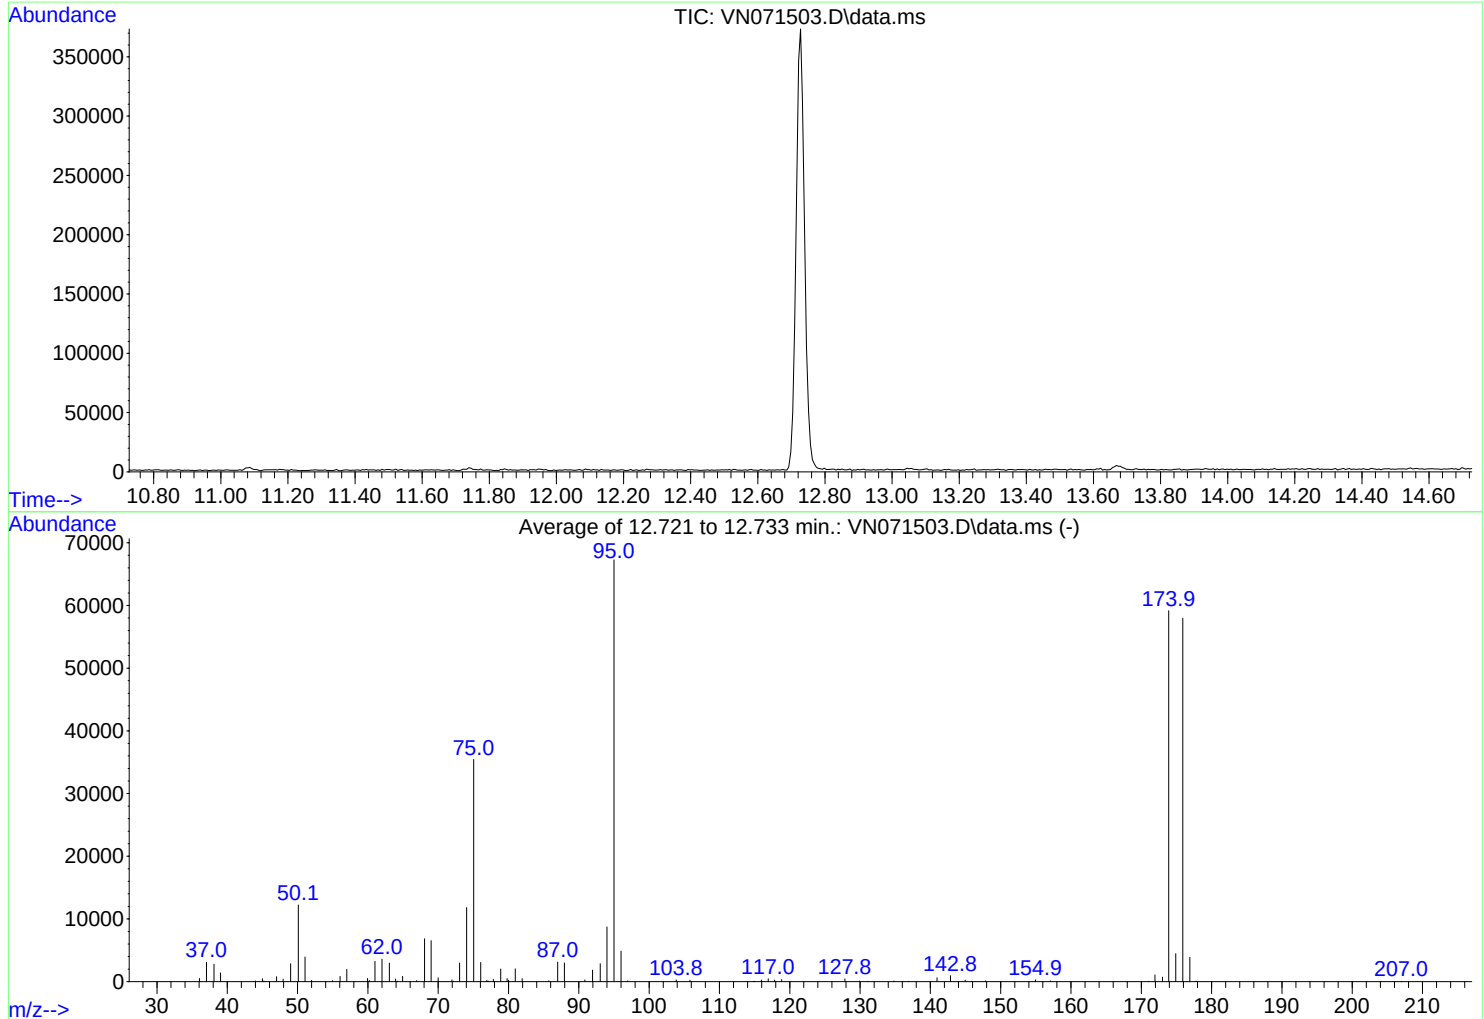

AutoFind: Scans 1825, 1826, 1827; Background Corrected with Scan 1818

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.2	12221	PASS
75	95	30	60	52.7	35443	PASS
95	95	100	100	100.0	67277	PASS
96	95	5	9	7.3	4880	PASS
173	174	0.00	2	1.2	722	PASS
174	95	50	100	87.9	59147	PASS
175	174	5	9	7.5	4460	PASS
176	174	95	101	98.0	57965	PASS
177	176	5	9	6.7	3895	PASS