


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032422\
Data File : VN071510.D
Acq On : 24 Mar 2022 09:22
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N032422W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Thu Mar 24 12:03:44 2022

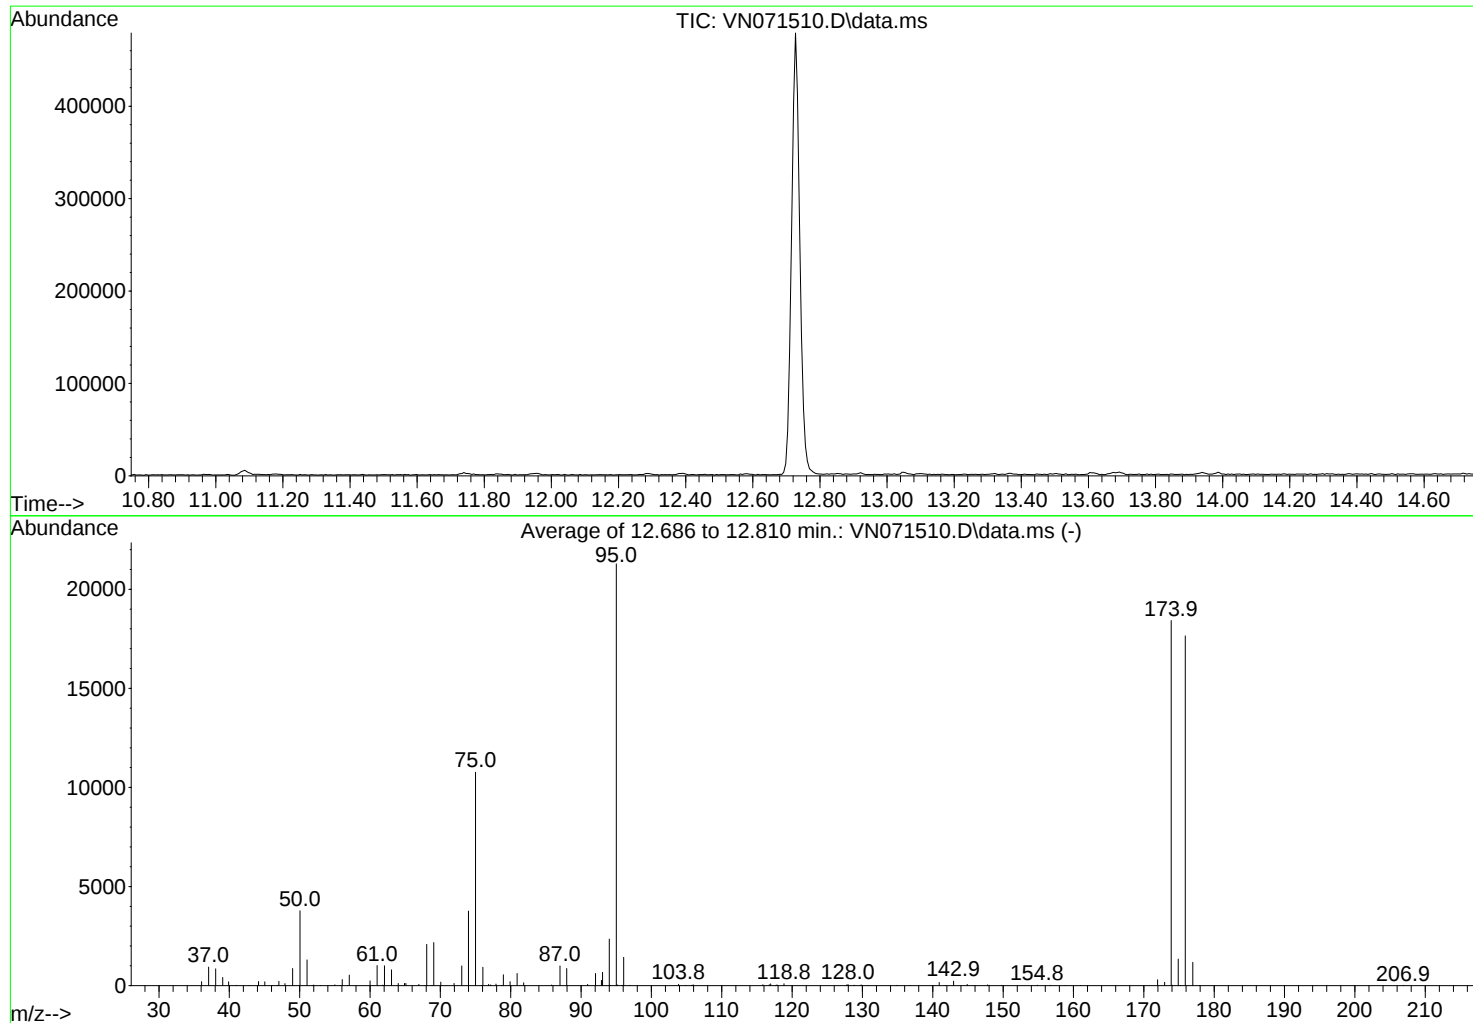

AutoFind: Averaged scan 1819 to 1840; Bkg corrected with scan 1818

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.8	3781	PASS
75	95	30	60	50.6	10768	PASS
95	95	100	100	100.0	21282	PASS
96	95	5	9	6.7	1426	PASS
173	174	0.00	2	0.9	170	PASS
174	95	50	100	86.5	18419	PASS
175	174	5	9	7.3	1339	PASS
176	174	95	101	95.8	17650	PASS
177	176	5	9	6.7	1178	PASS