

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032425\
 Data File : VN086067.D
 Acq On : 24 Mar 2025 13:02
 Operator : JC\MD
 Sample : VN0324WBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0324WBL01

Quant Time: Mar 25 01:21:09 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031825W.M
 Quant Title : SW846 8260
 QLast Update : Wed Mar 19 03:20:56 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	131247	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	230937	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	213386	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.788	152	85734	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	104038	57.888	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	115.780%
35) Dibromofluoromethane	8.165	113	90332	56.040	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	112.080%
50) Toluene-d8	10.565	98	287377	49.123	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	98.240%
62) 4-Bromofluorobenzene	12.847	95	88547	42.442	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	84.880%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032425\
Data File : VN086067.D
Acq On : 24 Mar 2025 13:02
Operator : JC\MD
Sample : VN0324WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0324WBL01

Quant Time: Mar 25 01:21:09 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031825W.M
Quant Title : SW846 8260
QLast Update : Wed Mar 19 03:20:56 2025
Response via : Initial Calibration




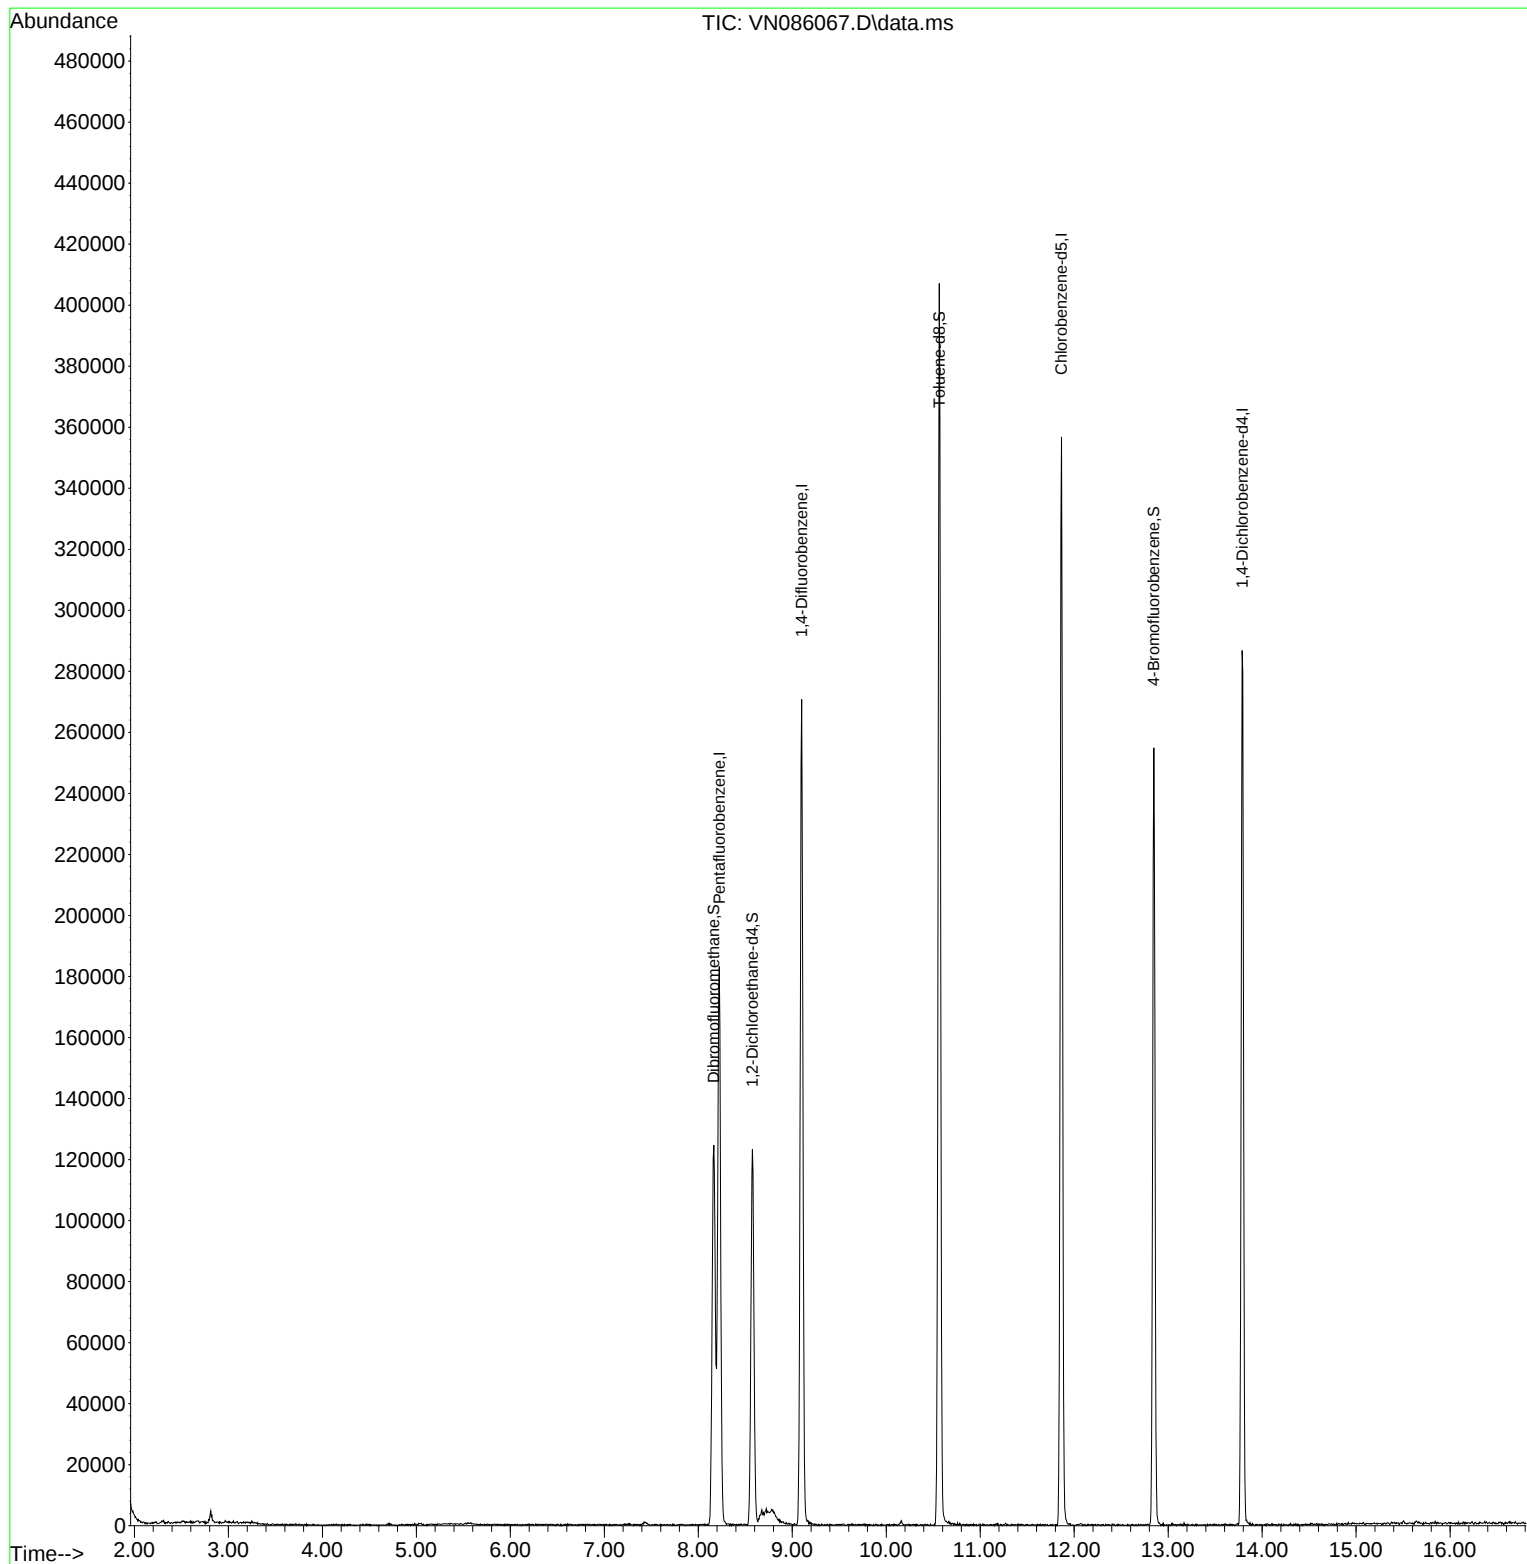


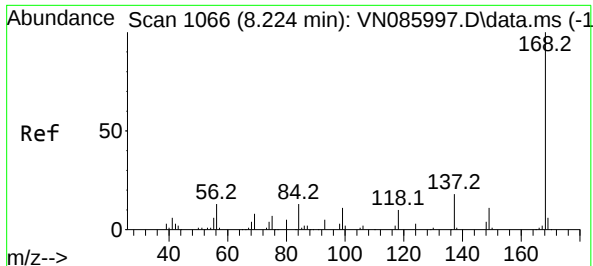

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.000 min
Lab File: VN086067.D
Acq: 24 Mar 2025 13:02




Instrument :
MSVOA_N
ClientSampleId :
VN0324WBL01


Tgt Ion:168 Resp: 131247
Ion Ratio Lower Upper
168 100
99 60.0 49.4 74.2

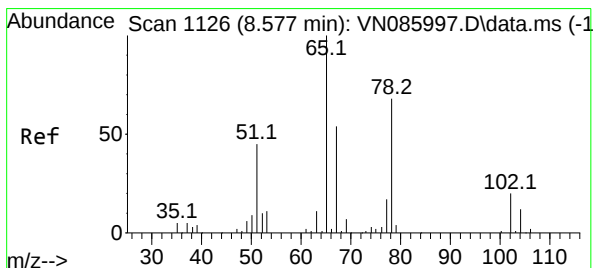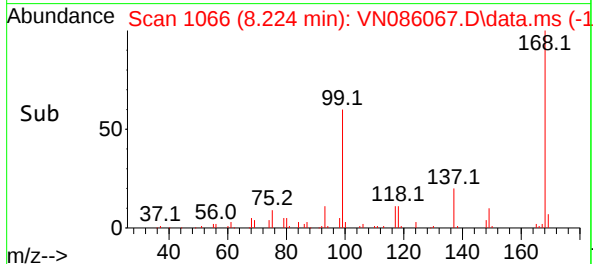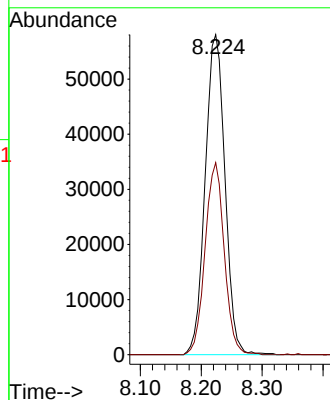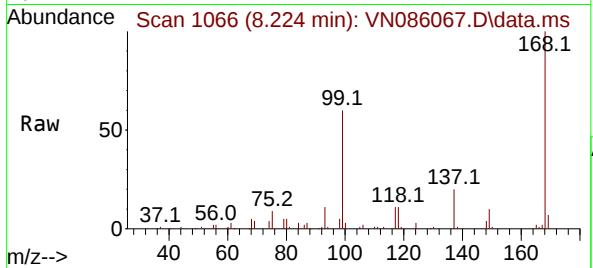

#33
1,2-Dichloroethane-d4
Concen: 57.888 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. -0.000 min
Lab File: VN086067.D
Acq: 24 Mar 2025 13:02

Tgt Ion: 65 Resp: 104038
Ion Ratio Lower Upper
65 100
67 51.9 0.0 102.2

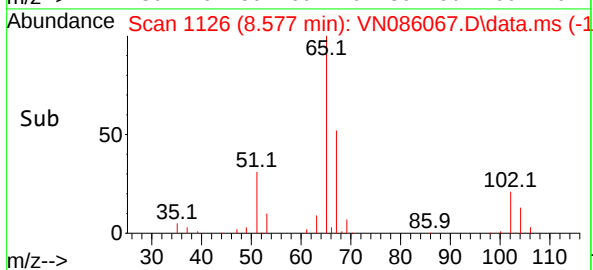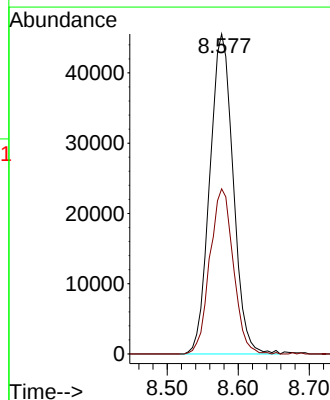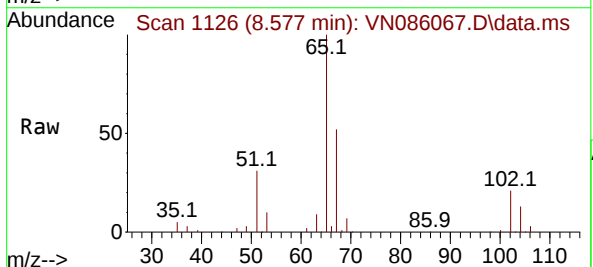

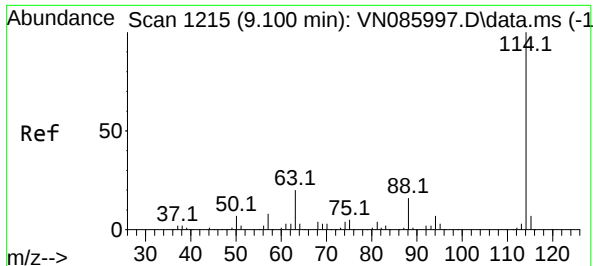

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN086067.D

Acq: 24 Mar 2025 13:02

Instrument :

MSVOA_N

ClientSampleId :

VN0324WBL01





Tgt Ion:114 Resp: 230937

Ion Ratio Lower Upper

114 100

63 18.2 0.0 39.6

88 18.0 0.0 32.6

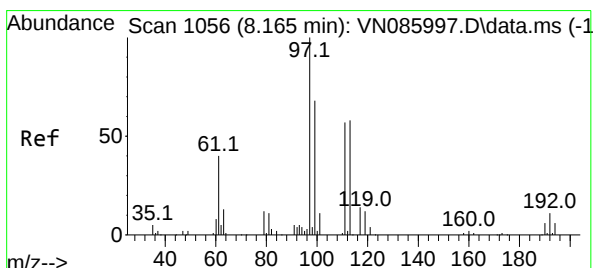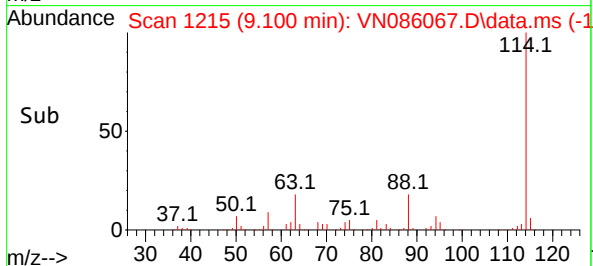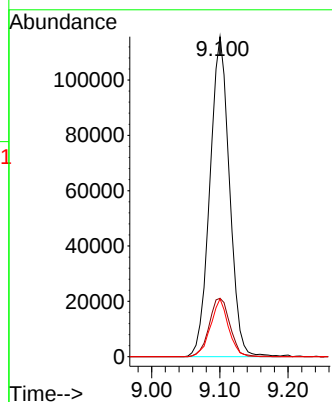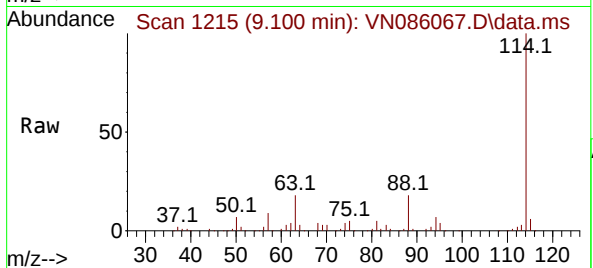

#35

Dibromofluoromethane

Concen: 56.040 ug/l

RT: 8.165 min Scan# 1056

Delta R.T. -0.000 min

Lab File: VN086067.D

Acq: 24 Mar 2025 13:02




Tgt Ion:113 Resp: 90332


Ion Ratio Lower Upper

113 100

111 104.9 81.8 122.8

192 20.1 15.9 23.9


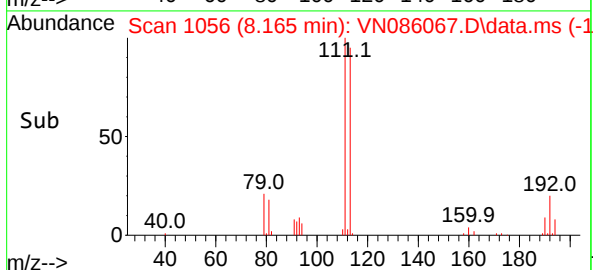
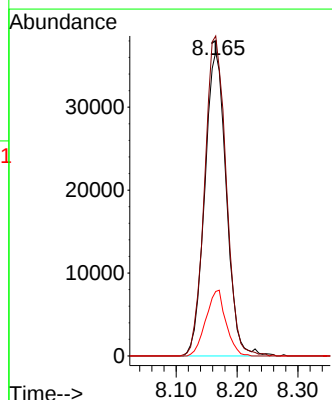
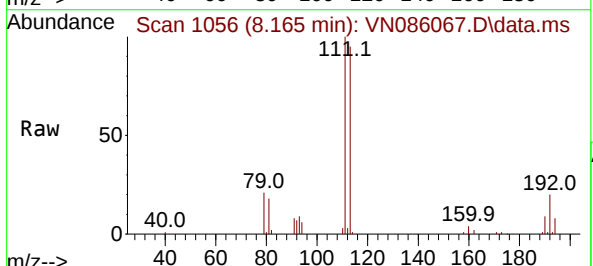


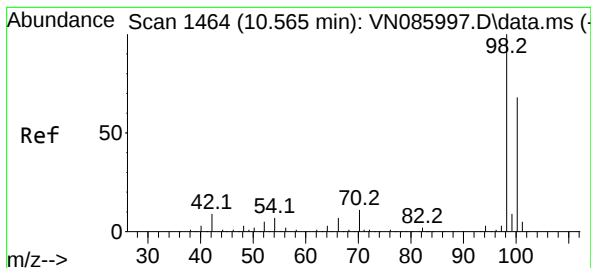

#50
Toluene-d8
Concen: 49.123 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. -0.000 min
Lab File: VN086067.D
Acq: 24 Mar 2025 13:02




Instrument :
MSVOA_N
ClientSampleId :
VN0324WBL01


Tgt Ion: 98 Resp: 287377
Ion Ratio Lower Upper
98 100
100 64.2 53.1 79.7

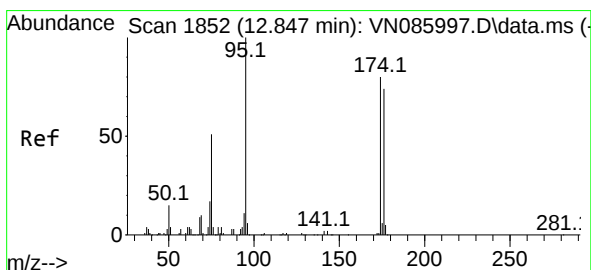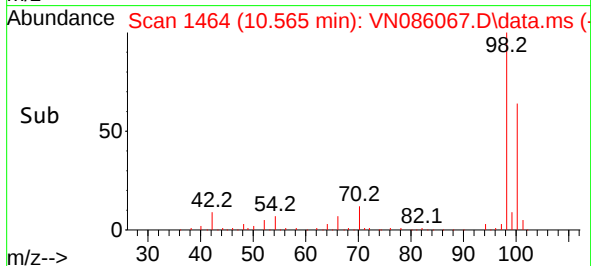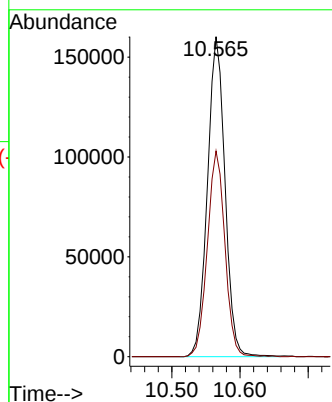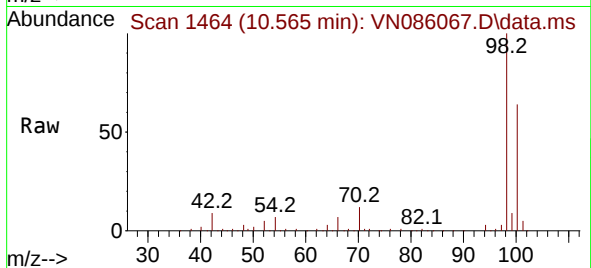

#62
4-Bromofluorobenzene
Concen: 42.442 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.000 min
Lab File: VN086067.D
Acq: 24 Mar 2025 13:02

Tgt Ion: 95 Resp: 88547
Ion Ratio Lower Upper
95 100
174 83.9 0.0 156.8
176 80.3 0.0 152.2


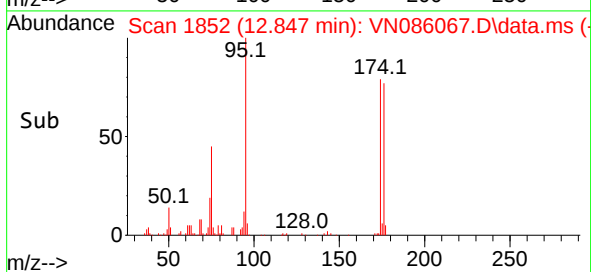
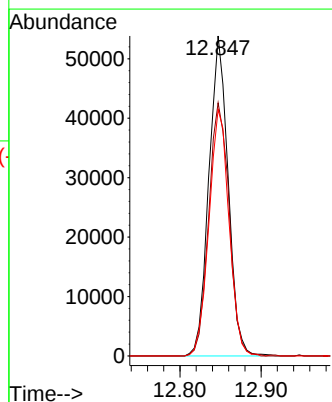
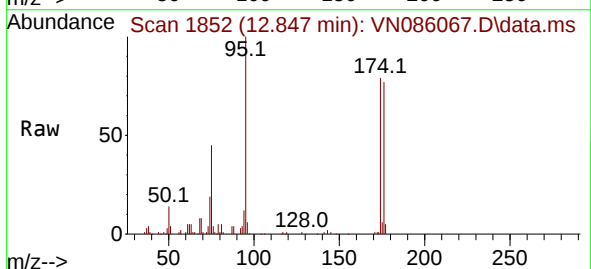


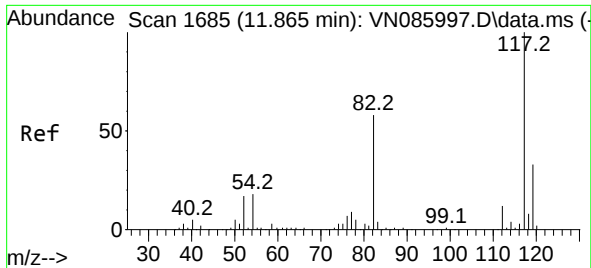

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 117
Delta R.T. -0.000 min
Lab File: VN086067.D
Acq: 24 Mar 2025 13:02

Instrument :
MSVOA_N
ClientSampleId :
VN0324WBL01

Tgt Ion:117 Resp: 213386
Ion Ratio Lower Upper
117 100
82 54.2 46.7 70.1
119 33.5 26.5 39.7

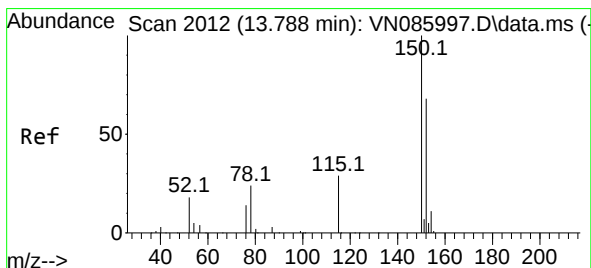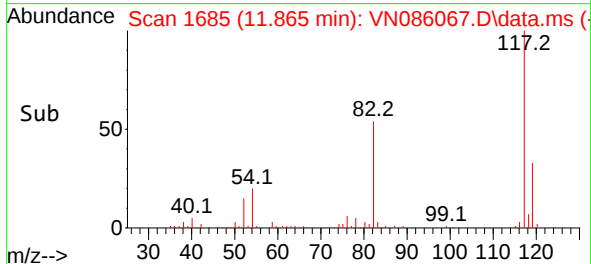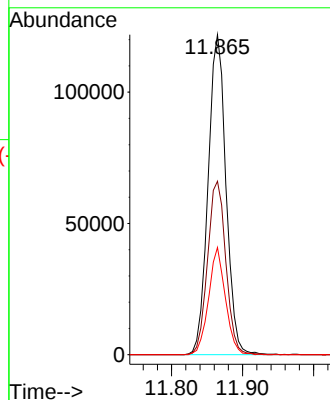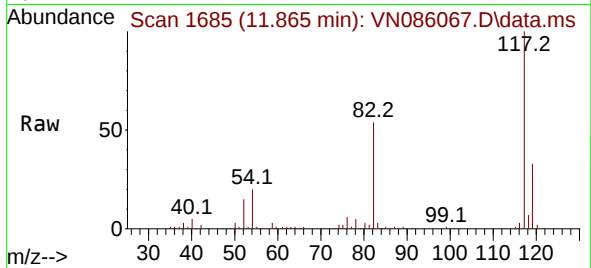

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.788 min Scan# 2012
Delta R.T. -0.000 min
Lab File: VN086067.D
Acq: 24 Mar 2025 13:02

Tgt Ion:152 Resp: 85734
Ion Ratio Lower Upper
152 100
115 59.8 31.1 93.2
150 155.7 0.0 359.6

