


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032425\
Data File : VN086064.D
Acq On : 24 Mar 2025 11:38
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031825W.M
Title : SW846 8260
Last Update : Wed Mar 19 03:20:56 2025

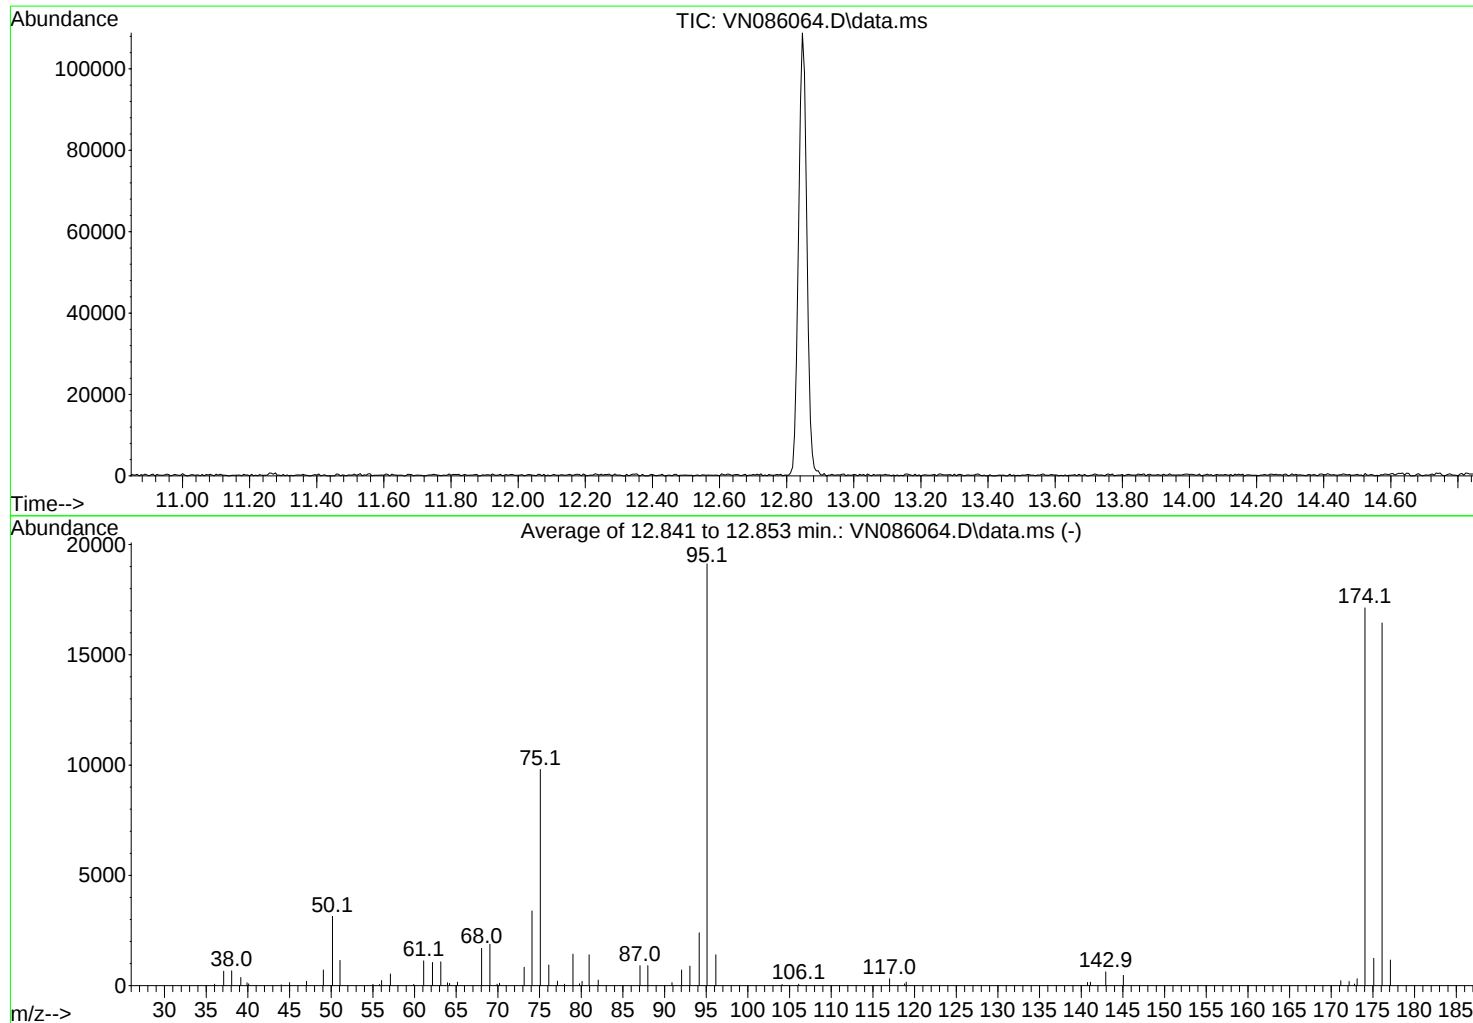

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	3138	PASS
75	95	30	60	51.3	9802	PASS
95	95	100	100	100.0	19125	PASS
96	95	5	9	7.3	1399	PASS
173	174	0.00	2	1.8	314	PASS
174	95	50	100	89.6	17128	PASS
175	174	5	9	7.2	1239	PASS
176	174	95	101	96.0	16445	PASS
177	176	5	9	7.1	1163	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	69	51.05	1149	65.15	157	79.00	143
37.10	656	55.00	55	68.05	1691	79.80	84
38.05	673	55.80	51	69.05	1876	80.10	19
39.15	372	56.05	233	69.90	63	80.95	139
39.90	133	57.10	529	70.20	107	82.05	257
40.10	78	59.90	58	73.15	837	87.05	906
44.00	40	61.10	1127	74.10	3388	88.00	904
45.00	137	62.15	1054	75.10	9802	90.90	135
47.05	195	63.15	1082	76.10	939	92.05	710
49.05	712	63.95	132	77.15	202	93.05	887
50.15	3138	64.20	103	78.00	68	94.15	2394

Average of 12.841 to 12.853 min.: VN086064.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
95.10	19125	171.15	224				
96.15	1399	172.15	189				
104.10	53	172.80	71				
106.10	64	173.10	314				
117.00	311	174.05	17128				
118.80	80	175.10	1239				
119.00	161	176.10	16445				
140.75	148	177.10	1163				
141.10	163						
142.95	626						
145.05	461						

Instrument :

MSVOA_N

ClientSampleId :

BFB