

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN032519\
 Data File : VN054665.D
 Acq On : 25 Mar 2019 11:55
 Operator : JC/SP
 Sample : K1931-02ME
 Misc : 4.49g/5mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 LSP-1ME

Quant Time: Mar 26 12:46:49 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N032019W.M
 Quant Title : SW846 8260
 QLast Update : Fri Mar 22 02:09:07 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.66	168	524995	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.58	114	830149	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	711956	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.34	152	285106	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.03	65	331887	50.82	ug/l	0.00
Spiked Amount	50.000		Recovery	=	101.64%	
35) Dibromofluoromethane	7.59	113	256480	47.96	ug/l	0.00
Spiked Amount	50.000		Recovery	=	95.92%	
50) Toluene-d8	10.09	98	1003024	49.89	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.78%	
62) 4-Bromofluorobenzene	12.40	95	324345	47.41	ug/l	0.00
Spiked Amount	50.000		Recovery	=	94.82%	


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN032519\
Data File : VN054665.D
Acq On : 25 Mar 2019 11:55
Operator : JC/SP
Sample : K1931-02ME
Misc : 4.49g/5mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
LSP-1ME

Quant Time: Mar 26 12:46:49 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N032019W.M
Quant Title : SW846 8260
QLast Update : Fri Mar 22 02:09:07 2019
Response via : Initial Calibration

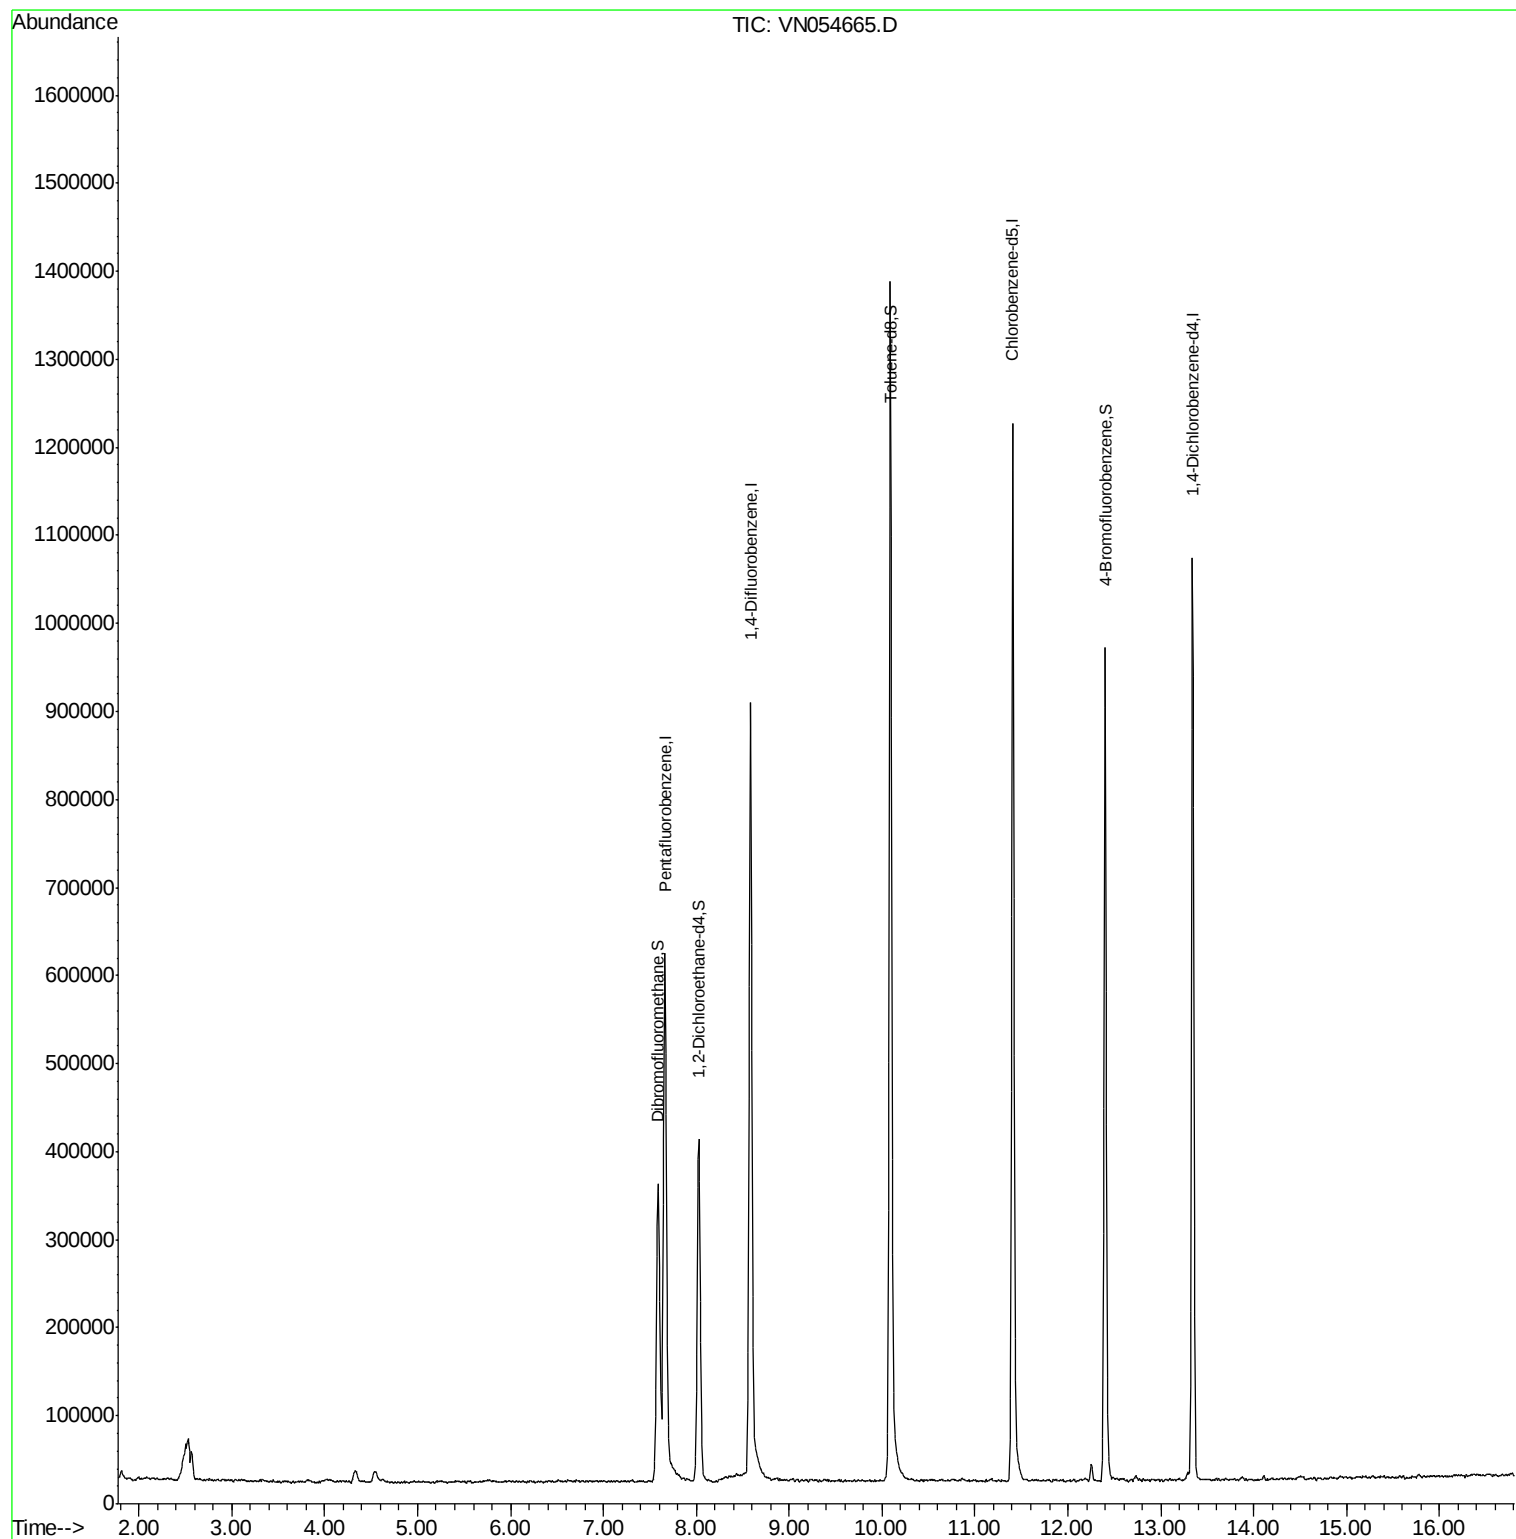



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.66 min Scan# 1832

Delta R.T. -0.00 min

Lab File: VN054665.D

Acq: 25 Mar 2019 11:55

Instrument :

MSVOA_N

ClientSampleId :


LSP-1ME

Tot Ion:168 Resp: 524995

Ion Ratio Lower Upper

168 100

99 53.2 37.1 55.7

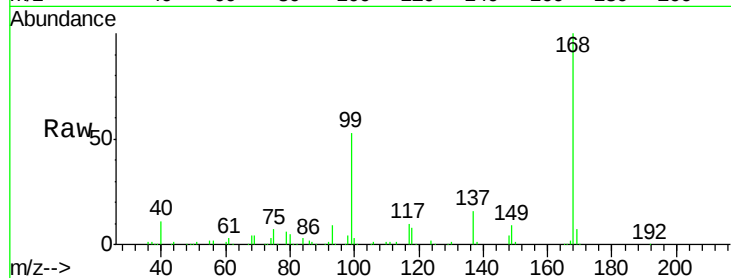

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VNO

7.66

200000



150000

100000

50000

0

Time-->

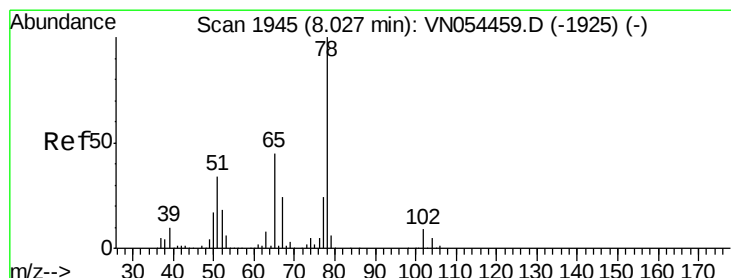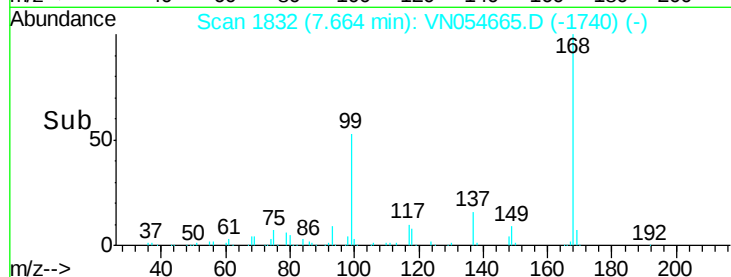

#33

1,2-Dichloroethane-d4

Concen: 50.824 ug/l

RT: 8.03 min Scan# 1945

Delta R.T. 0.00 min

Lab File: VN054665.D


Acq: 25 Mar 2019 11:55

Tgt Ion: 65 Resp: 331887

Ion Ratio Lower Upper

65 100

67 52.1 0.0 104.6

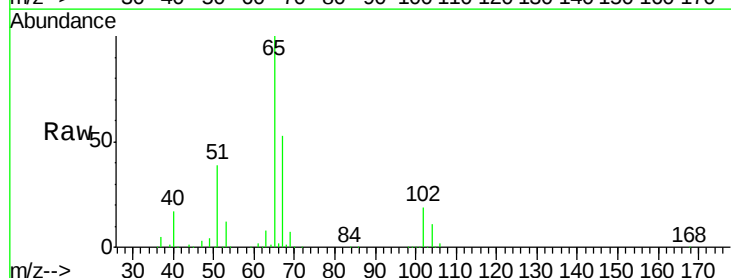

Abundance Ion 64.90 (64.60 to 65.60): VNO

Ion 66.90 (66.60 to 67.60): VNO

8.03


150000


100000

50000

0

Time-->

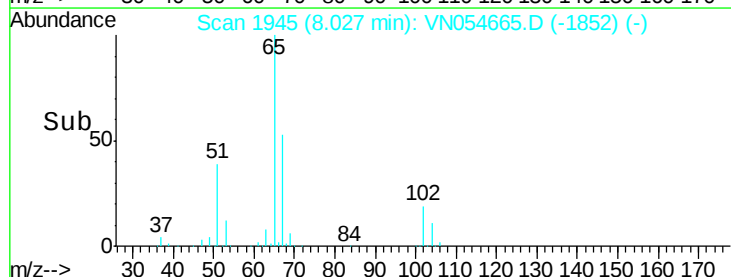


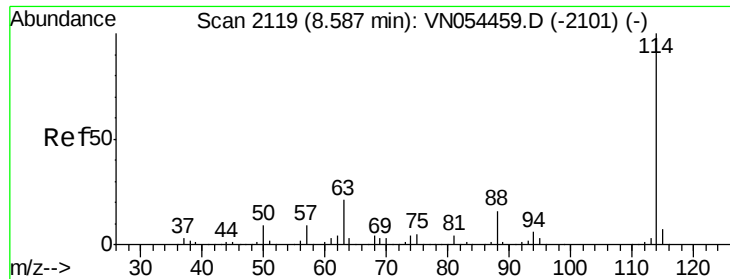




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.58 min Scan# 2119
Delta R.T. -0.00 min
Lab File: VN054665.D
Acq: 25 Mar 2019 11:55

Instrument :
MSVOA_N
ClientSampleId :
LSP-1ME

Tot Ion:114 Resp: 830149
Ion Ratio Lower Upper
114 100
63 22.6 0.0 35.2
88 16.1 0.0 30.2

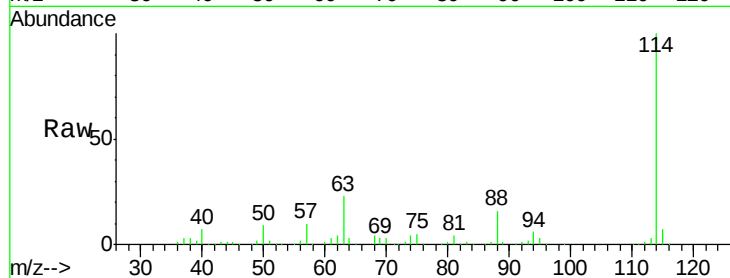


Abundance Ion 113.90 (113.60 to 114.60): V
Ion 63.00 (62.70 to 63.70): V
Ion 87.90 (87.60 to 88.60): V

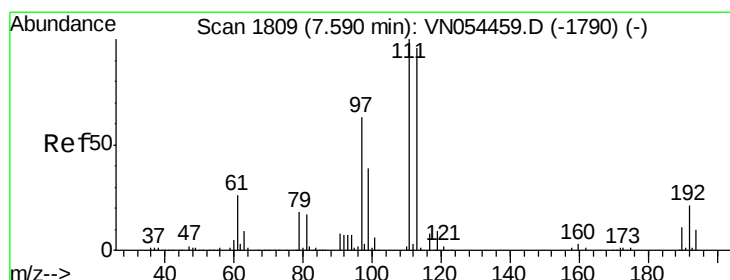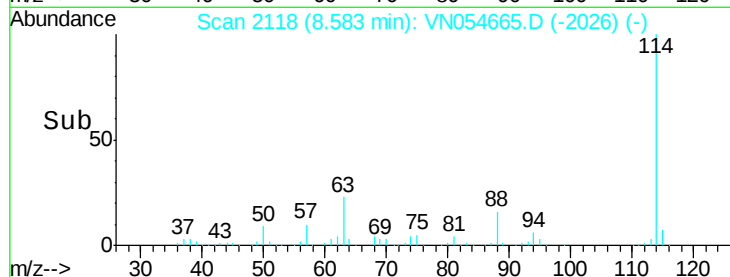
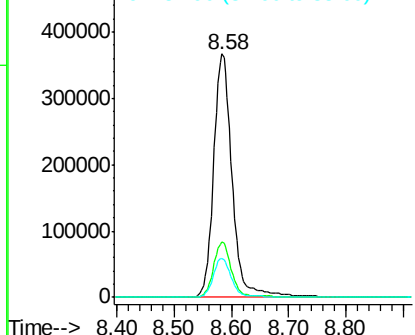



#35
Dibromofluoromethane
Concen: 47.956 ug/l
RT: 7.59 min Scan# 1809
Delta R.T. 0.00 min
Lab File: VN054665.D
Acq: 25 Mar 2019 11:55

Tgt Ion:113 Resp: 256480
Ion Ratio Lower Upper
113 100
111 101.0 82.2 123.4
192 20.2 19.2 28.8

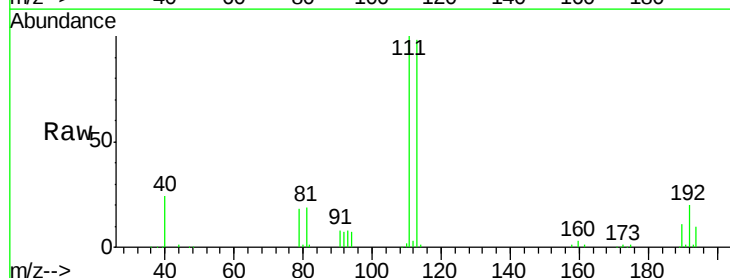

Abundance Ion 112.80 (112.50 to 113.50): V
Ion 110.80 (110.50 to 111.50): V
Ion 191.70 (191.40 to 192.40): V



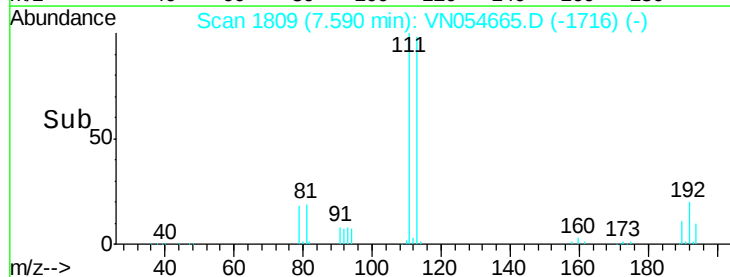
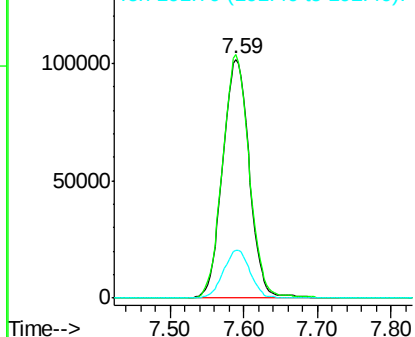


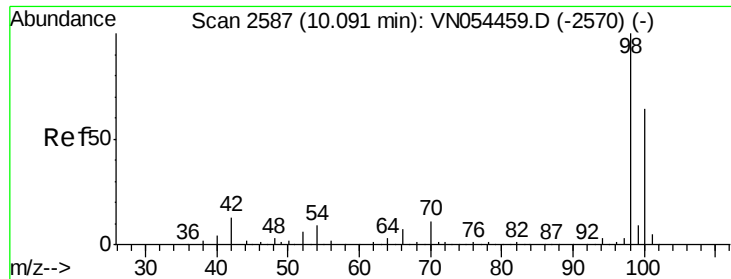

#50
Toluene-d8
Concen: 49.887 ug/l
RT: 10.09 min Scan# 2586
Delta R.T. -0.00 min
Lab File: VN054665.D
Acq: 25 Mar 2019 11:55




Instrument :
MSVOA_N
ClientSampled :
LSP-1ME


Tot Ion: 98 Resp: 1003024
Ion Ratio Lower Upper
98 100
100 64.3 51.2 76.8

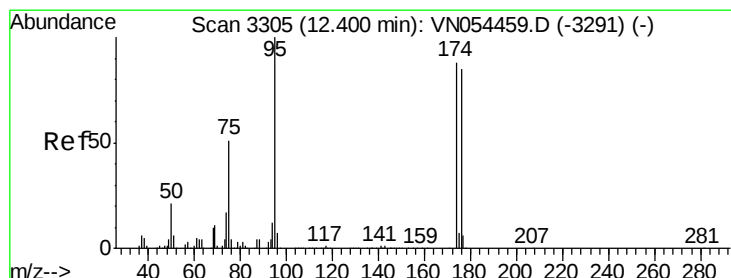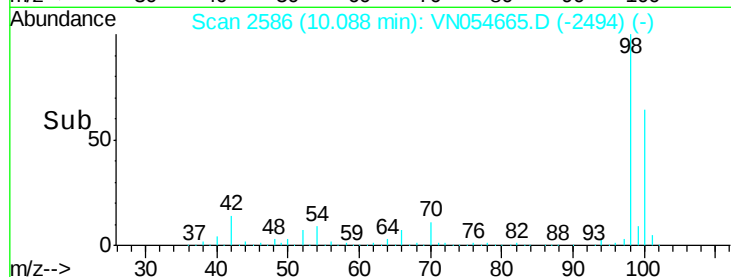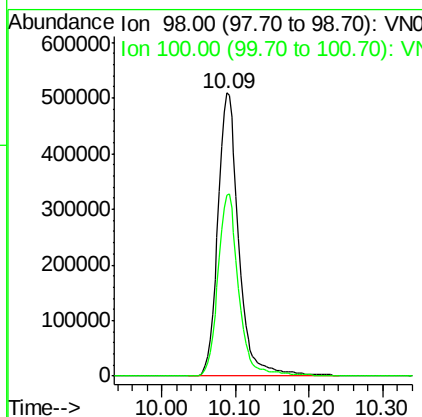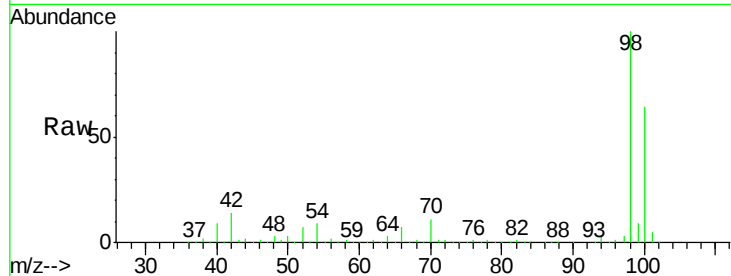

#62
4-Bromofluorobenzene
Concen: 47.407 ug/l
RT: 12.40 min Scan# 3305
Delta R.T. 0.00 min
Lab File: VN054665.D
Acq: 25 Mar 2019 11:55

Tgt Ion: 95 Resp: 324345
Ion Ratio Lower Upper
95 100
174 83.9 0.0 191.0
176 80.4 0.0 187.4

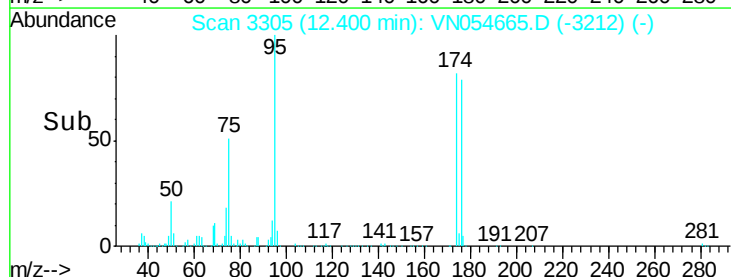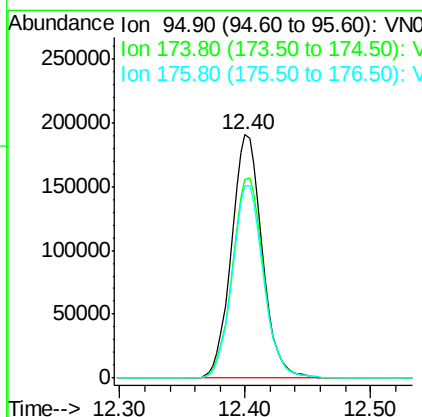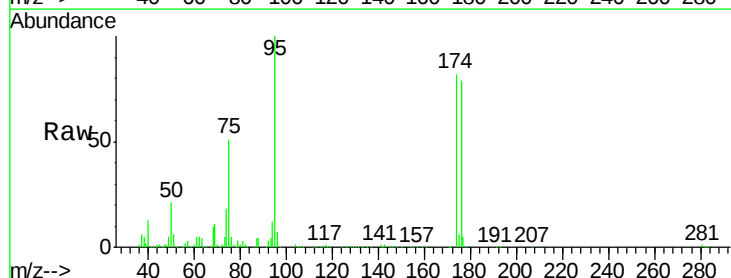


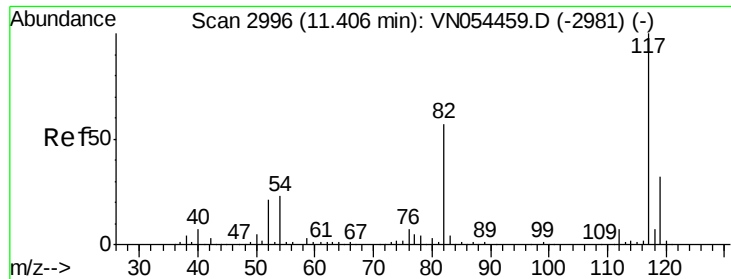




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.41 min Scan# 2996
Delta R.T. 0.00 min
Lab File: VN054665.D
Acq: 25 Mar 2019 11:55

Instrument :
MSVOA_N
ClientSampled :
LSP-1ME

Tot Ion:117 Resp: 711956
Ion Ratio Lower Upper
117 100
82 55.5 40.0 60.0
119 32.1 25.8 38.6

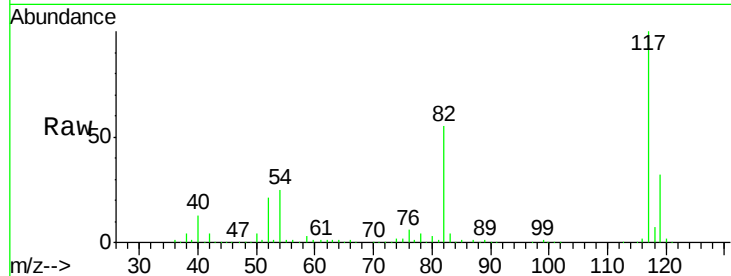


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V

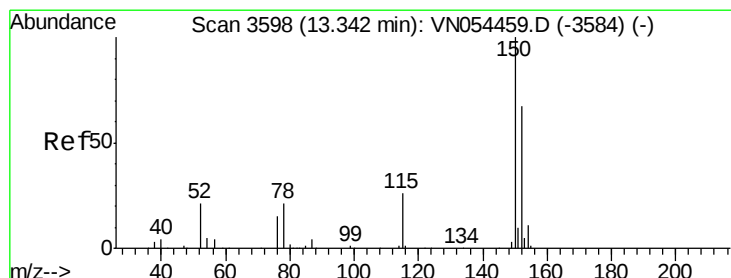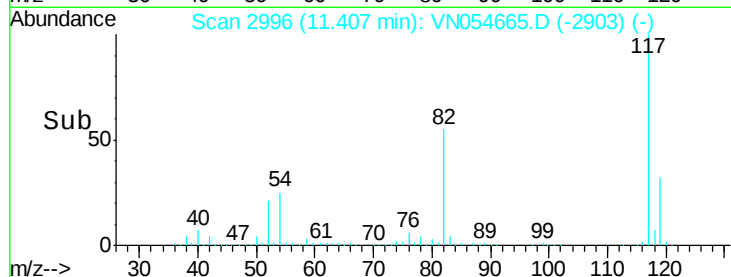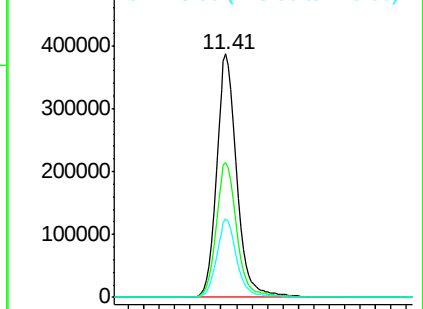

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.34 min Scan# 3598
Delta R.T. 0.00 min
Lab File: VN054665.D
Acq: 25 Mar 2019 11:55

Tgt Ion:152 Resp: 285106
Ion Ratio Lower Upper
152 100
115 56.7 27.2 81.6
150 155.2 0.0 349.2

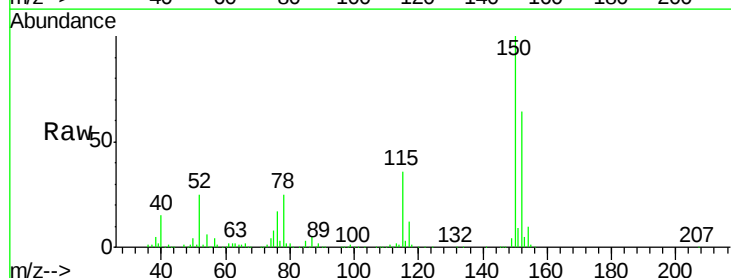

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

