

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN032519\
 Data File : VN054675.D
 Acq On : 25 Mar 2019 16:19
 Operator : JC/SP
 Sample : K2040-10
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 S4B(20)

Quant Time: Mar 26 03:33:04 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N032019W.M
 Quant Title : SW846 8260
 QLast Update : Fri Mar 22 02:09:07 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	559632	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	874708	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	741976	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.34	152	276277	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.03	65	353149	50.73	ug/l	0.00
Spiked Amount 50.000			Recovery	=	101.46%	
35) Dibromofluoromethane	7.59	113	273601	48.55	ug/l	0.00
Spiked Amount 50.000			Recovery	=	97.10%	
50) Toluene-d8	10.09	98	1062313	50.14	ug/l	0.00
Spiked Amount 50.000			Recovery	=	100.28%	
62) 4-Bromofluorobenzene	12.40	95	333317	46.24	ug/l	0.00
Spiked Amount 50.000			Recovery	=	92.48%	
Target Compounds						
16) Acetone	3.82	43	11900	5.686	ug/l #	76
20) Methylene Chloride	4.55	84	12335	1.999	ug/l #	85
43) Isopropyl Acetate	8.17	43	16232	1.652	ug/l	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN032519\
Data File : VN054675.D
Acq On : 25 Mar 2019 16:19
Operator : JC/SP
Sample : K2040-10
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
S4B(20)

Quant Time: Mar 26 03:33:04 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N032019W.M
Quant Title : SW846 8260
QLast Update : Fri Mar 22 02:09:07 2019
Response via : Initial Calibration

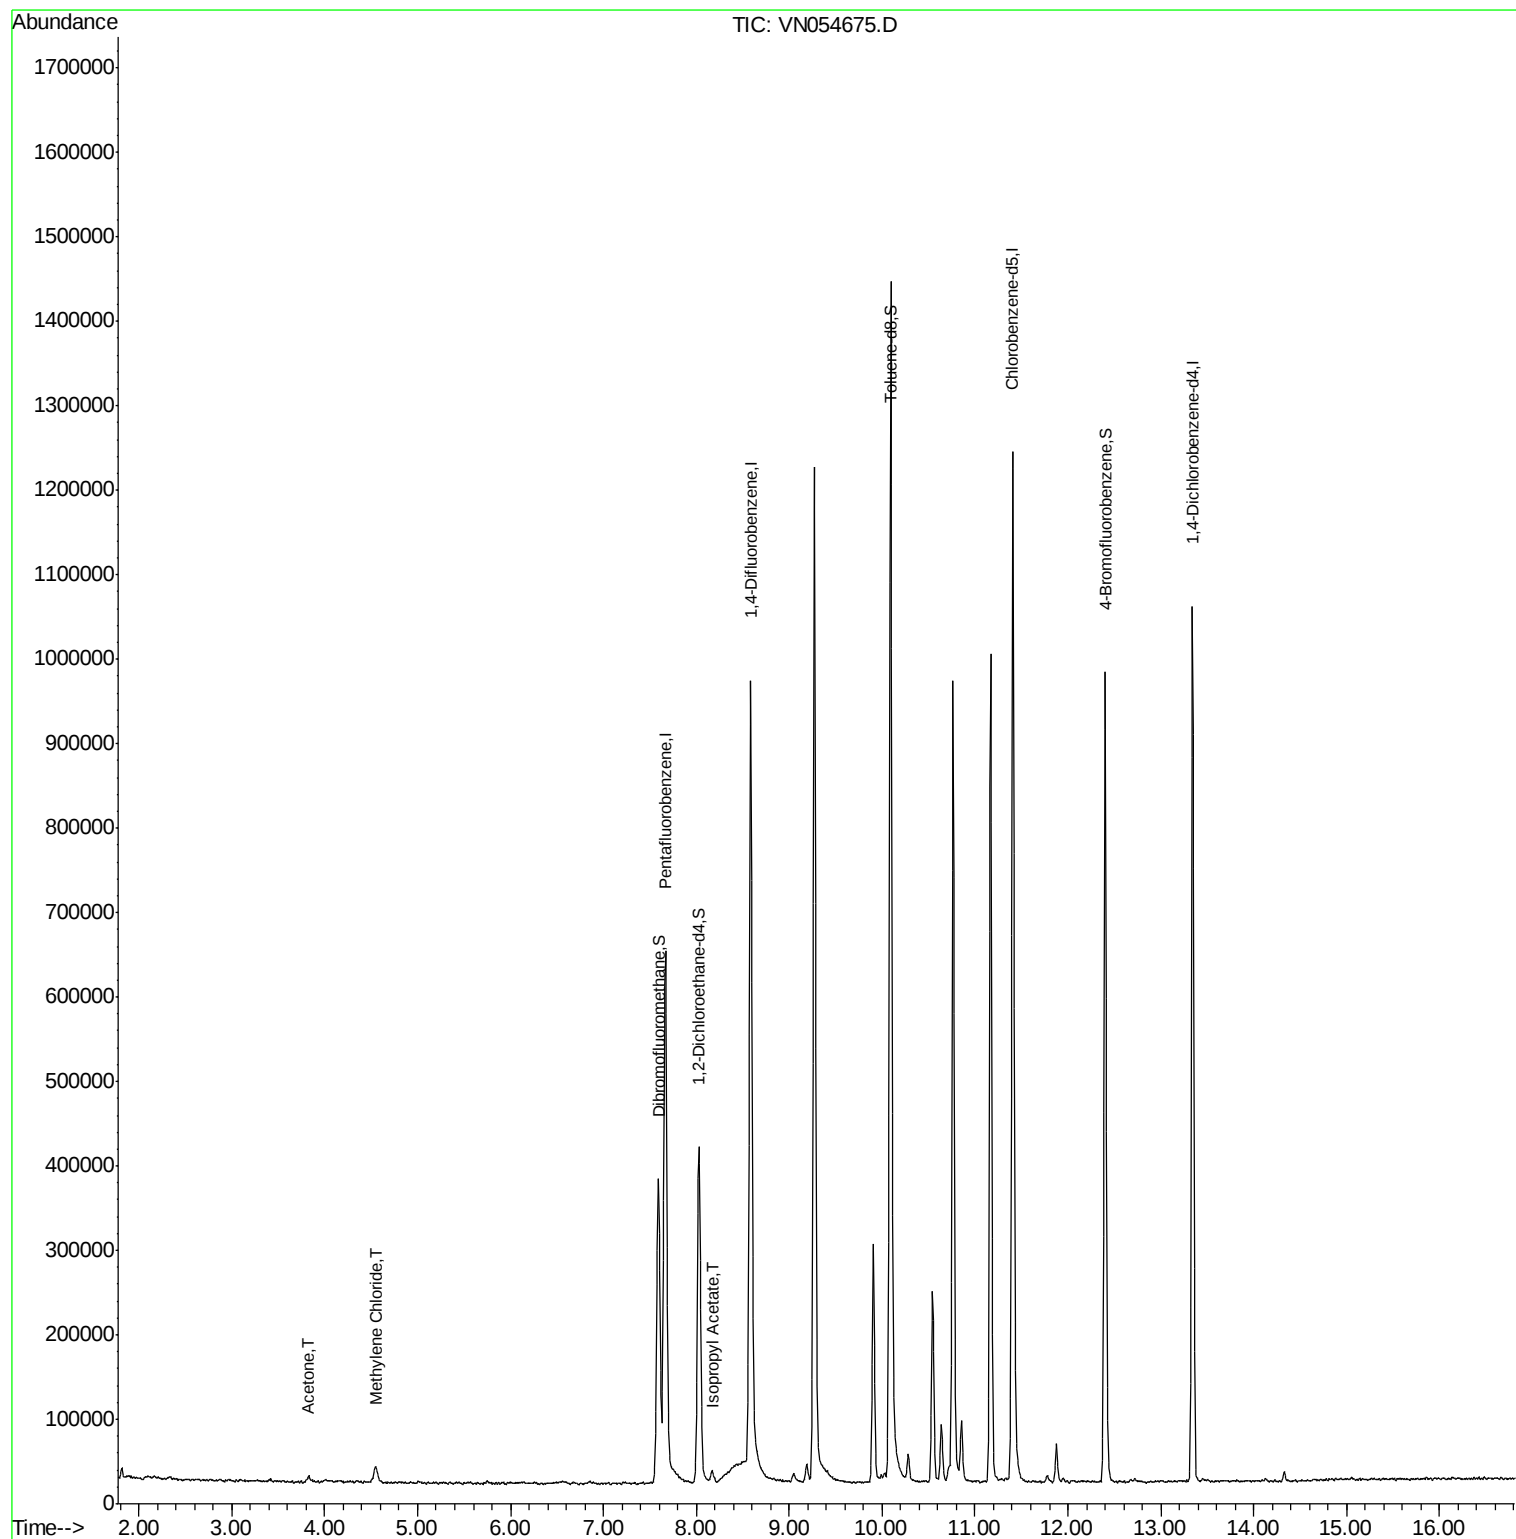



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.67 min Scan# 1833

Delta R.T. 0.00 min

Lab File: VN054675.D

Acq: 25 Mar 2019 16:19

Instrument :

MSVOA_N

ClientSampled :


S4B(20)

Tot Ion:168 Resp: 559632

Ion Ratio Lower Upper

168 100

99 55.1 37.1 55.7

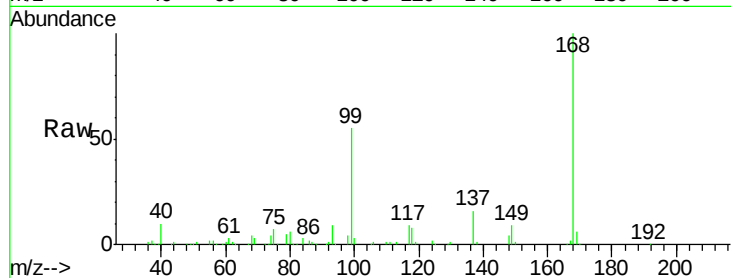

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VNO

7.67

200000



150000

100000

50000

0

Time--> 7.50 7.60 7.70 7.80 7.90

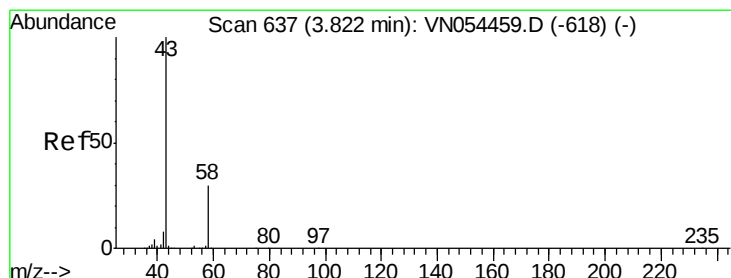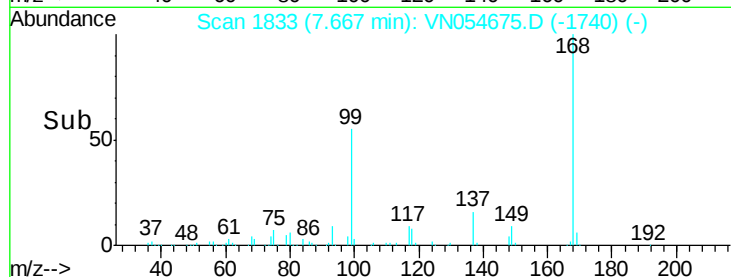

#16

Acetone

Concen: 5.686 ug/l

RT: 3.82 min Scan# 638

Delta R.T. 0.00 min

Lab File: VN054675.D


Acq: 25 Mar 2019 16:19

Tgt Ion: 43 Resp: 11900

Ion Ratio Lower Upper

43 100

58 22.9 29.9 44.9#

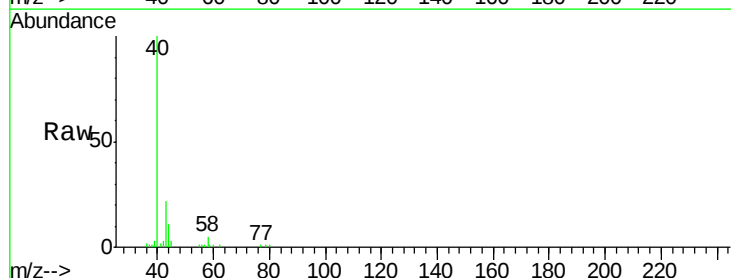

Abundance Ion 43.00 (42.70 to 43.70): VNO

Ion 58.00 (57.70 to 58.70): VNO

3.82

5000

4000


3000


2000

1000

0

Time--> 3.75 3.80 3.85 3.90




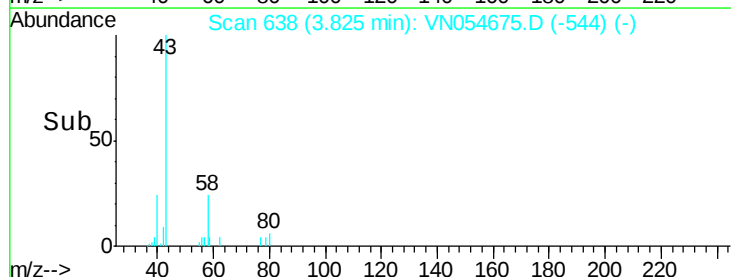


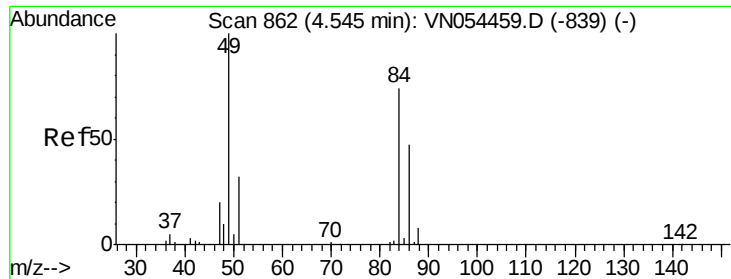

#20
Methylene Chloride
Concen: 1.999 ug/l
RT: 4.55 min Scan# 862
Delta R.T. 0.00 min
Lab File: VN054675.D
Acq: 25 Mar 2019 16:19




Instrument :
MSVOA_N
ClientSampleId :
S4B(20)


Tot Ion	84	Resp	12335
Ion	Ratio	Lower	Upper
84	100		
49	131.1	89.7	134.5
51	43.8	28.2	42.4
86	56.2	50.8	76.2

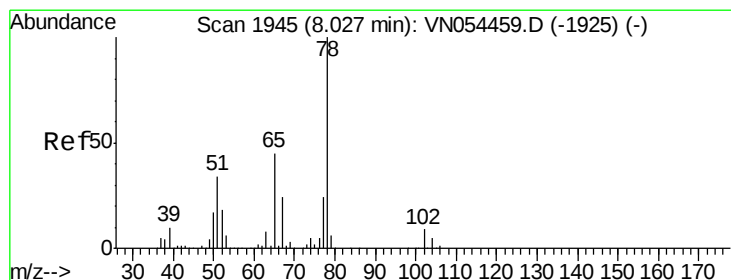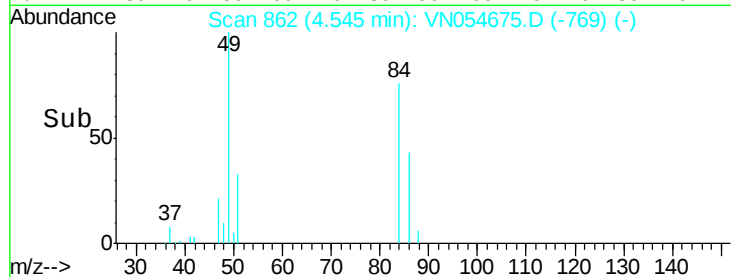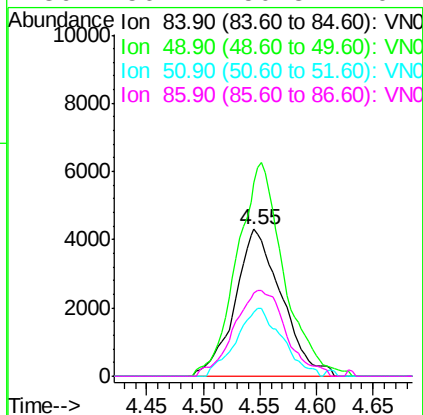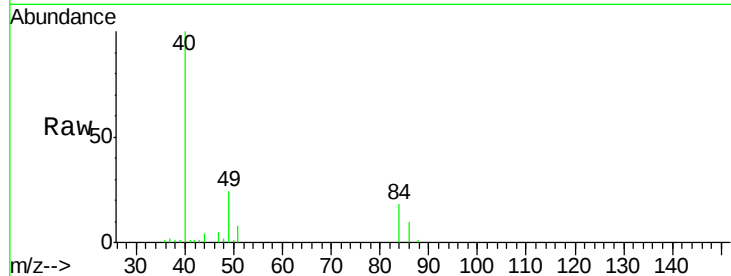

#33
1,2-Dichloroethane-d4
Concen: 50.733 ug/l
RT: 8.03 min Scan# 1945
Delta R.T. 0.00 min
Lab File: VN054675.D
Acq: 25 Mar 2019 16:19

Tgt Ion	65	Resp	353149
Ion	Ratio	Lower	Upper
65	100		
67	51.8	0.0	104.6

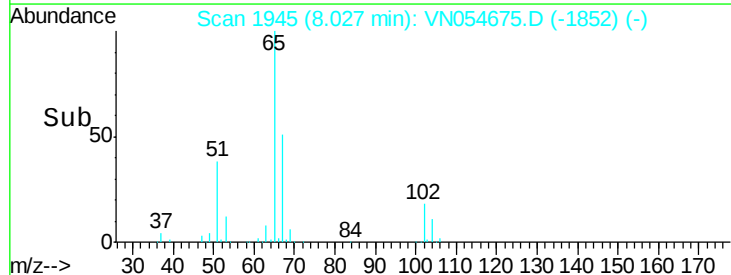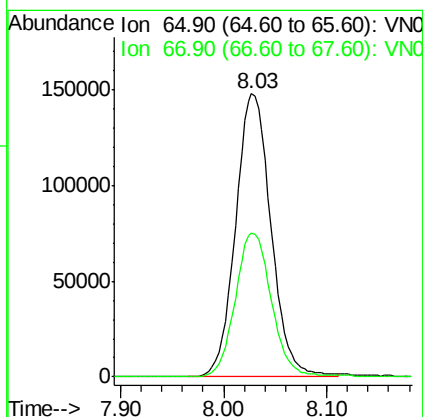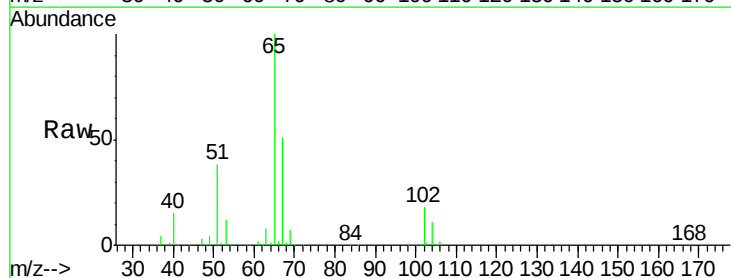

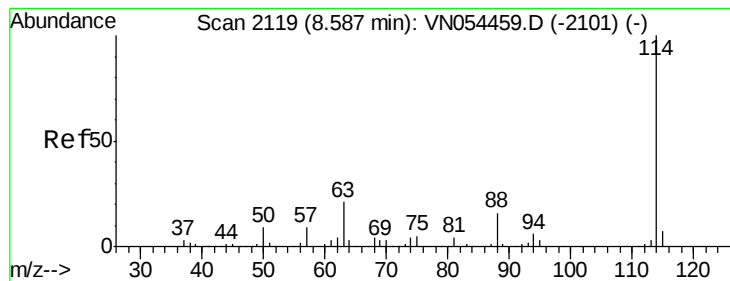

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.59 min Scan# 2119

Delta R.T. 0.00 min

Lab File: VN054675.D

Acq: 25 Mar 2019 16:19

Instrument :

MSVOA_N

ClientSampleId :

S4B(20)


Tot Ion:114 Resp: 874708

Ion Ratio Lower Upper

114 100

63 22.3 0.0 35.2




88 15.6 0.0 30.2

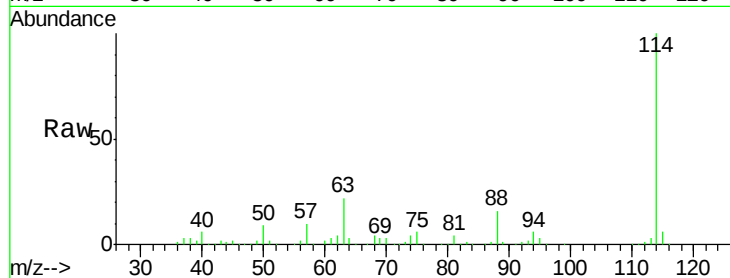

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VN0

Ion 87.90 (87.60 to 88.60): VN0

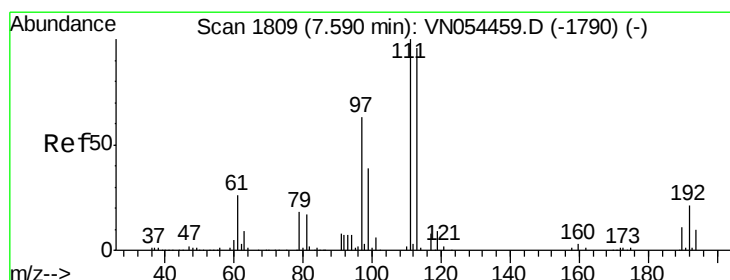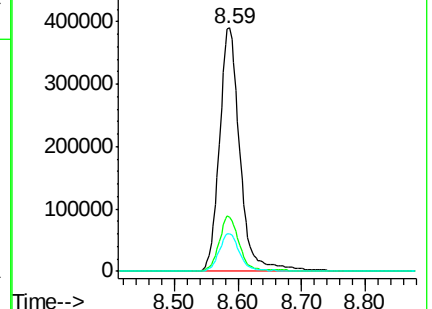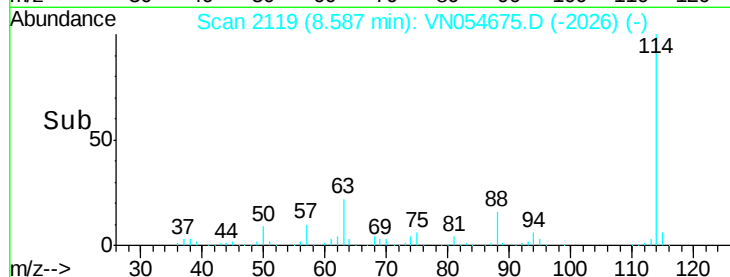

#35

Dibromofluoromethane

Concen: 48.551 ug/l

RT: 7.59 min Scan# 1810

Delta R.T. 0.00 min

Lab File: VN054675.D

Acq: 25 Mar 2019 16:19


Tgt Ion:113 Resp: 273601

Ion Ratio Lower Upper

113 100

111 102.4 82.2 123.4



192 20.3 19.2 28.8

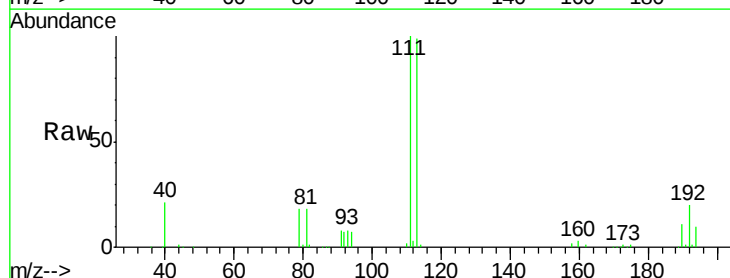


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

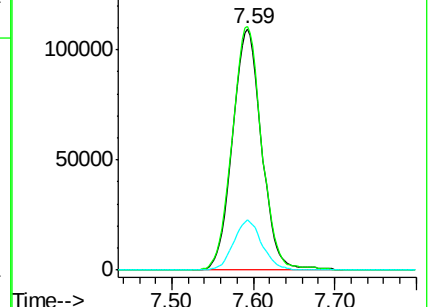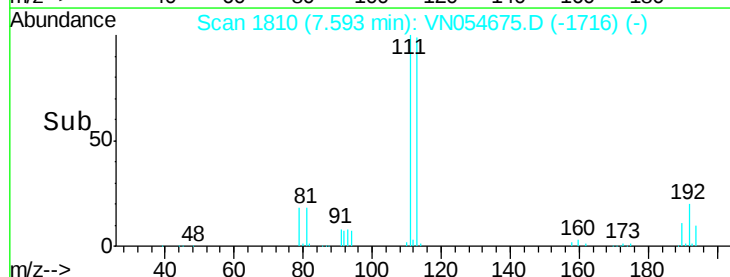

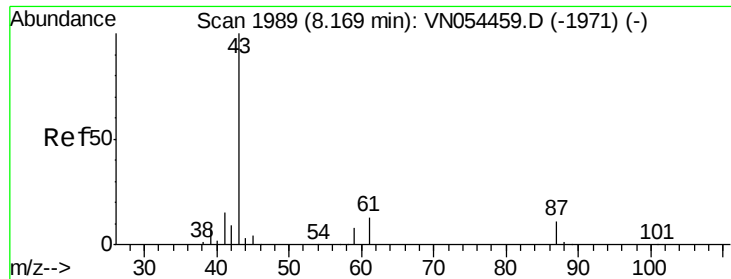

#43

Isopropyl Acetate

Concen: 1.652 ug/l

RT: 8.17 min Scan# 1990

Delta R.T. 0.00 min

Lab File: VN054675.D

Acq: 25 Mar 2019 16:19

Instrument :

MSVOA_N

ClientSampleId :

S4B(20)





Tot Ion: 43 Resp: 16232

Ion Ratio Lower Upper

43 100

61 19.1 15.8 23.8

87 13.3 12.0 18.0

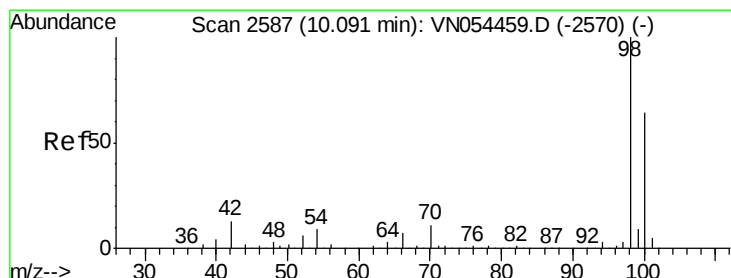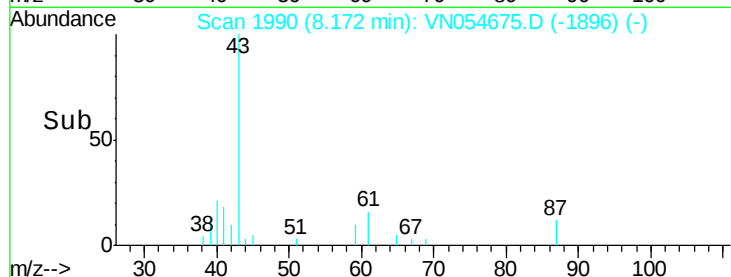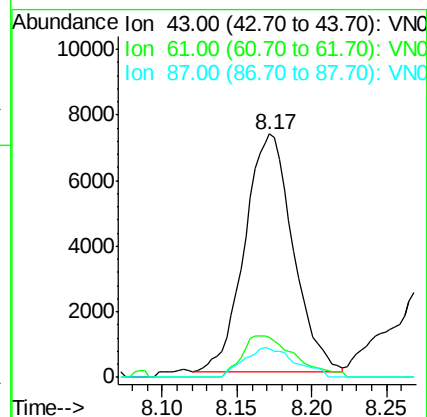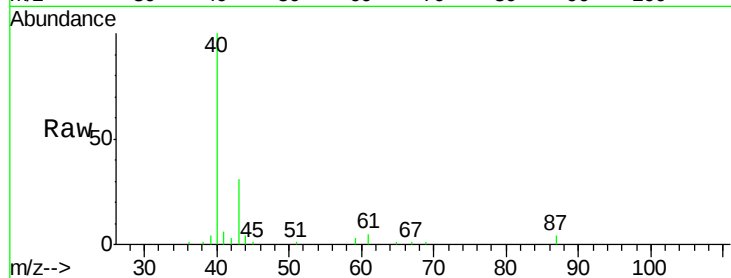

#50

Toluene-d8

Concen: 50.144 ug/l

RT: 10.09 min Scan# 2587

Delta R.T. 0.00 min

Lab File: VN054675.D




Acq: 25 Mar 2019 16:19


Tgt Ion: 98 Resp: 1062313

Ion Ratio Lower Upper

98 100

100 63.0 51.2 76.8

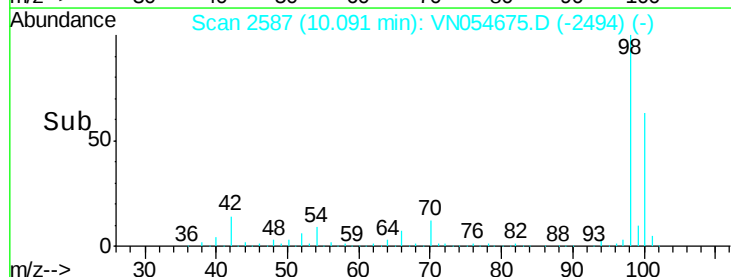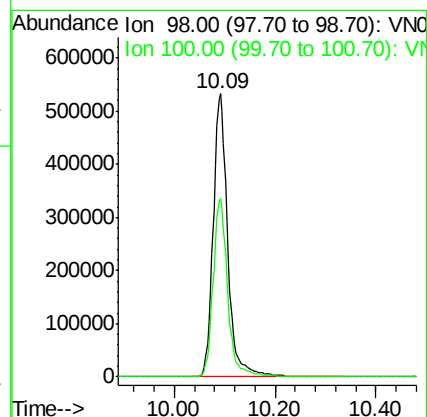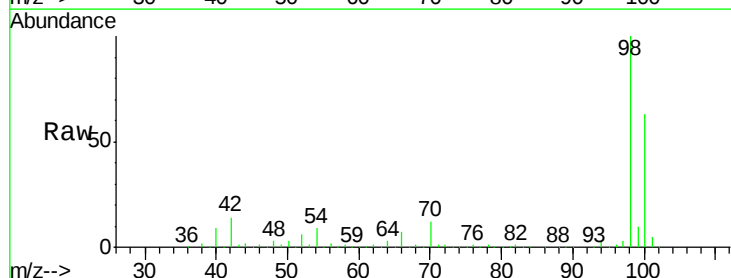

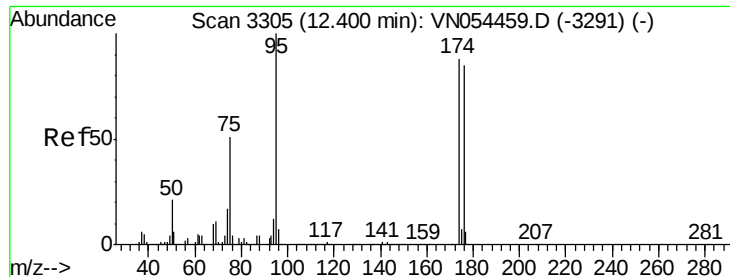

#62

4-Bromofluorobenzene

Concen: 46.236 ug/l

RT: 12.40 min Scan# 3305

Delta R.T. 0.00 min

Lab File: VN054675.D

Acq: 25 Mar 2019 16:19

Instrument :

MSVOA_N

ClientSampled :

S4B(20)


Tot Ion: 95 Resp: 333317

Ion Ratio Lower Upper

95 100

174 83.4 0.0 191.0




176 80.9 0.0 187.4

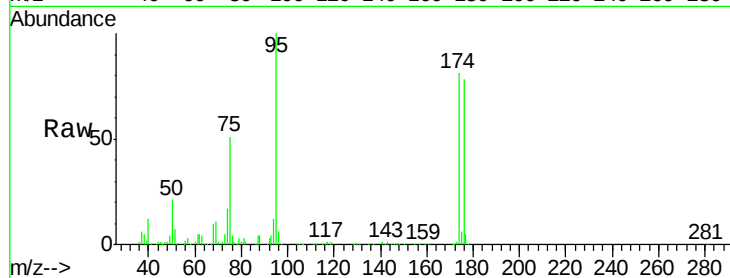

Abundance Ion 94.90 (94.60 to 95.60): VN054459.D (-3291) (-)

Ion 173.80 (173.50 to 174.50): VN054459.D (-3291) (-)

Ion 175.80 (175.50 to 176.50): VN054459.D (-3291) (-)

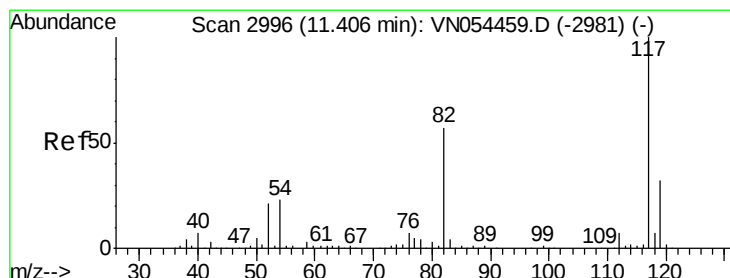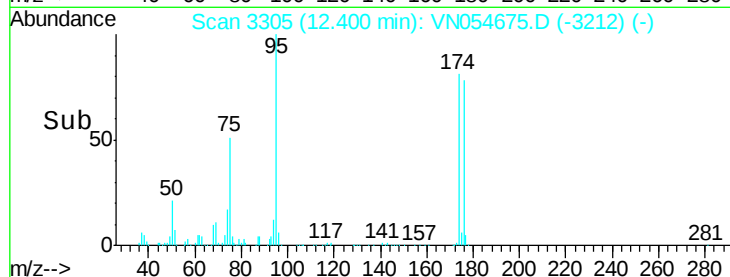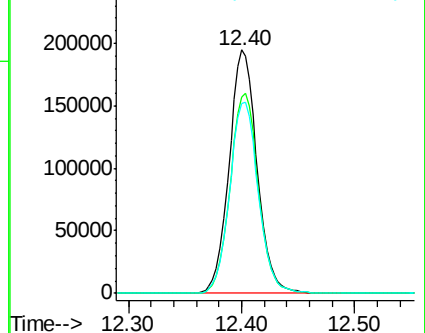

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.41 min Scan# 2996

Delta R.T. 0.00 min

Lab File: VN054675.D

Acq: 25 Mar 2019 16:19


Tgt Ion: 117 Resp: 741976

Ion Ratio Lower Upper

117 100

82 58.0 40.0 60.0



119 32.9 25.8 38.6

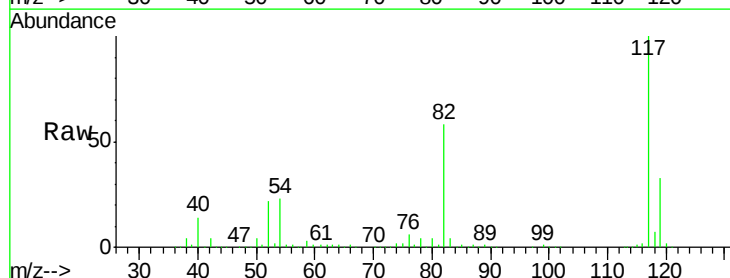


Abundance Ion 116.90 (116.60 to 117.60): VN054459.D (-2981) (-)

Ion 82.00 (81.70 to 82.70): VN054459.D (-2981) (-)

Ion 118.90 (118.60 to 119.60): VN054459.D (-2981) (-)

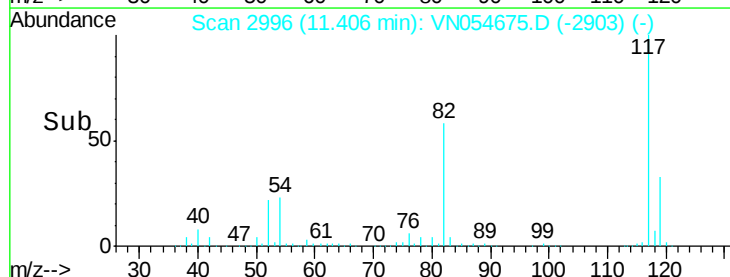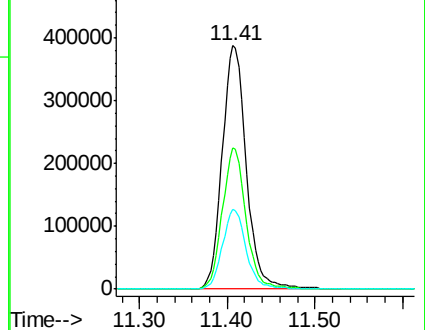

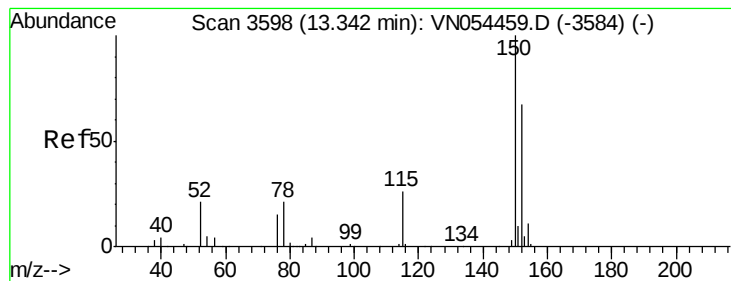

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.34 min Scan# 3598

Delta R.T. 0.00 min

Lab File: VN054675.D

Acq: 25 Mar 2019 16:19

Instrument :

MSVOA_N

ClientSampleId :

S4B(20)


Tot Ion:152 Resp: 276277

Ion Ratio Lower Upper

152 100

115 58.0 27.2 81.6

150 157.2 0.0 349.2

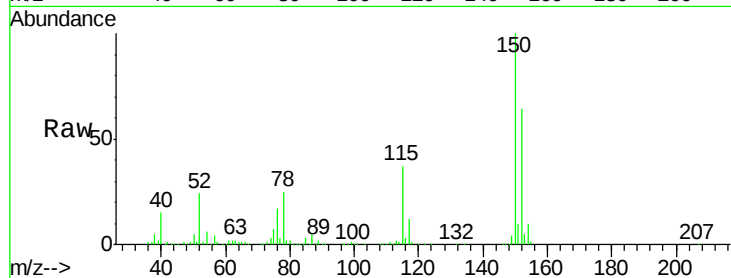

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

