


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN032520\
 Data File : VN060686.D
 Acq On : 25 Mar 2020 10:36
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N031820W.M
 Title : SW846 8260
 Last Update : Wed Mar 18 08:49:09 2020

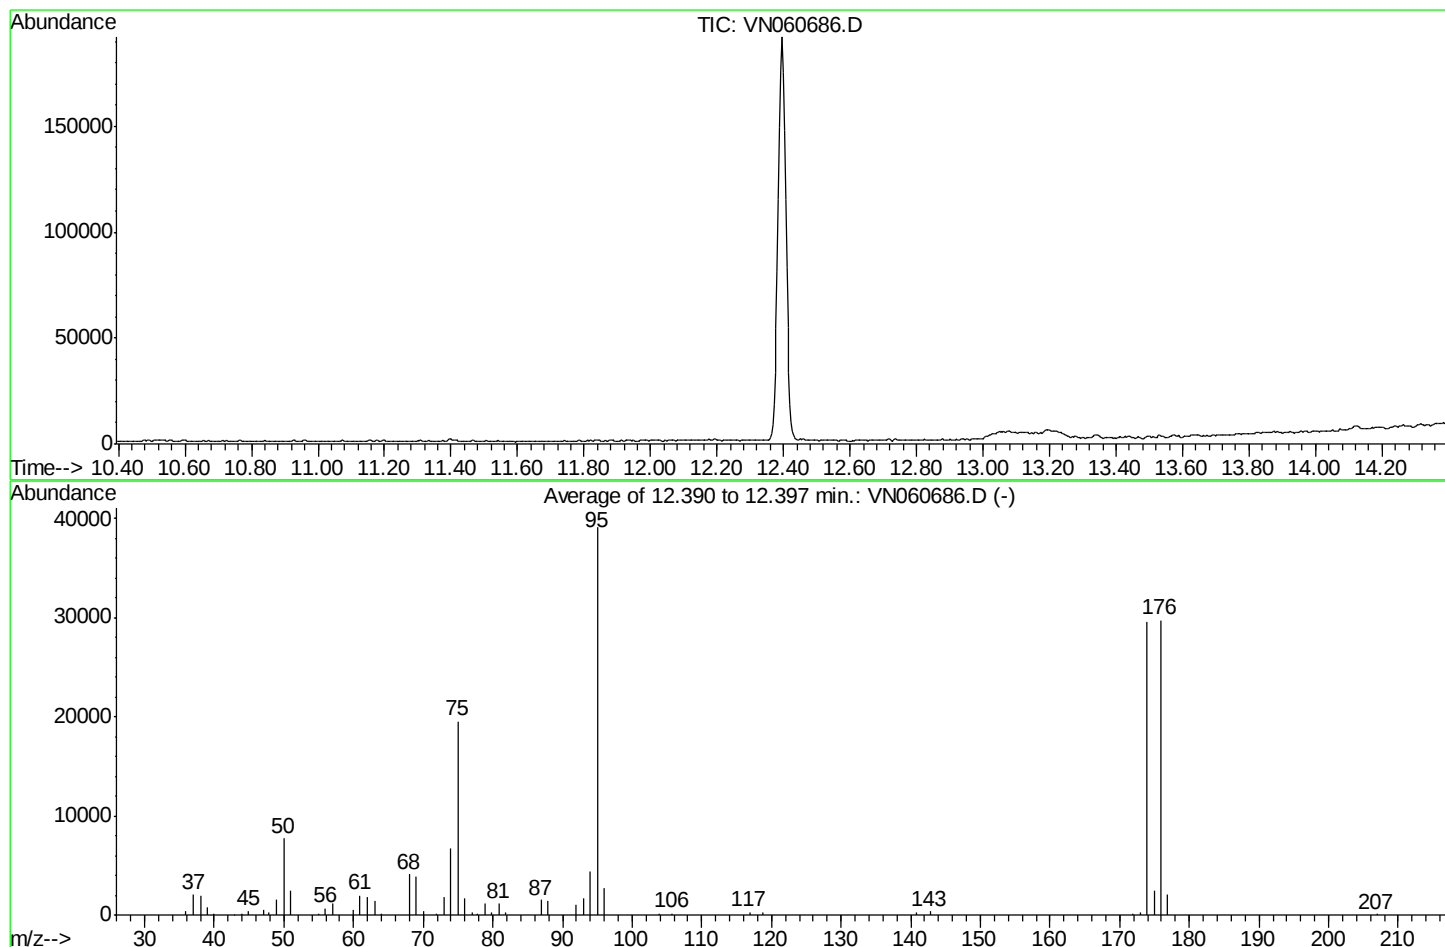

AutoFind: Scans 3302, 3303, 3304; Background Corrected with Scan 3289

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	7741	PASS
75	95	30	60	50.0	19546	PASS
95	95	100	100	100.0	39074	PASS
96	95	5	9	7.1	2761	PASS
173	174	0.00	2	0.8	225	PASS
174	95	50	100	75.7	29560	PASS
175	174	5	9	8.2	2414	PASS
176	174	95	101	100.4	29682	PASS
177	176	5	9	6.8	2007	PASS