


Chloromethane

Response Ratio

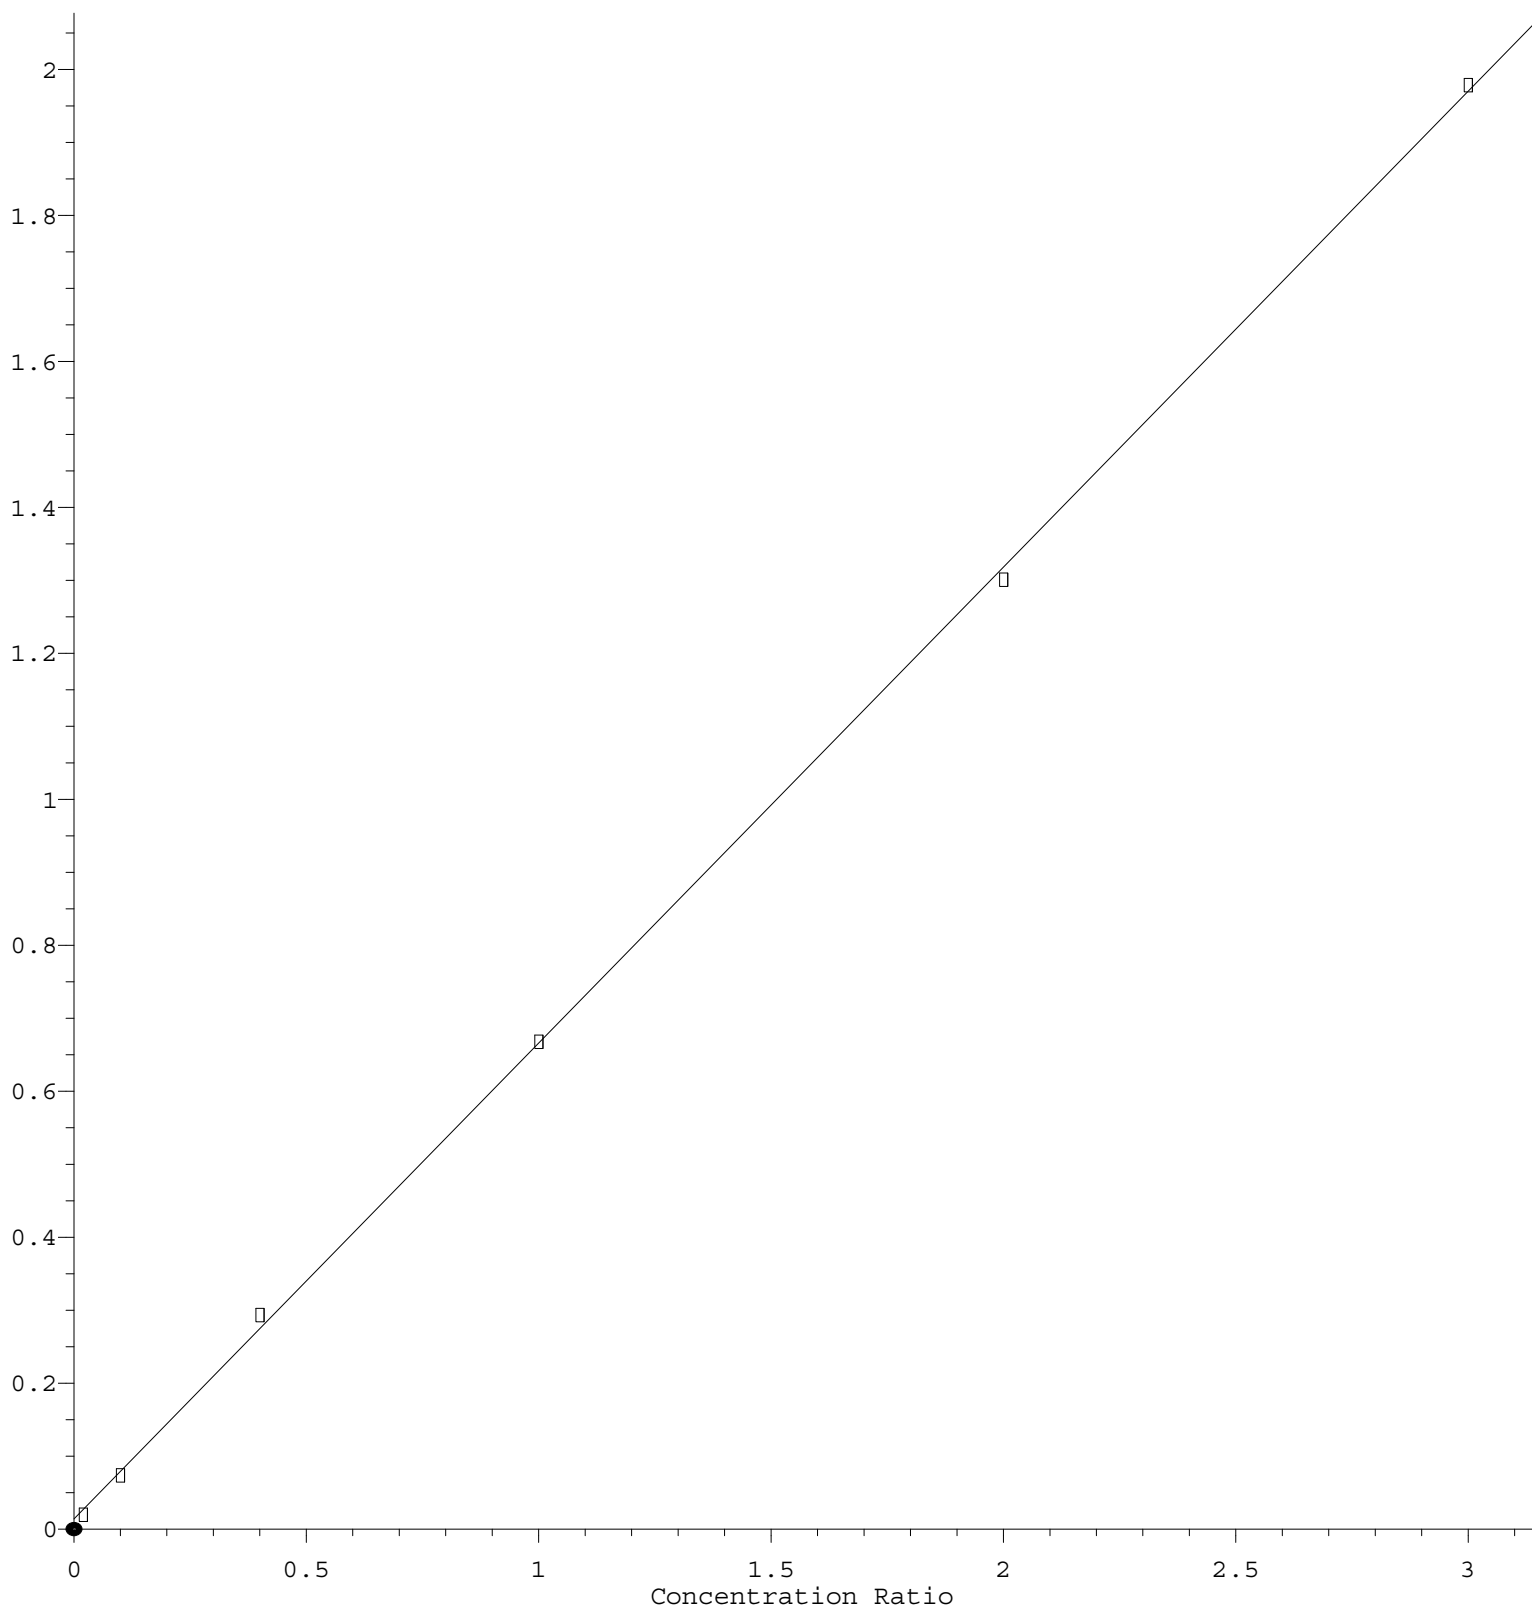

$$\text{Response} = 6.521\text{e-}001 * \text{Amt} + 1.364\text{e-}002$$


Coef of Det (r^2) = 0.999734 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N032521W.M

Calibration Table Last Updated: Fri Mar 26 16:26:01 2021

Methylene Chloride

Response Ratio

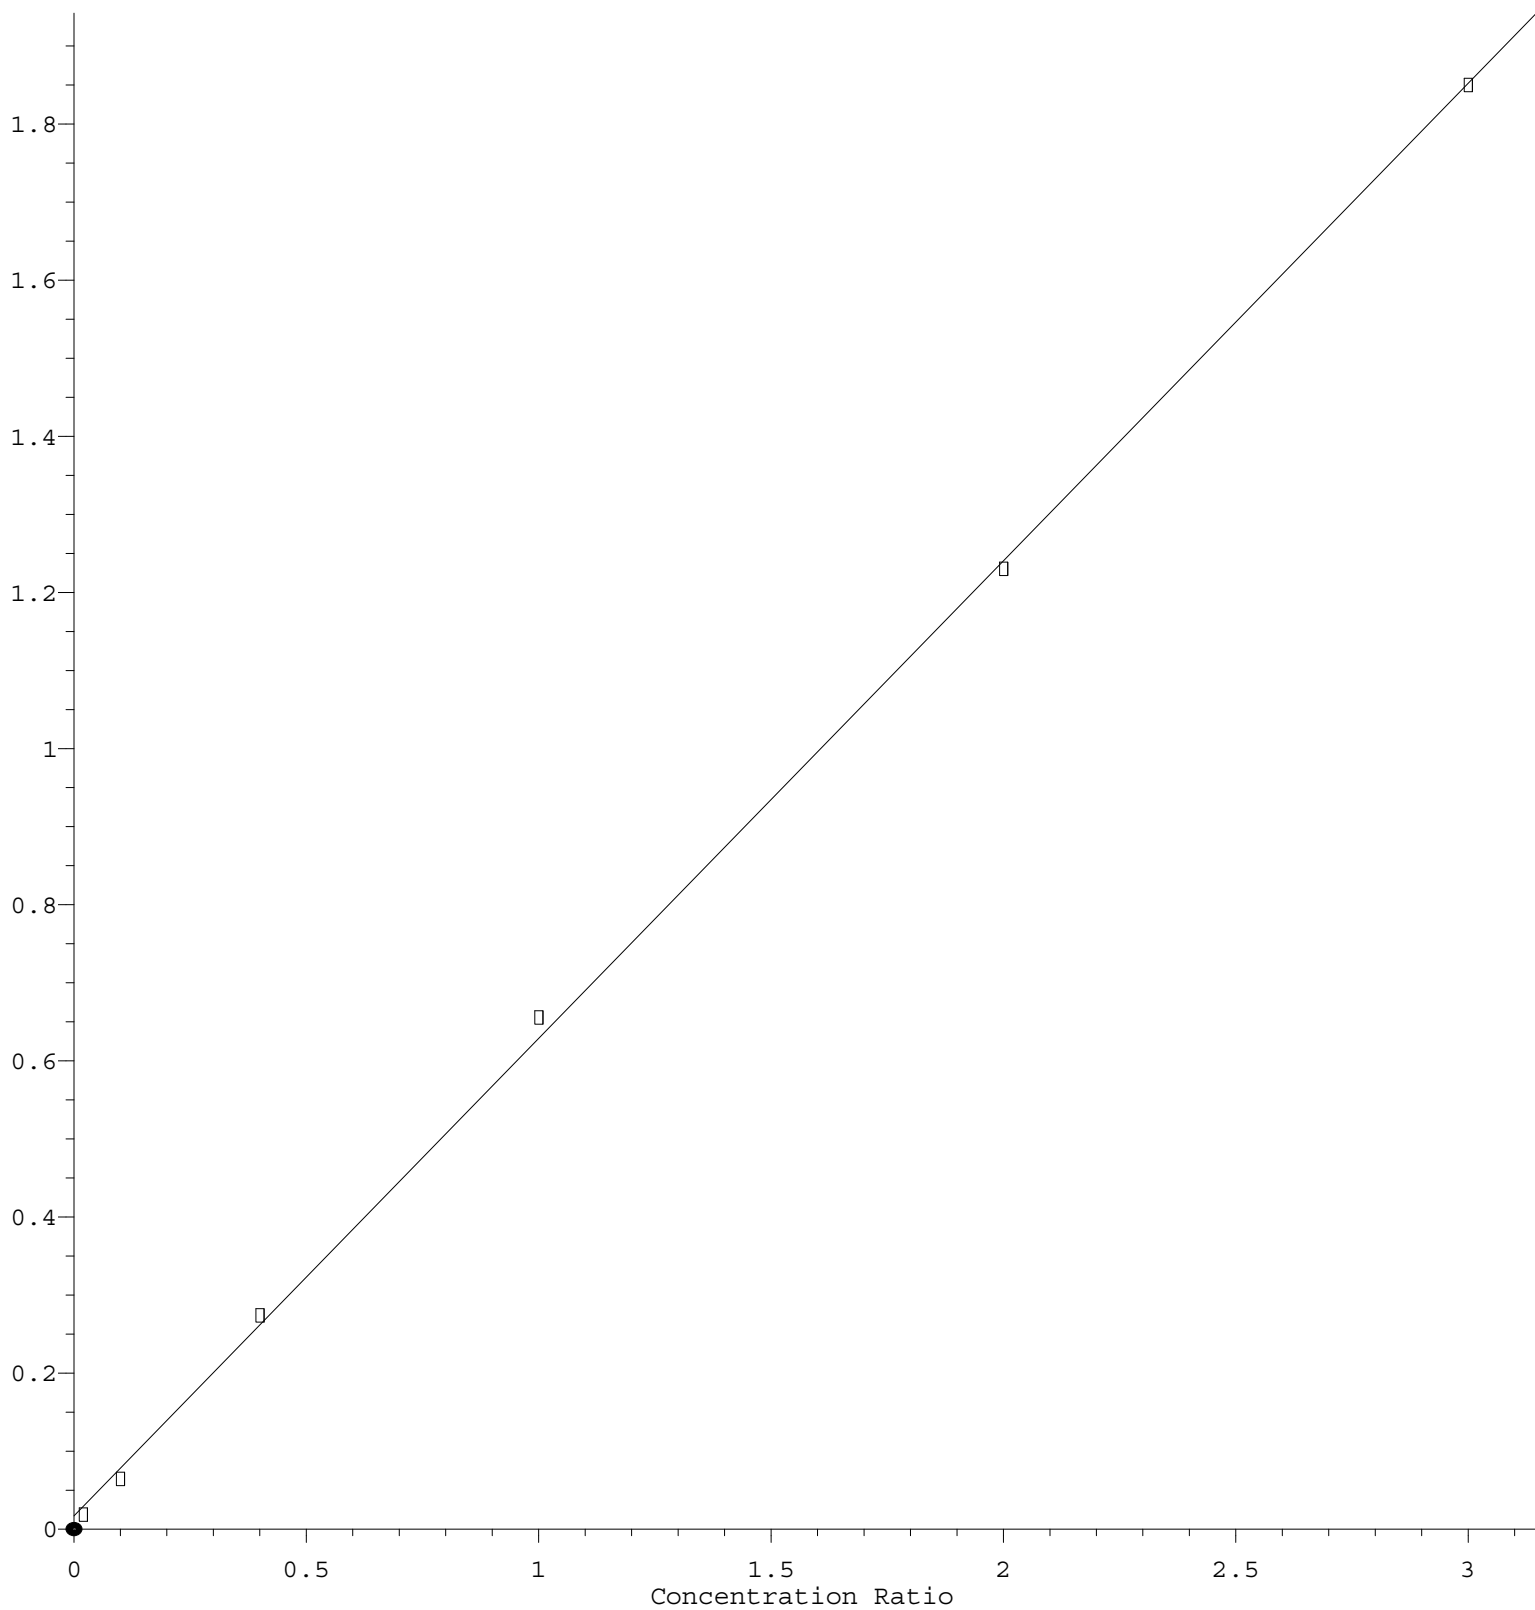


$$\text{Response} = 6.118\text{e-}001 * \text{Amt} + 1.725\text{e-}002$$

Coef of Det (r^2) = 0.999521 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N032521W.M

Calibration Table Last Updated: Fri Mar 26 16:26:01 2021


Acrolein

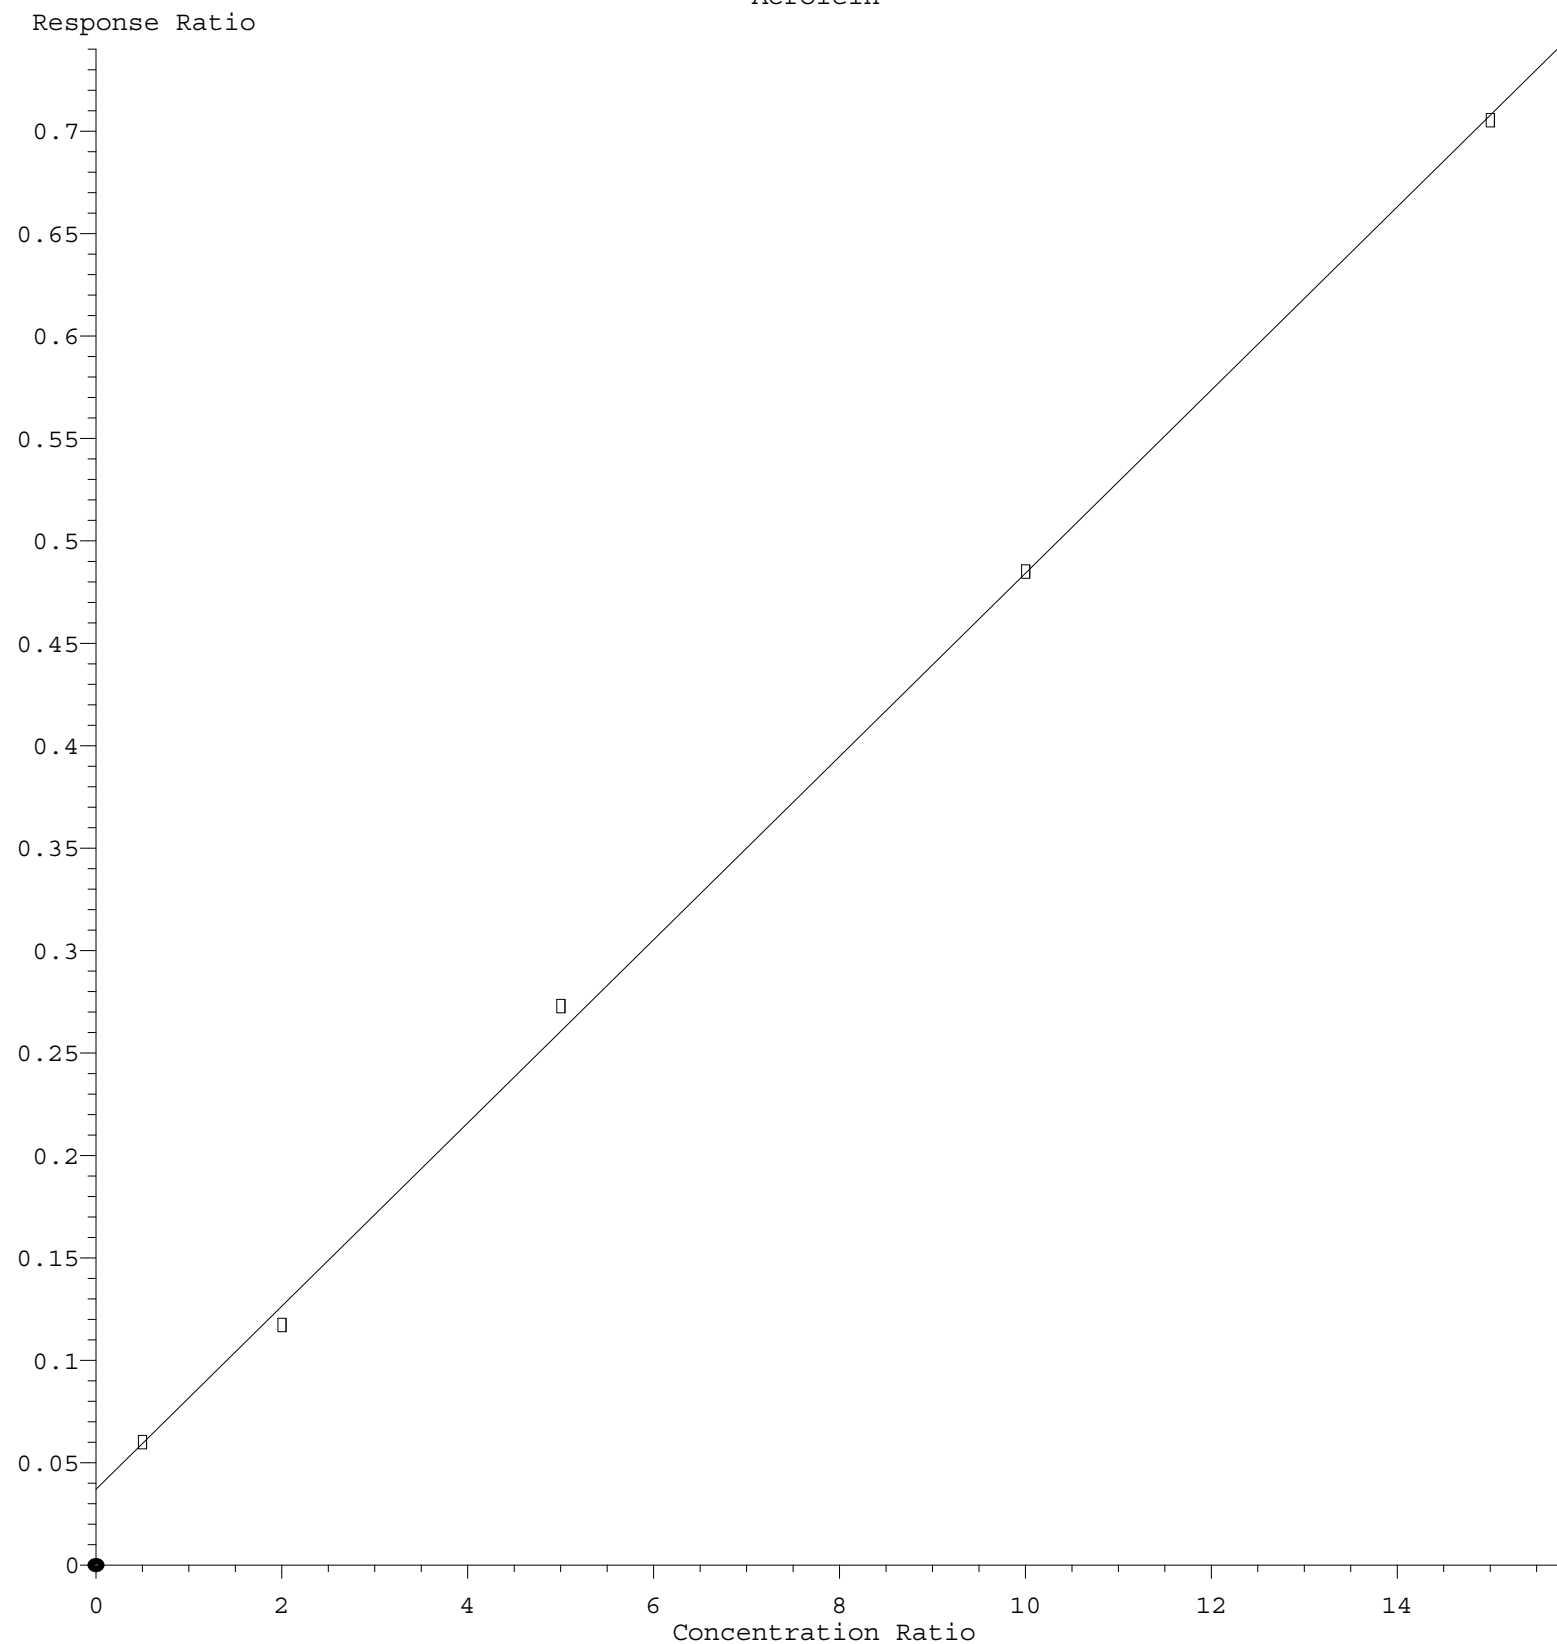

Response = $4.472 \times 10^{-2} \times \text{Amt} + 3.740 \times 10^{-2}$
 Coef of Det (r^2) = 0.999154 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N032521W.M
 Calibration Table Last Updated: Fri Mar 26 16:26:01 2021

Naphthalene


Response Ratio

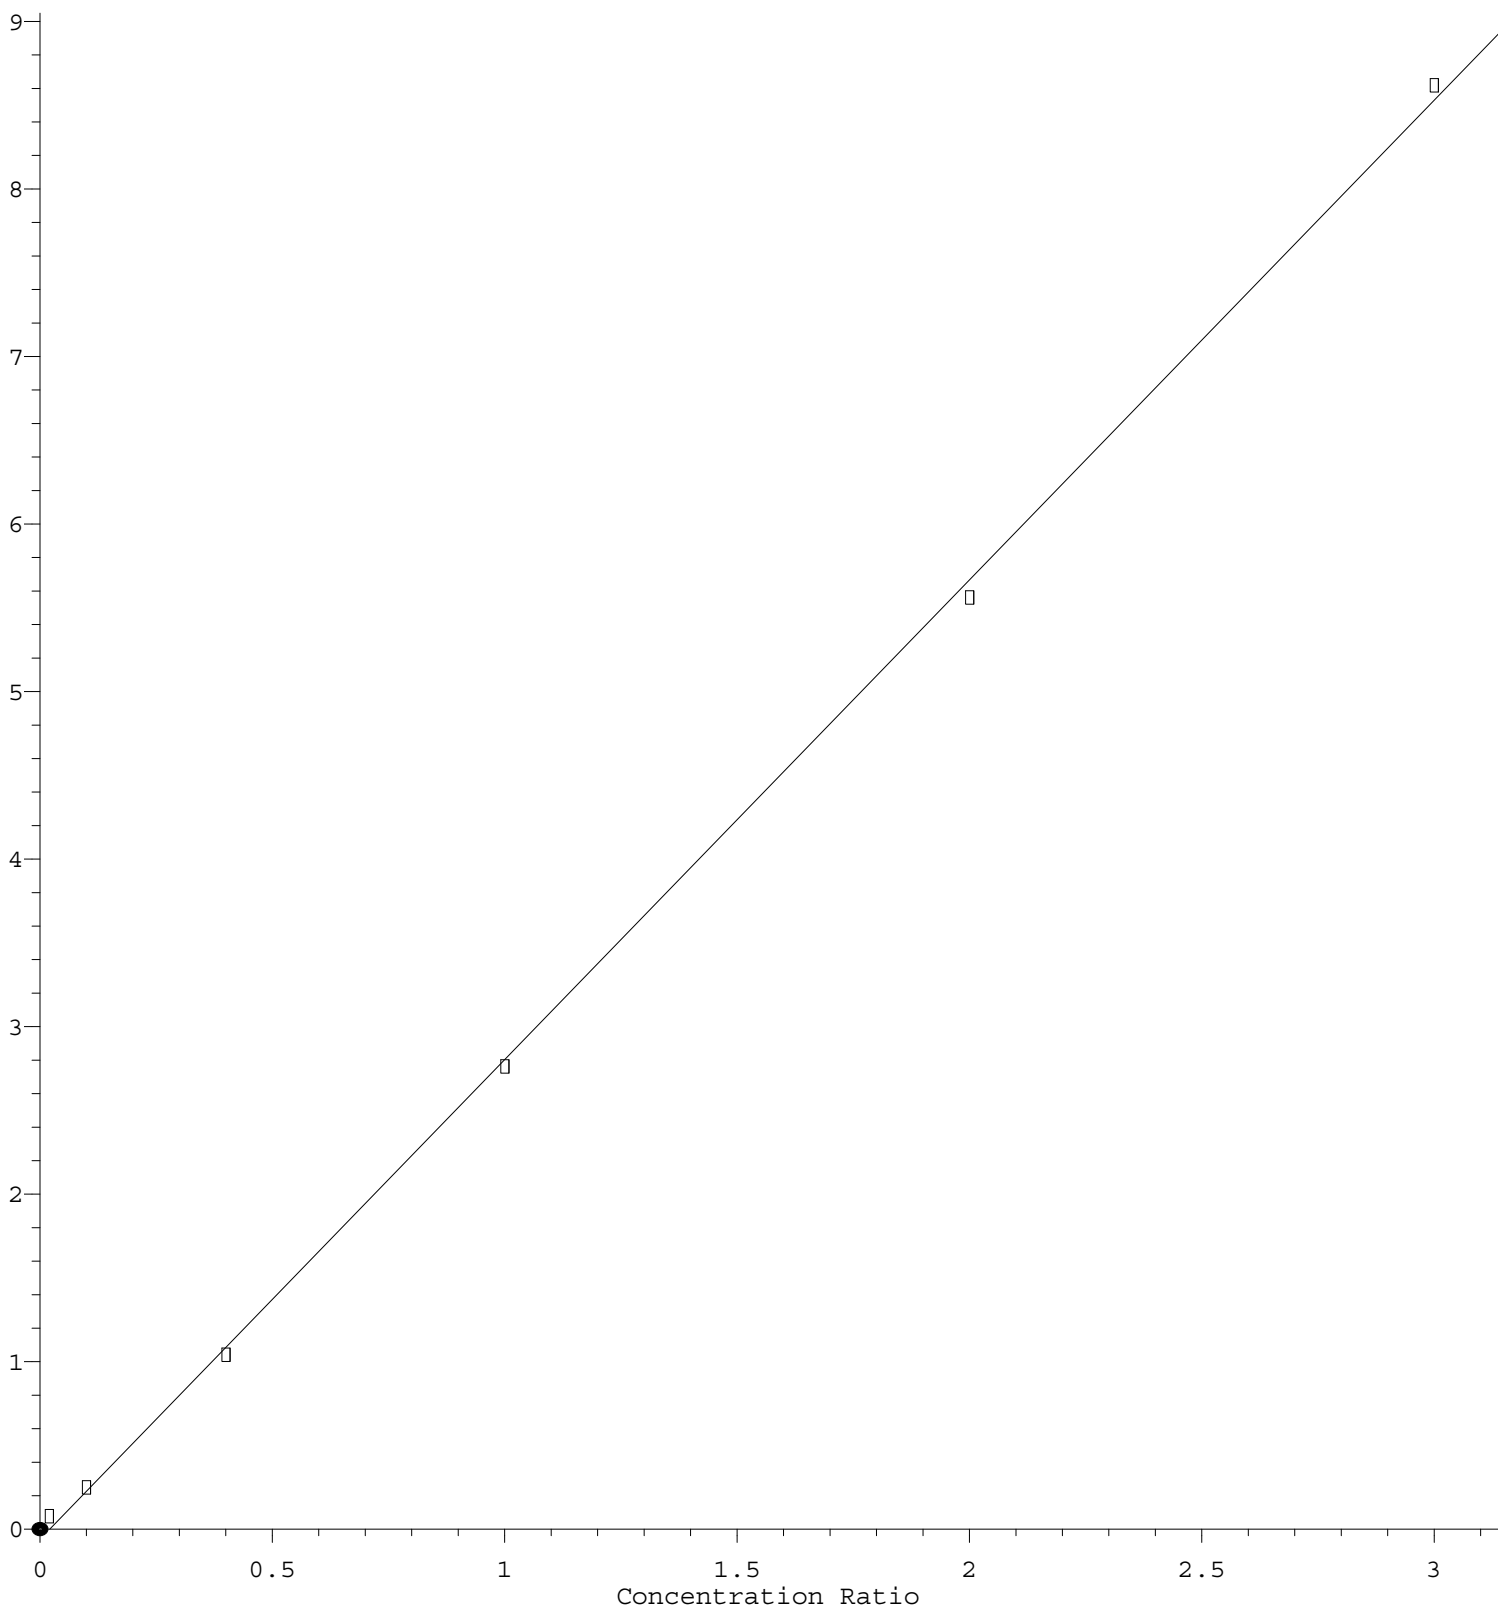

Response = 2.863e+000 * Amt - 5.968e-002
 Coef of Det (r^2) = 0.999490 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N032521W.M
 Calibration Table Last Updated: Fri Mar 26 16:26:01 2021

N-amyl acetate

Response Ratio

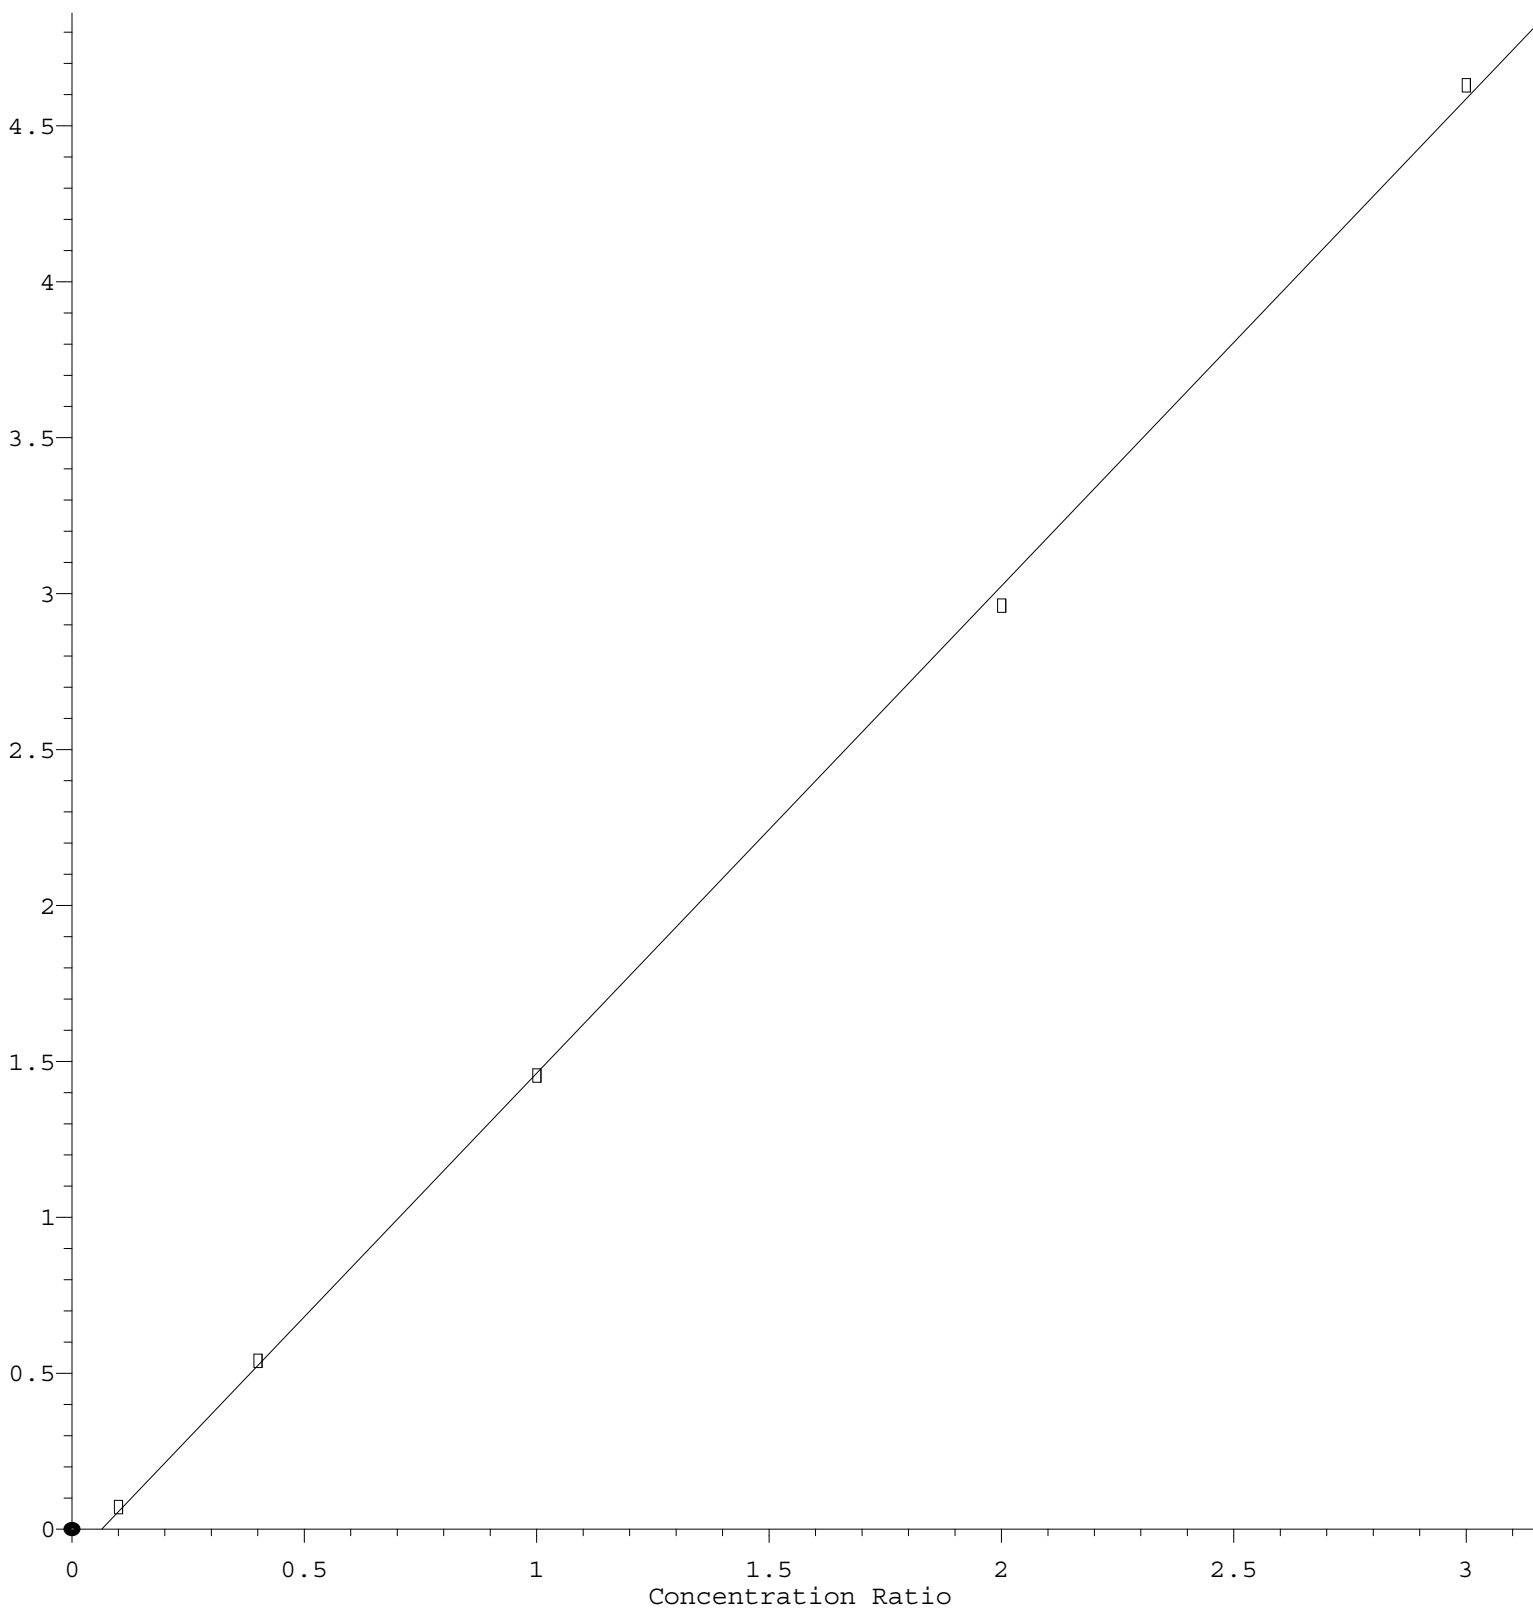

$$\text{Response} = 1.562e+000 * \text{Amt} - 9.980e-002$$


Coef of Det (r^2) = 0.999545 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N032521W.M

Calibration Table Last Updated: Fri Mar 26 16:26:01 2021

2-Chloroethyl Vinyl ether

Response Ratio

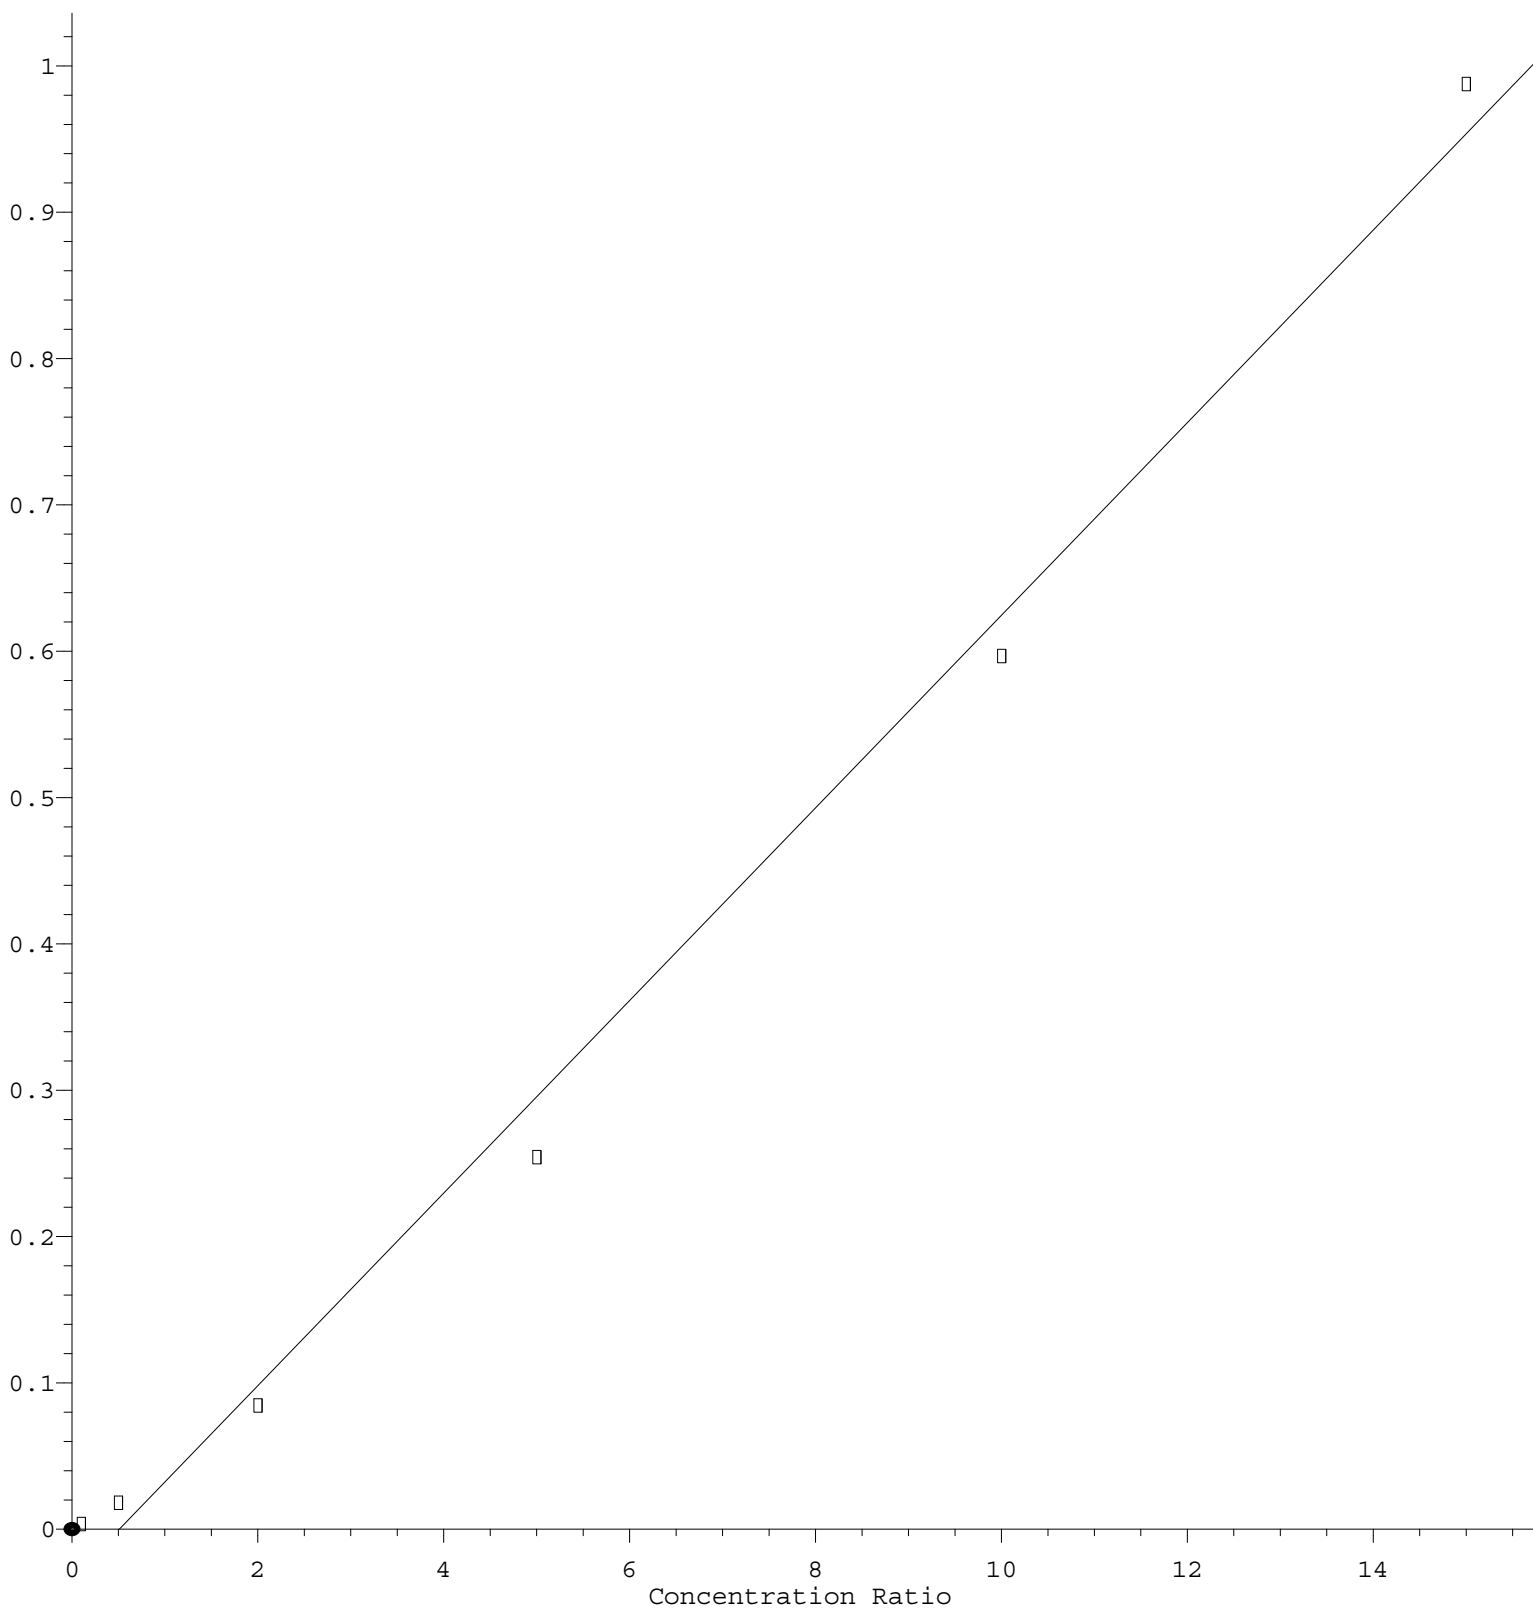

$$\text{Response} = 6.586\text{e-}002 * \text{Amt} - 3.372\text{e-}002$$

Coef of Det (r^2) = 0.993413 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N032521W.M

Calibration Table Last Updated: Fri Mar 26 16:26:01 2021