


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032521\
Data File : VN066329.D
Acq On : 25 Mar 2021 13:48
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N032521W.M
Title : SW846 8260
Last Update : Fri Mar 26 16:26:01 2021

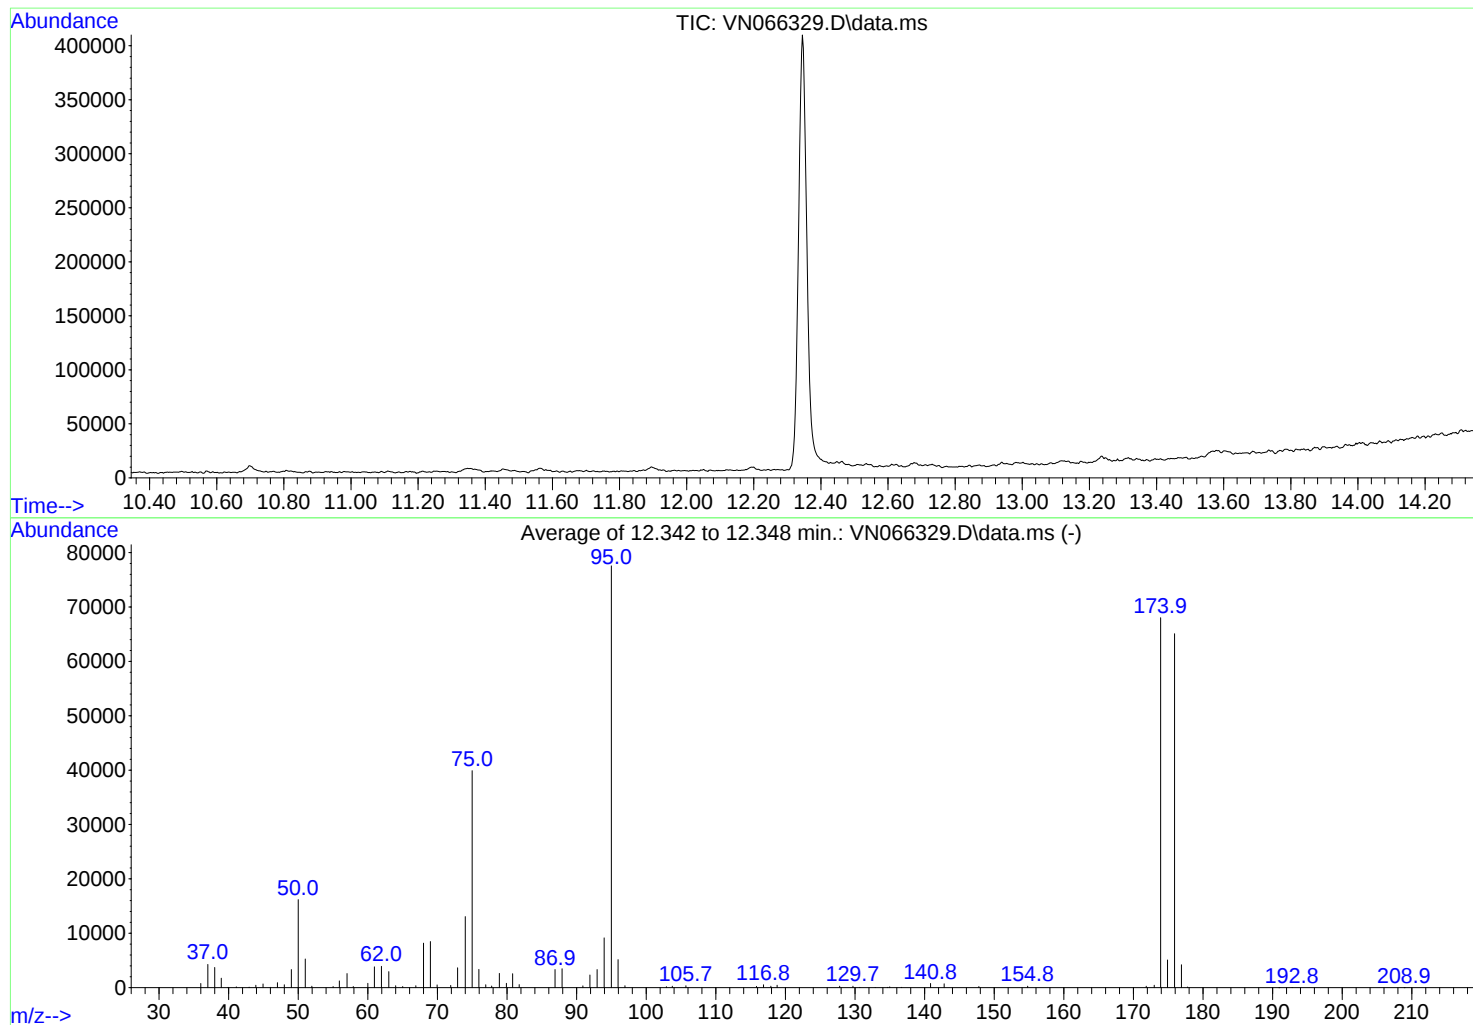

AutoFind: Scans 3972, 3973, 3974; Background Corrected with Scan 3956

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.9	16173	PASS
75	95	30	60	51.4	39901	PASS
95	95	100	100	100.0	77568	PASS
96	95	5	9	6.6	5142	PASS
173	174	0.00	2	0.7	455	PASS
174	95	50	100	87.7	68016	PASS
175	174	5	9	7.5	5100	PASS
176	174	95	101	95.7	65099	PASS
177	176	5	9	6.5	4217	PASS