

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032522\
 Data File : VN071542.D
 Acq On : 25 Mar 2022 13:04
 Operator : JC\MD
 Sample : PB143557ZHE#01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB143557ZHE#01

Quant Time: Mar 26 04:00:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N032522W.M
 Quant Title : SW846 8260
 QLast Update : Fri Mar 25 09:52:40 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.081	168	861291	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.963	114	1440344	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.739	117	1428182	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.674	152	527744	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.433	65	497987	46.538	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	93.080%		
35) Dibromofluoromethane	8.022	113	414968	45.842	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	91.680%		
50) Toluene-d8	10.439	98	1801746	49.347	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	98.700%		
62) 4-Bromofluorobenzene	12.727	95	606664	50.709	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	101.420%		
Target Compounds						Qvalue
3) Chloromethane	2.293	50	4918	Below Cal	#	77
5) Bromomethane	2.875	94	2811	0.439	ug/l #	70
6) Chloroethane	2.769	64	1692	0.208	ug/l #	64
8) Diethyl Ether	3.834	74	15098	2.589	ug/l	95
11) Tert butyl alcohol	5.316	59	3928	1.970	ug/l #	72
16) Acetone	4.293	43	26150	5.962	ug/l	97
18) Methyl Acetate	4.863	43	10468	Below Cal		100
20) Methylene Chloride	5.087	84	14103	1.380	ug/l #	93
25) 2-Butanone	7.334	43	6694	0.951	ug/l #	82
29) Tetrahydrofuran	7.692	42	1432	0.306	ug/l #	89
31) Cyclohexane	8.081	56	16148	1.055	ug/l #	27
36) 1,1-Dichloropropene	8.081	75	61271	4.695	ug/l #	48
38) Carbon Tetrachloride	8.086	117	78998	6.209	ug/l #	17
43) Isopropyl Acetate	8.557	43	71520	2.760	ug/l #	90
45) 1,2-Dichloropropane	9.622	63	5120	0.509	ug/l #	44
48) Methyl methacrylate	9.539	41	17631	1.717	ug/l #	10
49) 1,4-Dioxane	9.580	88	110	0.464	ug/l #	25
51) 4-Methyl-2-Pentanone	10.322	43	12626	0.886	ug/l	94
54) cis-1,3-Dichloropropene	10.239	75	115394	7.249	ug/l #	62
57) 1,3-Dichloropropane	11.086	76	73476	4.236	ug/l #	43
58) 2-Chloroethyl Vinyl ether	10.080	63	60	18.695	ug/l #	44
59) 2-Hexanone	11.086	43	972525	94.719	ug/l #	46
75) 1,1,2,2-Tetrachloroethane	12.827	83	250	Below Cal	#	25
76) 1,2,3-Trichloropropane	12.727	75	299974	25.491	ug/l #	1
80) 1,3,5-Trimethylbenzene	13.057	105	11818	0.322	ug/l	96
81) trans-1,4-Dichloro-2-b...	12.727	75	299974	68.246	ug/l #	10
93) 1,2,4-Trichlorobenzene	15.268	180	2116	0.253	ug/l	96
95) Naphthalene	15.504	128	6707	3.448	ug/l #	92
96) 1,2,3-Trichlorobenzene	15.692	180	2271	0.274	ug/l	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032522\
Data File : VN071542.D
Acq On : 25 Mar 2022 13:04
Operator : JC\MD
Sample : PB143557ZHE#01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB143557ZHE#01

Quant Time: Mar 26 04:00:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N032522W.M
Quant Title : SW846 8260
QLast Update : Fri Mar 25 09:52:40 2022
Response via : Initial Calibration




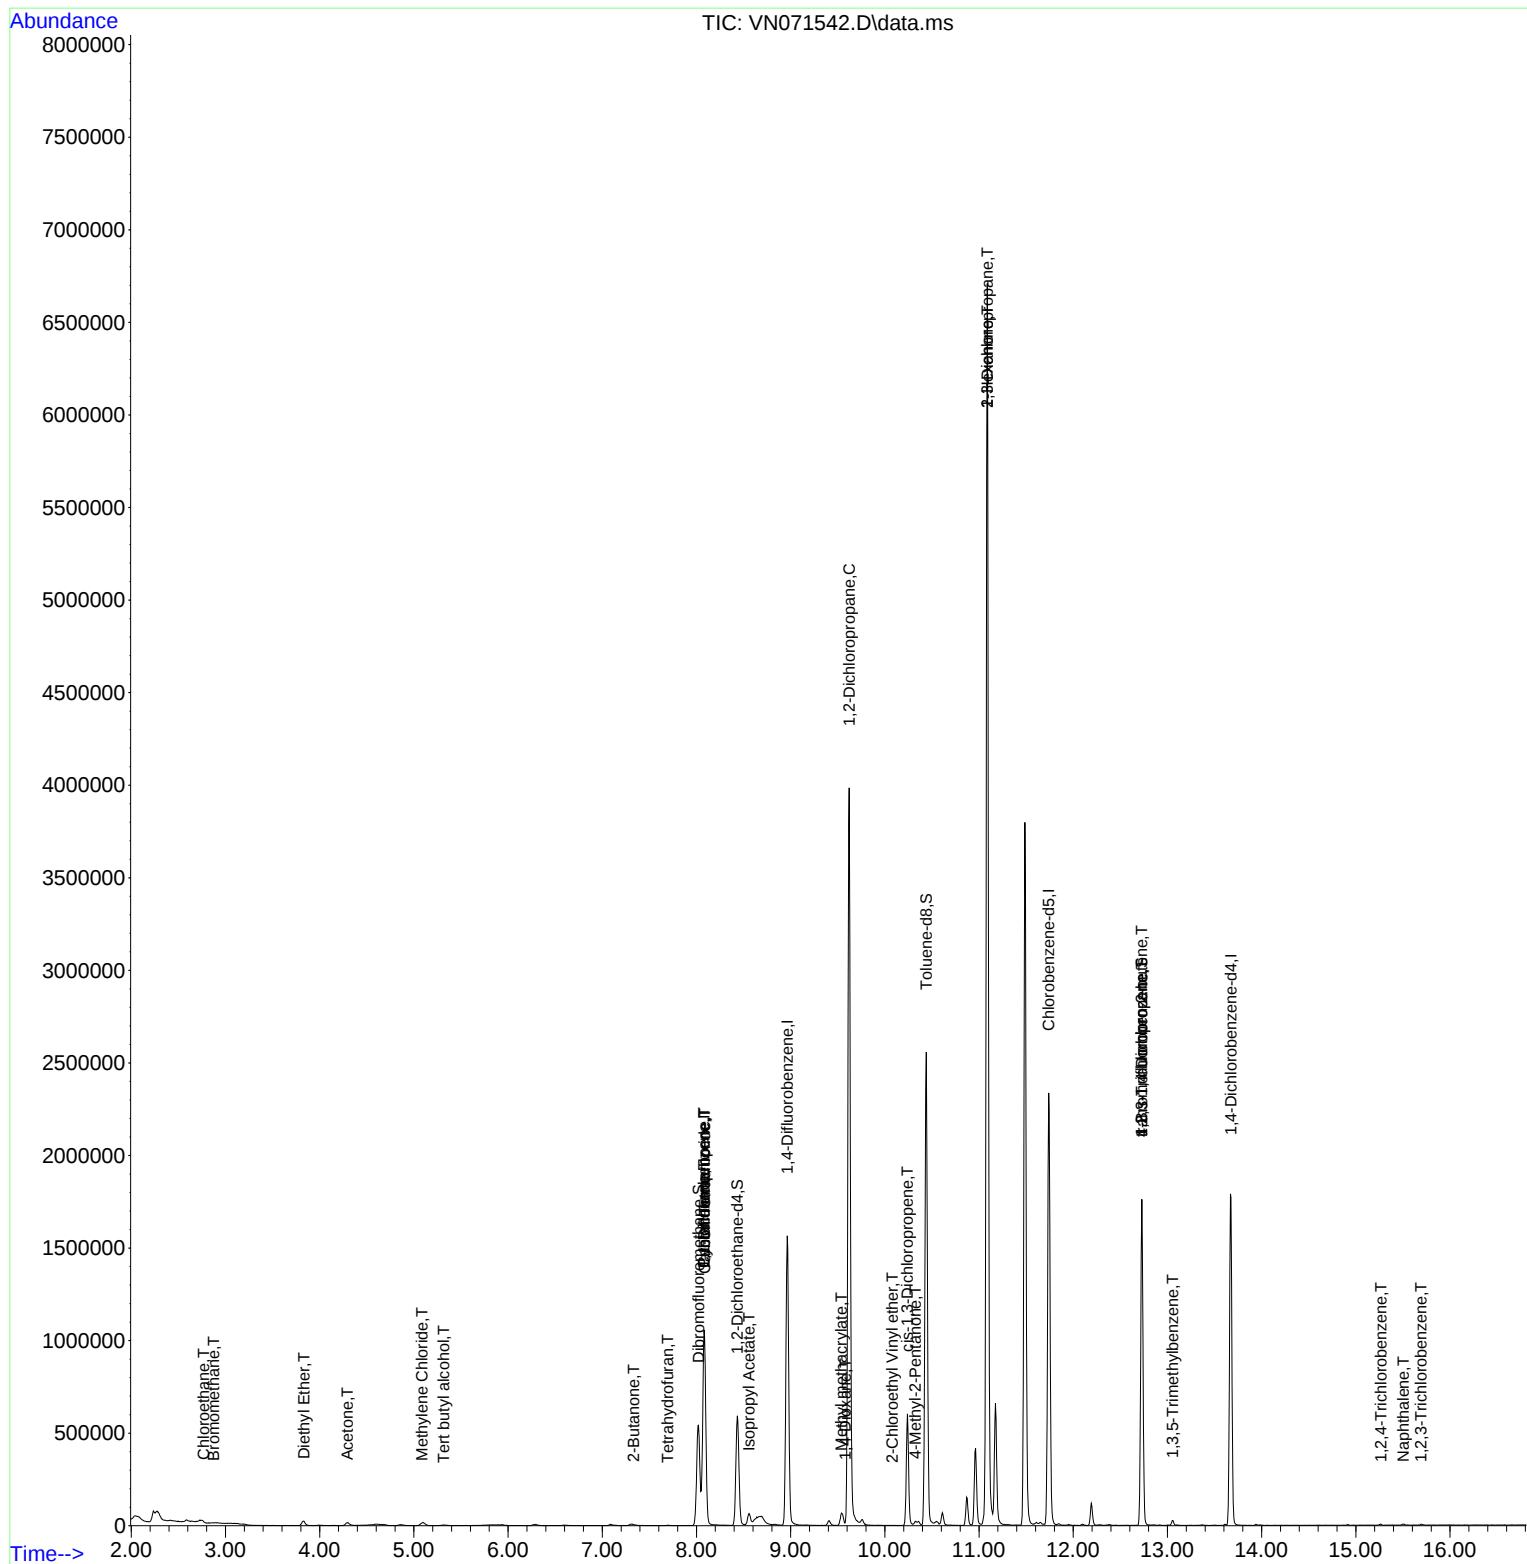




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.081 min Scan# 10
Delta R.T. -0.000 min
Lab File: VN071542.D
Acq: 25 Mar 2022 13:04




Instrument :
MSVOA_N
ClientSampleId :
PB143557ZHE#01


Tgt Ion:168 Resp: 861291
Ion Ratio Lower Upper
168 100
99 55.6 42.3 63.5

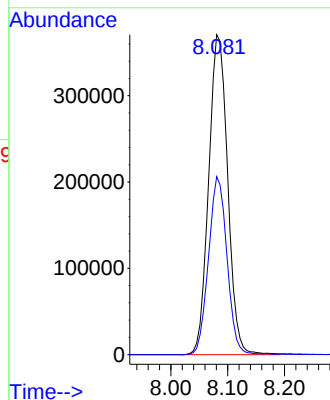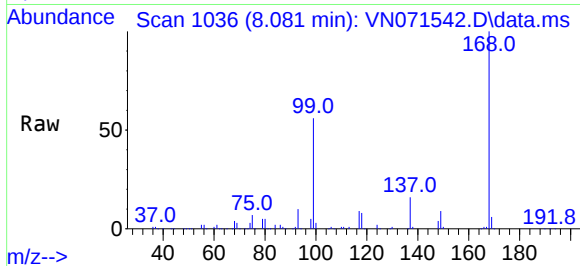

#3
Chloromethane
Concen: Below Cal
RT: 2.293 min Scan# 52
Delta R.T. -0.006 min
Lab File: VN071542.D
Acq: 25 Mar 2022 13:04

Tgt Ion: 50 Resp: 4918
Ion Ratio Lower Upper
50 100
52 19.1 25.7 38.5#



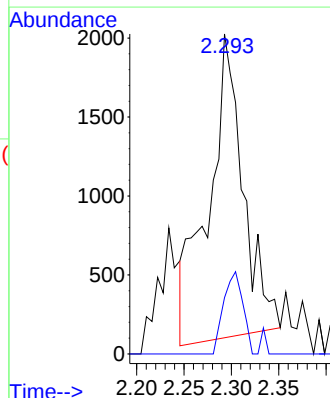
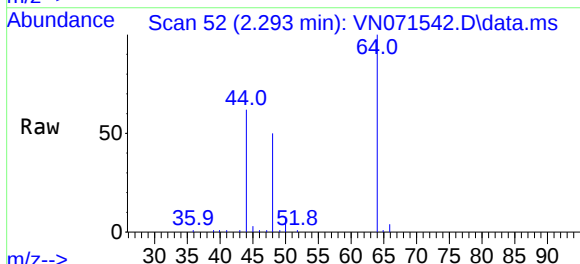




#5
Bromomethane
Concen: 0.439 ug/l
RT: 2.875 min Scan# 11
Delta R.T. 0.041 min
Lab File: VN071542.D
Acq: 25 Mar 2022 13:04




Instrument :
MSVOA_N
ClientSampleId :
PB143557ZHE#01


Tgt Ion: 94 Resp: 2811
Ion Ratio Lower Upper
94 100
96 65.7 76.0 114.0#

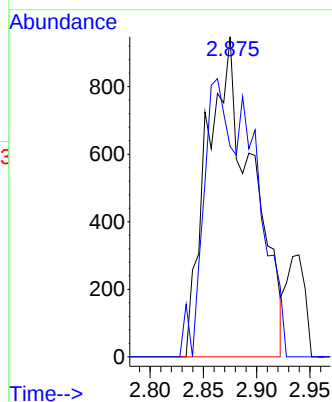

#6
Chloroethane
Concen: 0.208 ug/l
RT: 2.769 min Scan# 133
Delta R.T. -0.236 min
Lab File: VN071542.D
Acq: 25 Mar 2022 13:04

Tgt Ion: 64 Resp: 1692
Ion Ratio Lower Upper
64 100
66 12.6 26.2 39.4#


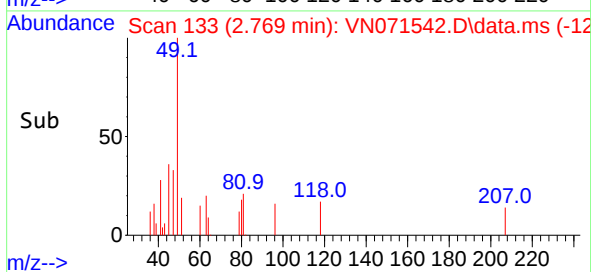
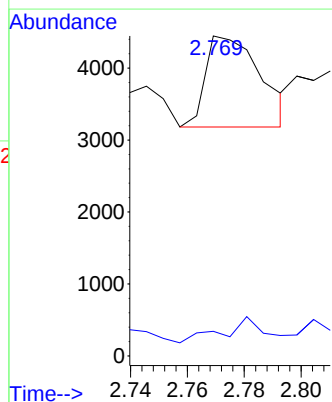





#8
Diethyl Ether
Concen: 2.589 ug/l
RT: 3.834 min Scan# 31
Delta R.T. 0.012 min
Lab File: VN071542.D
Acq: 25 Mar 2022 13:04




Instrument :
MSVOA_N
ClientSampleId :
PB143557ZHE#01


Tgt Ion: 74 Resp: 15098
Ion Ratio Lower Upper
74 100
45 90.7 42.9 128.5

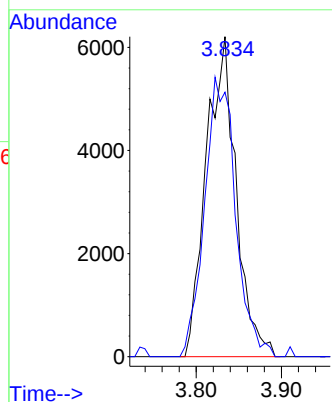

#11
Tert butyl alcohol
Concen: 1.970 ug/l
RT: 5.316 min Scan# 566
Delta R.T. -0.047 min
Lab File: VN071542.D
Acq: 25 Mar 2022 13:04

Tgt Ion: 59 Resp: 3928
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#


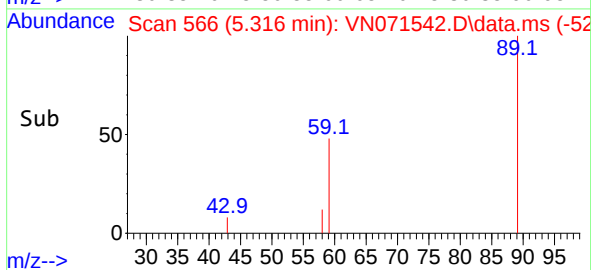
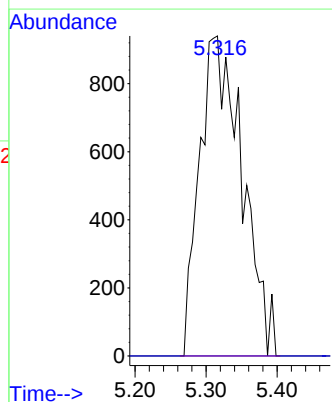





#16
Acetone
Concen: 5.962 ug/l
RT: 4.293 min Scan# 391
Delta R.T. 0.012 min
Lab File: VN071542.D
Acq: 25 Mar 2022 13:04




Instrument :
MSVOA_N
ClientSampleId :
PB143557ZHE#01


Tgt Ion: 43 Resp: 26150
Ion Ratio Lower Upper
43 100
58 30.8 26.0 39.0

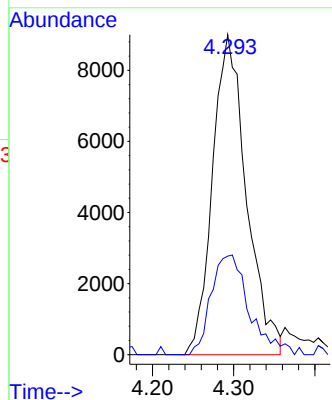

#18
Methyl Acetate
Concen: Below Cal
RT: 4.863 min Scan# 489
Delta R.T. 0.017 min
Lab File: VN071542.D
Acq: 25 Mar 2022 13:04

Tgt Ion: 43 Resp: 10468
Ion Ratio Lower Upper
43 100
74 26.8 21.6 32.4

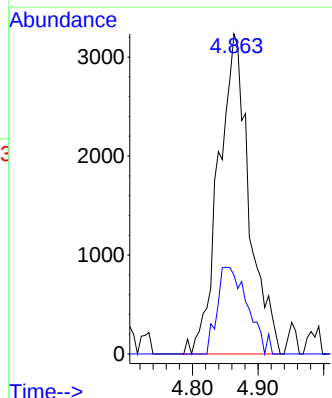




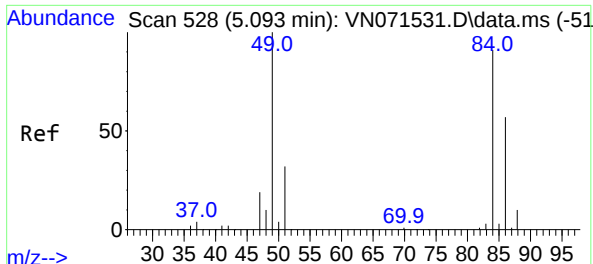


#20
Methylene Chloride
Concen: 1.380 ug/l
RT: 5.087 min Scan# 51
Delta R.T. -0.006 min
Lab File: VN071542.D
Acq: 25 Mar 2022 13:04

Instrument :
MSVOA_N
ClientSampleId :
PB143557ZHE#01

Tgt Ion: 84 Resp: 14103




Ion	Ratio	Lower	Upper
84	100		
49	110.3	88.3	132.5
51	26.1	28.2	42.2#
86	75.5	50.6	76.0

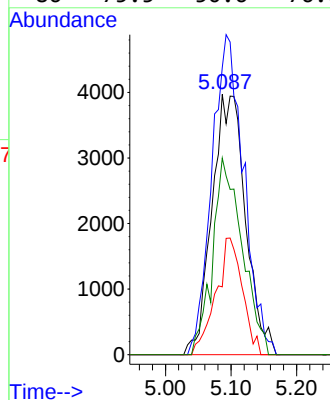


#25
2-Butanone
Concen: 0.951 ug/l
RT: 7.334 min Scan# 909
Delta R.T. 0.006 min
Lab File: VN071542.D
Acq: 25 Mar 2022 13:04

Tgt Ion: 43 Resp: 6694

Ion	Ratio	Lower	Upper
43	100		
72	20.1	23.7	35.5#


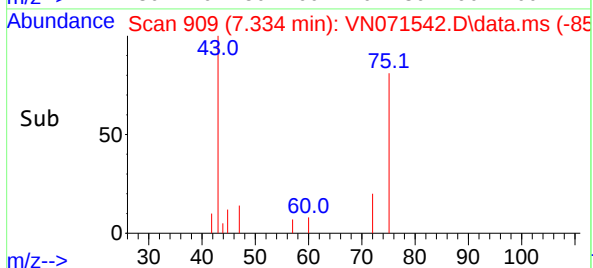
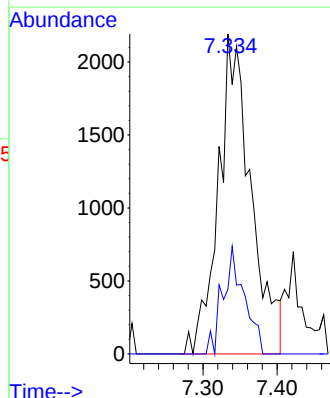
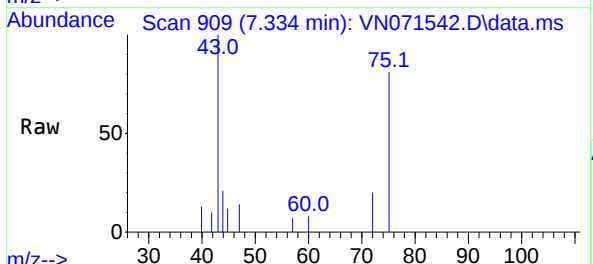




#29
Tetrahydrofuran
Concen: 0.306 ug/l
RT: 7.692 min Scan# 91
Delta R.T. 0.012 min
Lab File: VN071542.D
Acq: 25 Mar 2022 13:04




Instrument :
MSVOA_N
ClientSampleId :
PB143557ZHE#01


Tgt Ion: 42 Resp: 1432
Ion Ratio Lower Upper
42 100
72 37.6 39.7 59.5#
71 43.6 36.6 55.0

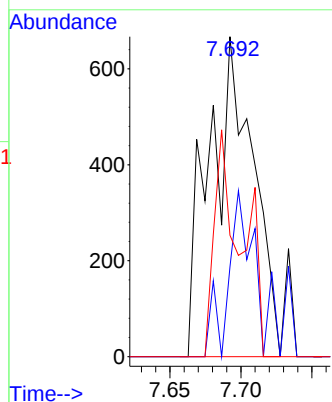

#31
Cyclohexane
Concen: 1.055 ug/l
RT: 8.081 min Scan# 1036
Delta R.T. -0.012 min
Lab File: VN071542.D
Acq: 25 Mar 2022 13:04

Tgt Ion: 56 Resp: 16148
Ion Ratio Lower Upper
56 100
69 154.9 27.8 41.8#
84 119.6 76.9 115.3#

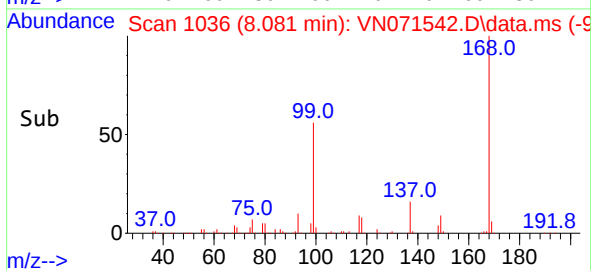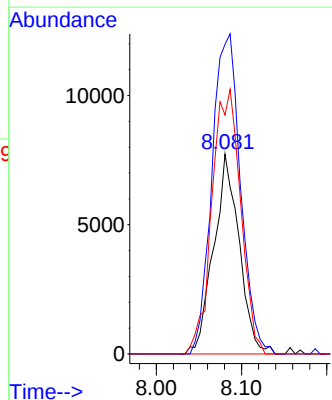



#33

1,2-Dichloroethane-d4

Concen: 46.538 ug/l

RT: 8.433 min Scan# 1096

Delta R.T. -0.000 min

Lab File: VN071542.D

Acq: 25 Mar 2022 13:04

Instrument :

MSVOA_N

ClientSampleId :





PB143557ZHE#01

Tgt Ion: 65 Resp: 497987

Ion Ratio Lower Upper

65 100

67 52.7 0.0 104.8

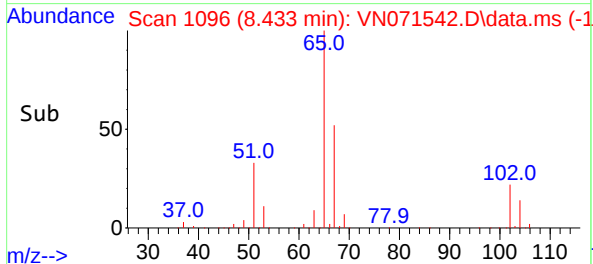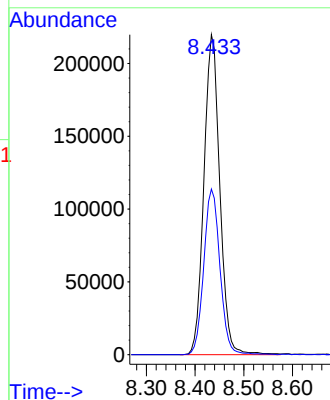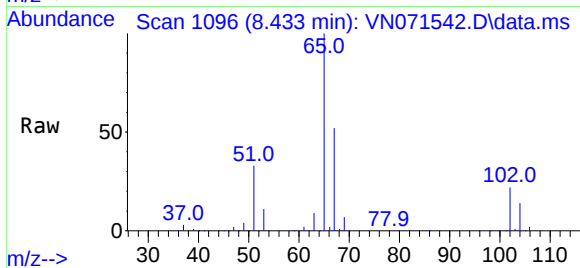

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.963 min Scan# 1186

Delta R.T. -0.000 min

Lab File: VN071542.D

Acq: 25 Mar 2022 13:04




Tgt Ion: 114 Resp: 1440344


Ion Ratio Lower Upper

114 100

63 19.8 0.0 40.0

88 15.9 0.0 32.6


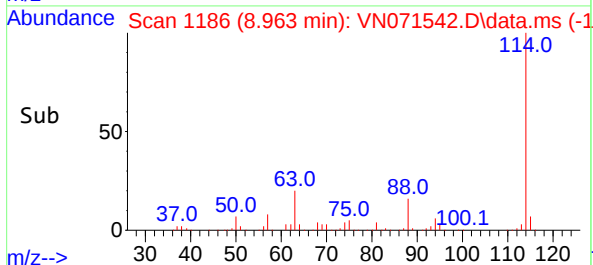
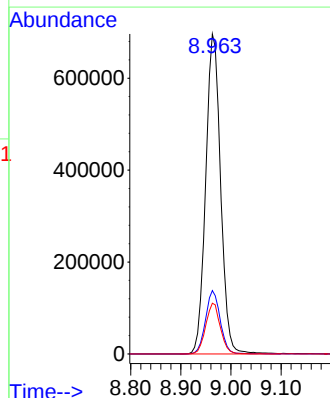
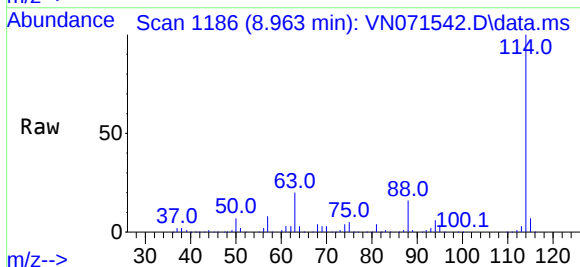




#35
Dibromofluoromethane
Concen: 45.842 ug/l
RT: 8.022 min Scan# 1026
Delta R.T. 0.006 min
Lab File: VN071542.D
Acq: 25 Mar 2022 13:04




Instrument :
MSVOA_N
ClientSampleId :
PB143557ZHE#01


Tgt Ion:113 Resp: 414968
Ion Ratio Lower Upper
113 100
111 101.8 81.4 122.0
192 21.6 17.0 25.6

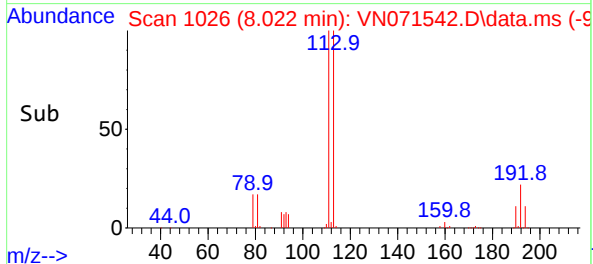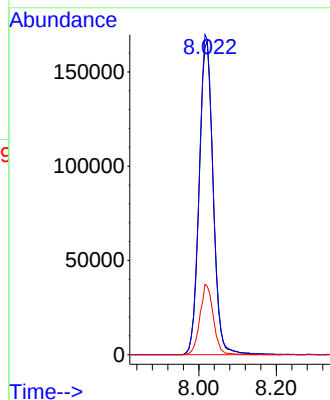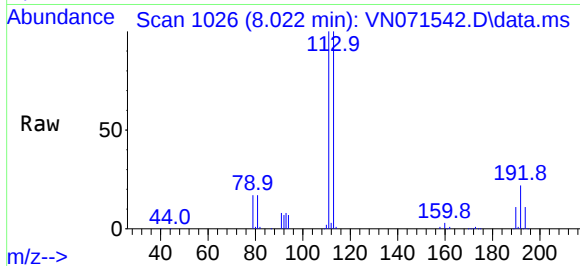

#36
1,1-Dichloropropene
Concen: 4.695 ug/l
RT: 8.081 min Scan# 1036
Delta R.T. -0.135 min
Lab File: VN071542.D
Acq: 25 Mar 2022 13:04

Tgt Ion: 75 Resp: 61271
Ion Ratio Lower Upper
75 100
110 7.9 18.3 54.8#
77 0.0 25.1 37.7#


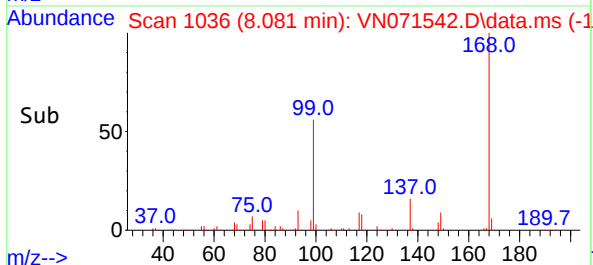
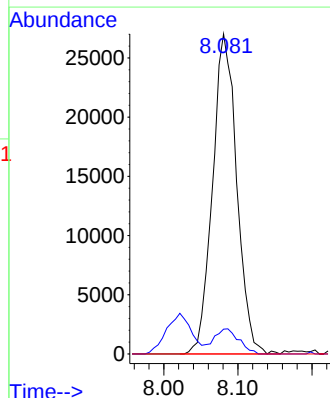
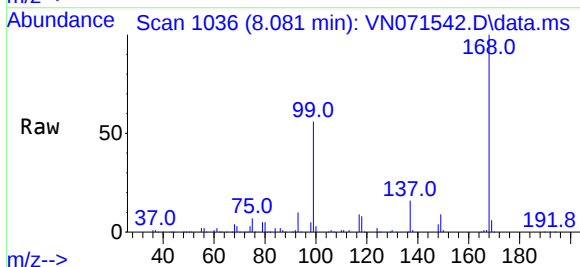




#38
Carbon Tetrachloride
Concen: 6.209 ug/l
RT: 8.086 min Scan# 1107
Delta R.T. -0.118 min
Lab File: VN071542.D
Acq: 25 Mar 2022 13:04




Instrument :
MSVOA_N
ClientSampleId :
PB143557ZHE#01


Tgt Ion:117 Resp: 78998
Ion Ratio Lower Upper
117 100
119 5.3 75.8 113.8#
121 0.0 24.6 37.0#

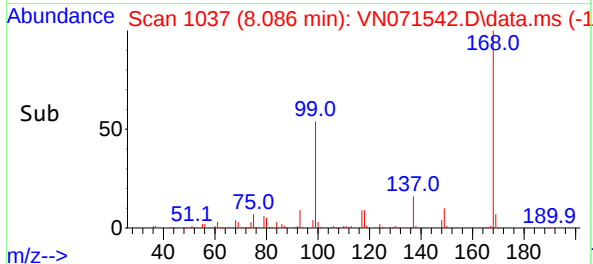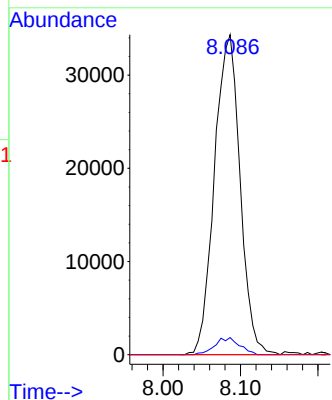

#43
Isopropyl Acetate
Concen: 2.760 ug/l
RT: 8.557 min Scan# 1117
Delta R.T. -0.000 min
Lab File: VN071542.D
Acq: 25 Mar 2022 13:04

Tgt Ion: 43 Resp: 71520
Ion Ratio Lower Upper
43 100
61 20.8 21.9 32.9#
87 13.4 12.0 18.0

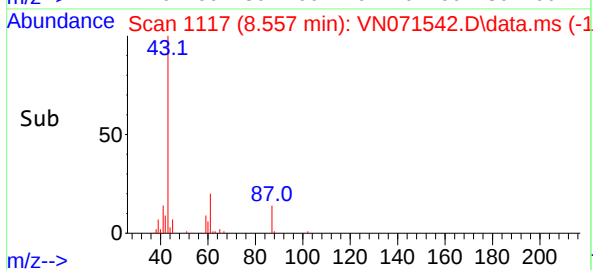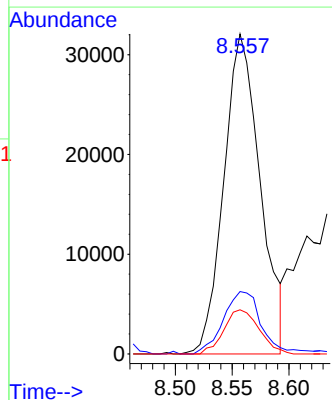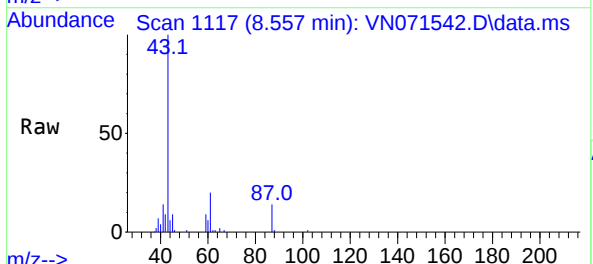



#45

1,2-Dichloropropane

Concen: 0.509 ug/l

RT: 9.622 min Scan# 1

Delta R.T. 0.135 min

Lab File: VN071542.D

Acq: 25 Mar 2022 13:04

Instrument :

MSVOA_N

ClientSampleId :





PB143557ZHE#01

Tgt Ion: 63 Resp: 5120

Ion Ratio Lower Upper

63 100

65 0.0 24.9 37.3#

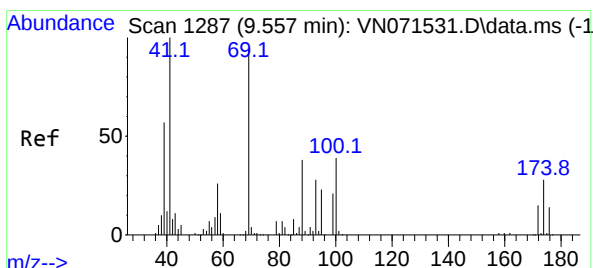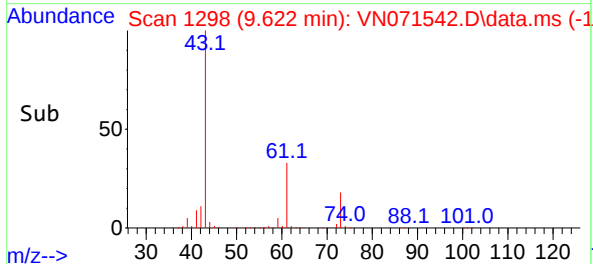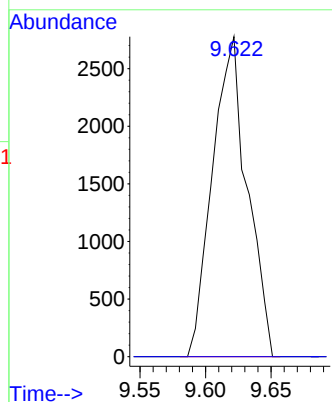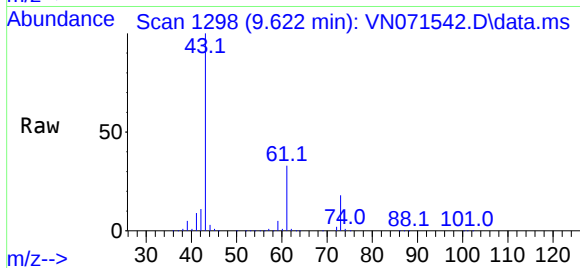

#48

Methyl methacrylate

Concen: 1.717 ug/l

RT: 9.539 min Scan# 1284

Delta R.T. -0.018 min

Lab File: VN071542.D

Acq: 25 Mar 2022 13:04




Tgt Ion: 41 Resp: 17631


Ion Ratio Lower Upper

41 100

69 0.0 74.7 112.1#

39 0.0 45.6 68.4#


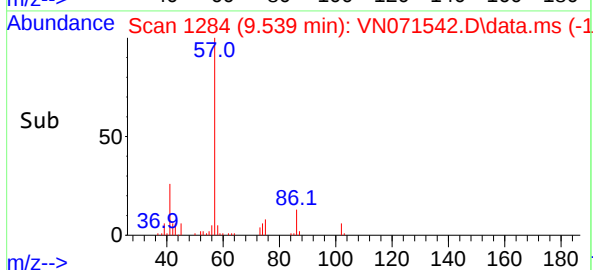
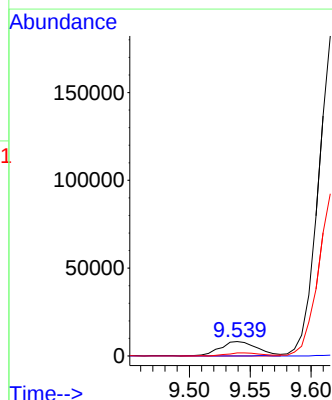
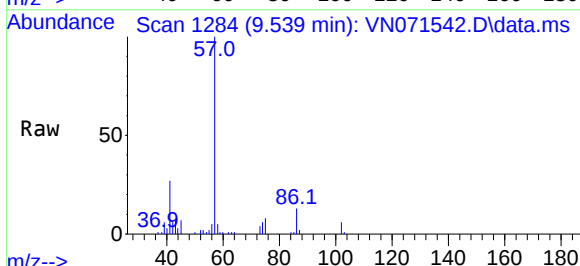




#49
1,4-Dioxane
Concen: 0.464 ug/l
RT: 9.580 min Scan# 11
Delta R.T. 0.018 min
Lab File: VN071542.D
Acq: 25 Mar 2022 13:04




Instrument :
MSVOA_N
ClientSampleId :
PB143557ZHE#01


Tgt Ion: 88 Resp: 110
Ion Ratio Lower Upper
88 100
43 0.0 20.2 30.4#
58 0.0 54.2 81.4#

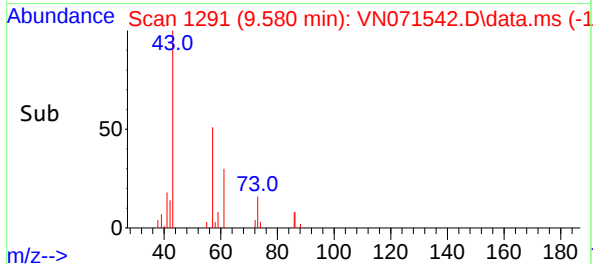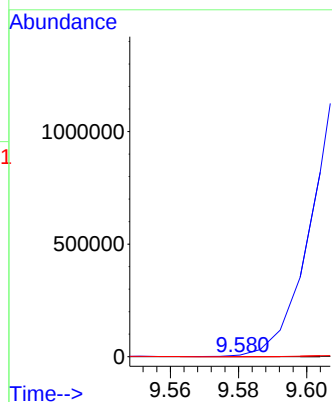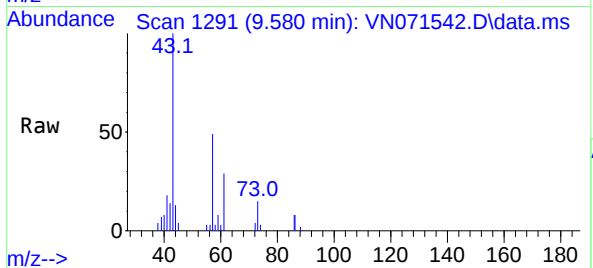

#50
Toluene-d8
Concen: 49.347 ug/l
RT: 10.439 min Scan# 1437
Delta R.T. -0.000 min
Lab File: VN071542.D
Acq: 25 Mar 2022 13:04

Tgt Ion: 98 Resp: 1801746
Ion Ratio Lower Upper
98 100
100 64.8 52.6 78.8


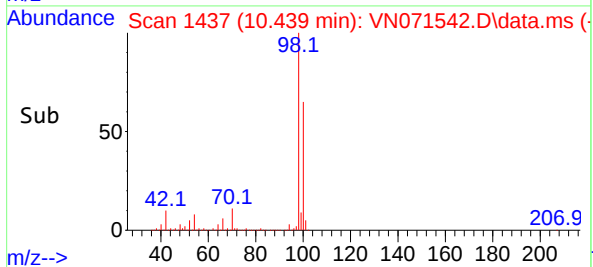
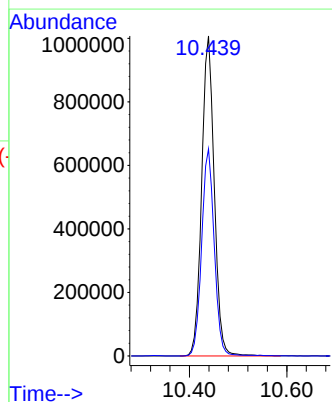
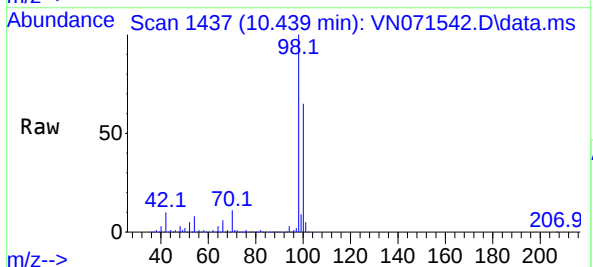




#51
4-Methyl-2-Pentanone
Concen: 0.886 ug/l
RT: 10.322 min Scan# 1418
Delta R.T. -0.006 min
Lab File: VN071542.D
Acq: 25 Mar 2022 13:04




Instrument :
MSVOA_N
ClientSampleId :
PB143557ZHE#01


Tgt Ion: 43 Resp: 12626
Ion Ratio Lower Upper
43 100
58 46.3 34.1 51.1

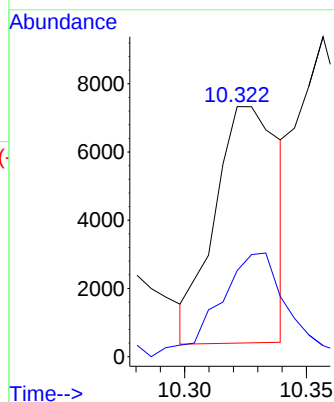

#54
cis-1,3-Dichloropropene
Concen: 7.249 ug/l
RT: 10.239 min Scan# 1403
Delta R.T. 0.053 min
Lab File: VN071542.D
Acq: 25 Mar 2022 13:04

Tgt Ion: 75 Resp: 115394
Ion Ratio Lower Upper
75 100
77 0.5 25.2 37.8#
39 27.9 35.7 53.5#

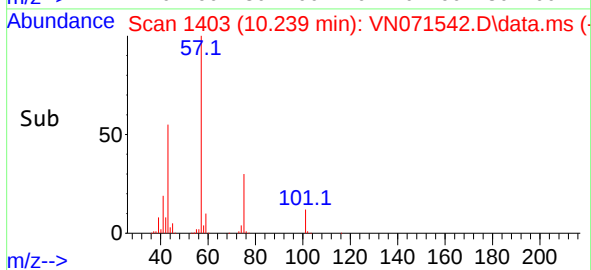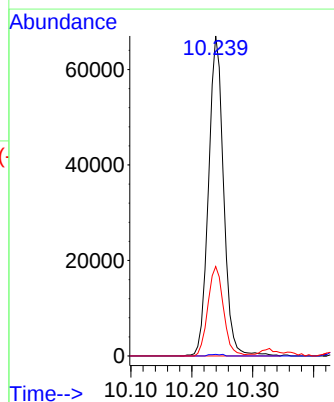



#57

1,3-Dichloropropane

Concen: 4.236 ug/l

RT: 11.086 min Scan# 11

Delta R.T. 0.047 min

Lab File: VN071542.D

Acq: 25 Mar 2022 13:04

Instrument :

MSVOA_N

ClientSampleId :





PB143557ZHE#01

Tgt Ion: 76 Resp: 73476

Ion Ratio Lower Upper

76 100

78 0.4 26.2 39.2#

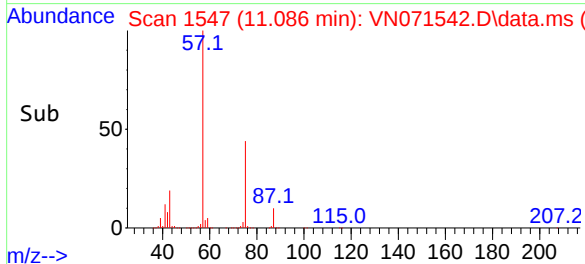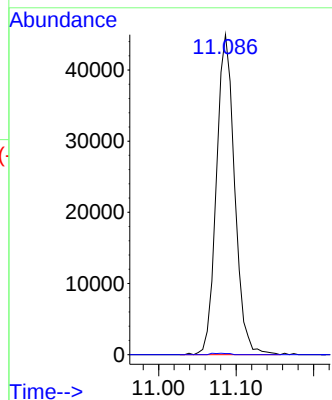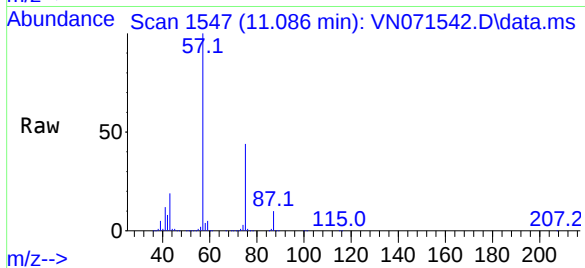

#58

2-Chloroethyl Vinyl ether

Concen: 18.695 ug/l

RT: 10.080 min Scan# 1376

Delta R.T. 0.041 min

Lab File: VN071542.D




Acq: 25 Mar 2022 13:04


Tgt Ion: 63 Resp: 60

Ion Ratio Lower Upper

63 100

106 0.0 24.6 36.8#


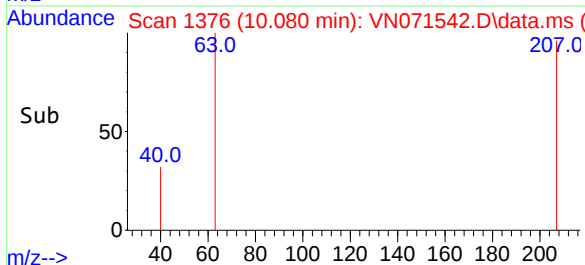
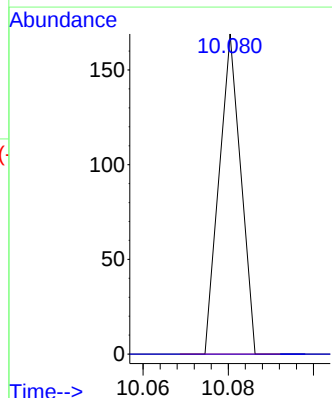
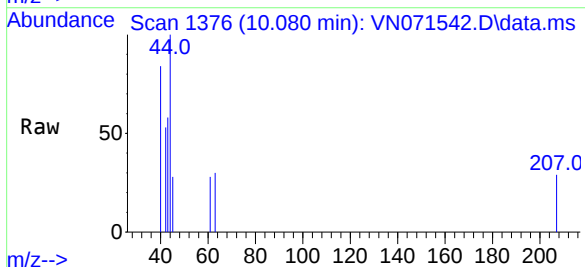




#59
2-Hexanone
Concen: 94.719 ug/l
RT: 11.086 min Scan# 1154
Delta R.T. 0.006 min
Lab File: VN071542.D
Acq: 25 Mar 2022 13:04




Instrument :
MSVOA_N
ClientSampleId :
PB143557ZHE#01


Tgt Ion: 43 Resp: 972525
Ion Ratio Lower Upper
43 100
58 19.1 29.7 89.1#

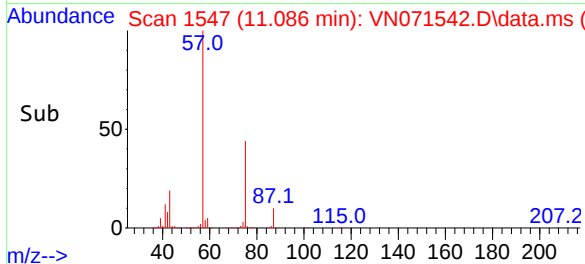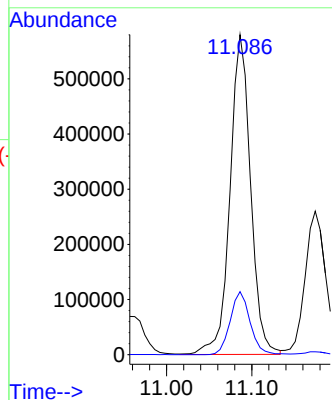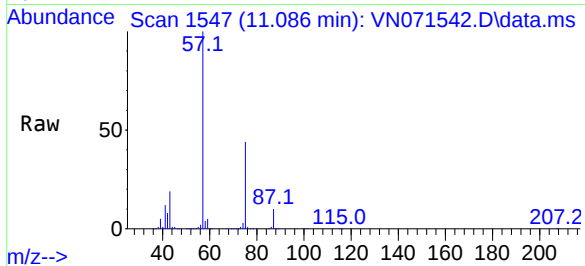

#62
4-Bromofluorobenzene
Concen: 50.709 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. -0.000 min
Lab File: VN071542.D
Acq: 25 Mar 2022 13:04

Tgt Ion: 95 Resp: 606664
Ion Ratio Lower Upper
95 100
174 84.2 0.0 167.6
176 81.7 0.0 163.4


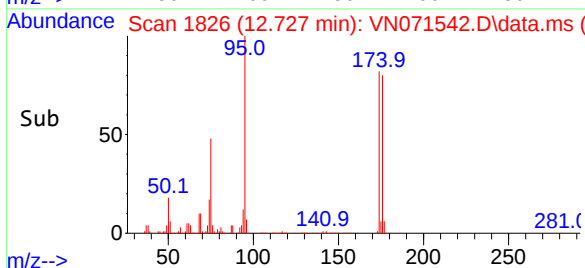
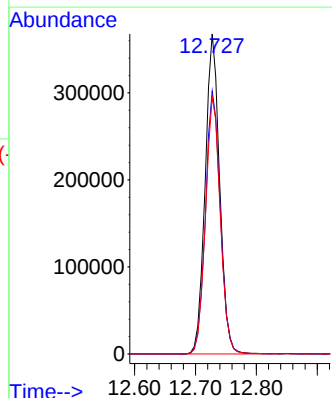
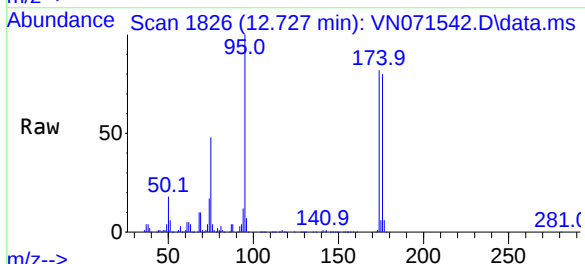




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.739 min Scan# 117
Delta R.T. -0.000 min
Lab File: VN071542.D
Acq: 25 Mar 2022 13:04




Instrument :
MSVOA_N
ClientSampleId :
PB143557ZHE#01


Tgt Ion:117 Resp: 1428182
Ion Ratio Lower Upper
117 100
82 54.9 44.2 66.2
119 32.6 25.4 38.0

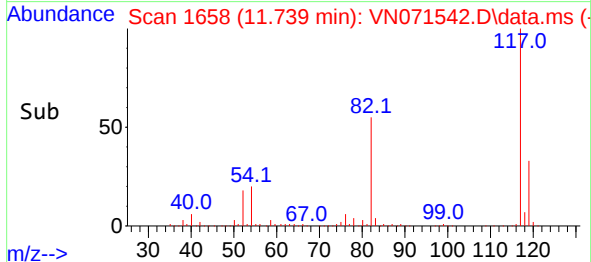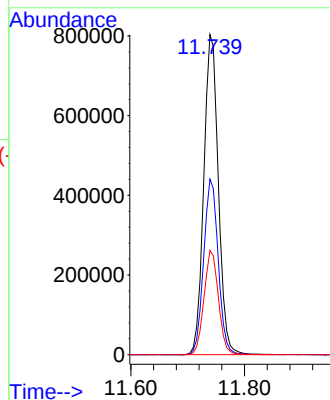

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.674 min Scan# 1987
Delta R.T. 0.006 min
Lab File: VN071542.D
Acq: 25 Mar 2022 13:04

Tgt Ion:152 Resp: 527744
Ion Ratio Lower Upper
152 100
115 56.9 28.9 86.7
150 157.8 0.0 356.2


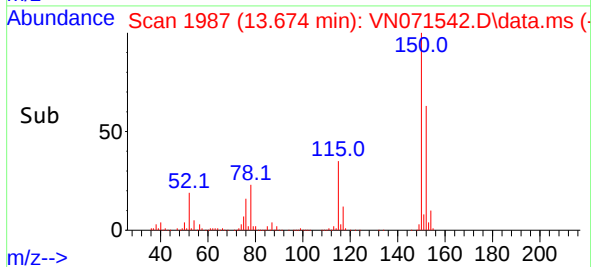
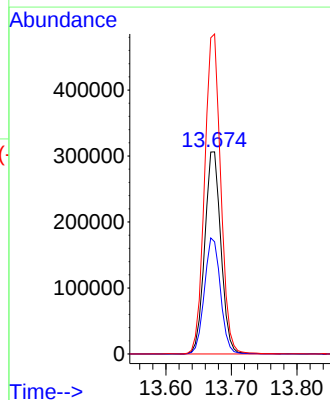
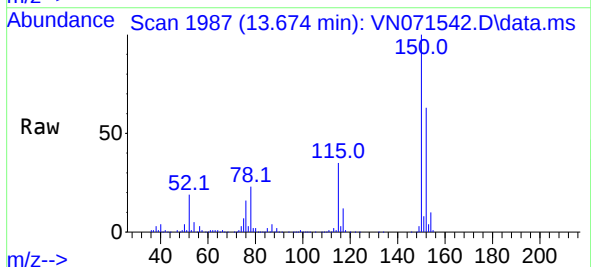




#75
1,1,2,2-Tetrachloroethane
Concen: Below Cal
RT: 12.827 min Scan# 1842
Delta R.T. 0.005 min
Lab File: VN071542.D
Acq: 25 Mar 2022 13:04




Instrument :
MSVOA_N
ClientSampleId :
PB143557ZHE#01


Tgt Ion: 83 Resp: 250
Ion Ratio Lower Upper
83 100
131 0.0 5.3 15.9#
85 0.0 32.3 96.9#

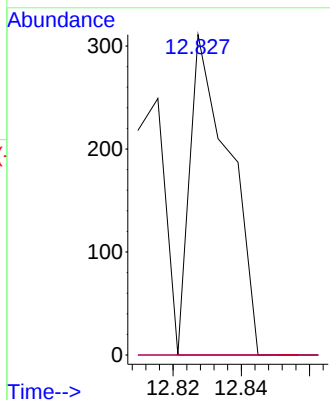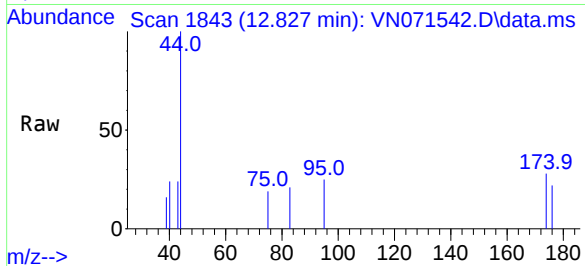

#76
1,2,3-Trichloropropane
Concen: 25.491 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. -0.147 min
Lab File: VN071542.D
Acq: 25 Mar 2022 13:04

Tgt Ion: 75 Resp: 299974
Ion Ratio Lower Upper
75 100
77 1.1 98.5 295.5#


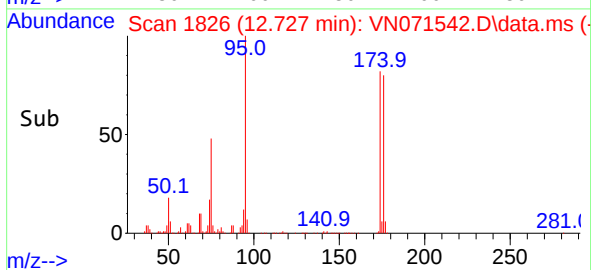
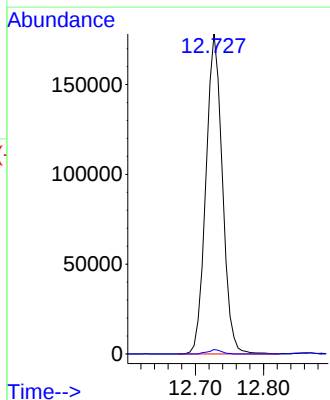
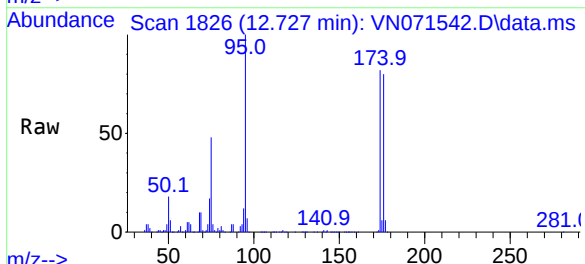




#80
1,3,5-Trimethylbenzene
Concen: 0.322 ug/l
RT: 13.057 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN071542.D
Acq: 25 Mar 2022 13:04




Instrument :
MSVOA_N
ClientSampleId :
PB143557ZHE#01


Tgt Ion:105 Resp: 11818
Ion Ratio Lower Upper
105 100
120 52.2 24.9 74.7

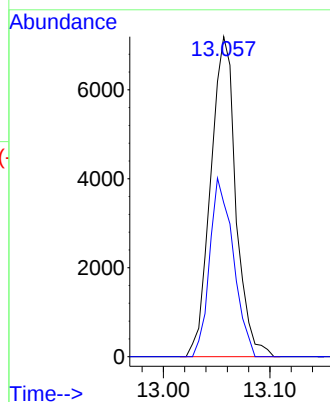

#81
trans-1,4-Dichloro-2-butene
Concen: 68.246 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.106 min
Lab File: VN071542.D
Acq: 25 Mar 2022 13:04

Tgt Ion: 75 Resp: 299974
Ion Ratio Lower Upper
75 100
53 0.0 78.0 117.0#
89 0.0 37.2 55.8#


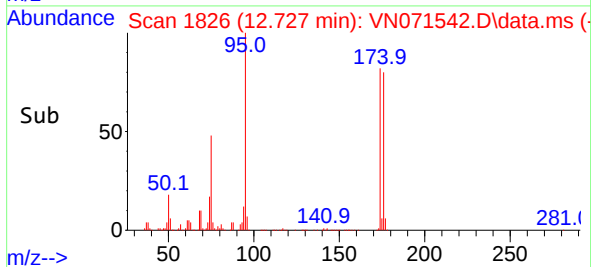
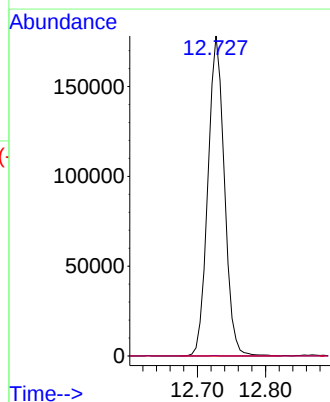
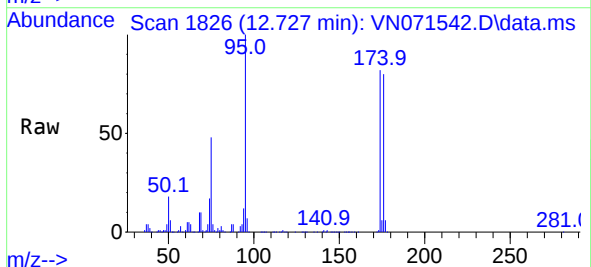




#93
1,2,4-Trichlorobenzene
Concen: 0.253 ug/l
RT: 15.268 min Scan# 2116
Delta R.T. 0.012 min
Lab File: VN071542.D
Acq: 25 Mar 2022 13:04




Instrument :
MSVOA_N
ClientSampleId :
PB143557ZHE#01


Tgt Ion:	180	Resp:	2116
Ion Ratio	Lower	Upper	
180	100		
182	96.3	47.5	142.5
145	22.0	14.5	43.5

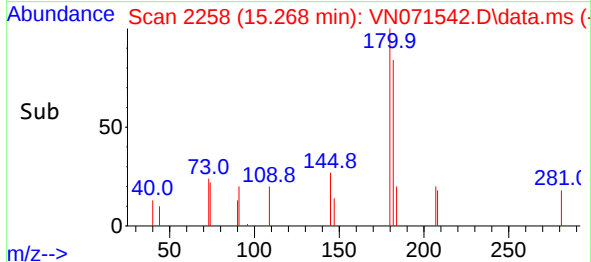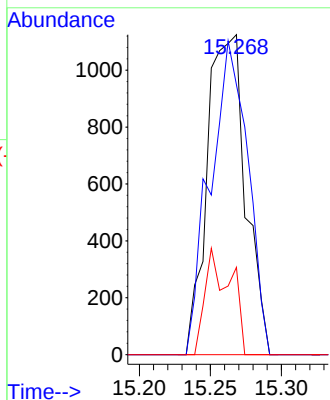

#95
Naphthalene
Concen: 3.448 ug/l
RT: 15.504 min Scan# 2298
Delta R.T. 0.006 min
Lab File: VN071542.D
Acq: 25 Mar 2022 13:04


Tgt Ion:	128	Resp:	6707
Ion Ratio	Lower	Upper	
128	100		
127	9.7	10.3	15.5#
129	8.2	8.6	13.0#

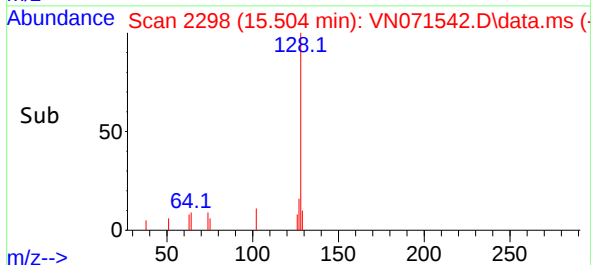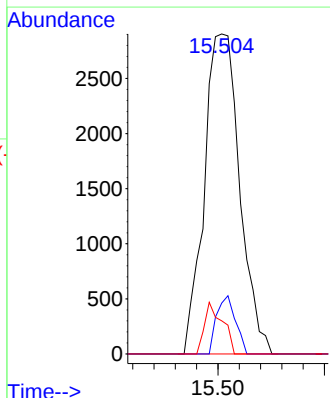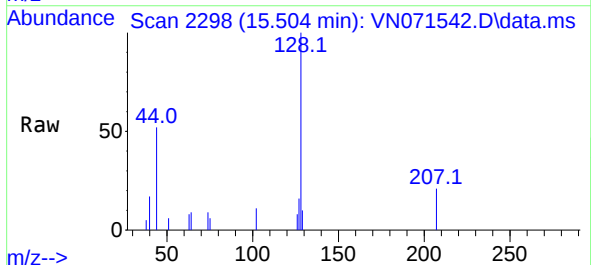



#96
 1,2,3-Trichlorobenzene
 Concen: 0.274 ug/l
 RT: 15.692 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: VN071542.D
 Acq: 25 Mar 2022 13:04

Instrument :
 MSVOA_N
 ClientSampleId :
 PB143557ZHE#01



Tgt Ion:	180	Resp:	2271
Ion	Ratio	Lower	Upper
180	100		
182	89.2	47.8	143.3
145	24.1	15.5	46.5

