
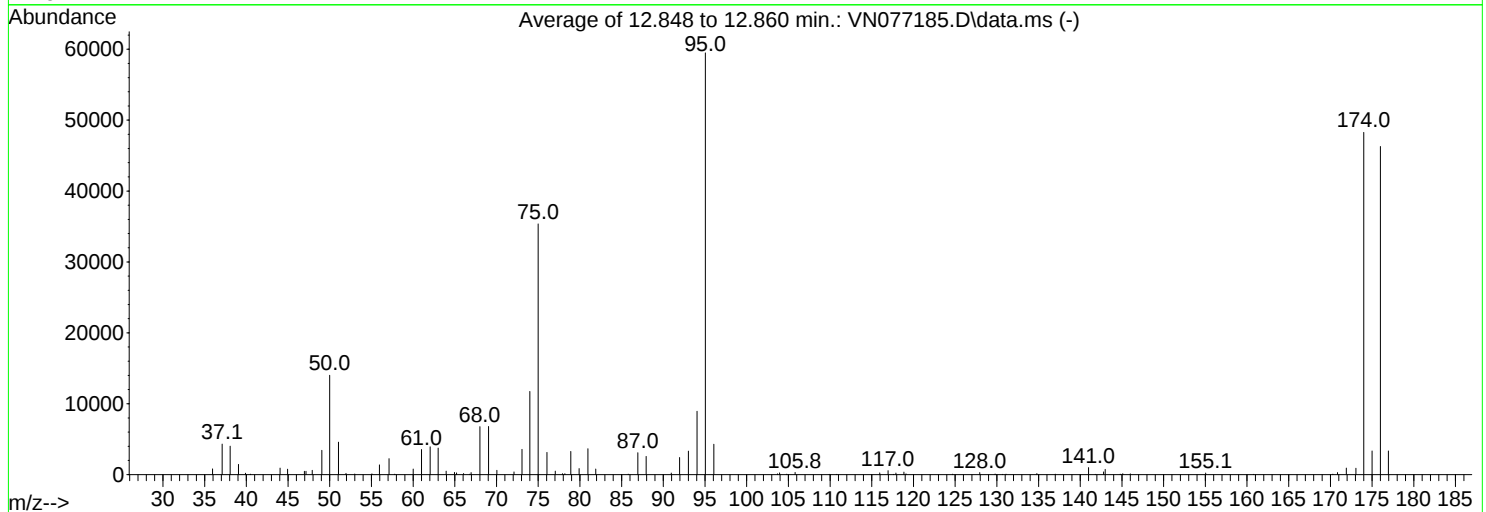


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032523\
Data File : VN077185.D
Acq On : 24 Mar 2023 19:03
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N032523W.M
Title : SW846 8260
Last Update : Mon Mar 27 02:47:06 2023

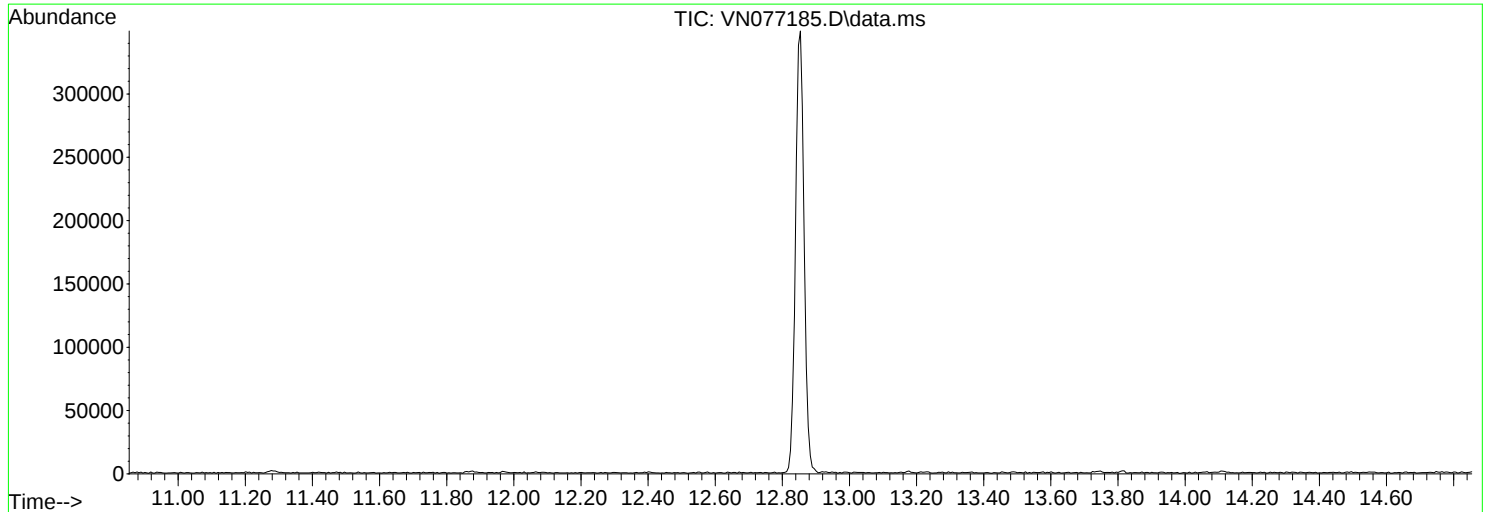

AutoFind: Scans 1855, 1856, 1857; Background Corrected with Scan 1847

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.6	14026	PASS
75	95	30	60	59.4	35365	PASS
95	95	100	100	100.0	59491	PASS
96	95	5	9	7.2	4298	PASS
173	174	0.00	2	1.9	905	PASS
174	95	50	100	81.2	48280	PASS
175	174	5	9	6.9	3346	PASS
176	174	95	101	95.9	46293	PASS
177	176	5	9	7.2	3345	PASS

Average of 12.848 to 12.860 min.: VN077185.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	806	49.05	3438	62.05	3925	72.10	381
37.10	4317	50.00	14026	63.00	3757	73.05	356
38.05	4029	51.05	4582	63.95	492	74.00	1174
39.05	1452	51.95	193	64.95	321	75.00	3536
39.90	202	53.00	86	65.20	239	76.05	3137
40.50	78	55.05	118	66.05	159	77.05	493
44.05	934	55.95	1373	66.80	78	77.90	131
44.95	763	57.10	2250	66.95	284	78.20	126
46.95	478	57.80	78	68.00	6769	78.90	3270
47.15	482	60.00	799	69.05	6802	79.90	849
47.90	607	61.00	3541	70.05	617	80.95	3665

Average of 12.848 to 12.860 min.: VN077185.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
81.90	783	103.95	253	124.70	60	144.80	72
85.80	79	104.80	77	127.95	298	145.10	132
86.95	3085	105.80	307	129.80	96	146.00	105
87.95	2577	109.90	52	130.70	53	155.05	223
90.95	229	110.80	54	131.10	59	160.80	53
91.95	2412	115.95	253	134.80	151	170.30	63
93.00	3325	116.95	560	137.00	60	170.85	288
94.05	8933	117.60	55	141.00	991	171.90	935
95.05	59491	117.90	230	141.80	52	173.05	905
96.05	4298	118.85	354	142.80	379	174.00	48280
103.70	107	119.10	112	143.00	737	175.00	3346

Average of 12.848 to 12.860 min.: VN077185.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
176.00	46293						
176.95	3345						