
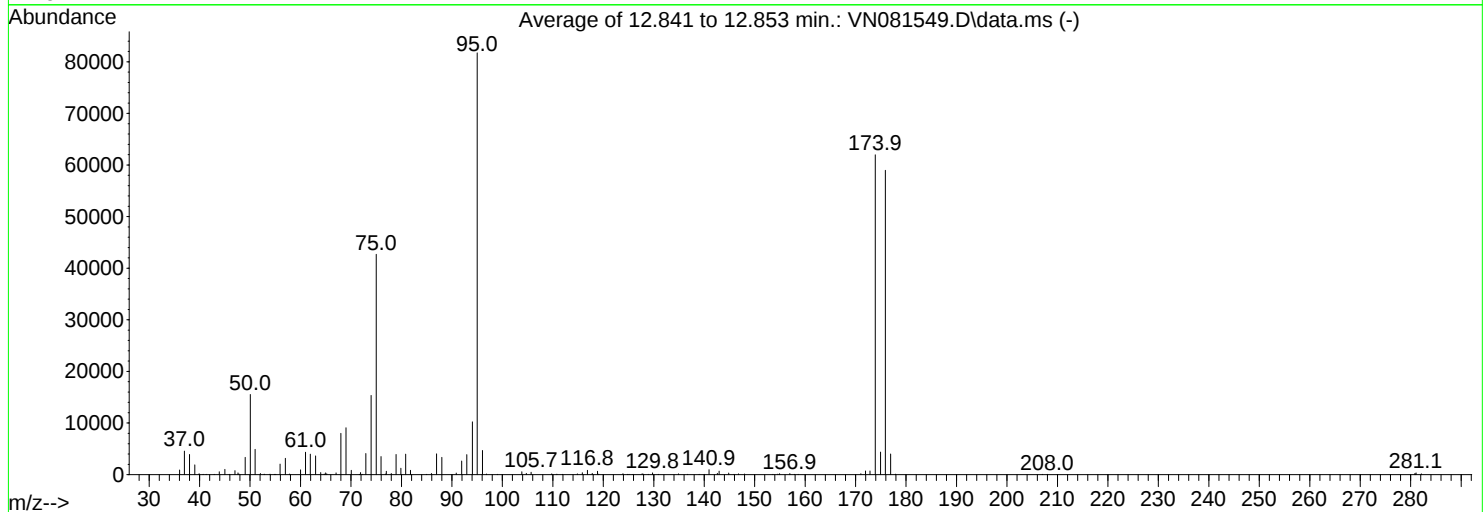


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032524\
Data File : VN081549.D
Acq On : 25 Mar 2024 09:02
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031824W.M
Title : SW846 8260
Last Update : Tue Mar 19 06:00:00 2024

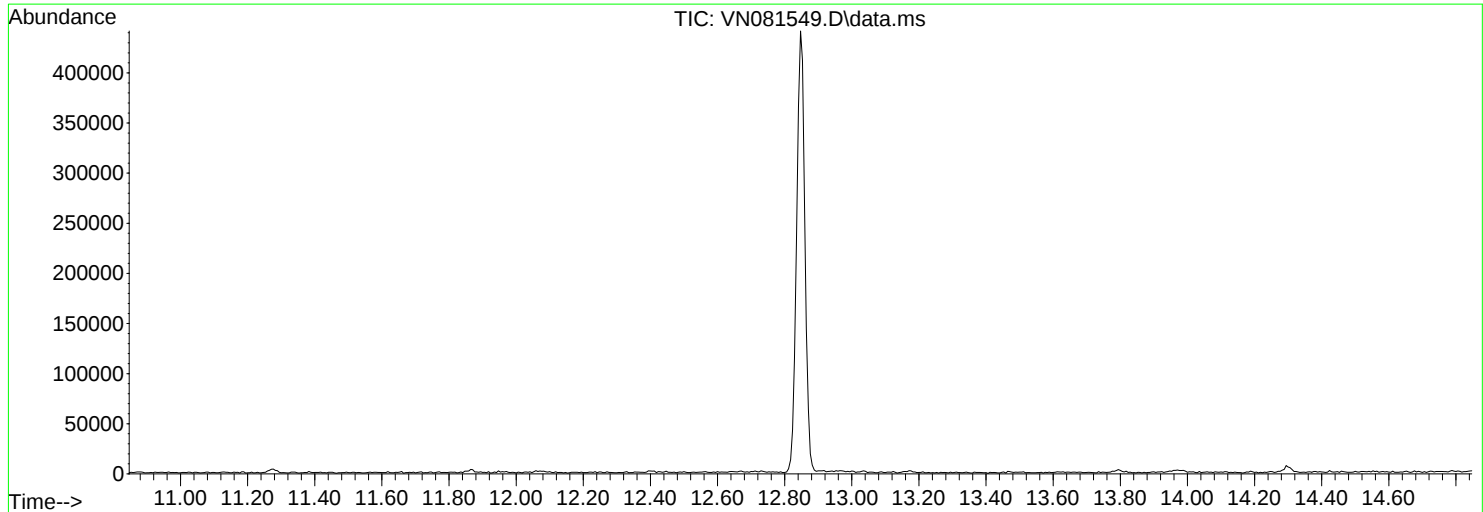

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	15521	PASS
75	95	30	60	52.2	42693	PASS
95	95	100	100	100.0	81736	PASS
96	95	5	9	5.7	4670	PASS
173	174	0.00	2	1.2	730	PASS
174	95	50	100	75.8	61965	PASS
175	174	5	9	7.1	4381	PASS
176	174	95	101	95.2	58960	PASS
177	176	5	9	6.8	4011	PASS

Average of 12.841 to 12.853 min.: VN081549.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	898	47.00	776	55.95	2035	67.05	341
37.00	4559	47.60	349	57.00	3165	68.00	801
38.00	3908	47.80	124	57.85	124	69.00	909
39.05	1893	49.05	3359	60.00	936	70.05	82
39.90	184	50.05	15521	61.00	4357	71.70	69
40.70	62	51.00	4897	61.95	3975	71.90	414
41.30	59	52.05	230	63.00	3621	72.20	74
42.90	72	52.80	80	64.00	410	72.95	4101
43.90	574	53.95	109	64.70	138	74.00	15349
45.00	1021	54.80	54	65.00	359	75.00	42693
45.90	59	55.10	78	65.20	156	75.95	3504

Average of 12.841 to 12.853 min.: VN081549.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
76.80	123	90.85	322	109.80	171	125.10	62
77.00	640	91.95	2631	110.80	96	125.90	51
78.00	216	92.95	3866	111.90	61	127.70	181
78.95	3909	94.05	10238	114.85	155	128.00	86
79.90	1258	95.00	81736	115.85	382	128.90	51
80.85	3977	96.05	4670	116.85	845	129.75	346
81.80	834	96.85	141	117.80	263	130.90	53
85.00	53	99.00	68	118.85	641	134.90	145
85.95	215	103.85	553	119.10	98	136.70	52
86.95	4022	104.75	262	123.90	201	139.00	53
88.00	3354	105.70	464	124.80	68	140.00	53

Average of 12.841 to 12.853 min.: VN081549.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
140.95	963	157.90	51	208.00	59		
142.60	267	158.60	56	280.80	191		
142.95	684	171.05	173	280.90	161		
144.85	321	171.95	716	281.05	340		
145.90	76	172.85	730	282.10	144		
146.80	144	173.90	61965				
148.00	131	174.95	4381				
153.60	55	175.90	58960				
154.60	82	176.95	4011				
154.95	190	177.90	104				
156.95	208	207.00	53				

Instrument :

MSVOA_N

ClientSampleId :

BFB