

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032525\
 Data File : VN086092.D
 Acq On : 25 Mar 2025 11:26
 Operator : JC\MD
 Sample : VN0325WBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0325WBL01

Quant Time: Mar 26 03:14:17 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031825W.M
 Quant Title : SW846 8260
 QLast Update : Wed Mar 19 03:20:56 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	201384	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	370671	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	325680	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.788	152	130926	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	148116	53.711	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	107.420%
35) Dibromofluoromethane	8.165	113	130697	50.516	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	101.040%
50) Toluene-d8	10.565	98	447092	47.614	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	95.220%
62) 4-Bromofluorobenzene	12.847	95	144141	43.044	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	86.080%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032525\
Data File : VN086092.D
Acq On : 25 Mar 2025 11:26
Operator : JC\MD
Sample : VN0325WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0325WBL01


Quant Time: Mar 26 03:14:17 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031825W.M
Quant Title : SW846 8260
QLast Update : Wed Mar 19 03:20:56 2025
Response via : Initial Calibration

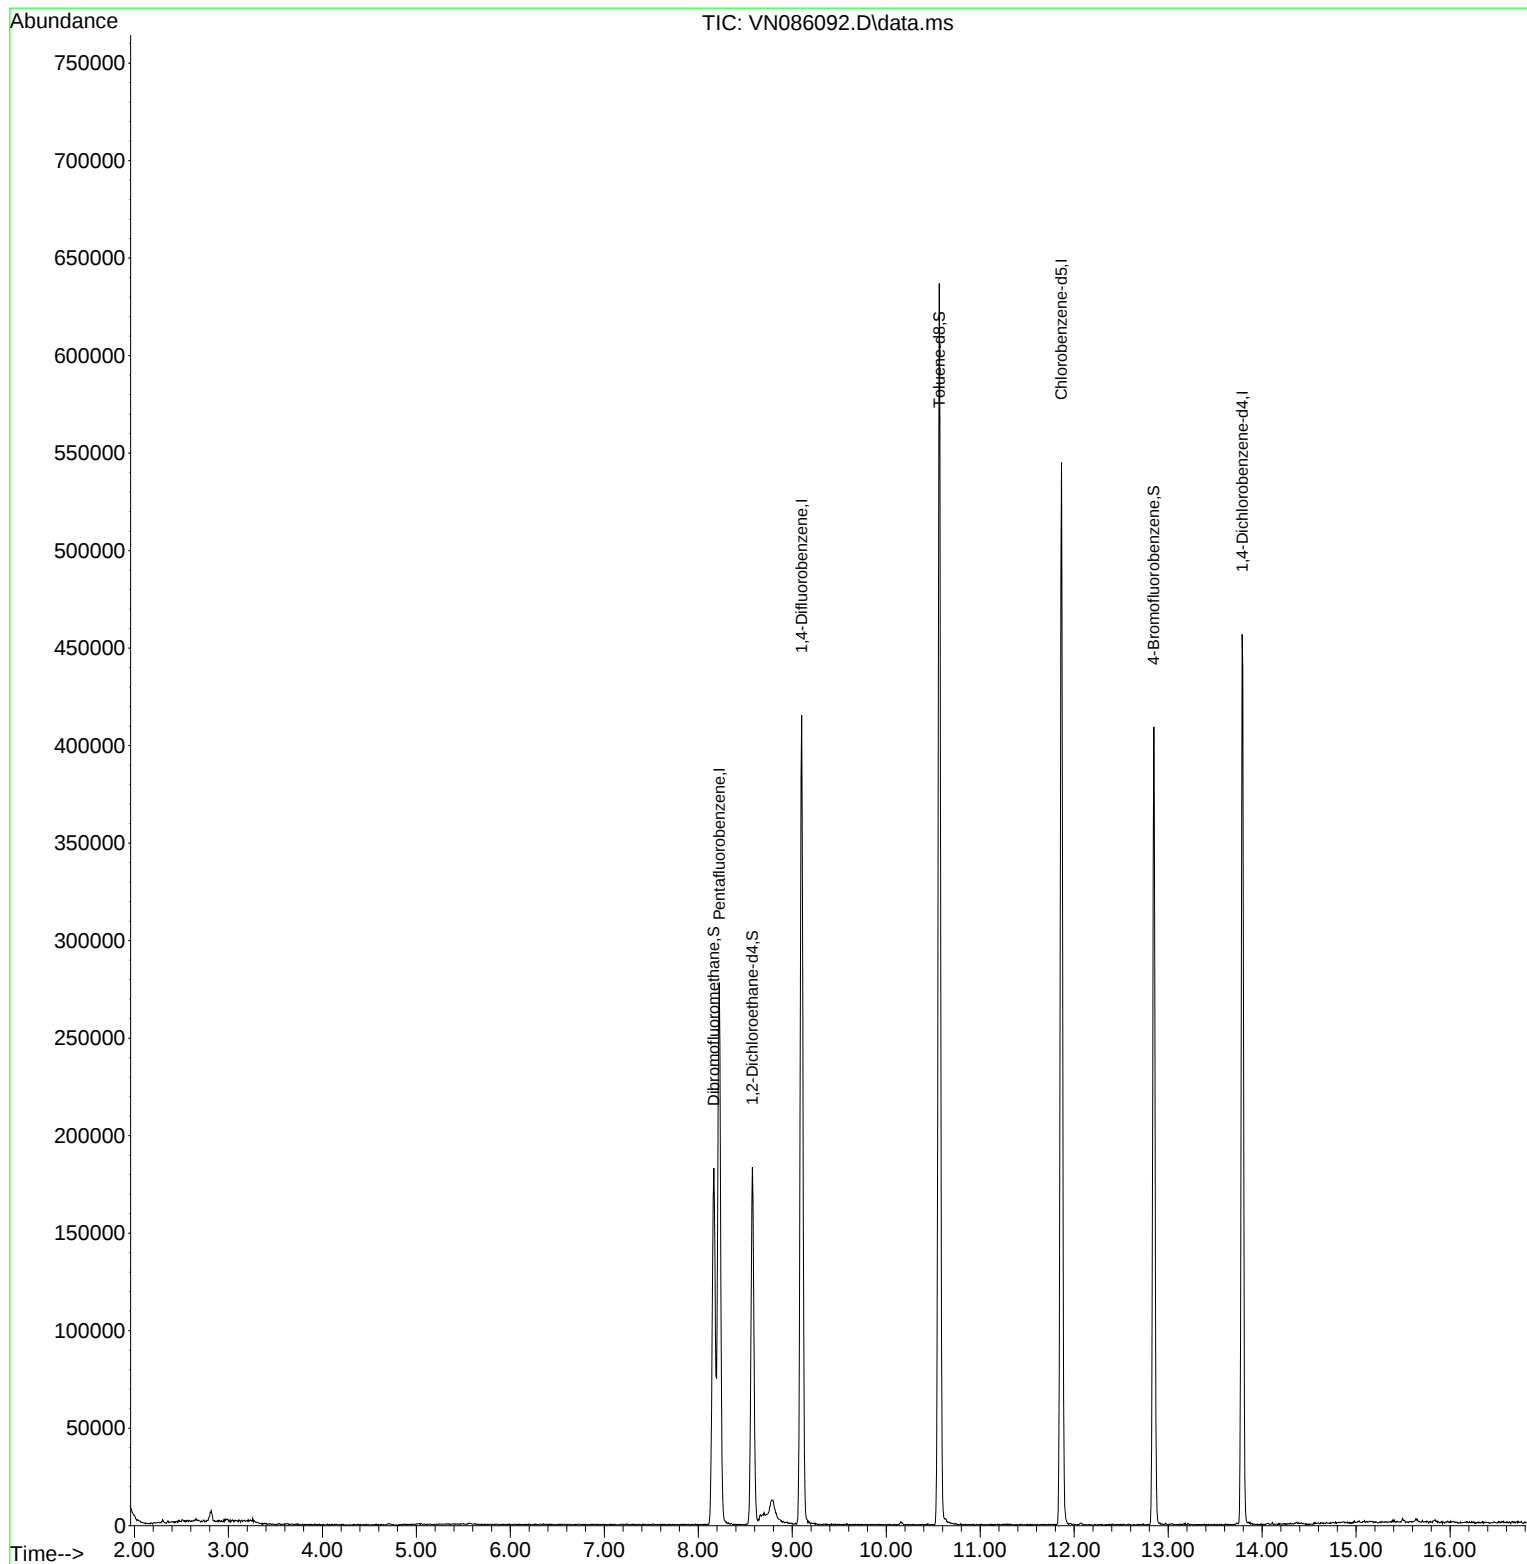



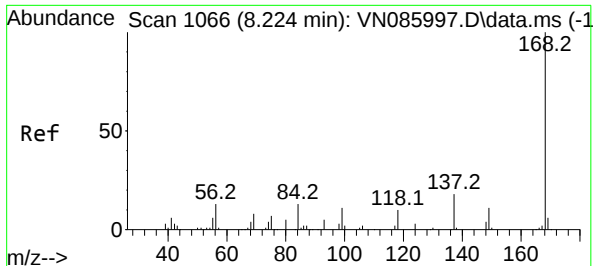


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.000 min
Lab File: VN086092.D
Acq: 25 Mar 2025 11:26

Instrument :
MSVOA_N
ClientSampleId :
VN0325WBL01



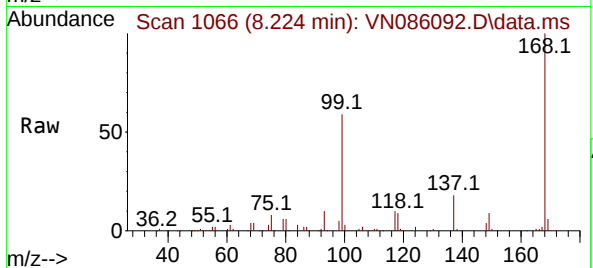



Tgt Ion:168 Resp: 201384
Ion Ratio Lower Upper
168 100
99 59.2 49.4 74.2

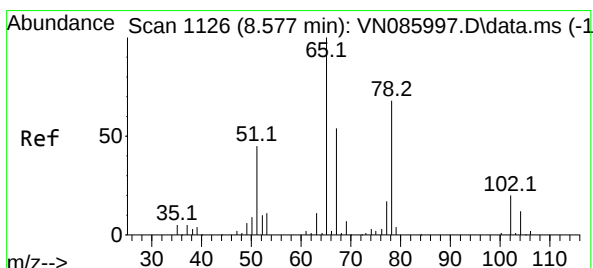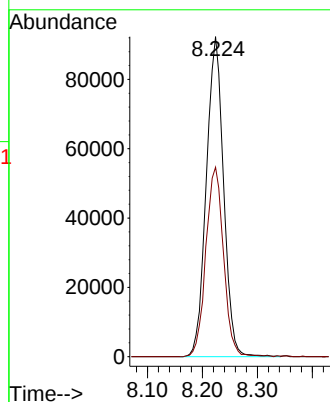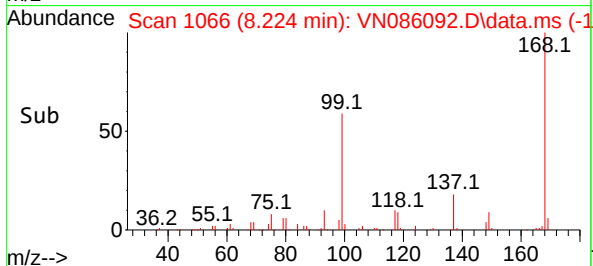

#33
1,2-Dichloroethane-d4
Concen: 53.711 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. -0.000 min
Lab File: VN086092.D
Acq: 25 Mar 2025 11:26

Tgt Ion: 65 Resp: 148116
Ion Ratio Lower Upper
65 100
67 52.8 0.0 102.2


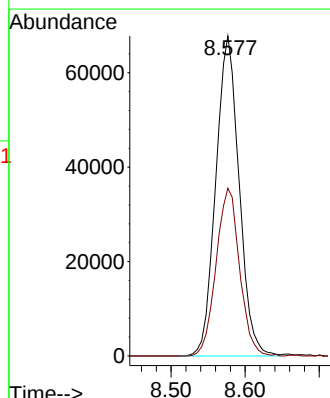
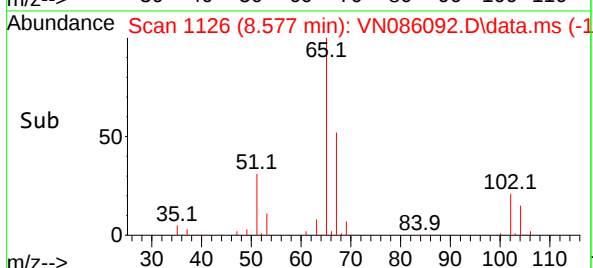
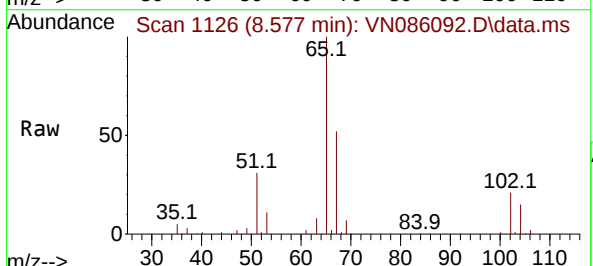


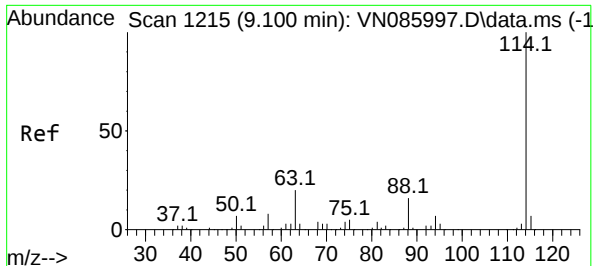

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.100 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN086092.D
Acq: 25 Mar 2025 11:26




Instrument :
MSVOA_N
ClientSampleId :
VN0325WBL01


Tgt Ion:114 Resp: 370671
Ion Ratio Lower Upper
114 100
63 18.6 0.0 39.6
88 17.5 0.0 32.6

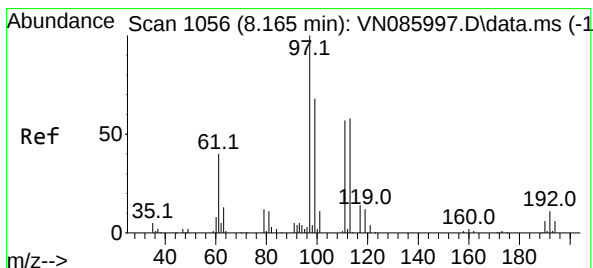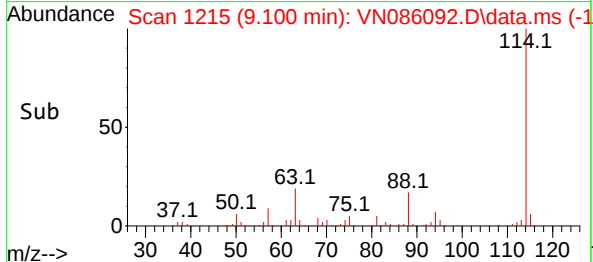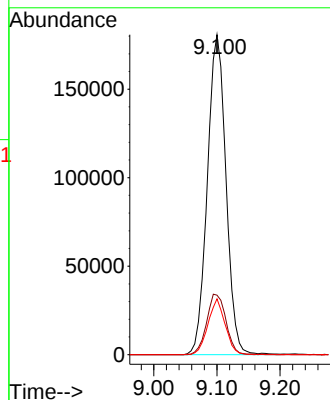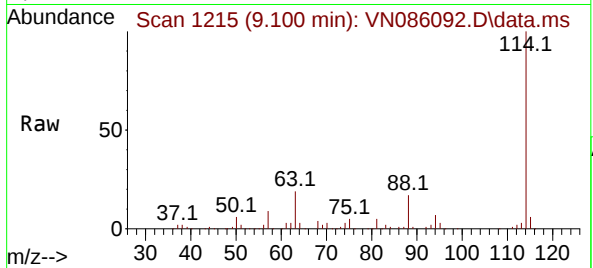

#35
Dibromofluoromethane
Concen: 50.516 ug/l
RT: 8.165 min Scan# 1056
Delta R.T. -0.000 min
Lab File: VN086092.D
Acq: 25 Mar 2025 11:26

Tgt Ion:113 Resp: 130697
Ion Ratio Lower Upper
113 100
111 103.1 81.8 122.8
192 19.7 15.9 23.9

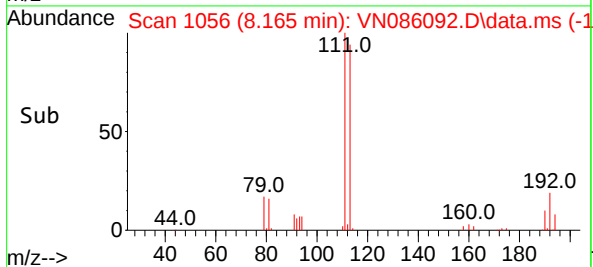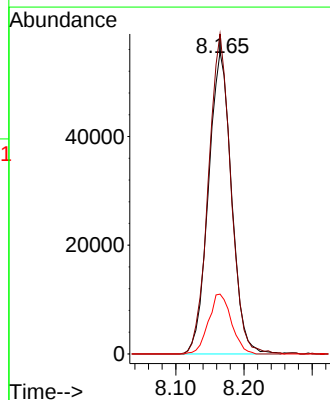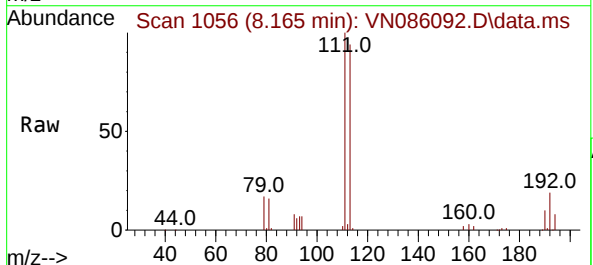

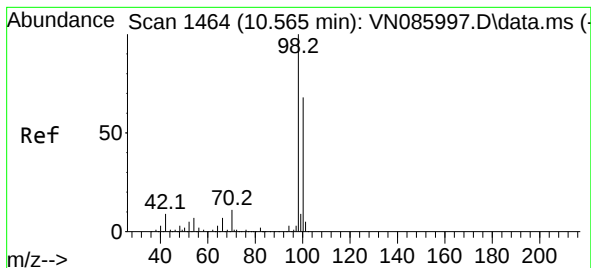

#50

Toluene-d8

Concen: 47.614 ug/l

RT: 10.565 min Scan# 1464

Delta R.T. -0.000 min

Lab File: VN086092.D

Acq: 25 Mar 2025 11:26

Instrument :

MSVOA_N

ClientSampleId :





VN0325WBL01

Tgt Ion: 98 Resp: 447092

Ion Ratio Lower Upper

98 100

100 65.1 53.1 79.7

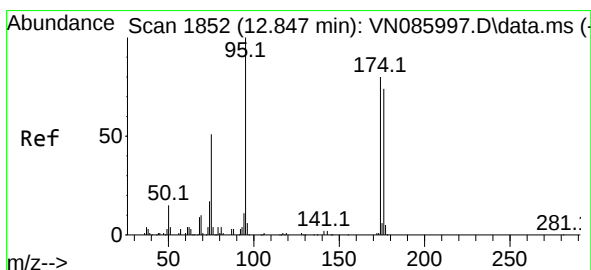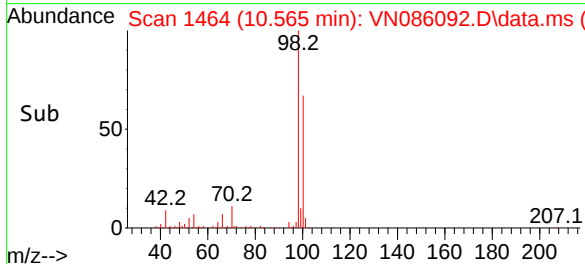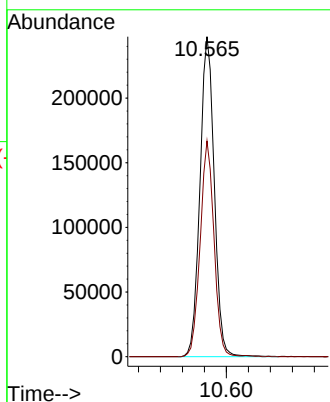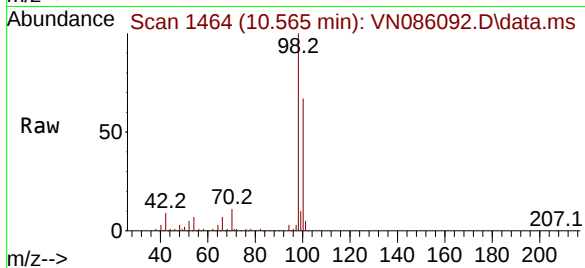

#62

4-Bromofluorobenzene

Concen: 43.044 ug/l

RT: 12.847 min Scan# 1852

Delta R.T. -0.000 min

Lab File: VN086092.D

Acq: 25 Mar 2025 11:26




Tgt Ion: 95 Resp: 144141


Ion Ratio Lower Upper

95 100

174 80.3 0.0 156.8

176 76.3 0.0 152.2


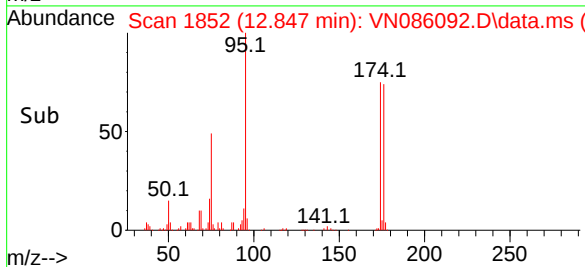
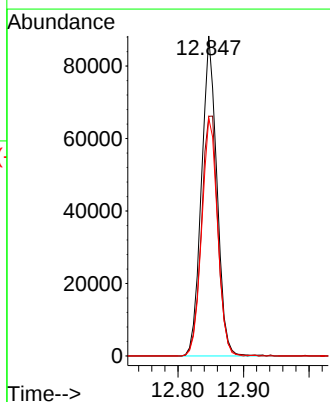
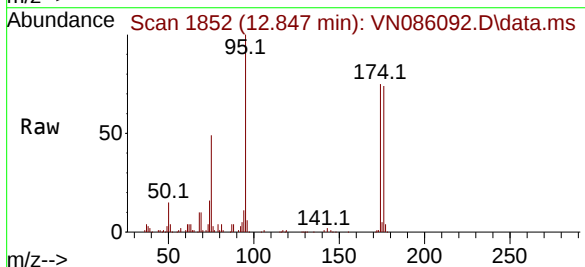


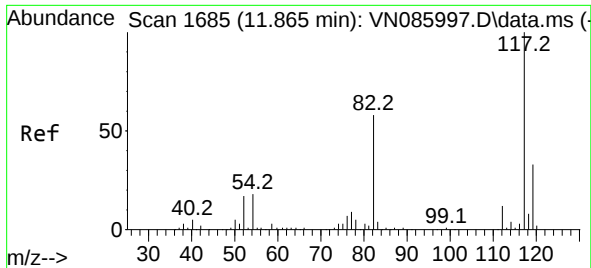

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN086092.D
Acq: 25 Mar 2025 11:26

Instrument :
MSVOA_N
ClientSampleId :
VN0325WBL01

Tgt Ion:117 Resp: 325680
Ion Ratio Lower Upper
117 100
82 55.2 46.7 70.1
119 31.9 26.5 39.7

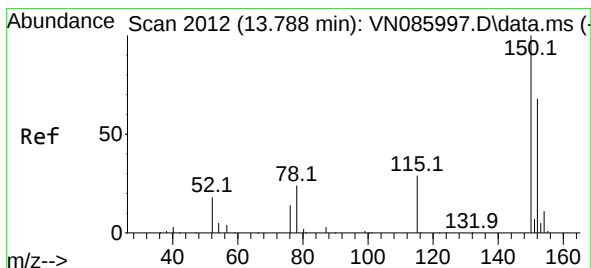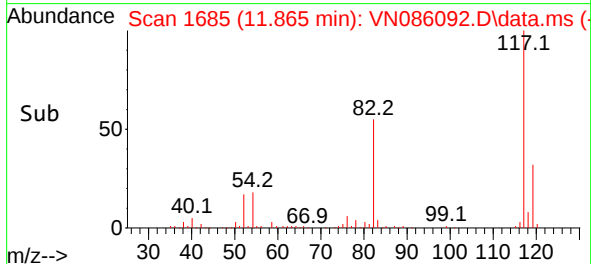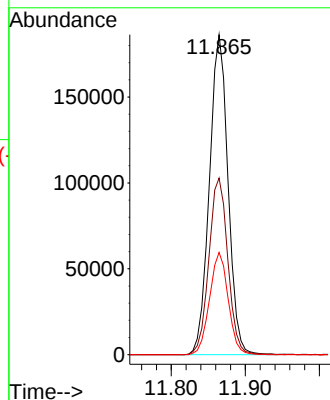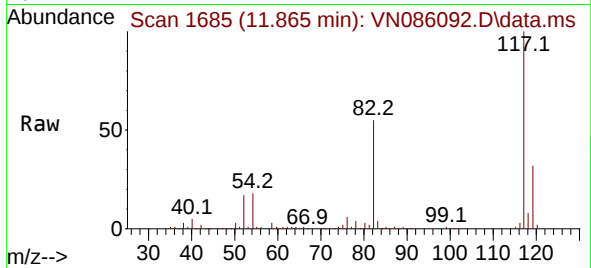

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.788 min Scan# 2012
Delta R.T. -0.000 min
Lab File: VN086092.D
Acq: 25 Mar 2025 11:26

Tgt Ion:152 Resp: 130926
Ion Ratio Lower Upper
152 100
115 60.4 31.1 93.2
150 157.9 0.0 359.6

