
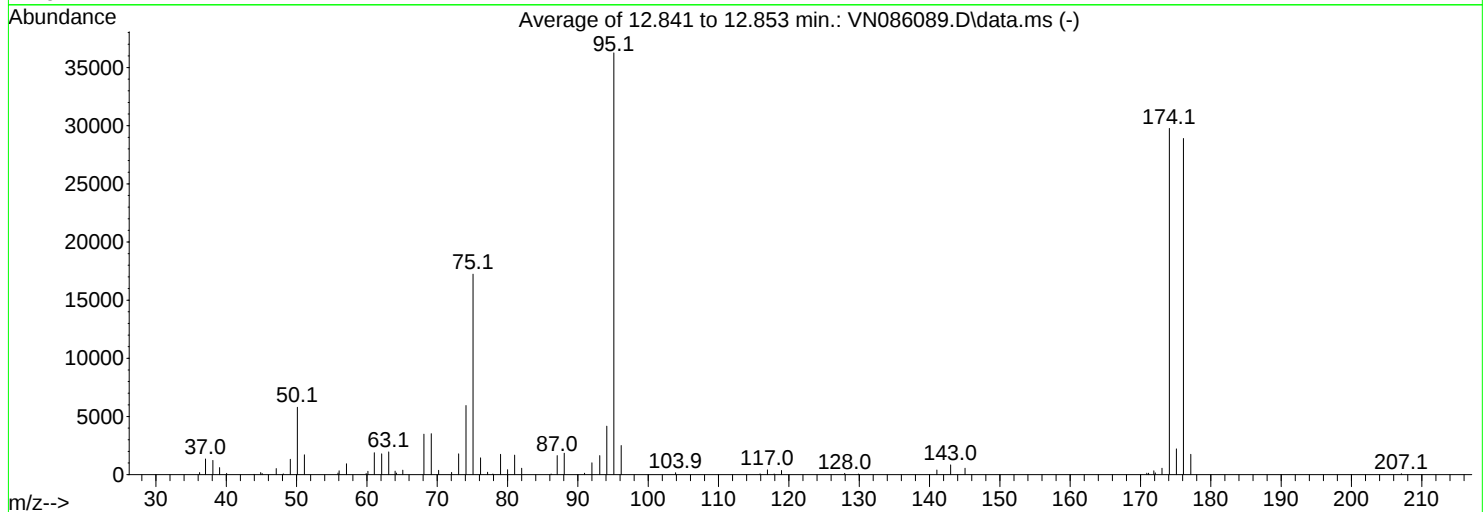


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032525\
Data File : VN086089.D
Acq On : 25 Mar 2025 09:39
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031825W.M
Title : SW846 8260
Last Update : Wed Mar 19 03:20:56 2025

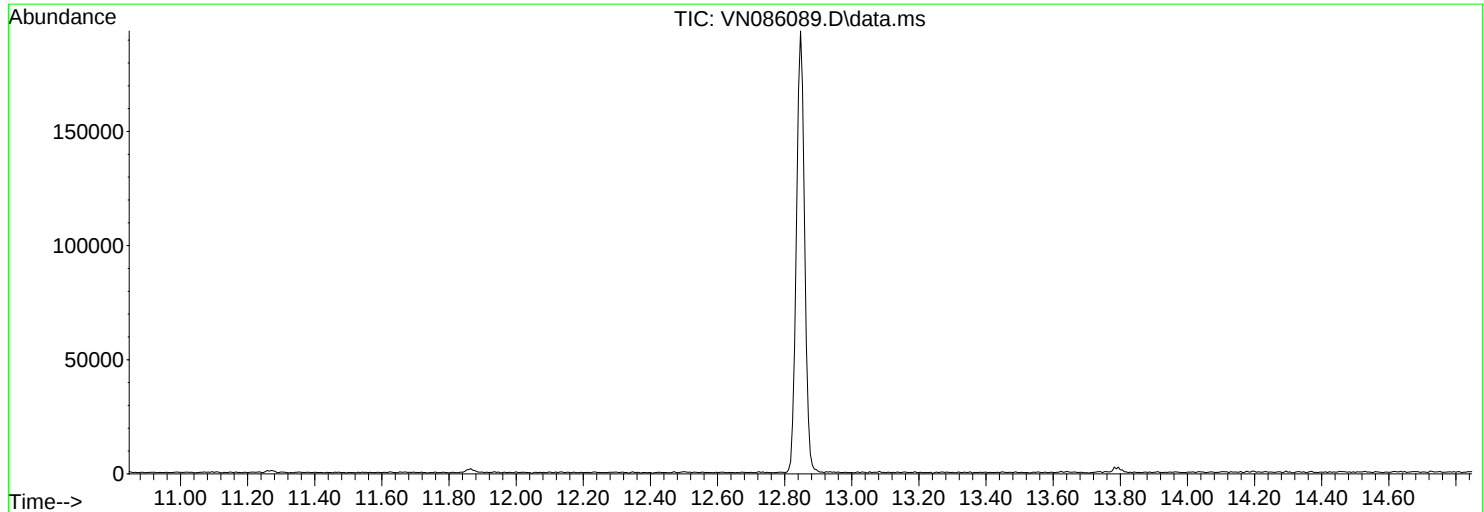

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	5790	PASS
75	95	30	60	47.5	17230	PASS
95	95	100	100	100.0	36261	PASS
96	95	5	9	6.9	2503	PASS
173	174	0.00	2	1.8	546	PASS
174	95	50	100	82.1	29765	PASS
175	174	5	9	7.4	2212	PASS
176	174	95	101	97.1	28901	PASS
177	176	5	9	6.1	1749	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.20	183	50.10	5790	64.20	135	77.90	51
37.05	1354	51.10	1700	65.10	388	79.00	174
38.10	1218	55.90	142	68.10	3487	80.00	43
39.05	605	56.05	326	69.15	3520	81.00	168
40.05	113	57.10	936	70.20	370	82.00	547
43.95	26	59.90	103	72.05	191	86.20	54
44.90	185	60.15	286	73.05	1785	87.05	1638
45.10	99	61.05	1887	74.10	5941	88.05	1851
47.10	521	62.10	1790	75.10	17230	90.95	121
48.10	70	63.10	1948	76.15	1451	92.00	1022
49.10	1325	64.00	302	77.15	209	93.10	1639

Average of 12.841 to 12.853 min.: VN086089.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
94.10	4162	143.00	846	207.10	86		
95.10	36261	145.05	551				
96.15	2503	170.90	119				
103.90	167	171.15	121				
115.90	77	171.90	337				
116.95	416	172.10	158				
117.90	54	173.05	546				
118.95	363	174.10	29765				
127.95	105	175.10	2212				
129.90	52	176.10	28901				
141.05	403	177.15	1749				

Instrument :

MSVOA_N

ClientSampleId :

BFB