

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN032620\
 Data File : VN060728.D
 Acq On : 26 Mar 2020 20:46
 Operator : JC/MD
 Sample : L2026-03
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 SLUDGE-PIT

Quant Time: Mar 27 05:37:01 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N031820W.M
 Quant Title : SW846 8260
 QLast Update : Wed Mar 18 08:49:09 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.64	168	193556	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.57	114	318519	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.40	117	302819	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.34	152	142997	50.00	ug/l	0.00


System Monitoring Compounds

33) 1,2-Dichloroethane-d4	8.00	65	123851	46.61	ug/l	0.00
Spiked Amount	50.000		Recovery	=	93.22%	
35) Dibromofluoromethane	7.57	113	94245	48.93	ug/l	0.00
Spiked Amount	50.000		Recovery	=	97.86%	
50) Toluene-d8	10.08	98	396501	50.40	ug/l	0.00
Spiked Amount	50.000		Recovery	=	100.80%	
62) 4-Bromofluorobenzene	12.40	95	149422	51.83	ug/l	0.00
Spiked Amount	50.000		Recovery	=	103.66%	

Target Compounds

						Qvalue
11) Tert butyl alcohol	4.72	59	258	0.660	ug/l #	72
16) Acetone	3.78	43	50775	53.947	ug/l	97
18) Methyl Acetate	4.30	43	1888	0.713	ug/l #	65
20) Methylene Chloride	4.53	84	5945	2.568	ug/l	92
25) 2-Butanone	6.80	43	17957	11.790	ug/l	98
29) Tetrahydrofuran	7.18	42	345	0.320	ug/l #	35
31) Cyclohexane	7.64	56	4153	0.970	ug/l #	1
36) 1,1-Dichloropropene	7.64	75	14638	4.746	ug/l #	50
37) Ethyl Acetate	6.80	43	17957	5.388	ug/l #	70
38) Carbon Tetrachloride	7.64	117	18180	6.577	ug/l #	17
40) Benzene	8.02	78	2308	0.248	ug/l	99
41) Methacrylonitrile	7.16	41	893	0.628	ug/l #	100
43) Isopropyl Acetate	8.14	43	21675	3.944	ug/l #	90
48) Methyl methacrylate	9.16	41	3554	1.452	ug/l #	28
51) 4-Methyl-2-Pentanone	9.97	43	88005	28.139	ug/l	98
52) Toluene	10.14	92	12376	2.201	ug/l	98
54) cis-1,3-Dichloropropene	9.89	75	15768	4.054	ug/l #	62
56) Ethyl methacrylate	10.34	69	9017	2.673	ug/l #	62
57) 1,3-Dichloropropane	10.75	76	1249	0.333	ug/l #	42
59) 2-Hexanone	10.75	43	18536	8.228	ug/l #	58
68) m/p-Xylenes	11.61	106	1106	0.267	ug/l	85
71) Bromoform	12.40	173	120	1.745	ug/l #	1
74) N-amyl acetate	12.02	43	4555	0.919	ug/l #	47
76) 1,2,3-Trichloropropane	12.40	75	75002	24.307	ug/l #	100
81) trans-1,4-Dichloro-2-buten	12.40	75	75002	62.428	ug/l #	13
92) 1,2-Dibromo-3-Chloropropan	14.45	75	62	Below Cal	#	3
95) Naphthalene	15.13	128	1659	0.206	ug/l #	69

(#) = qualifier out of range (m) = manual integration (+) = signals summed

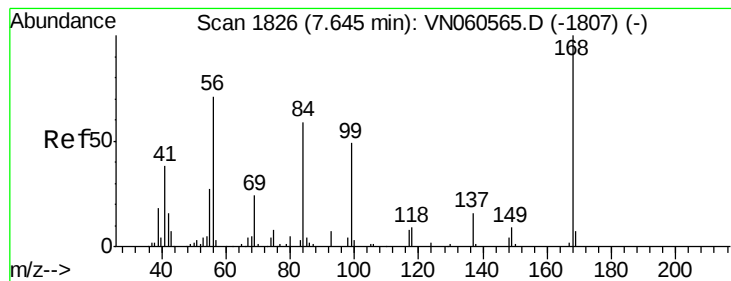

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.64 min Scan# 1826

Delta R.T. -0.00 min

Lab File: VN060728.D

Acq: 26 Mar 2020 20:46

Instrument :

MSVOA_N

ClientSampleId :


SLUDGE-PIT

Tgt Ion: 168 Resp: 193556




Ion Ratio Lower Upper

168 100

99 56.6 44.0 66.0



Abundance Ion 167.90 (167.60 to 168.60): VN060728.D (-1733) (-)

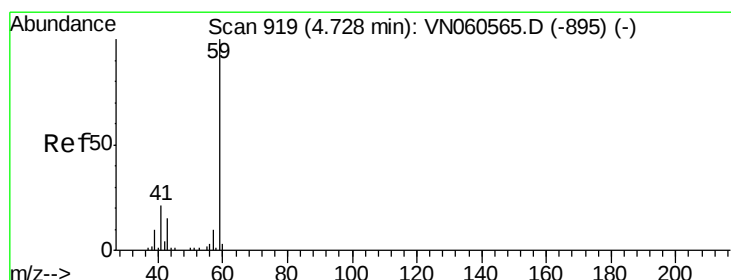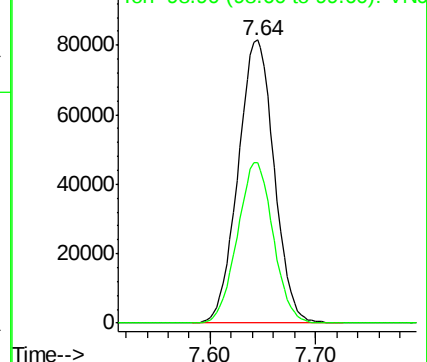

#11

Tert butyl alcohol

Concen: 0.660 ug/l

RT: 4.72 min Scan# 917

Delta R.T. -0.01 min

Lab File: VN060728.D


Acq: 26 Mar 2020 20:46

Tgt Ion: 59 Resp: 258



Ion Ratio Lower Upper


59 100

57 0.0 8.2 12.4#



Abundance Ion 59.00 (58.70 to 59.70): VN060728.D (-826) (-)



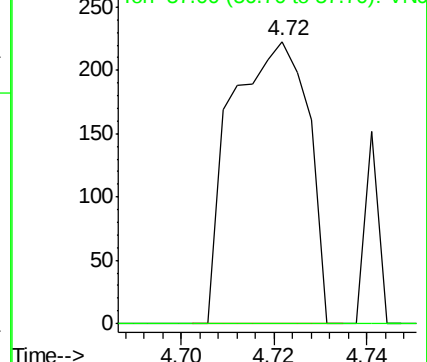





#16
Acetone
Concen: 53.947 ug/l
RT: 3.78 min Scan# 624
Delta R.T. -0.00 min
Lab File: VN060728.D
Acq: 26 Mar 2020 20:46




Instrument :
MSVOA_N
ClientSampleId :
SLUDGE-PIT


Tgt Ion: 43 Resp: 50775
Ion Ratio Lower Upper
43 100
58 29.6 25.1 37.7

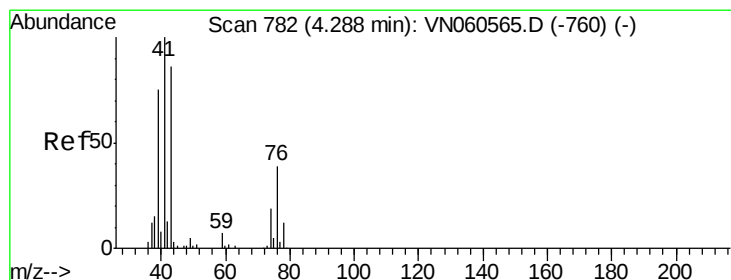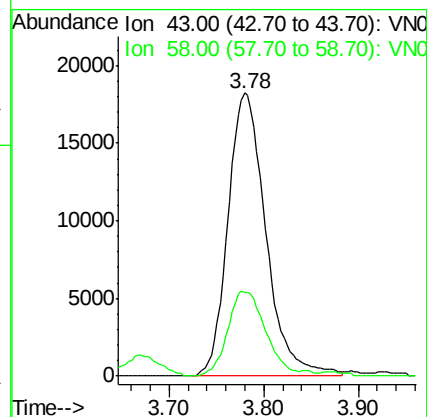

#18
Methyl Acetate
Concen: 0.713 ug/l
RT: 4.30 min Scan# 785
Delta R.T. 0.01 min
Lab File: VN060728.D
Acq: 26 Mar 2020 20:46

Tgt Ion: 43 Resp: 1888
Ion Ratio Lower Upper
43 100
74 5.1 17.5 26.3#

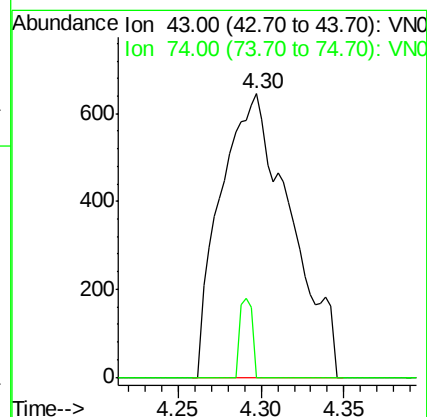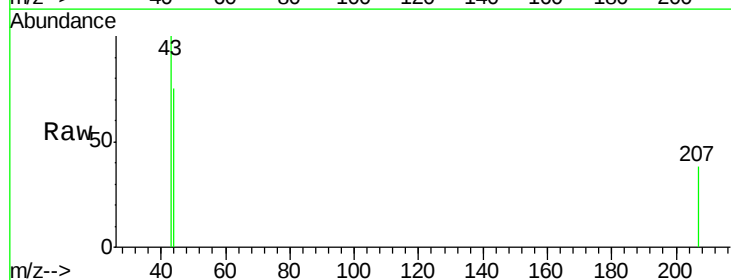


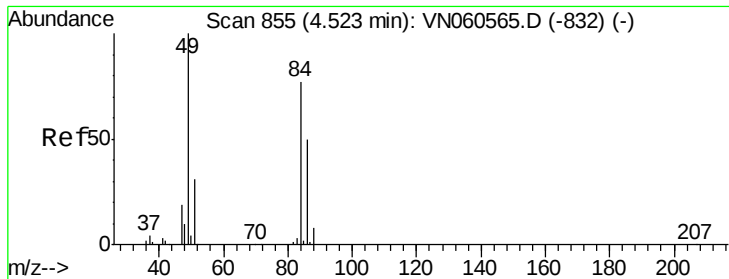

#20
Methylene Chloride
Concen: 2.568 ug/l
RT: 4.53 min Scan# 857
Delta R.T. 0.01 min
Lab File: VN060728.D
Acq: 26 Mar 2020 20:46

Instrument :
MSVOA_N
ClientSampleId :
SLUDGE-PIT

Tgt Ion:	84	Resp:	5945
Ion	Ratio	Lower	Upper
84	100		
49	119.2	103.3	154.9
51	34.9	31.6	47.4
86	58.5	52.0	78.0



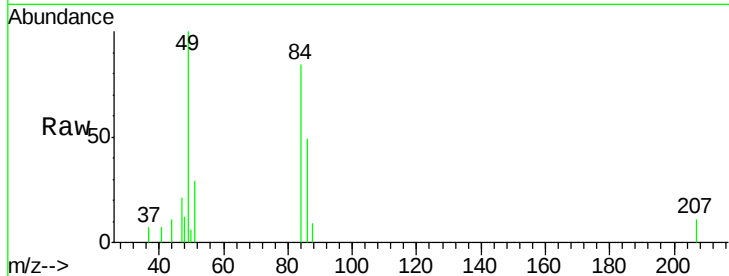


Abundance Ion 83.90 (83.60 to 84.60): VN060728.D (-1469) (-)

Ion 48.90 (48.60 to 49.60): VN060728.D (-1469) (-)


Ion 50.90 (50.60 to 51.60): VN060728.D (-1469) (-)

Ion 85.90 (85.60 to 86.60): VN060728.D (-1469) (-)

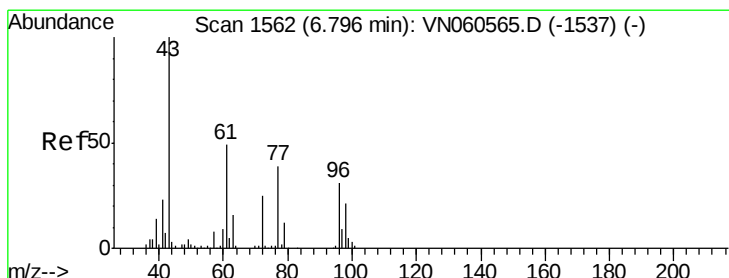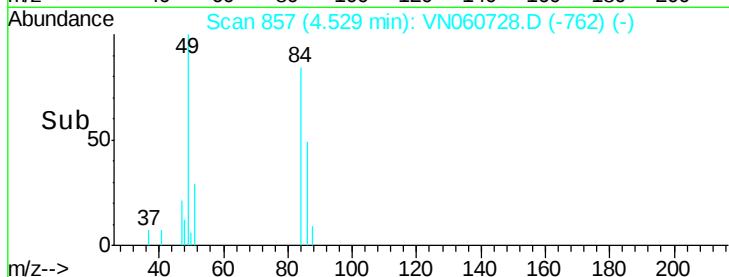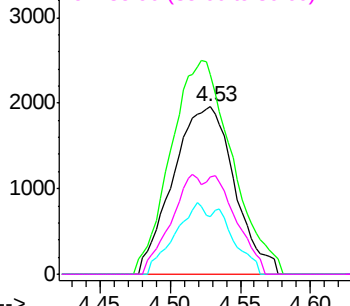



#25
2-Butanone
Concen: 11.790 ug/l
RT: 6.80 min Scan# 1563
Delta R.T. 0.00 min
Lab File: VN060728.D
Acq: 26 Mar 2020 20:46


Tgt Ion:	43	Resp:	17957
Ion	Ratio	Lower	Upper
43	100		
72	24.5	20.4	30.6

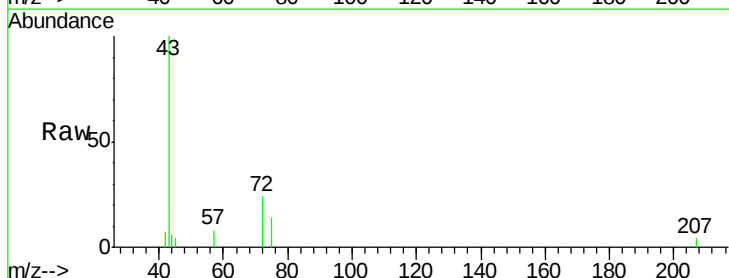

Abundance Ion 43.00 (42.70 to 43.70): VN060728.D (-1469) (-)

Ion 72.00 (71.70 to 72.70): VN060728.D (-1469) (-)

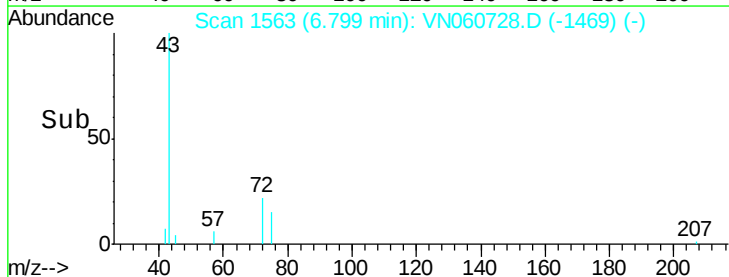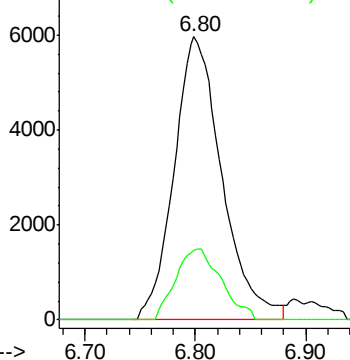



#29

Tetrahydrofuran

Concen: 0.320 ug/l

RT: 7.18 min Scan# 1682

Delta R.T. 0.00 min

Lab File: VN060728.D

Acq: 26 Mar 2020 20:46

Instrument :

MSVOA_N

ClientSampleId :

SLUDGE-PIT


Tgt Ion: 42 Resp: 345

Ion Ratio Lower Upper

42 100

72 0.0 33.2 49.8#




71 0.0 31.1 46.7#

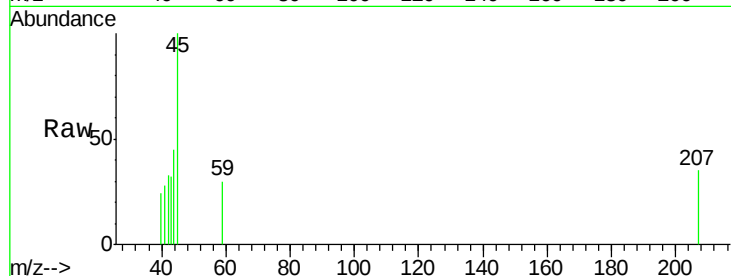

Abundance Ion 42.00 (41.70 to 42.70): VN0

Ion 72.00 (71.70 to 72.70): VN0

Ion 71.00 (70.70 to 71.70): VN0

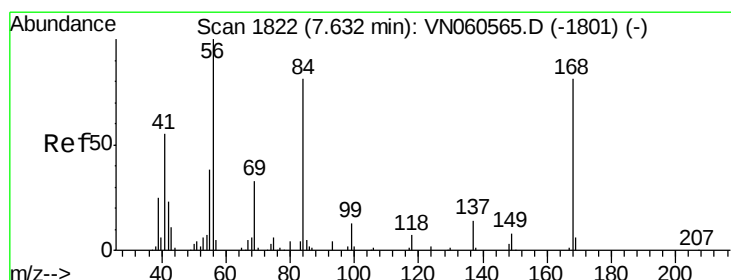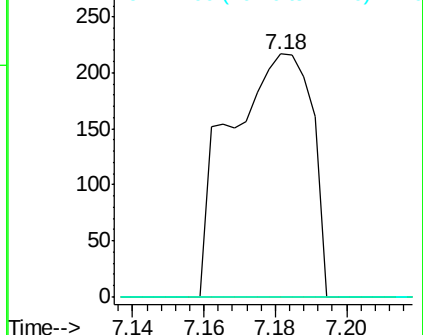

#31

Cyclohexane

Concen: 0.970 ug/l

RT: 7.64 min Scan# 1826

Delta R.T. 0.01 min

Lab File: VN060728.D

Acq: 26 Mar 2020 20:46


Tgt Ion: 56 Resp: 4153

Ion Ratio Lower Upper

56 100

69 181.1 26.6 40.0#



84 141.8 64.3 96.5#




Abundance Ion 56.00 (55.70 to 56.70): VN0

Ion 69.00 (68.70 to 69.70): VN0

Ion 84.00 (83.70 to 84.70): VN0




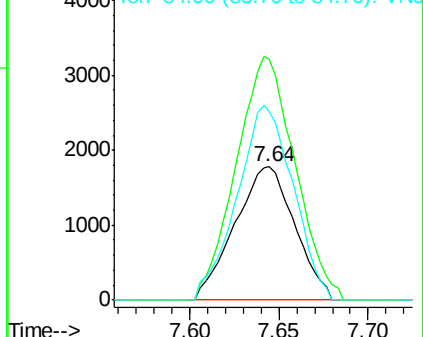




#33
 1,2-Dichloroethane-d4
 Concen: 46.612 ug/l
 RT: 8.00 min Scan# 1938
 Delta R.T. -0.00 min
 Lab File: VN060728.D
 Acq: 26 Mar 2020 20:46




Instrument :
 MSVOA_N
 ClientSampleId :
 SLUDGE-PIT


Tgt Ion: 65 Resp: 123851
 Ion Ratio Lower Upper
 65 100
 67 54.2 0.0 107.6

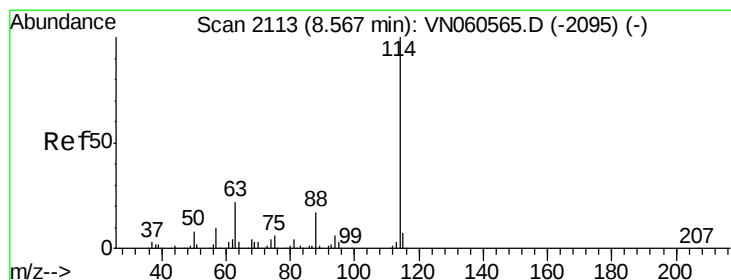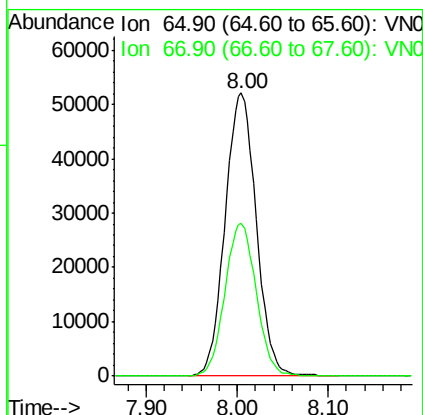

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.57 min Scan# 2113
 Delta R.T. -0.00 min
 Lab File: VN060728.D
 Acq: 26 Mar 2020 20:46

Tgt Ion: 114 Resp: 318519
 Ion Ratio Lower Upper
 114 100
 63 22.9 0.0 43.8
 88 16.5 0.0 33.0



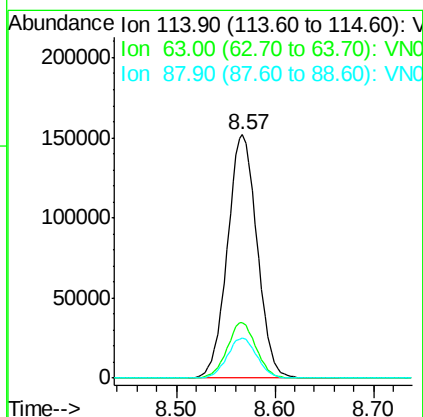
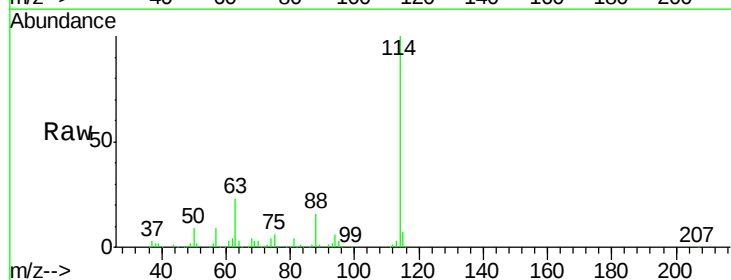




#35
 Dibromofluoromethane
 Concen: 48.933 ug/l
 RT: 7.57 min Scan# 1802
 Delta R.T. 0.00 min
 Lab File: VN060728.D
 Acq: 26 Mar 2020 20:46




Instrument :
 MSVOA_N
 ClientSampleId :
 SLUDGE-PIT


Tgt Ion:113 Resp: 94245
 Ion Ratio Lower Upper
 113 100
 111 103.7 82.9 124.3
 192 19.8 15.8 23.8

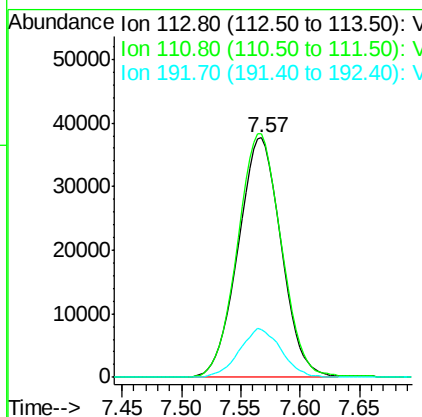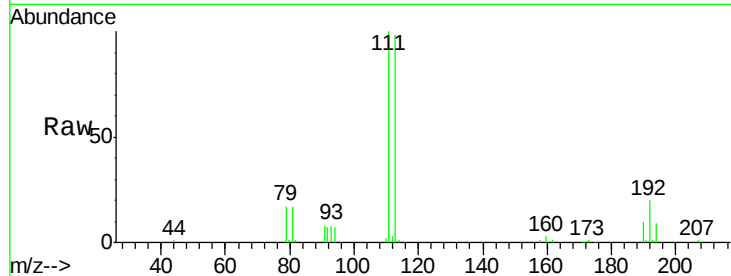

#36
 1,1-Dichloropropene
 Concen: 4.746 ug/l
 RT: 7.64 min Scan# 1825
 Delta R.T. -0.13 min
 Lab File: VN060728.D
 Acq: 26 Mar 2020 20:46

Tgt Ion: 75 Resp: 14638
 Ion Ratio Lower Upper
 75 100
 110 7.9 16.9 50.6#
 77 0.0 24.6 36.8#



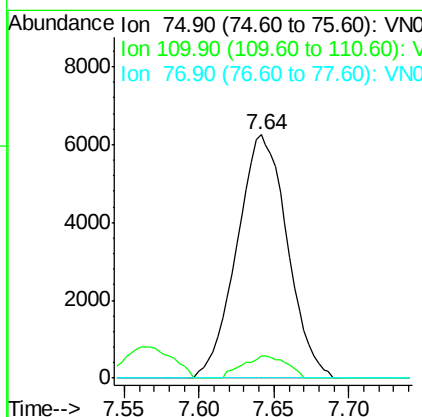
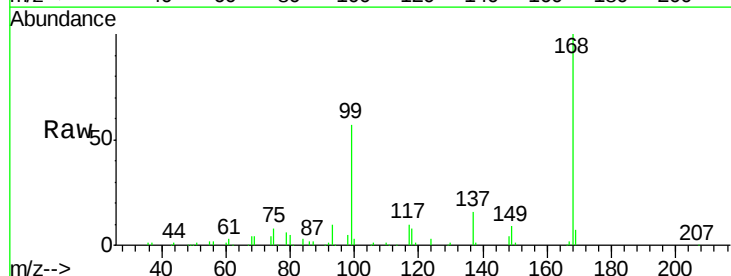




#37
 Ethyl Acetate
 Concen: 5.388 ug/l
 RT: 6.80 min Scan# 1563
 Delta R.T. -0.10 min
 Lab File: VN060728.D
 Acq: 26 Mar 2020 20:46




Instrument :
 MSVOA_N
 ClientSampleId :
 SLUDGE-PIT


Tgt Ion: 43 Resp: 17957
 Ion Ratio Lower Upper
 43 100
 61 0.0 10.6 15.8#
 70 0.0 7.9 11.9#

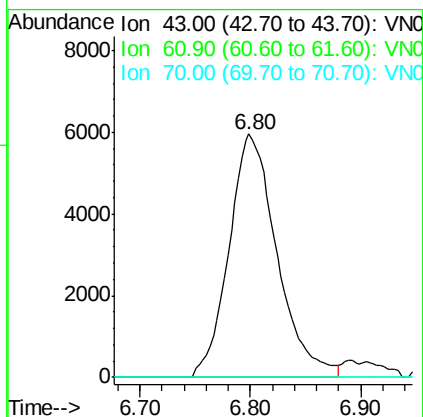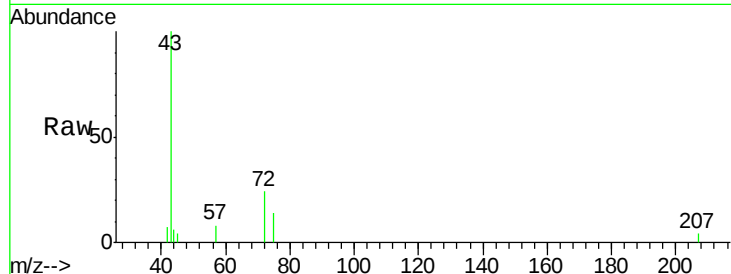

#38
 Carbon Tetrachloride
 Concen: 6.577 ug/l
 RT: 7.64 min Scan# 1825
 Delta R.T. -0.11 min
 Lab File: VN060728.D
 Acq: 26 Mar 2020 20:46

Tgt Ion: 117 Resp: 18180
 Ion Ratio Lower Upper
 117 100
 119 6.2 76.2 114.2#
 121 0.0 23.7 35.5#

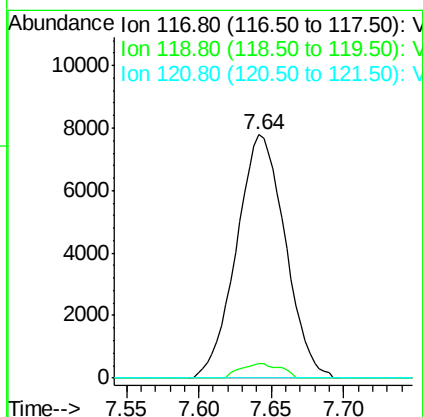



#40

Benzene

Concen: 0.248 ug/l

RT: 8.02 min Scan# 1943

Delta R.T. -0.00 min

Lab File: VN060728.D

Acq: 26 Mar 2020 20:46

Instrument :

MSVOA_N

ClientSampleId :





SLUDGE-PIT

Tgt Ion: 78 Resp: 2308

Ion Ratio Lower Upper

78 100

77 23.8 18.6 28.0

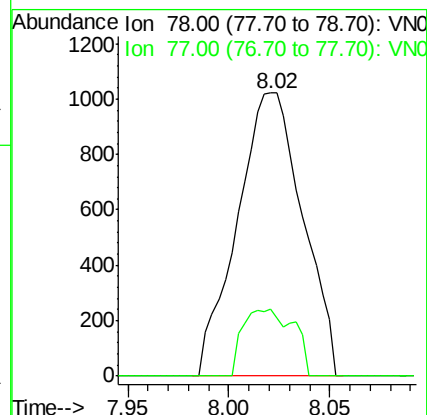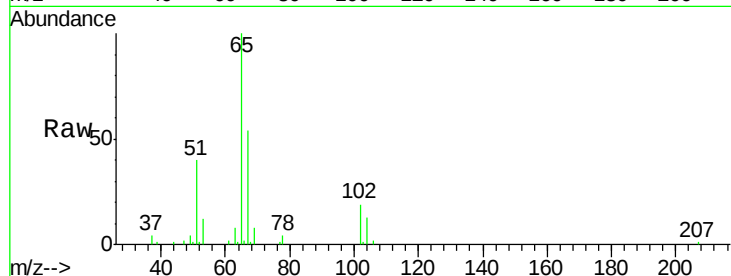

#41

Methacrylonitrile

Concen: 0.628 ug/l

RT: 7.16 min Scan# 1676

Delta R.T. 0.02 min

Lab File: VN060728.D

Acq: 26 Mar 2020 20:46

Tgt Ion: 41 Resp: 893




Ion Ratio Lower Upper


41 100

39 0.0 0.0 0.0

67 0.0 0.0 0.0

52 0.0 0.0 0.0

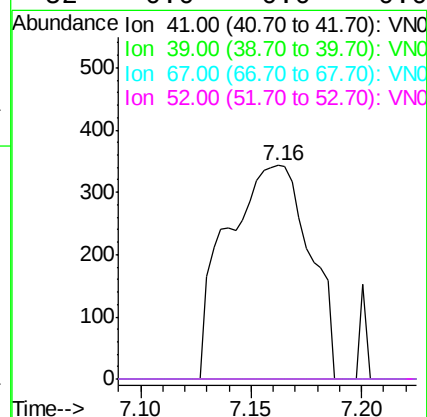







#43
Isopropyl Acetate
Concen: 3.944 ug/l
RT: 8.14 min Scan# 1980
Delta R.T. -0.00 min
Lab File: VN060728.D
Acq: 26 Mar 2020 20:46

Instrument :
MSVOA_N
ClientSampled :
SLUDGE-PIT

Tgt Ion: 43 Resp: 21675
Ion Ratio Lower Upper
43 100
61 19.1 20.7 31.1#
87 11.7 9.8 14.8




Abundance Ion 43.00 (42.70 to 43.70): VN0
Ion 61.00 (60.70 to 61.70): VN0
Ion 87.00 (86.70 to 87.70): VN0


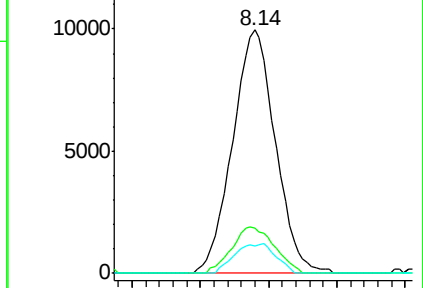



#48
Methyl methacrylate
Concen: 1.452 ug/l
RT: 9.16 min Scan# 2297
Delta R.T. -0.02 min
Lab File: VN060728.D
Acq: 26 Mar 2020 20:46

Tgt Ion: 41 Resp: 3554
Ion Ratio Lower Upper
41 100
69 0.0 65.4 98.0#
39 23.4 44.0 66.0#



Abundance Ion 41.00 (40.70 to 41.70): VN0
Ion 69.00 (68.70 to 69.70): VN0
Ion 39.00 (38.70 to 39.70): VN0

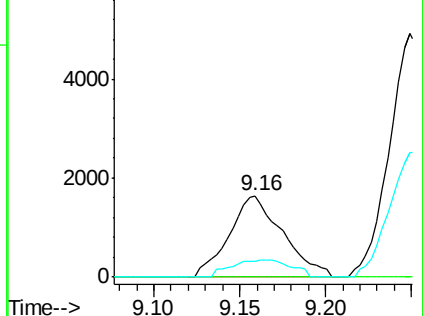



#50

Toluene-d8

Concen: 50.401 ug/l

RT: 10.08 min Scan# 2583

Delta R.T. -0.00 min

Lab File: VN060728.D

Acq: 26 Mar 2020 20:46

Instrument :

MSVOA_N

ClientSampleId :





SLUDGE-PIT

Tgt Ion: 98 Resp: 396501

Ion Ratio Lower Upper

98 100

100 65.6 51.8 77.8

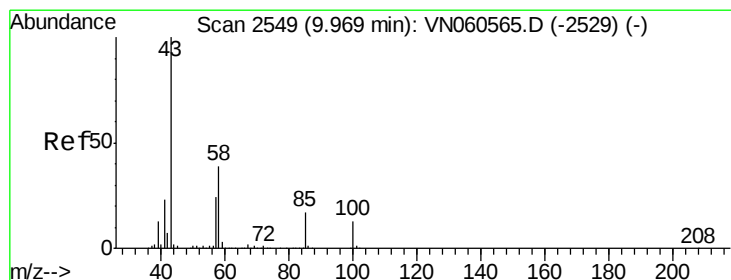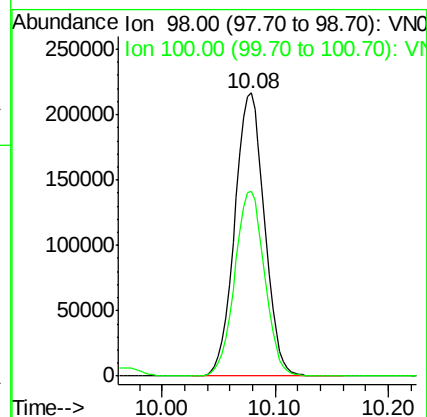

#51

4-Methyl-2-Pentanone

Concen: 28.139 ug/l

RT: 9.97 min Scan# 2549

Delta R.T. -0.00 min

Lab File: VN060728.D




Acq: 26 Mar 2020 20:46


Tgt Ion: 43 Resp: 88005

Ion Ratio Lower Upper

43 100

58 37.1 30.8 46.2

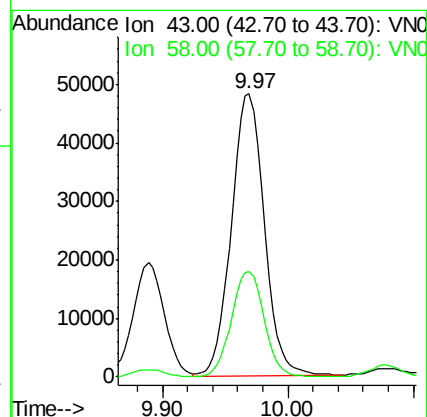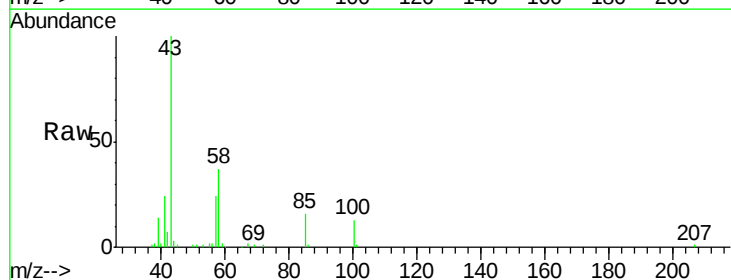



#52

Toluene

Concen: 2.201 ug/l

RT: 10.14 min Scan# 2603

Delta R.T. -0.00 min

Lab File: VN060728.D

Acq: 26 Mar 2020 20:46

Instrument :

MSVOA_N

ClientSampled :





SLUDGE-PIT

Tgt Ion: 92 Resp: 12376

Ion Ratio Lower Upper

92 100

91 175.2 137.6 206.4

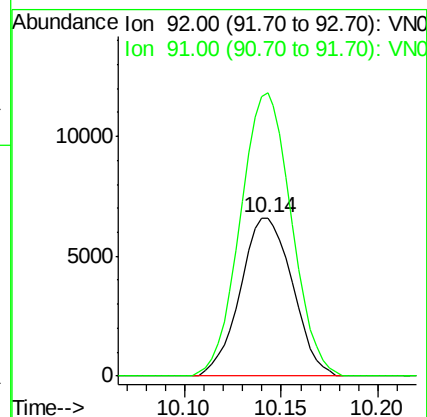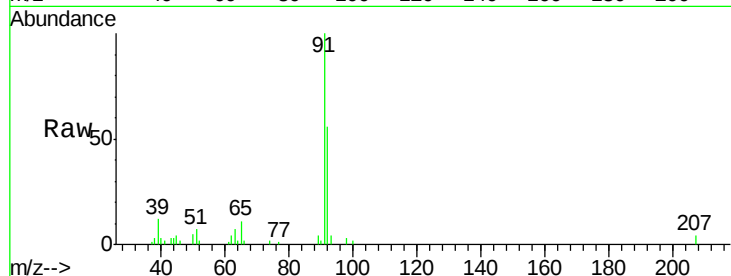

#54

cis-1,3-Dichloropropene

Concen: 4.054 ug/l

RT: 9.89 min Scan# 2524

Delta R.T. 0.06 min

Lab File: VN060728.D

Acq: 26 Mar 2020 20:46




Tgt Ion: 75 Resp: 15768


Ion Ratio Lower Upper

75 100

77 0.0 25.4 38.0#

39 31.8 40.2 60.4#

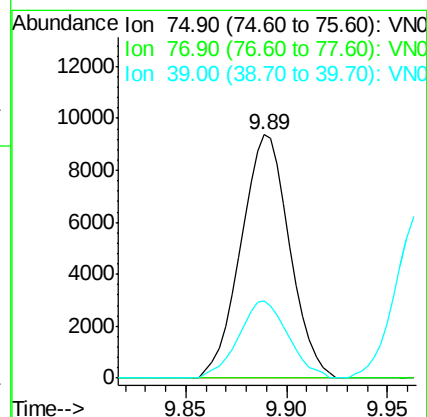



#56

Ethyl methacrylate

Concen: 2.673 ug/l

RT: 10.34 min Scan# 2664

Delta R.T. -0.08 min

Lab File: VN060728.D

Acq: 26 Mar 2020 20:46

Instrument :





MSVOA_N

ClientSampleId :

SLUDGE-PIT

Tgt Ion: 69 Resp: 9017

Ion	Ratio	Lower	Upper
69	100		
41	104.7	55.4	83.2#
39	53.9	29.4	44.0#

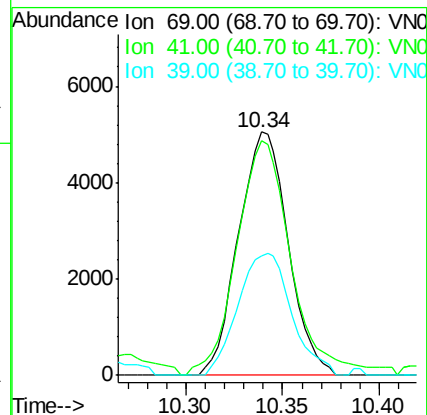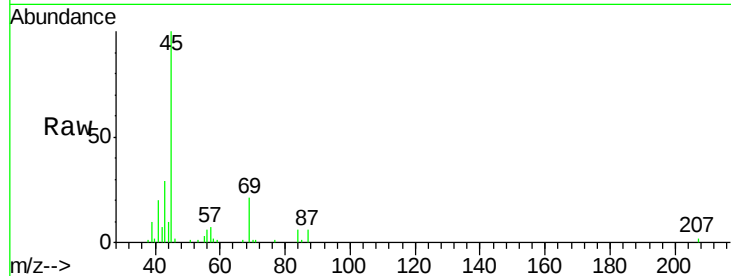

#57

1,3-Dichloropropane

Concen: 0.333 ug/l

RT: 10.75 min Scan# 2793




Delta R.T. 0.06 min


Lab File: VN060728.D

Acq: 26 Mar 2020 20:46

Tgt Ion: 76 Resp: 1249

Ion	Ratio	Lower	Upper
76	100		
78	0.0	25.8	38.6#



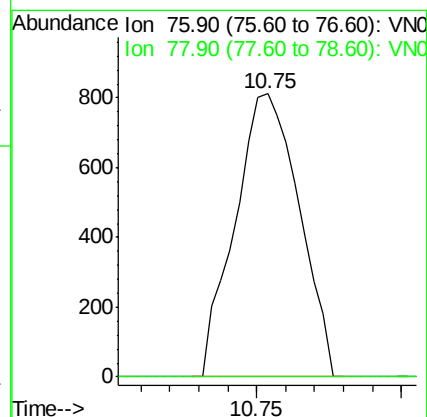



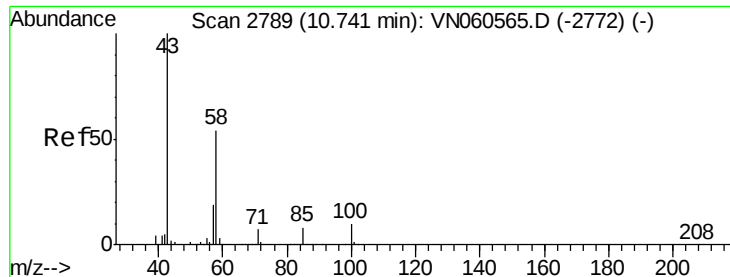

#59
2-Hexanone
Concen: 8.228 ug/l
RT: 10.75 min Scan# 2793
Delta R.T. 0.01 min
Lab File: VN060728.D
Acq: 26 Mar 2020 20:46




Instrument :
MSVOA_N
ClientSampleId :
SLUDGE-PIT


Tgt Ion: 43 Resp: 18536
Ion Ratio Lower Upper
43 100
58 23.2 26.7 80.1#

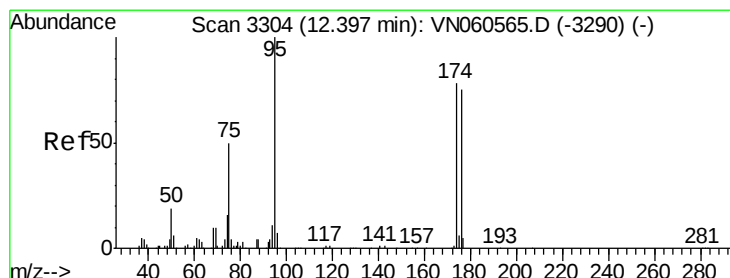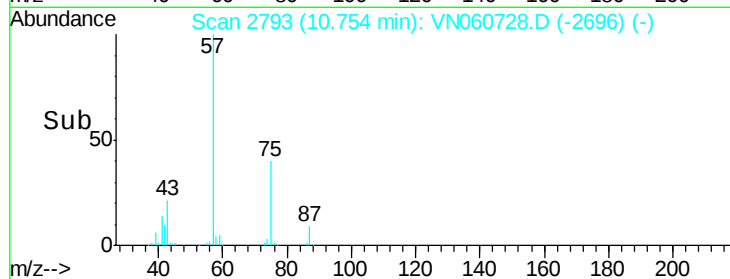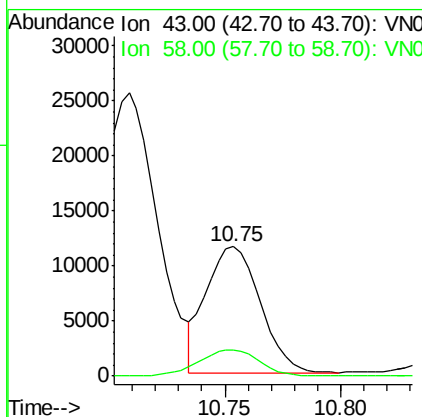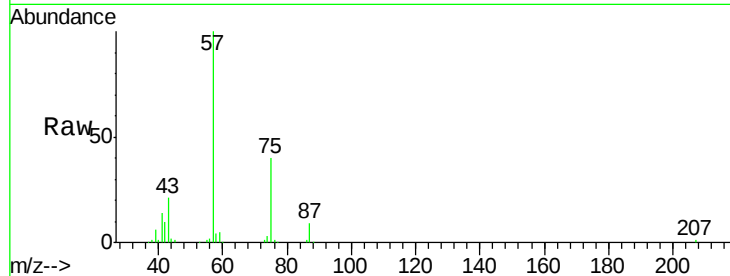

#62
4-Bromofluorobenzene
Concen: 51.827 ug/l
RT: 12.40 min Scan# 3304
Delta R.T. -0.00 min
Lab File: VN060728.D
Acq: 26 Mar 2020 20:46

Tgt Ion: 95 Resp: 149422
Ion Ratio Lower Upper
95 100
174 78.0 0.0 157.6
176 75.2 0.0 150.6

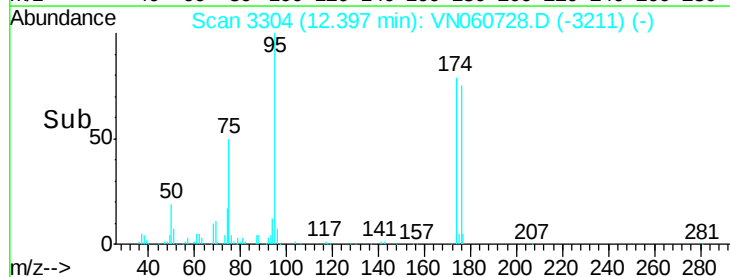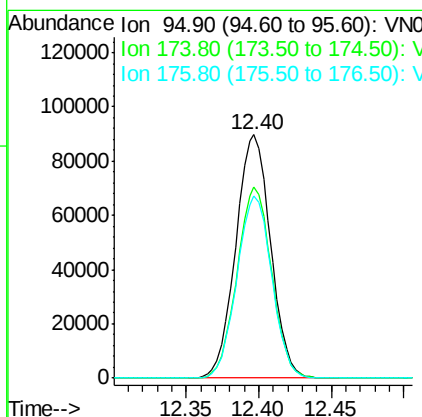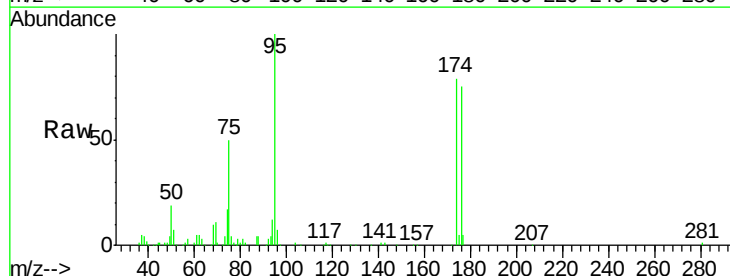


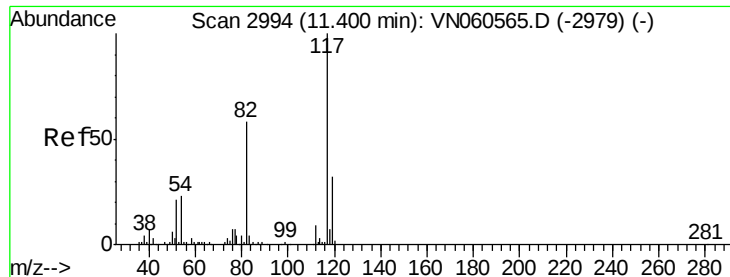




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.40 min Scan# 2994
Delta R.T. -0.00 min
Lab File: VN060728.D
Acq: 26 Mar 2020 20:46

Instrument :
MSVOA_N
ClientSampleId :
SLUDGE-PIT

Tgt Ion:117 Resp: 302819
Ion Ratio Lower Upper
117 100
82 58.5 46.7 70.1
119 32.1 25.5 38.3

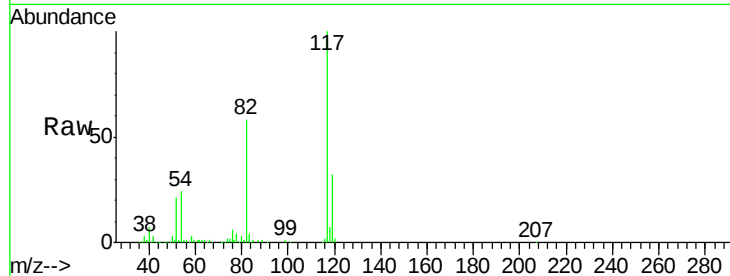


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VN
Ion 118.90 (118.60 to 119.60): V

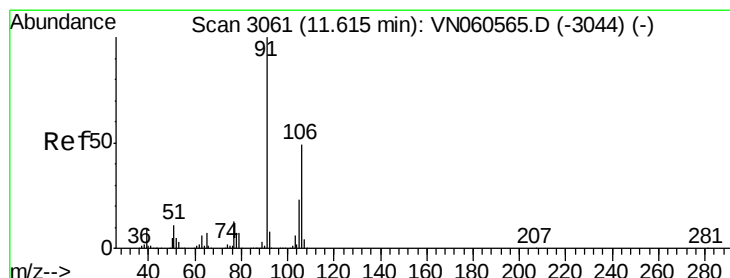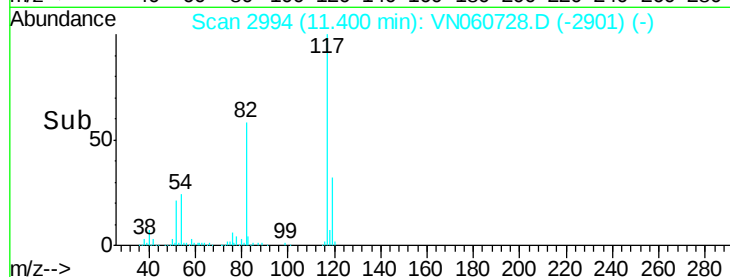
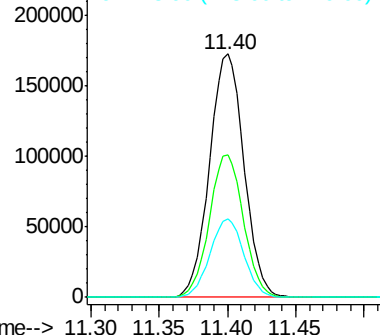



#68
m/p-Xylenes
Concen: 0.267 ug/l
RT: 11.61 min Scan# 3060
Delta R.T. -0.00 min
Lab File: VN060728.D
Acq: 26 Mar 2020 20:46

Tgt Ion:106 Resp: 1106
Ion Ratio Lower Upper
106 100
91 229.1 165.0 247.4

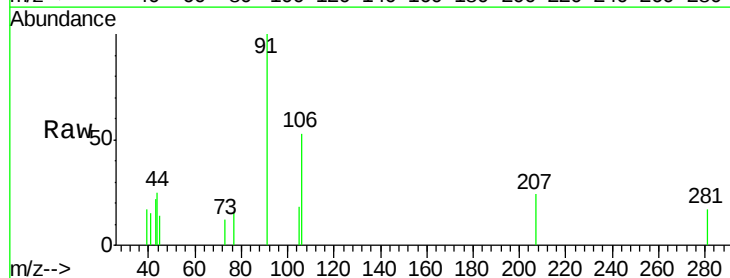

Abundance Ion 106.00 (105.70 to 106.70): V
Ion 91.00 (90.70 to 91.70): VN

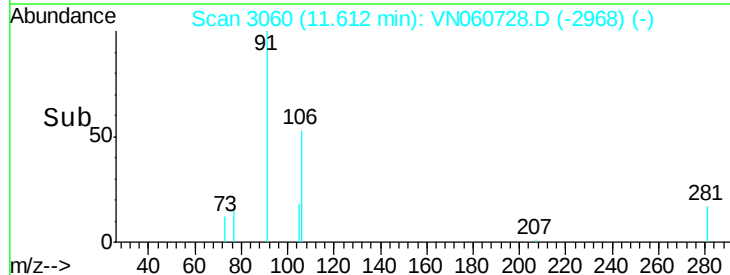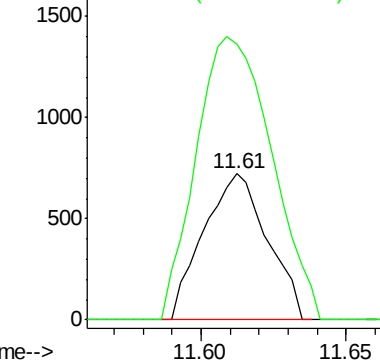


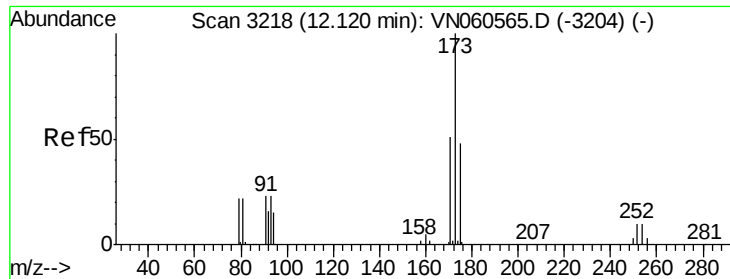




#71
Bromoform
Concen: 1.745 ug/l
RT: 12.40 min Scan# 3305
Delta R.T. 0.28 min
Lab File: VN060728.D
Acq: 26 Mar 2020 20:46

Instrument :
MSVOA_N
ClientSampleId :
SLUDGE-PIT

Tgt Ion:173 Resp: 120
Ion Ratio Lower Upper
173 100
175 5972.5 24.1 72.4#
254 0.0 0.0 0.0

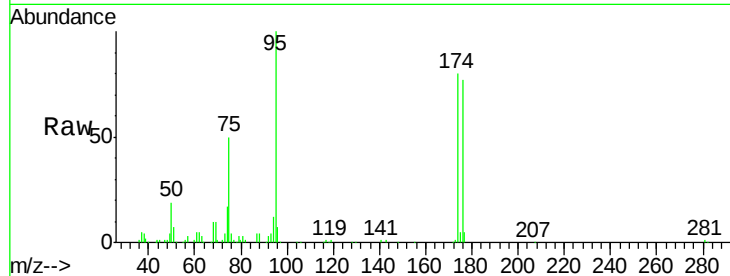


Abundance Ion 172.70 (172.40 to 173.40): V
Ion 174.70 (174.40 to 175.40): V
Ion 254.40 (254.10 to 255.10): V

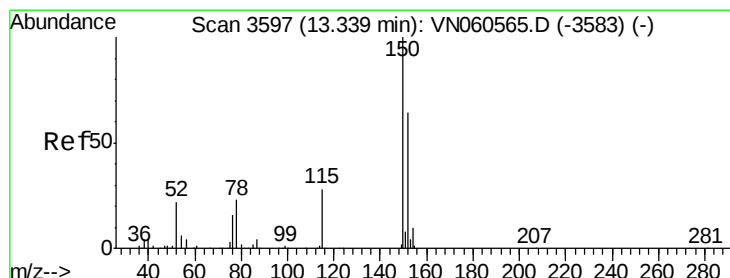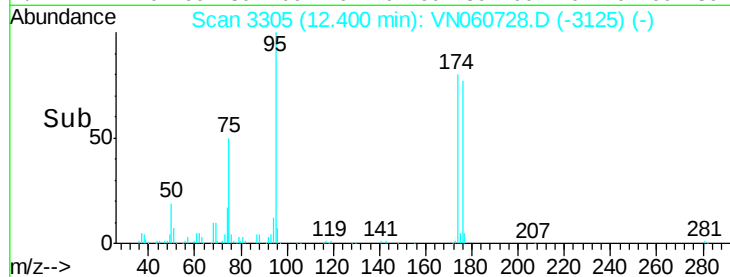
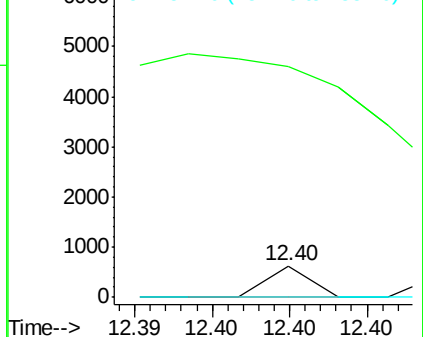



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.34 min Scan# 3597
Delta R.T. -0.00 min
Lab File: VN060728.D
Acq: 26 Mar 2020 20:46

Tgt Ion:152 Resp: 142997
Ion Ratio Lower Upper
152 100
115 60.0 30.2 90.6
150 157.2 0.0 350.2

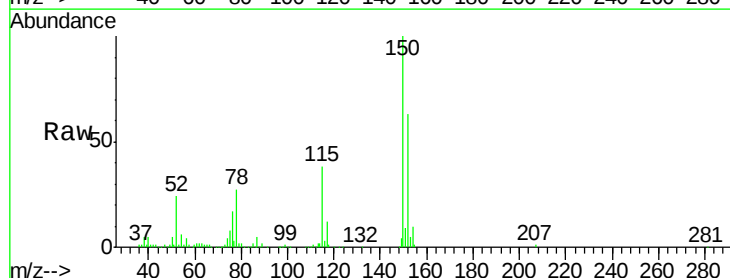

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

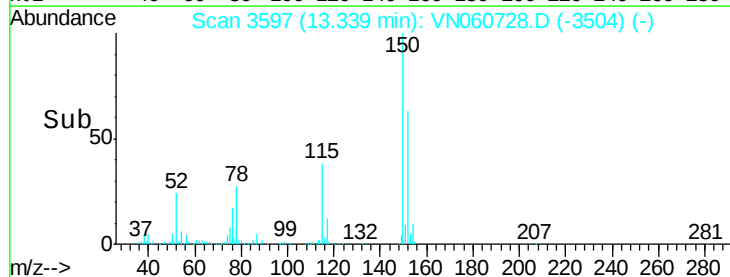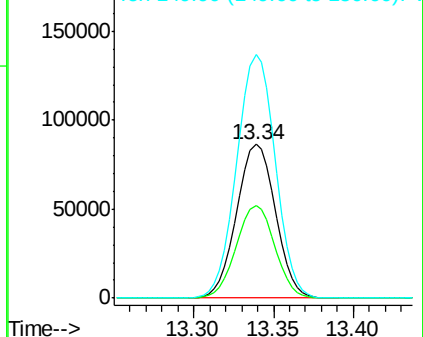

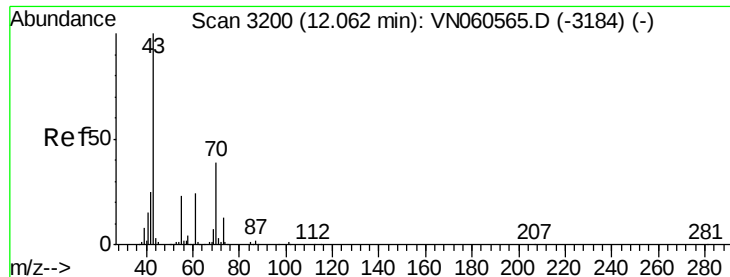

#74

N-ethyl acetate

Concen: 0.919 ug/l

RT: 12.02 min Scan# 3187

Delta R.T. -0.04 min

Lab File: VN060728.D

Acq: 26 Mar 2020 20:46

Instrument :

MSVOA_N

ClientSampleId :

SLUDGE-PIT

Tgt Ion: 43 Resp: 4555


Ion Ratio Lower Upper

43 100

70 0.0 31.1 46.7#

55 4.4 18.6 27.8#

61 0.0 18.9 28.3#



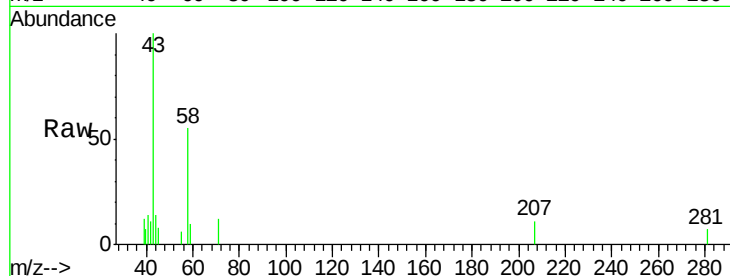


Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 70.00 (69.70 to 70.70): VN0

Ion 55.00 (54.70 to 55.70): VN0

Ion 61.00 (60.70 to 61.70): VN0

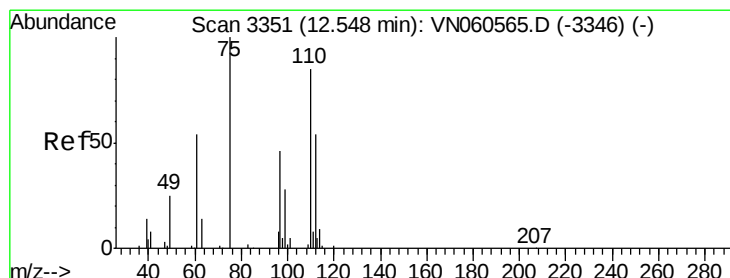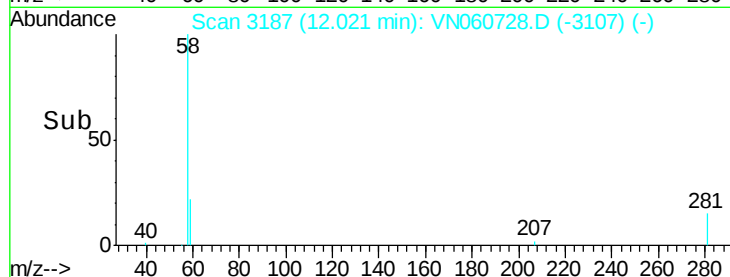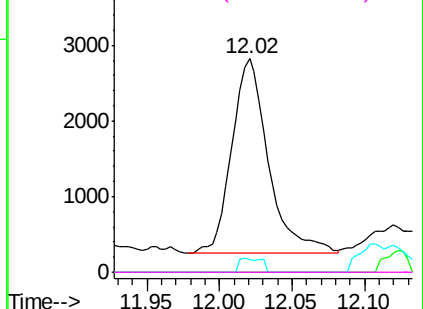

#76

1,2,3-Trichloropropane

Concen: 24.307 ug/l

RT: 12.40 min Scan# 3304

Delta R.T. -0.15 min

Lab File: VN060728.D


Acq: 26 Mar 2020 20:46

Tgt Ion: 75 Resp: 75002

Ion Ratio Lower Upper



75 100


77 1.2 0.0 0.0#

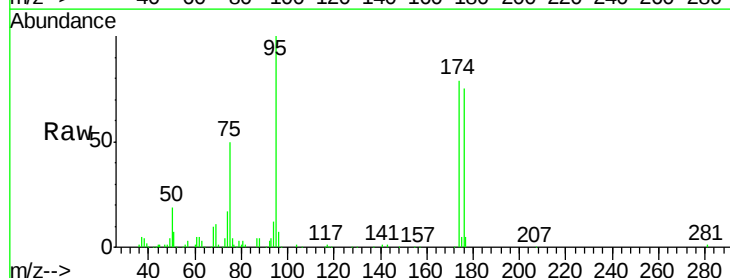

Abundance Ion 74.90 (74.60 to 75.60): VN0

Ion 77.00 (76.70 to 77.70): VN0



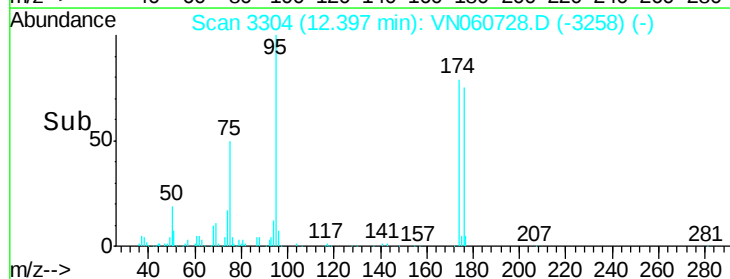
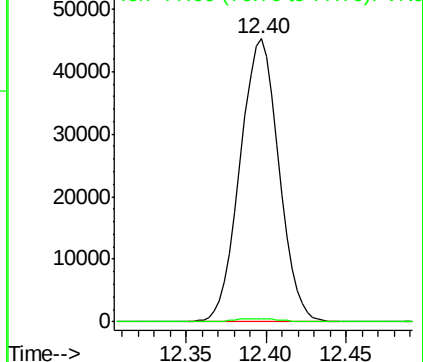


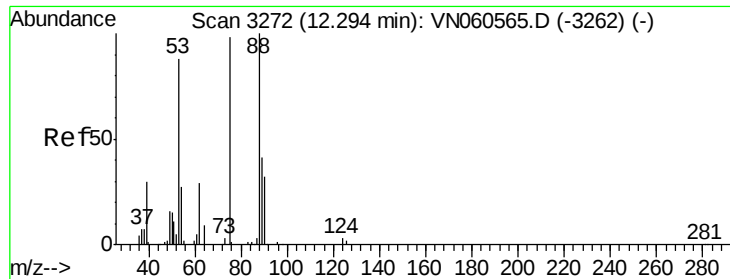

#81
trans-1,4-Dichloro-2-butene
Concen: 62.428 ug/l
RT: 12.40 min Scan# 3304
Delta R.T. 0.10 min
Lab File: VN060728.D
Acq: 26 Mar 2020 20:46

Instrument :
MSVOA_N
ClientSampleId :
SLUDGE-PIT

Tgt Ion: 75 Resp: 75002
Ion Ratio Lower Upper
75 100
53 0.0 73.0 109.4#
89 0.0 34.8 52.2#

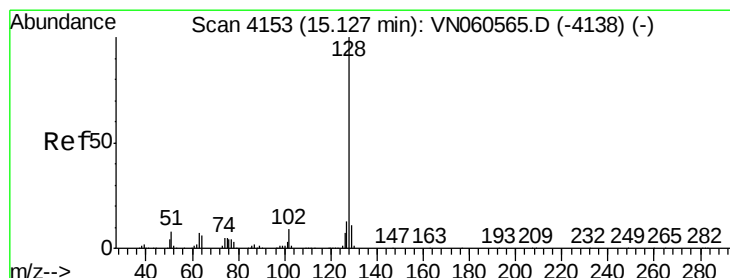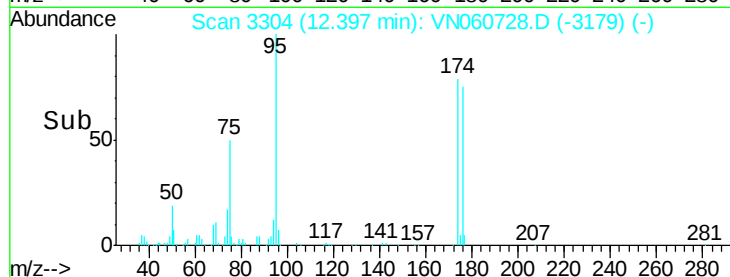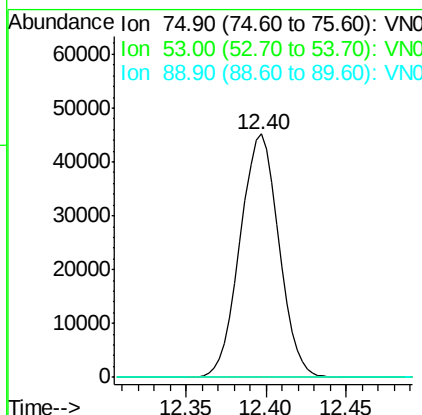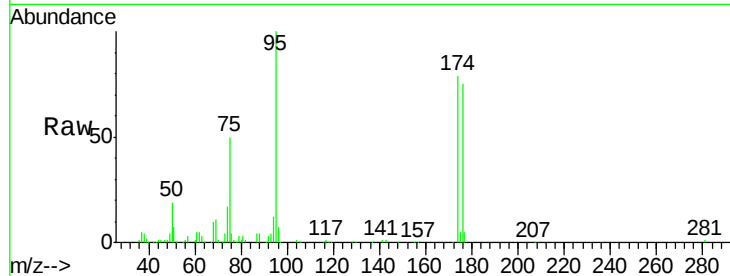

#95
Naphthalene
Concen: 0.206 ug/l
RT: 15.13 min Scan# 4154
Delta R.T. 0.00 min
Lab File: VN060728.D
Acq: 26 Mar 2020 20:46

Tgt Ion: 128 Resp: 1659
Ion Ratio Lower Upper
128 100
127 0.0 10.2 15.2#
129 0.0 8.8 13.2#

