


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN032620\
 Data File : VN060705.D
 Acq On : 26 Mar 2020 10:04
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N031820W.M
 Title : SW846 8260
 Last Update : Wed Mar 18 08:49:09 2020

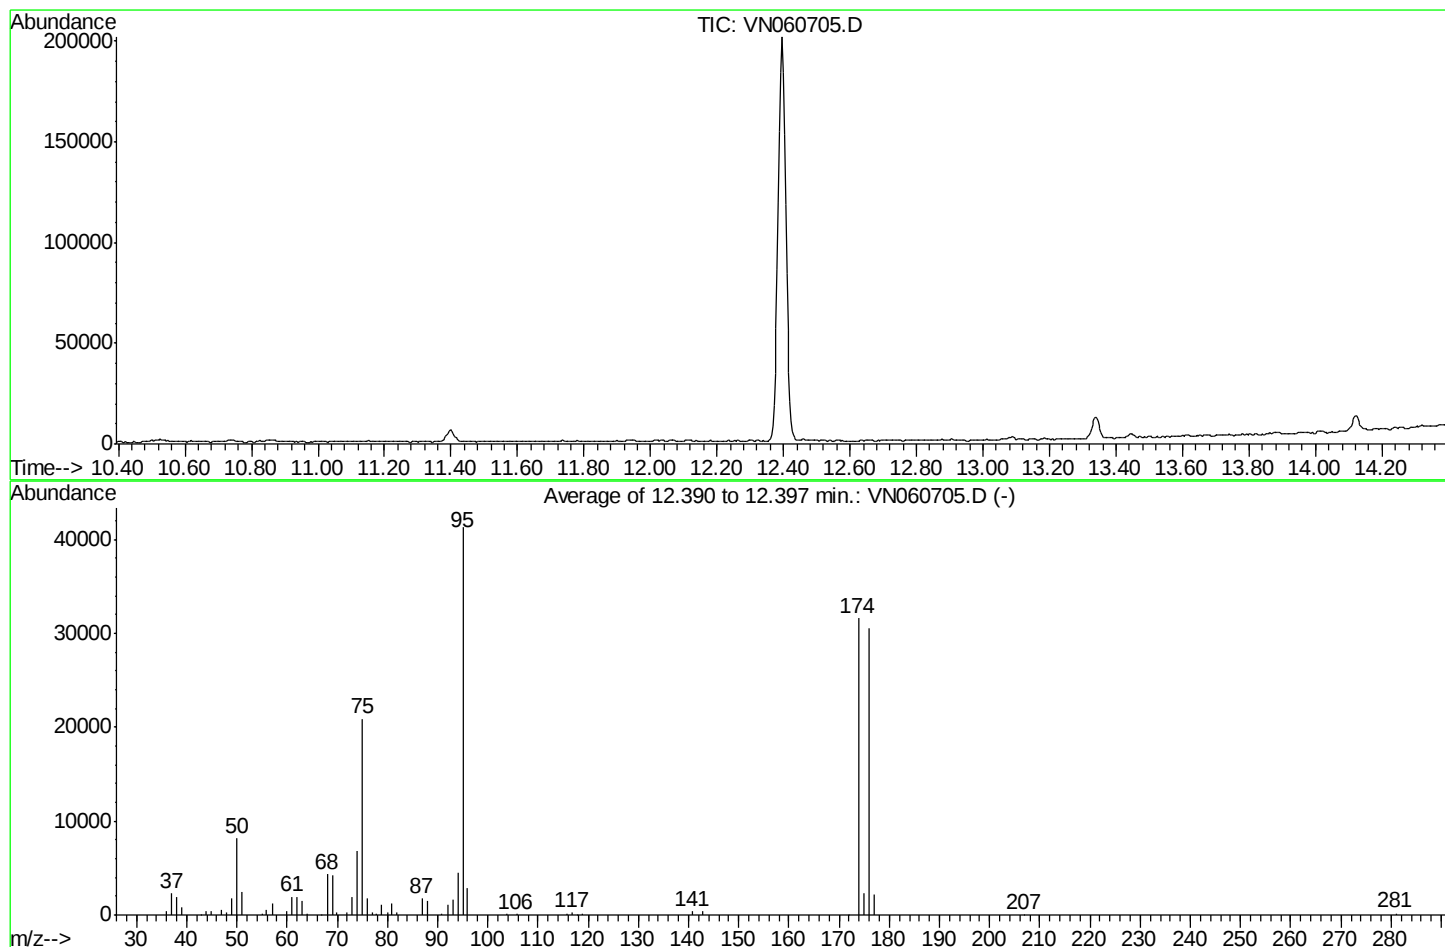

AutoFind: Scans 3302, 3303, 3304; Background Corrected with Scan 3289

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	8157	PASS
75	95	30	60	50.6	20882	PASS
95	95	100	100	100.0	41290	PASS
96	95	5	9	6.9	2838	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	76.5	31597	PASS
175	174	5	9	7.5	2363	PASS
176	174	95	101	96.5	30504	PASS
177	176	5	9	6.9	2118	PASS