

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032621\
 Data File : VN066352.D
 Acq On : 26 Mar 2021 16:22
 Operator : JC/MD
 Sample : M1788-02
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW201D-20210320

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N032521W.M

Title : SW846 8260

Signal : TIC: VN066352.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.389	252	261	263	rBV	24721	29006	1.15%	0.253%
2	7.507	2149	2169	2183	rBV	332602	823853	32.60%	7.174%
3	7.584	2184	2198	2225	rVB	533647	1252336	49.55%	10.905%
4	7.949	2311	2334	2358	rBV	383907	895087	35.42%	7.794%
5	8.515	2523	2545	2567	rBV	756787	1569146	62.09%	13.664%
6	8.764	2625	2638	2655	rVB4	28354	58976	2.33%	0.514%
7	10.028	3092	3109	3141	rBV	1389824	2527293	100.00%	22.007%
8	10.572	3301	3312	3323	rBV4	14989	26084	1.03%	0.227%
9	11.350	3585	3602	3628	rBV	1006785	1731867	68.53%	15.081%
10	12.345	3958	3973	3997	rBV2	808863	1402577	55.50%	12.213%
11	13.289	4309	4325	4366	rBV	576291	1167857	46.21%	10.169%




Sum of corrected areas: 11484082

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032621\
Data File : VN066352.D
Acq On : 26 Mar 2021 16:22
Operator : JC/MD
Sample : M1788-02
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW201D-20210320

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N032521W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

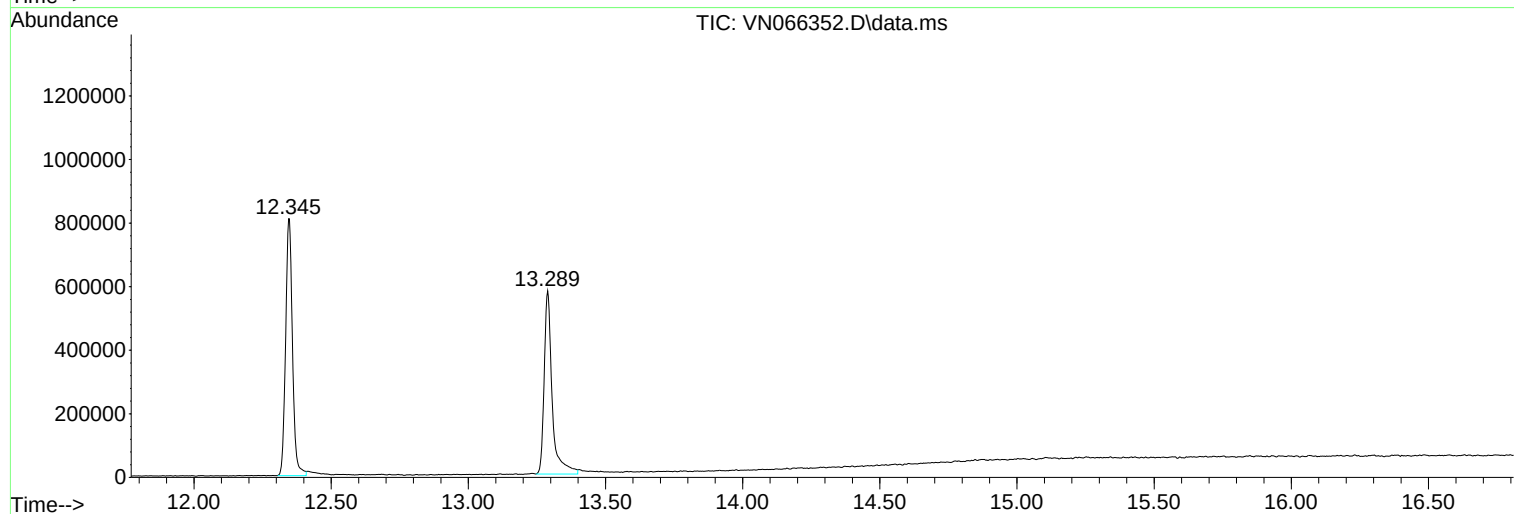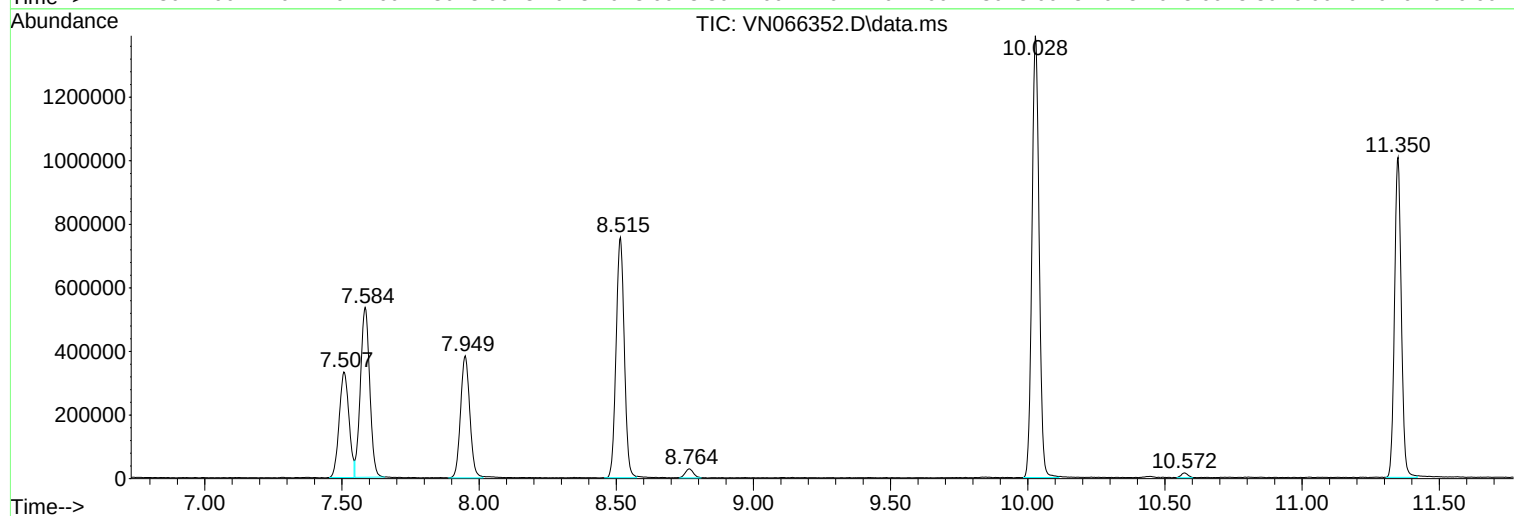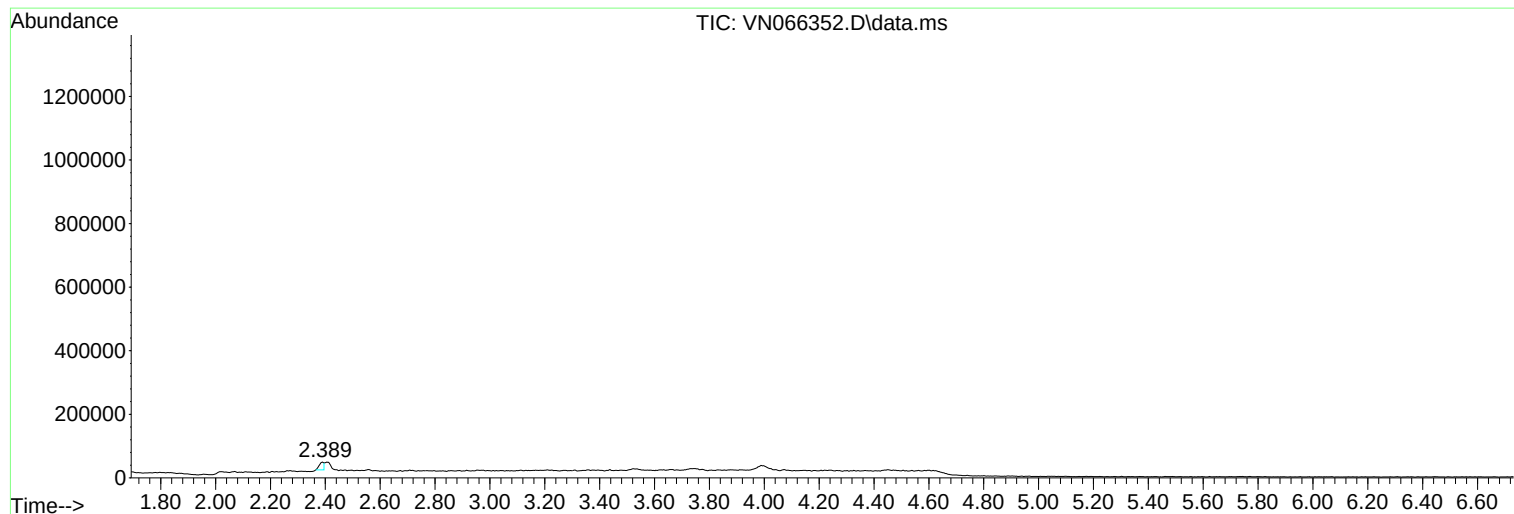

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032621\
Data File : VN066352.D
Acq On : 26 Mar 2021 16:22
Operator : JC/MD
Sample : M1788-02
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW201D-20210320

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N032521W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032621\
Data File : VN066352.D
Acq On : 26 Mar 2021 16:22
Operator : JC/MD
Sample : M1788-02
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW201D-20210320

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N032521W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
