
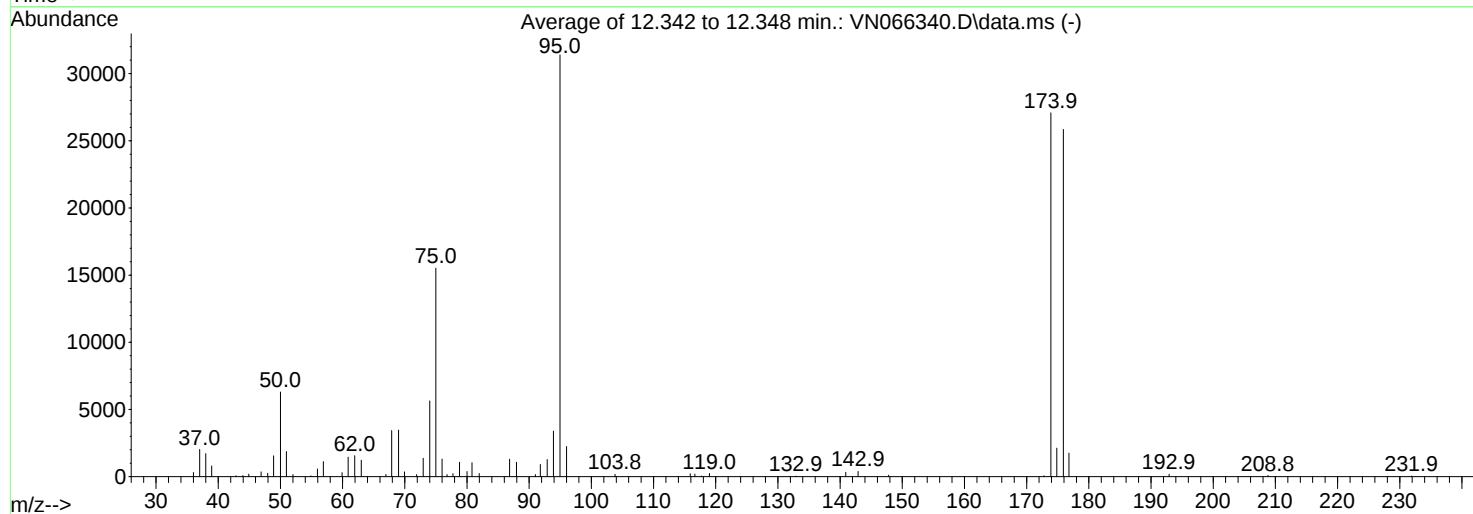


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032621\
 Data File : VN066340.D
 Acq On : 26 Mar 2021 8:50
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N032521W.M
 Title : SW846 8260
 Last Update : Fri Mar 26 16:26:01 2021

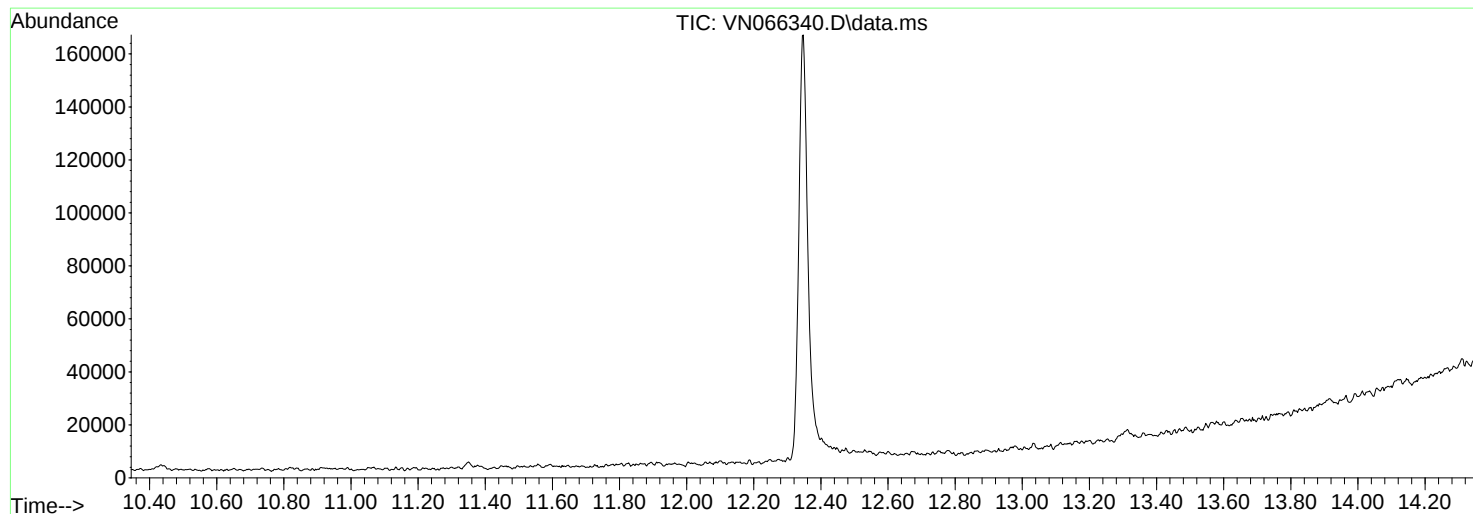

AutoFind: Scans 3972, 3973, 3974; Background Corrected with Scan 3957

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	6297	PASS
75	95	30	60	49.4	15525	PASS
95	95	100	100	100.0	31400	PASS
96	95	5	9	7.1	2240	PASS
173	174	0.00	2	0.3	68	PASS
174	95	50	100	86.3	27088	PASS
175	174	5	9	7.8	2125	PASS
176	174	95	101	95.4	25853	PASS
177	176	5	9	6.8	1757	PASS