

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032622\
 Data File : VN071592.D
 Acq On : 26 Mar 2022 23:04
 Operator : JC\MD
 Sample : N2109-02
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 TP-1

Quant Time: Mar 28 02:22:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N032522W.M
 Quant Title : SW846 8260
 QLast Update : Fri Mar 25 09:52:40 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.081	168	794834	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.963	114	1325716	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.739	117	1332076	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.674	152	500541	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.433	65	451285	45.700	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	91.400%		
35) Dibromofluoromethane	8.022	113	371668	44.609	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	89.220%		
50) Toluene-d8	10.439	98	1659452	49.379	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	98.760%		
62) 4-Bromofluorobenzene	12.727	95	568455	51.624	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	103.240%		
Target Compounds						
					Qvalue	
3) Chloromethane	2.304	50	3035	Below Cal	#	78
11) Tert butyl alcohol	5.322	59	3065	1.666	ug/l #	72
16) Acetone	4.287	43	23707	5.857	ug/l	99
20) Methylene Chloride	5.098	84	67933	7.203	ug/l	99
25) 2-Butanone	7.345	43	9617	1.481	ug/l #	80
29) Tetrahydrofuran	7.692	42	1317	0.305	ug/l #	50
31) Cyclohexane	8.086	56	14111	0.999	ug/l #	1
36) 1,1-Dichloropropene	8.086	75	53889	4.486	ug/l #	49
38) Carbon Tetrachloride	8.081	117	71939	6.143	ug/l #	17
43) Isopropyl Acetate	8.563	43	135062	6.095	ug/l #	75
45) 1,2-Dichloropropane	9.616	63	5644	0.609	ug/l #	44
48) Methyl methacrylate	9.539	41	18289	1.935	ug/l #	10
49) 1,4-Dioxane	9.616	88	772	3.539	ug/l #	1
51) 4-Methyl-2-Pentanone	10.327	43	9743	0.743	ug/l #	85
52) Toluene	10.504	92	28625	1.223	ug/l	97
54) cis-1,3-Dichloropropene	10.239	75	118373	8.079	ug/l #	60
57) 1,3-Dichloropropane	11.086	76	75495	4.729	ug/l #	42
59) 2-Hexanone	11.086	43	951501	100.684	ug/l #	47
67) Ethyl Benzene	11.845	91	17374	0.358	ug/l	94
68) m/p-Xylenes	11.945	106	21585	1.163	ug/l	89
69) o-Xylene	12.280	106	10292	0.558	ug/l	94
70) Styrene	12.292	104	30562	1.063	ug/l	86
71) Bromoform	12.727	173	2808	0.357	ug/l #	1
75) 1,1,2,2-Tetrachloroethane	12.727	83	406	Below Cal	#	1
76) 1,2,3-Trichloropropane	12.727	75	285955	25.620	ug/l #	1
78) n-propylbenzene	12.916	91	9932	0.212	ug/l	98
80) 1,3,5-Trimethylbenzene	13.051	105	7194	0.207	ug/l	90
81) trans-1,4-Dichloro-2-b...	12.727	75	285955	68.592	ug/l #	10
84) 1,2,4-Trimethylbenzene	13.368	105	24385	0.725	ug/l	94
95) Naphthalene	15.504	128	130512	8.008	ug/l	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032622\
Data File : VN071592.D
Acq On : 26 Mar 2022 23:04
Operator : JC\MD
Sample : N2109-02
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
TP-1

Quant Time: Mar 28 02:22:41 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N032522W.M
Quant Title : SW846 8260
QLast Update : Fri Mar 25 09:52:40 2022
Response via : Initial Calibration




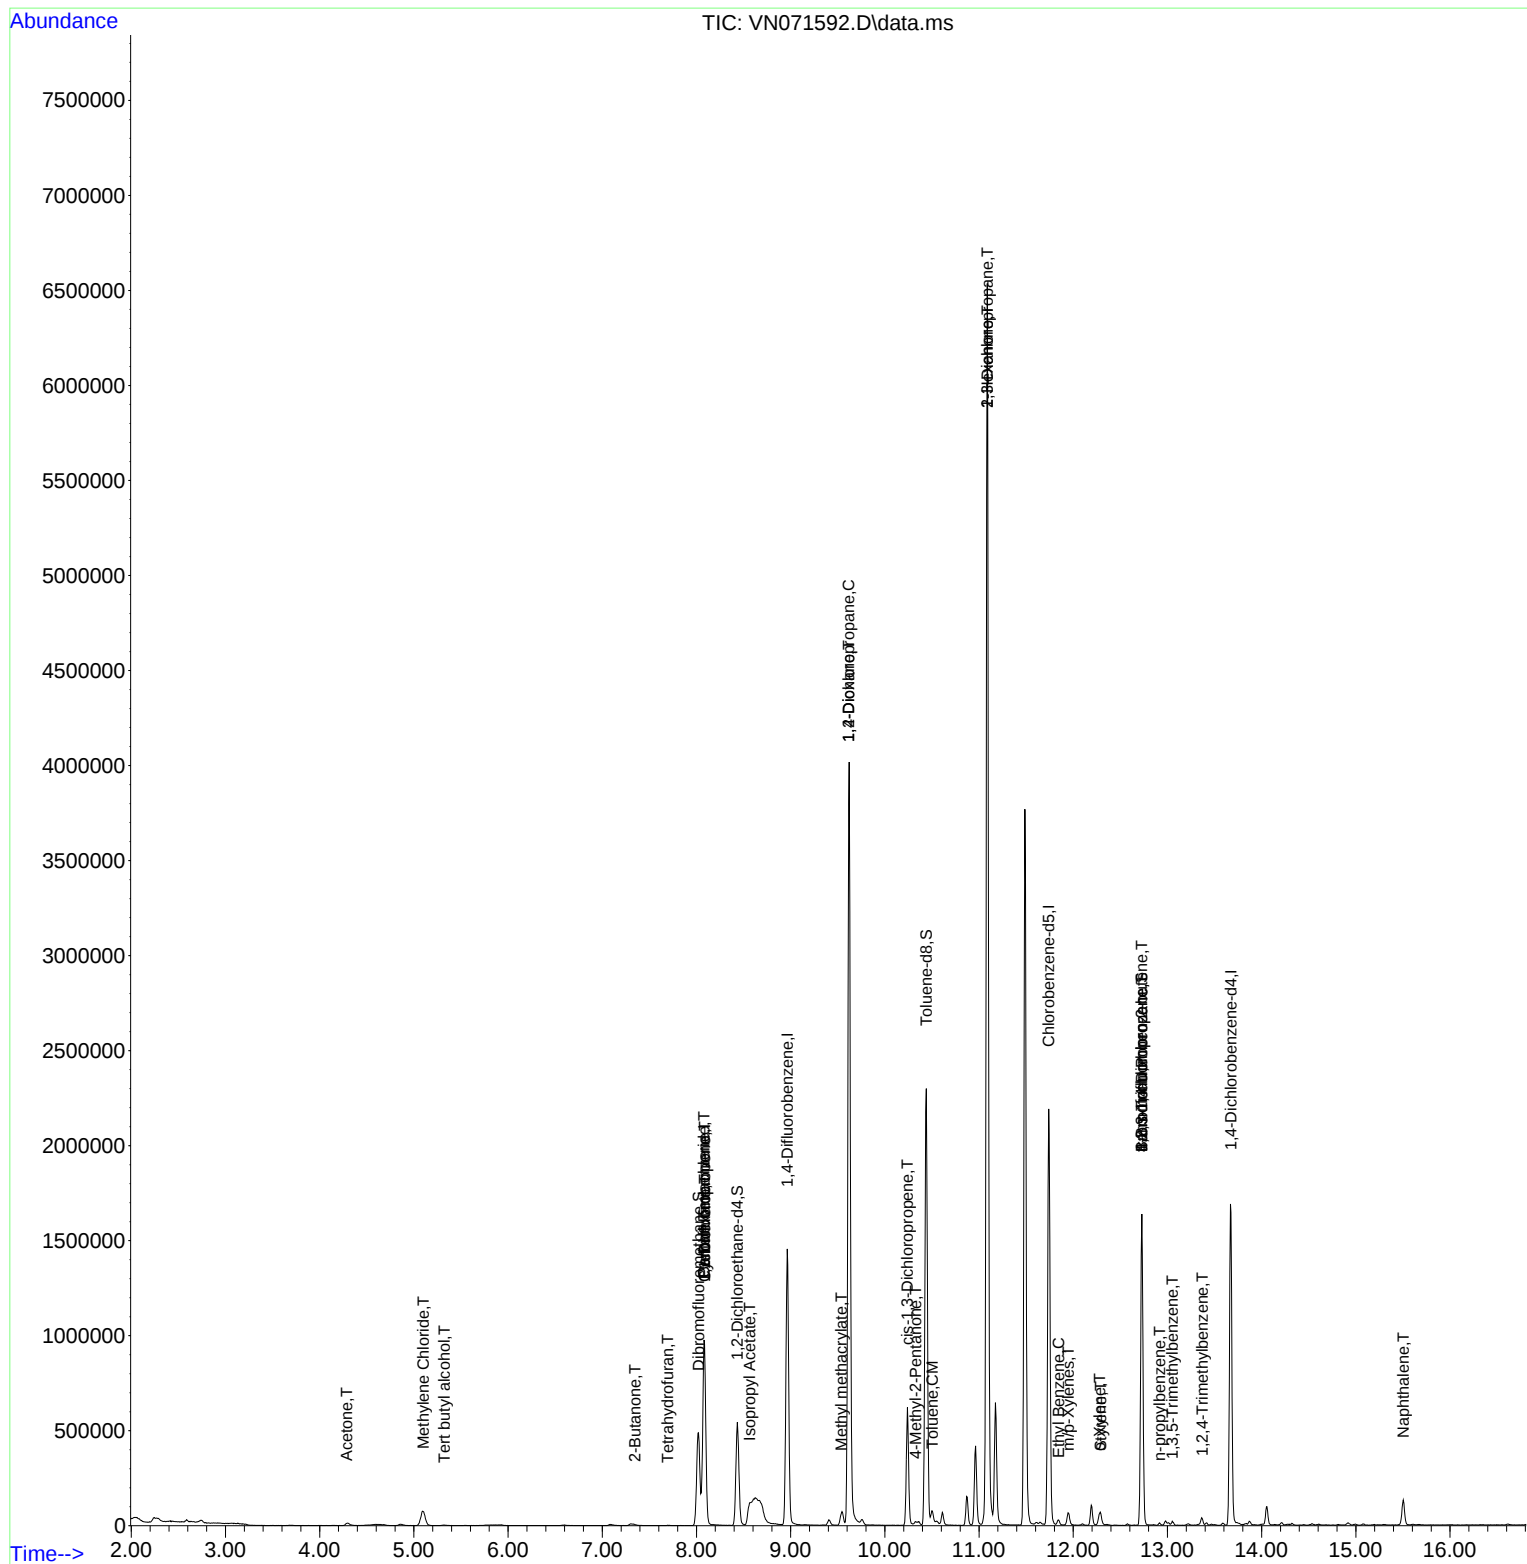




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.081 min Scan# 1036
Delta R.T. -0.000 min
Lab File: VN071592.D
Acq: 26 Mar 2022 23:04




Instrument :
MSVOA_N
ClientSampleId :
TP-1


Tgt Ion:168 Resp: 794834
Ion Ratio Lower Upper
168 100
99 52.4 42.3 63.5

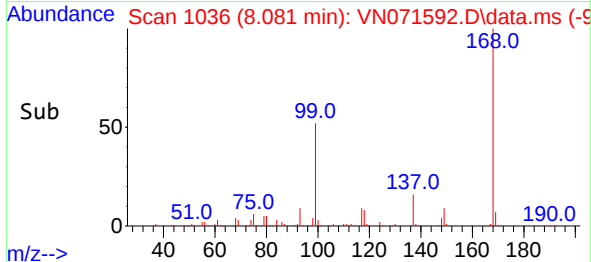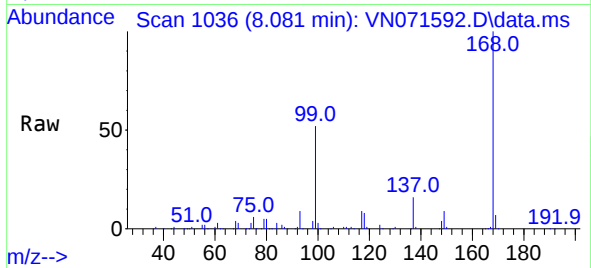

#3
Chloromethane
Concen: Below Cal
RT: 2.304 min Scan# 54
Delta R.T. 0.005 min
Lab File: VN071592.D
Acq: 26 Mar 2022 23:04

Tgt Ion: 50 Resp: 3035
Ion Ratio Lower Upper
50 100
52 20.0 25.7 38.5#


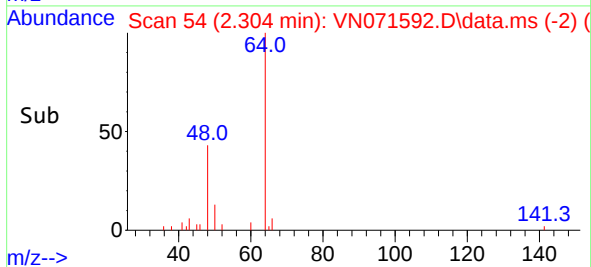

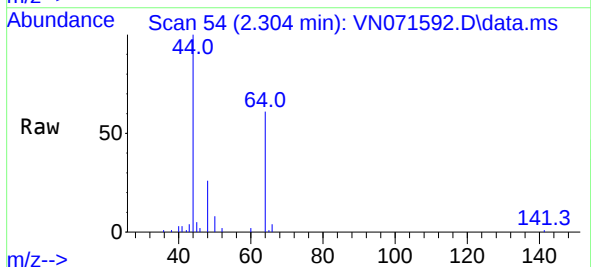




#11
Tert butyl alcohol
Concen: 1.666 ug/l
RT: 5.322 min Scan# 50
Delta R.T. -0.041 min
Lab File: VN071592.D
Acq: 26 Mar 2022 23:04




Instrument :
MSVOA_N
ClientSampleId :
TP-1


Tgt Ion: 59 Resp: 3065
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#



#16
Acetone
Concen: 5.857 ug/l
RT: 4.287 min Scan# 391
Delta R.T. 0.006 min
Lab File: VN071592.D
Acq: 26 Mar 2022 23:04

Tgt Ion: 43 Resp: 23707
Ion Ratio Lower Upper
43 100
58 31.8 26.0 39.0

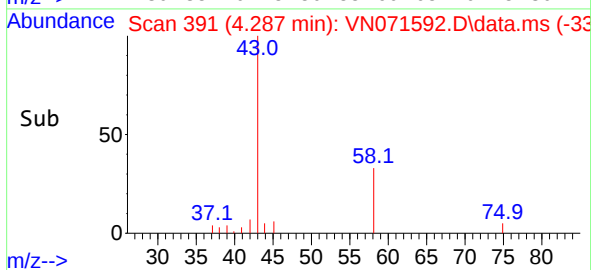







#20
Methylene Chloride
Concen: 7.203 ug/l
RT: 5.098 min Scan# 511
Delta R.T. 0.006 min
Lab File: VN071592.D
Acq: 26 Mar 2022 23:04

Instrument :
MSVOA_N
ClientSampleId :
TP-1

Tgt Ion: 84 Resp: 67933




Ion	Ratio	Lower	Upper
84	100		
49	109.5	88.3	132.5
51	35.6	28.2	42.2
86	63.3	50.6	76.0

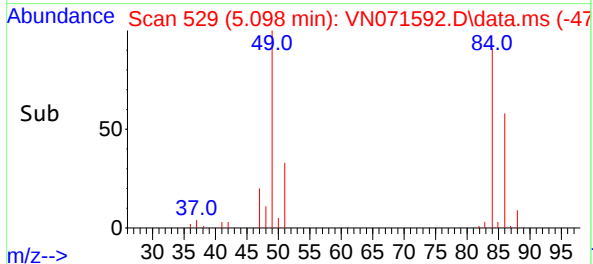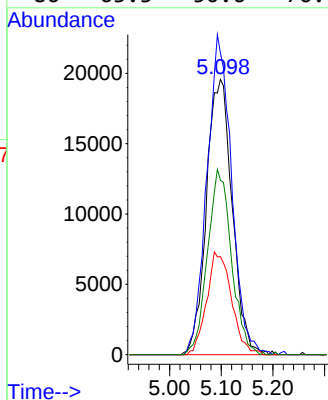


#25
2-Butanone
Concen: 1.481 ug/l
RT: 7.345 min Scan# 911
Delta R.T. 0.018 min
Lab File: VN071592.D
Acq: 26 Mar 2022 23:04

Tgt Ion: 43 Resp: 9617

Ion	Ratio	Lower	Upper
43	100		
72	19.1	23.7	35.5

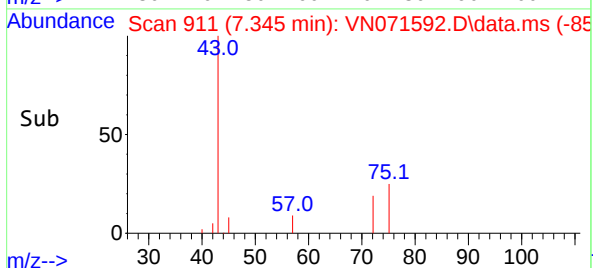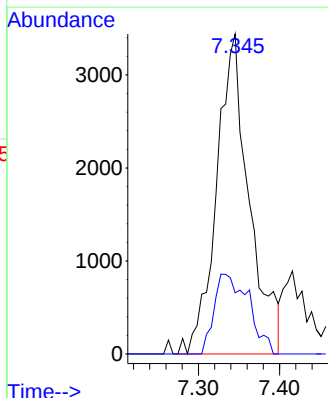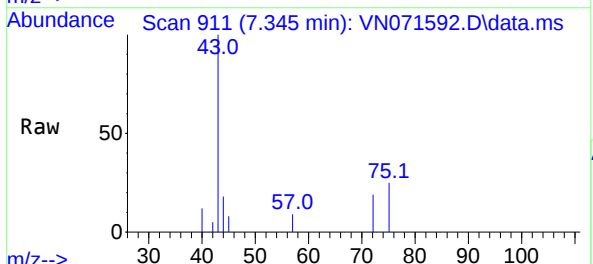



#29

Tetrahydrofuran

Concen: 0.305 ug/l

RT: 7.692 min Scan# 91

Delta R.T. 0.012 min

Lab File: VN071592.D

Acq: 26 Mar 2022 23:04

Instrument :

MSVOA_N

ClientSampleId :

TP-1





Tgt Ion: 42 Resp: 1317

Ion Ratio Lower Upper

42 100

72 15.3 39.7 59.5#

71 13.1 36.6 55.0#

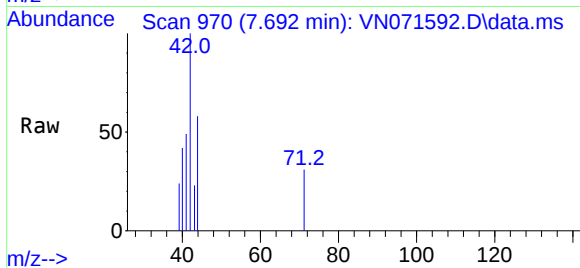

#31

Cyclohexane

Concen: 0.999 ug/l

RT: 8.086 min Scan# 1037

Delta R.T. -0.006 min

Lab File: VN071592.D

Acq: 26 Mar 2022 23:04




Tgt Ion: 56 Resp: 14111


Ion Ratio Lower Upper

56 100

69 167.5 27.8 41.8#

84 165.2 76.9 115.3#

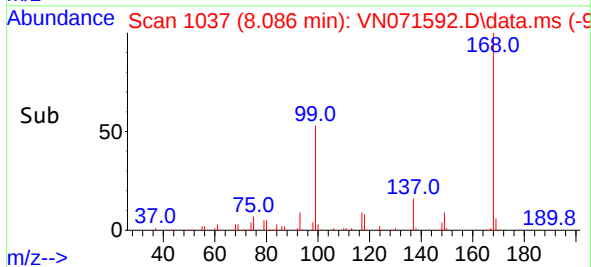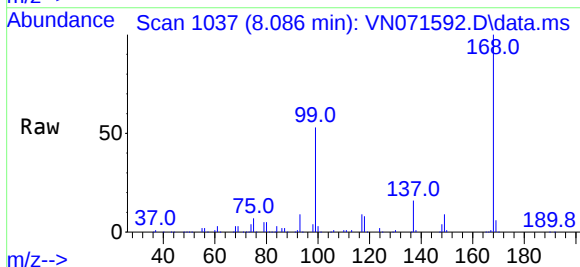



#33

1,2-Dichloroethane-d4

Concen: 45.700 ug/l

RT: 8.433 min Scan# 1096

Delta R.T. -0.000 min

Lab File: VN071592.D

Acq: 26 Mar 2022 23:04

Instrument :

MSVOA_N

ClientSampleId :





TP-1

Tgt Ion: 65 Resp: 451285

Ion Ratio Lower Upper

65 100

67 52.0 0.0 104.8

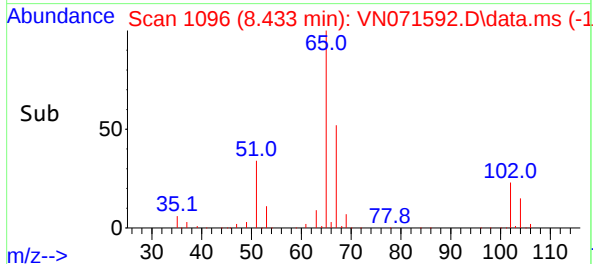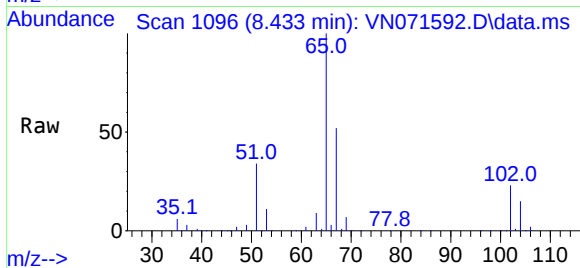

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.963 min Scan# 1186

Delta R.T. -0.000 min

Lab File: VN071592.D

Acq: 26 Mar 2022 23:04




Tgt Ion: 114 Resp: 1325716


Ion Ratio Lower Upper

114 100

63 19.2 0.0 40.0

88 15.6 0.0 32.6


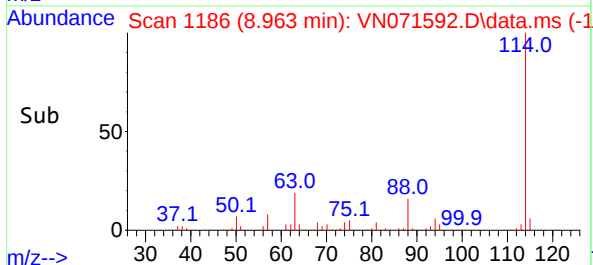
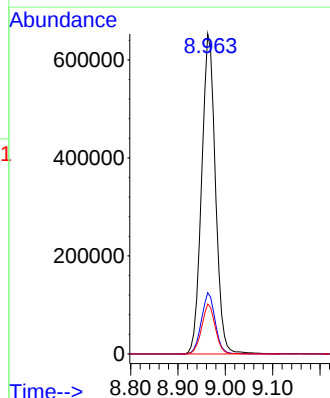
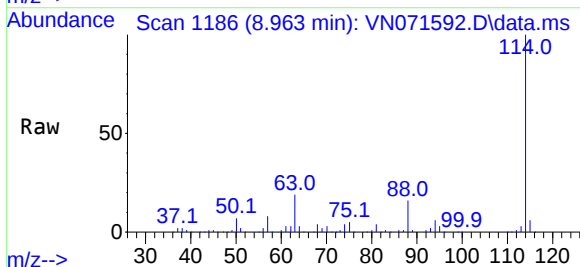




#35
Dibromofluoromethane
Concen: 44.609 ug/l
RT: 8.022 min Scan# 1026
Delta R.T. 0.006 min
Lab File: VN071592.D
Acq: 26 Mar 2022 23:04




Instrument :
MSVOA_N
ClientSampleId :
TP-1


Tgt Ion:113 Resp: 371668
Ion Ratio Lower Upper
113 100
111 102.1 81.4 122.0
192 21.6 17.0 25.6

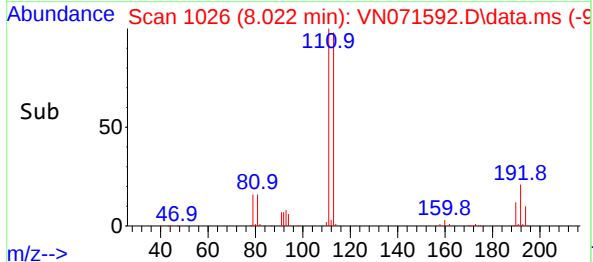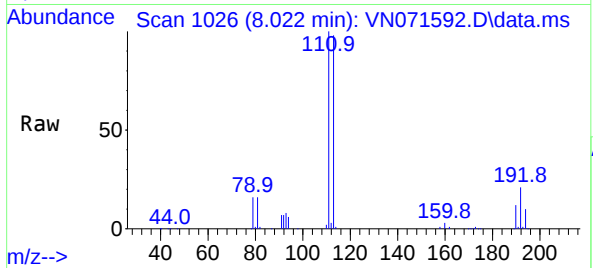

#36
1,1-Dichloropropene
Concen: 4.486 ug/l
RT: 8.086 min Scan# 1037
Delta R.T. -0.130 min
Lab File: VN071592.D
Acq: 26 Mar 2022 23:04

Tgt Ion: 75 Resp: 53889
Ion Ratio Lower Upper
75 100
110 9.1 18.3 54.8#
77 0.0 25.1 37.7#


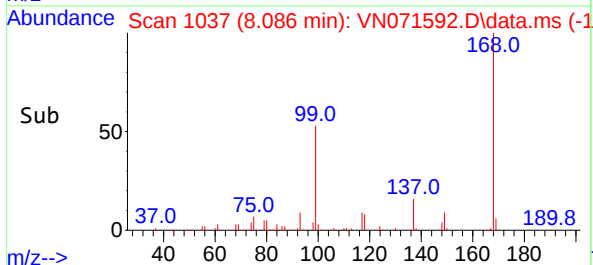
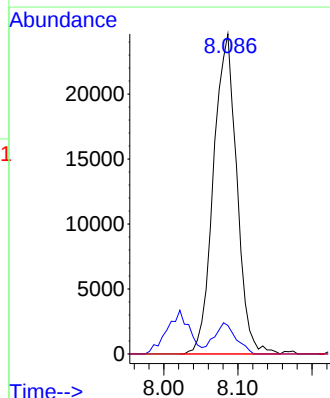
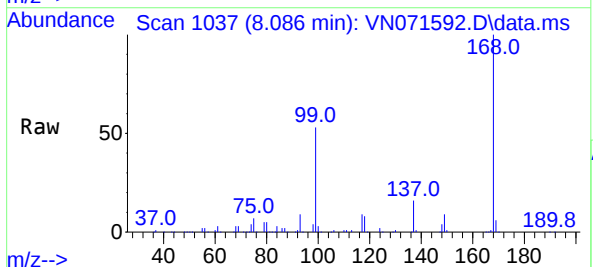




#38
Carbon Tetrachloride
Concen: 6.143 ug/l
RT: 8.081 min Scan# 1036
Delta R.T. -0.124 min
Lab File: VN071592.D
Acq: 26 Mar 2022 23:04




Instrument :
MSVOA_N
ClientSampleId :
TP-1


Tgt Ion:117 Resp: 71939
Ion Ratio Lower Upper
117 100
119 5.8 75.8 113.8#
121 0.0 24.6 37.0#

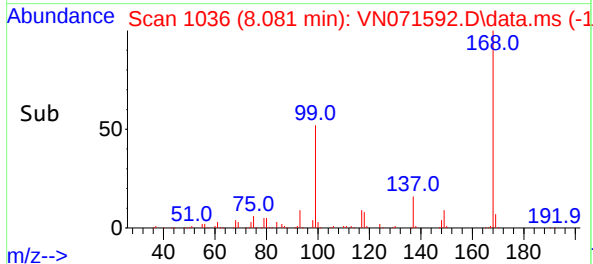

#43
Isopropyl Acetate
Concen: 6.095 ug/l
RT: 8.563 min Scan# 1118
Delta R.T. 0.006 min
Lab File: VN071592.D
Acq: 26 Mar 2022 23:04

Tgt Ion: 43 Resp: 135062
Ion Ratio Lower Upper
43 100
61 12.3 21.9 32.9#
87 7.5 12.0 18.0#

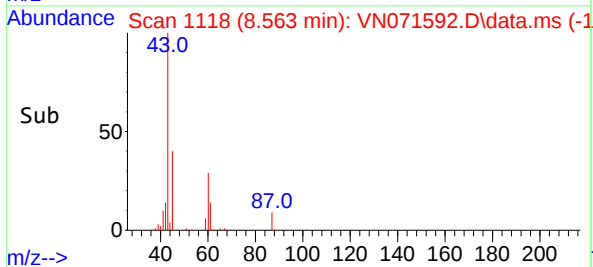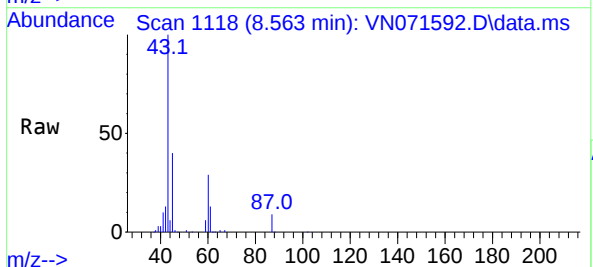



#45

1,2-Dichloropropane

Concen: 0.609 ug/l

RT: 9.616 min Scan# 11

Delta R.T. 0.129 min

Lab File: VN071592.D

Acq: 26 Mar 2022 23:04

Instrument :

MSVOA_N

ClientSampleId :





TP-1

Tgt Ion: 63 Resp: 5644

Ion Ratio Lower Upper

63 100

65 0.0 24.9 37.3#

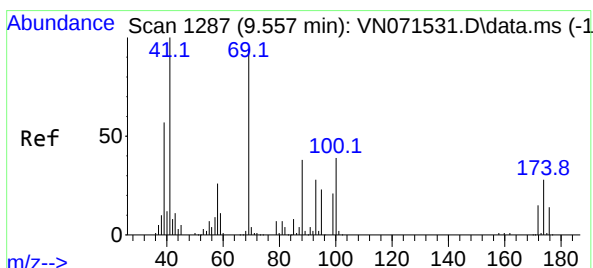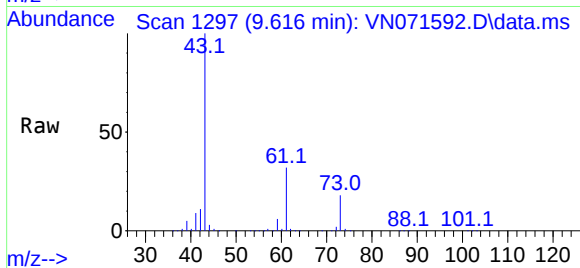

#48

Methyl methacrylate

Concen: 1.935 ug/l

RT: 9.539 min Scan# 1284

Delta R.T. -0.018 min

Lab File: VN071592.D

Acq: 26 Mar 2022 23:04




Tgt Ion: 41 Resp: 18289


Ion Ratio Lower Upper

41 100

69 0.0 74.7 112.1#

39 0.0 45.6 68.4#


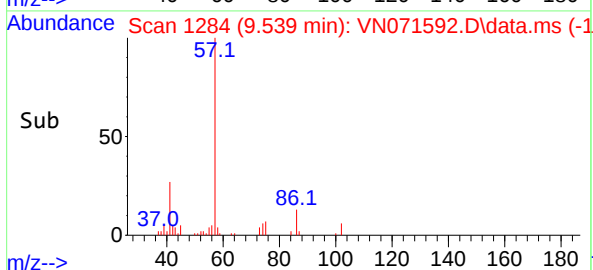

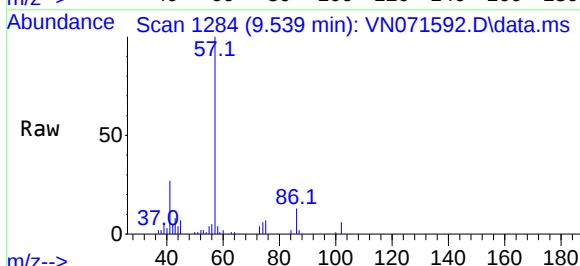


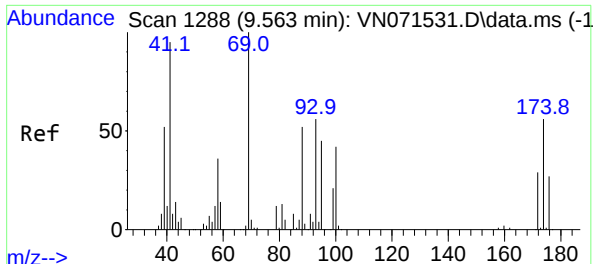

#49
1,4-Dioxane
Concen: 3.539 ug/l
RT: 9.616 min Scan# 1297
Delta R.T. 0.053 min
Lab File: VN071592.D
Acq: 26 Mar 2022 23:04




Instrument :
MSVOA_N
ClientSampleId :
TP-1


Tgt Ion: 88 Resp: 772
Ion Ratio Lower Upper
88 100
43 493014.5 20.2 30.4#
58 2130.4 54.2 81.4#

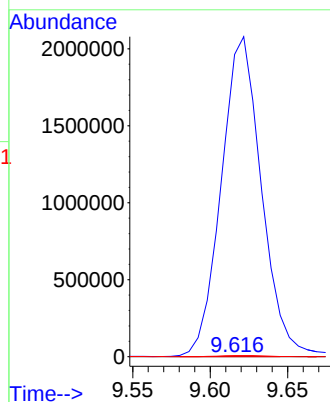

#50
Toluene-d8
Concen: 49.379 ug/l
RT: 10.439 min Scan# 1437
Delta R.T. -0.000 min
Lab File: VN071592.D
Acq: 26 Mar 2022 23:04

Tgt Ion: 98 Resp: 1659452
Ion Ratio Lower Upper
98 100
100 65.1 52.6 78.8


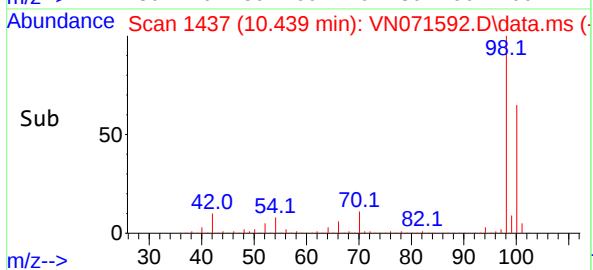
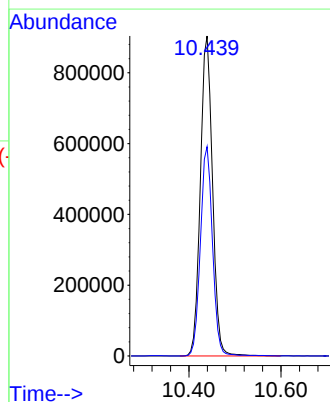
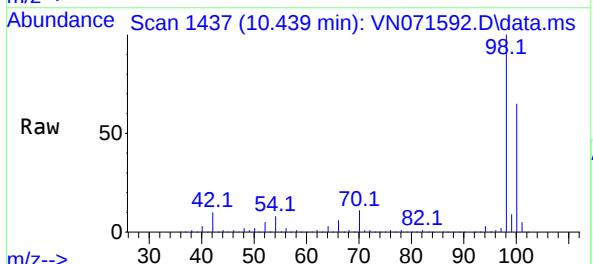




#51
4-Methyl-2-Pentanone
Concen: 0.743 ug/l
RT: 10.327 min Scan# 1418
Delta R.T. -0.000 min
Lab File: VN071592.D
Acq: 26 Mar 2022 23:04




Instrument :
MSVOA_N
ClientSampleId :
TP-1


Tgt Ion: 43 Resp: 9743
Ion Ratio Lower Upper
43 100
58 52.4 34.1 51.1#

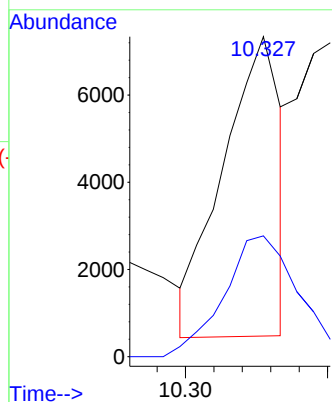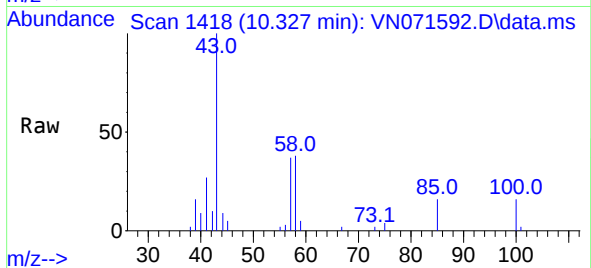

#52
Toluene
Concen: 1.223 ug/l
RT: 10.504 min Scan# 1448
Delta R.T. -0.000 min
Lab File: VN071592.D
Acq: 26 Mar 2022 23:04

Tgt Ion: 92 Resp: 28625
Ion Ratio Lower Upper
92 100
91 177.2 138.6 207.8


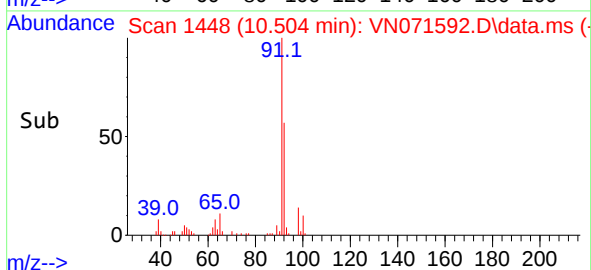






#54
cis-1,3-Dichloropropene
Concen: 8.079 ug/l
RT: 10.239 min Scan# 1403
Delta R.T. 0.053 min
Lab File: VN071592.D
Acq: 26 Mar 2022 23:04




Instrument :
MSVOA_N
ClientSampleId :
TP-1


Tgt Ion: 75 Resp: 118373
Ion Ratio Lower Upper
75 100
77 0.3 25.2 37.8#
39 26.3 35.7 53.5#

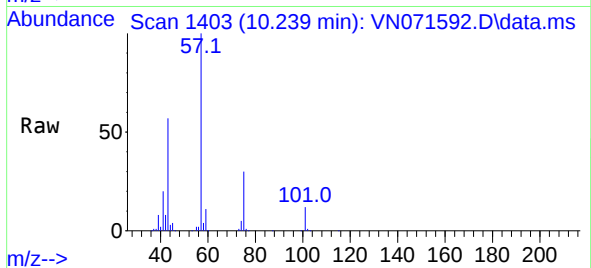

#57
1,3-Dichloropropane
Concen: 4.729 ug/l
RT: 11.086 min Scan# 1547
Delta R.T. 0.047 min
Lab File: VN071592.D
Acq: 26 Mar 2022 23:04

Tgt Ion: 76 Resp: 75495
Ion Ratio Lower Upper
76 100
78 0.3 26.2 39.2#


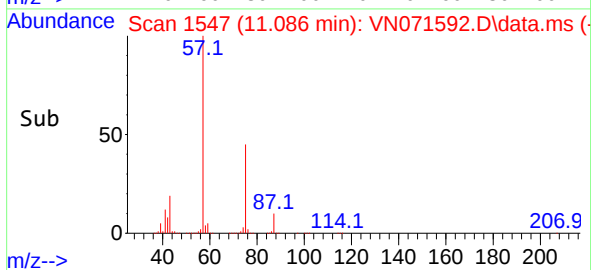






#59
2-Hexanone
Concen: 100.684 ug/l
RT: 11.086 min Scan# 1100
Delta R.T. 0.006 min
Lab File: VN071592.D
Acq: 26 Mar 2022 23:04




Instrument :
MSVOA_N
ClientSampleId :
TP-1


Tgt Ion: 43 Resp: 951501
Ion Ratio Lower Upper
43 100
58 19.6 29.7 89.1#

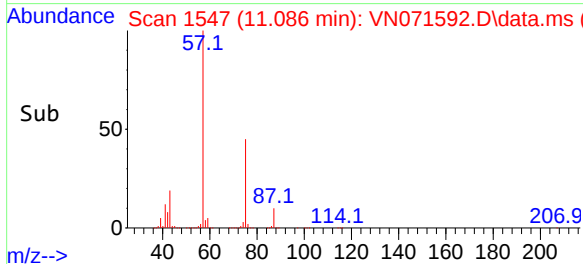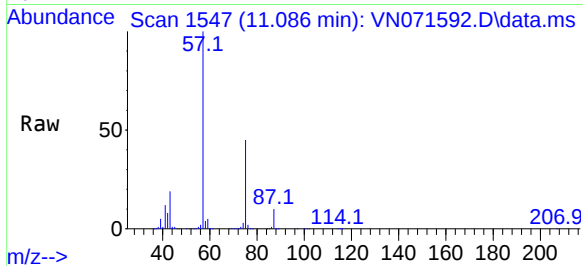

#62
4-Bromofluorobenzene
Concen: 51.624 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. -0.000 min
Lab File: VN071592.D
Acq: 26 Mar 2022 23:04

Tgt Ion: 95 Resp: 568455
Ion Ratio Lower Upper
95 100
174 85.1 0.0 167.6
176 82.2 0.0 163.4


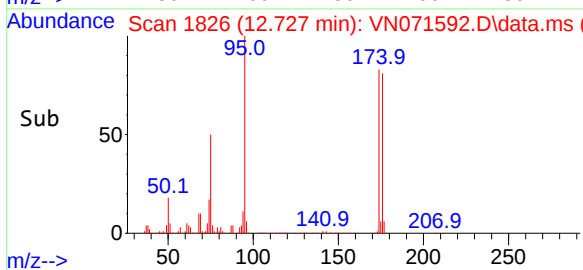

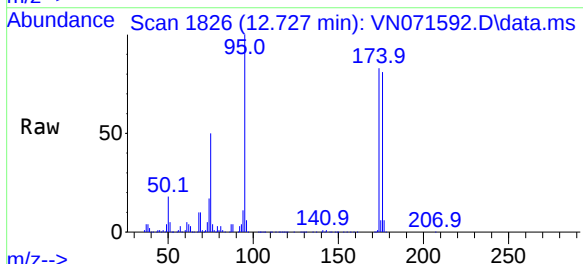




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.739 min Scan# 117
Delta R.T. -0.000 min
Lab File: VN071592.D
Acq: 26 Mar 2022 23:04




Instrument :
MSVOA_N
ClientSampleId :
TP-1


Tgt Ion:117 Resp: 1332076
Ion Ratio Lower Upper
117 100
82 54.0 44.2 66.2
119 32.0 25.4 38.0

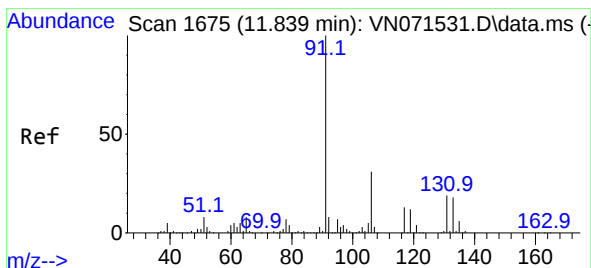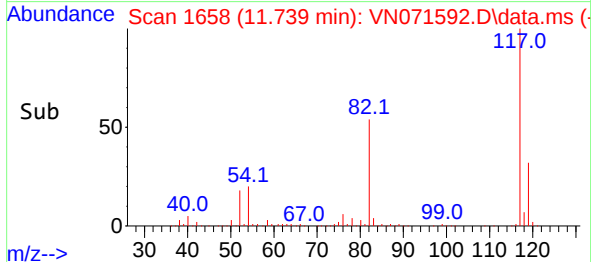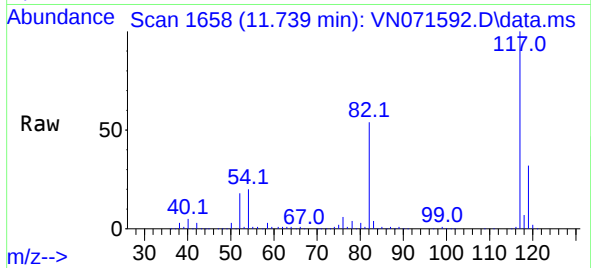

#67
Ethyl Benzene
Concen: 0.358 ug/l
RT: 11.845 min Scan# 1676
Delta R.T. 0.006 min
Lab File: VN071592.D
Acq: 26 Mar 2022 23:04

Tgt Ion: 91 Resp: 17374
Ion Ratio Lower Upper
91 100
106 34.4 24.9 37.3


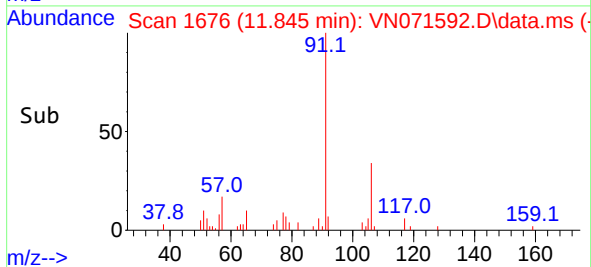

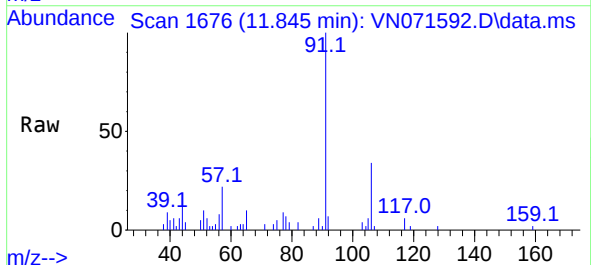




#68
m/p-Xylenes
Concen: 1.163 ug/l
RT: 11.945 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN071592.D
Acq: 26 Mar 2022 23:04




Instrument :
MSVOA_N
ClientSampleId :
TP-1


Tgt Ion:106 Resp: 21585
Ion Ratio Lower Upper
106 100
91 214.5 158.9 238.3



#69
o-Xylene
Concen: 0.558 ug/l
RT: 12.280 min Scan# 1750
Delta R.T. 0.006 min
Lab File: VN071592.D
Acq: 26 Mar 2022 23:04

Tgt Ion:106 Resp: 10292
Ion Ratio Lower Upper
106 100
91 201.9 106.0 318.0


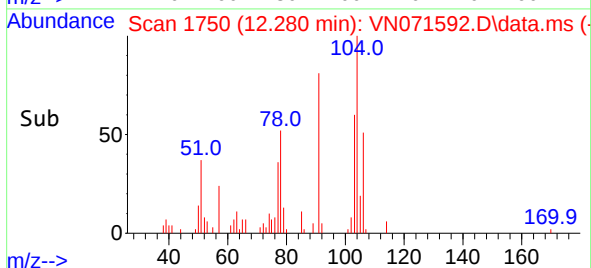






#70
Styrene
Concen: 1.063 ug/l
RT: 12.292 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN071592.D
Acq: 26 Mar 2022 23:04




Instrument :
MSVOA_N
ClientSampleId :
TP-1


Tgt Ion:104 Resp: 30562
Ion Ratio Lower Upper
104 100
78 39.9 39.5 59.3
103 45.2 44.0 66.0



#71
Bromoform
Concen: 0.357 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.270 min
Lab File: VN071592.D
Acq: 26 Mar 2022 23:04

Tgt Ion:173 Resp: 2808
Ion Ratio Lower Upper
173 100
175 945.3 24.6 73.6#
254 0.0 0.1 0.1#


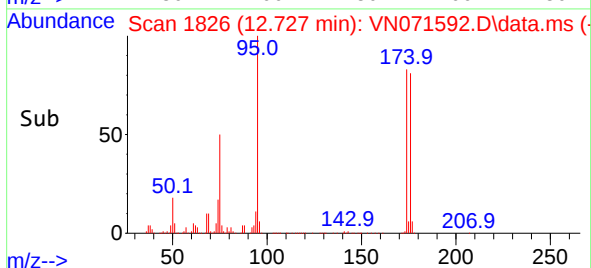
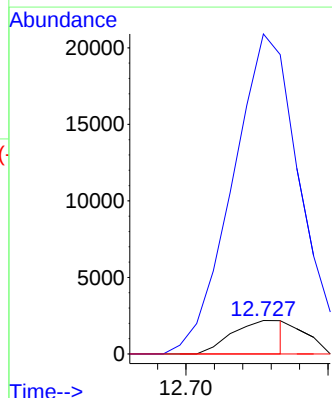





#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.674 min Scan# 1986
Delta R.T. 0.006 min
Lab File: VN071592.D
Acq: 26 Mar 2022 23:04




Instrument :
MSVOA_N
ClientSampleId :
TP-1


Tgt Ion:152 Resp: 500541
Ion Ratio Lower Upper
152 100
115 57.1 28.9 86.7
150 156.3 0.0 356.2



#75
1,1,2,2-Tetrachloroethane
Concen: Below Cal
RT: 12.727 min Scan# 1826
Delta R.T. -0.095 min
Lab File: VN071592.D
Acq: 26 Mar 2022 23:04

Tgt Ion: 83 Resp: 406
Ion Ratio Lower Upper
83 100
131 148.8 5.3 15.9#
85 0.0 32.3 96.9#


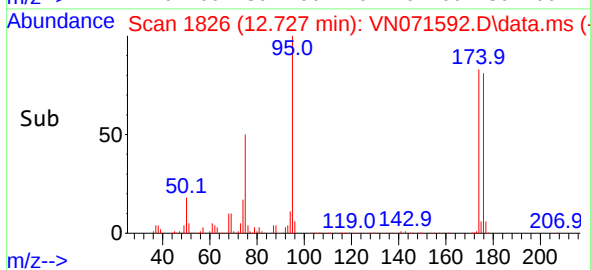






#76
1,2,3-Trichloropropane
Concen: 25.620 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. -0.147 min
Lab File: VN071592.D
Acq: 26 Mar 2022 23:04




Instrument :
MSVOA_N
ClientSampleId :
TP-1


Tgt Ion: 75 Resp: 285955
Ion Ratio Lower Upper
75 100
77 1.3 98.5 295.5#



#78
n-propylbenzene
Concen: 0.212 ug/l
RT: 12.916 min Scan# 1858
Delta R.T. -0.000 min
Lab File: VN071592.D
Acq: 26 Mar 2022 23:04

Tgt Ion: 91 Resp: 9932
Ion Ratio Lower Upper
91 100
120 22.5 11.9 35.5


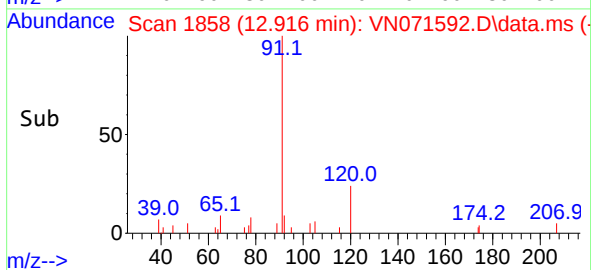






#80
1,3,5-Trimethylbenzene
Concen: 0.207 ug/l
RT: 13.051 min Scan# 1881
Delta R.T. -0.006 min
Lab File: VN071592.D
Acq: 26 Mar 2022 23:04




Instrument :
MSVOA_N
ClientSampleId :
TP-1


Tgt Ion:105 Resp: 7194
Ion Ratio Lower Upper
105 100
120 56.7 24.9 74.7

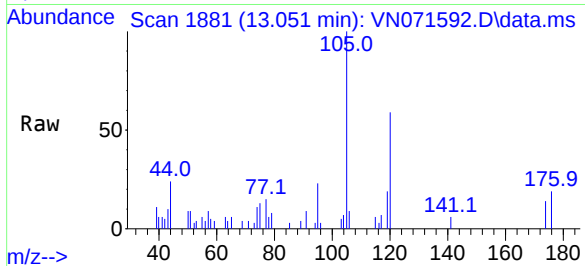

#81
trans-1,4-Dichloro-2-butene
Concen: 68.592 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.106 min
Lab File: VN071592.D
Acq: 26 Mar 2022 23:04

Tgt Ion: 75 Resp: 285955
Ion Ratio Lower Upper
75 100
53 0.0 78.0 117.0#
89 0.0 37.2 55.8#


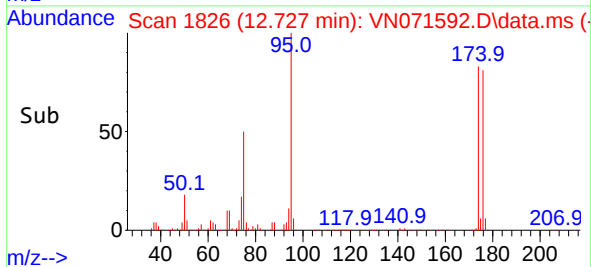

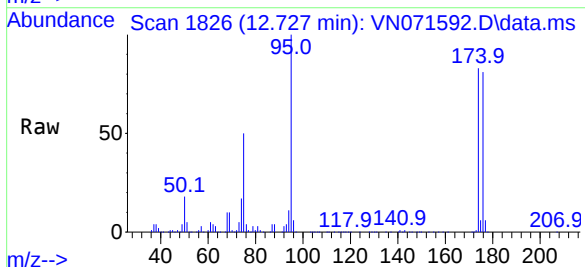




#84
1,2,4-Trimethylbenzene
Concen: 0.725 ug/l
RT: 13.368 min Scan# 1934
Delta R.T. 0.006 min
Lab File: VN071592.D
Acq: 26 Mar 2022 23:04

Instrument :
MSVOA_N
ClientSampleId :
TP-1

Tgt Ion:105 Resp: 24385
Ion Ratio Lower Upper
105 100
120 42.3 23.3 69.8

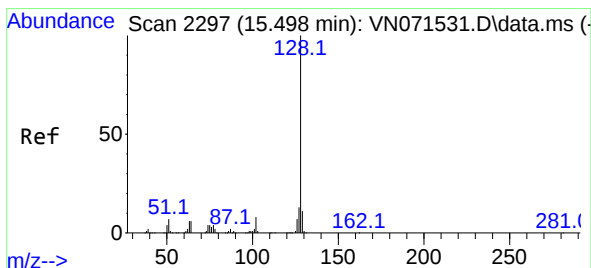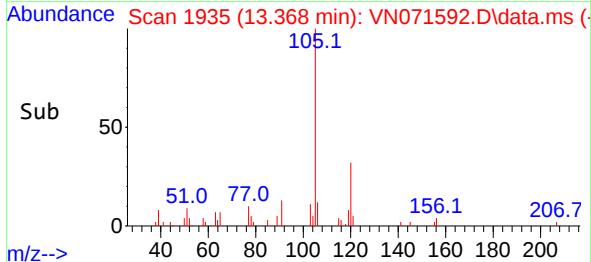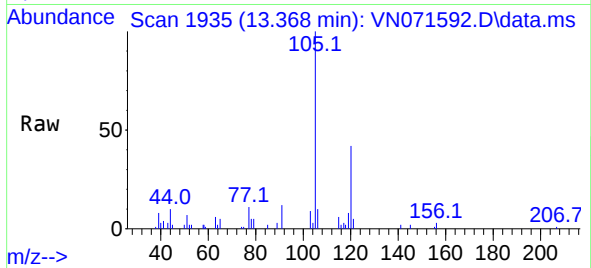

#95
Naphthalene
Concen: 8.008 ug/l
RT: 15.504 min Scan# 2298
Delta R.T. 0.006 min
Lab File: VN071592.D
Acq: 26 Mar 2022 23:04

Tgt Ion:128 Resp: 130512
Ion Ratio Lower Upper
128 100
127 13.1 10.3 15.5
129 10.7 8.6 13.0

