
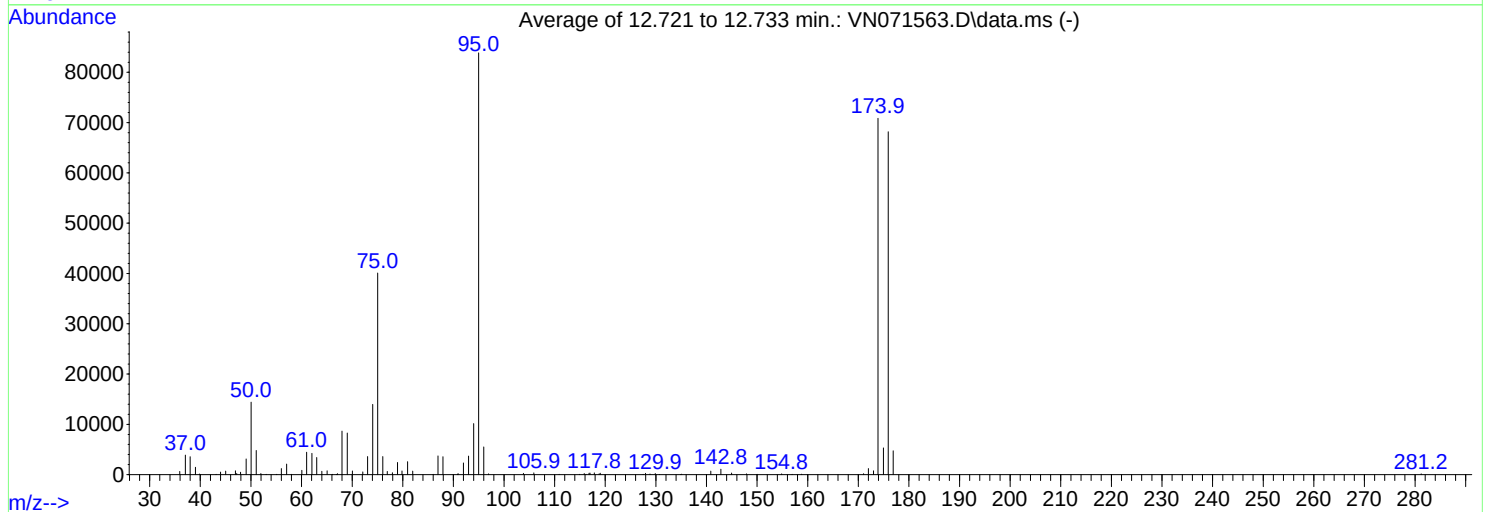


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032622\
 Data File : VN071563.D
 Acq On : 26 Mar 2022 09:31
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N032422W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Thu Mar 24 12:03:44 2022

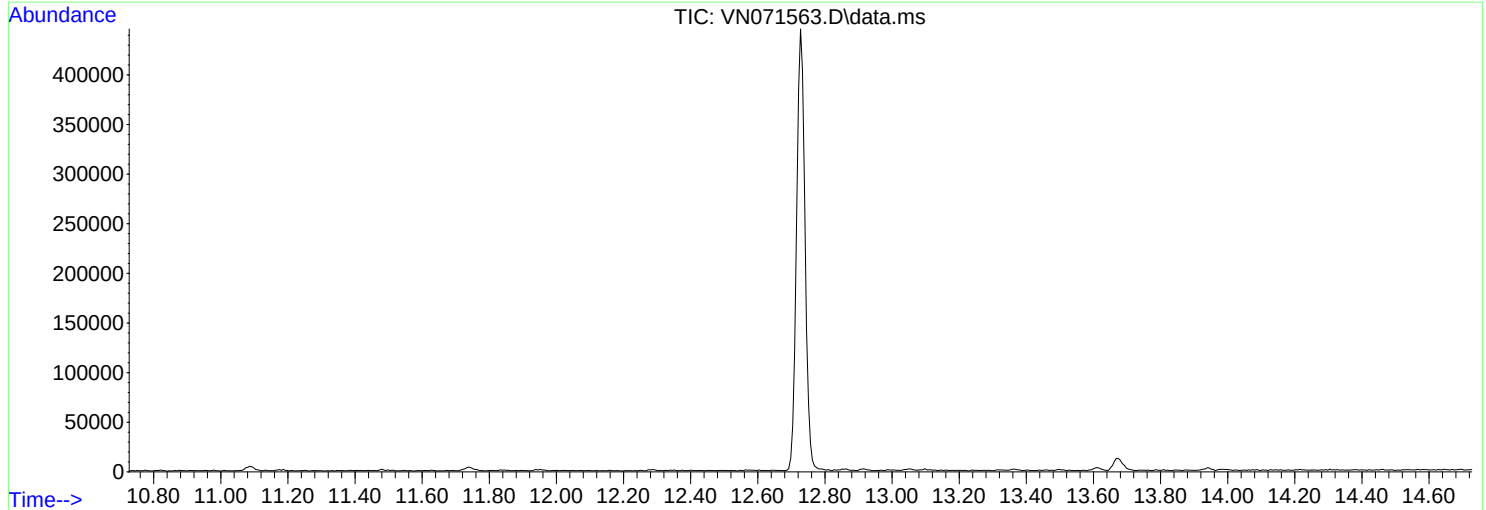

AutoFind: Scans 1825, 1826, 1827; Background Corrected with Scan 1817

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	14407	PASS
75	95	30	60	47.8	40072	PASS
95	95	100	100	100.0	83869	PASS
96	95	5	9	6.6	5499	PASS
173	174	0.00	2	1.1	763	PASS
174	95	50	100	84.5	70853	PASS
175	174	5	9	7.5	5329	PASS
176	174	95	101	96.2	68171	PASS
177	176	5	9	7.0	4759	PASS