
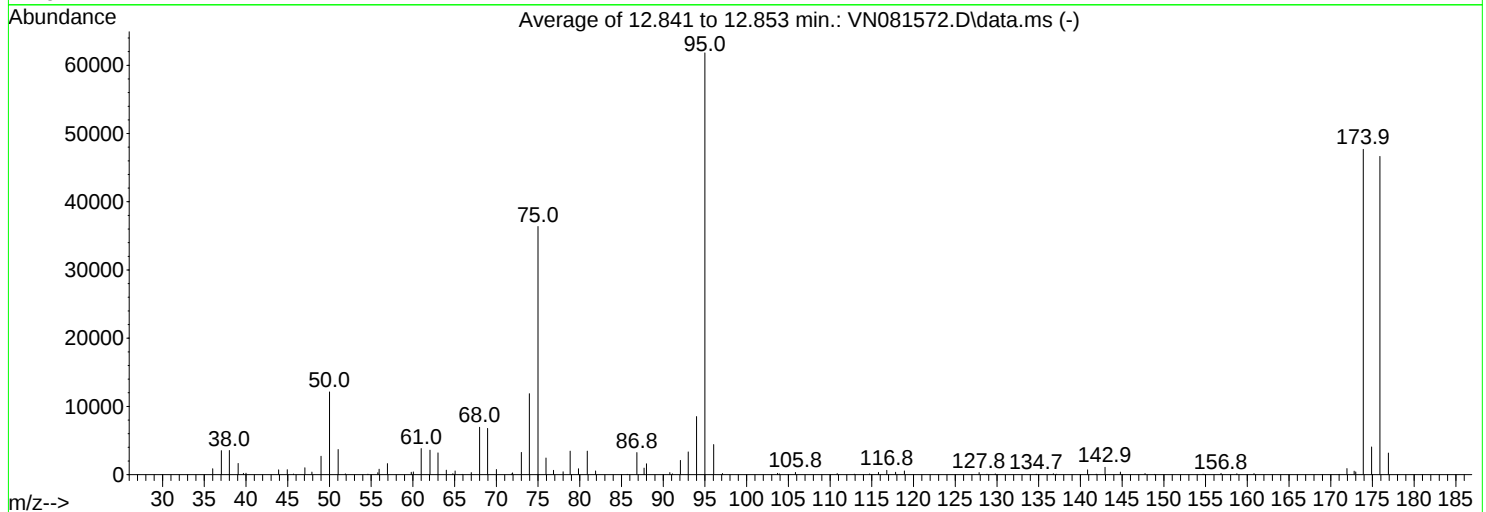


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032624\
Data File : VN081572.D
Acq On : 26 Mar 2024 08:35
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031824W.M
Title : SW846 8260
Last Update : Tue Mar 19 06:00:00 2024

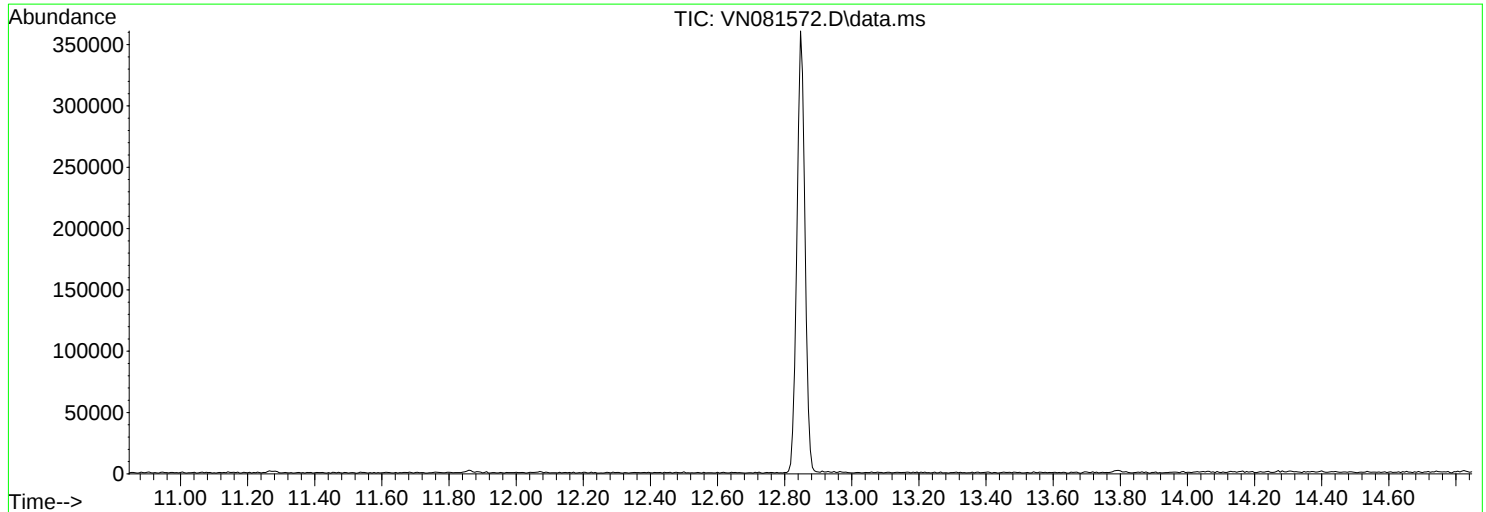

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.6	12117	PASS
75	95	30	60	58.8	36373	PASS
95	95	100	100	100.0	61827	PASS
96	95	5	9	7.1	4410	PASS
173	174	0.00	2	1.1	516	PASS
174	95	50	100	77.1	47691	PASS
175	174	5	9	8.5	4055	PASS
176	174	95	101	97.8	46656	PASS
177	176	5	9	6.8	3178	PASS

Average of 12.841 to 12.853 min.: VN081572.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	878	49.00	2701	62.05	3599	71.95	261
37.05	3510	50.00	12117	63.00	3185	73.00	326
38.00	3543	51.05	3687	64.00	656	73.95	1186
39.05	1633	51.90	125	64.80	143	75.00	3637
39.70	195	54.60	71	65.05	542	75.95	2440
40.00	208	55.80	280	65.90	51	76.85	640
43.90	695	55.95	801	67.00	296	78.00	435
44.95	724	56.95	1614	68.00	6945	78.85	3447
45.70	88	59.80	361	68.95	6783	79.85	881
47.05	1017	60.05	397	70.00	748	80.90	3446
47.90	382	61.00	3814	71.80	86	81.90	537

Average of 12.841 to 12.853 min.: VN081572.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
85.70	59	97.10	155	127.85	300	148.90	57
86.85	3247	103.70	193	128.80	62	154.70	79
87.70	955	103.90	129	129.80	124	154.90	55
88.00	1598	105.85	332	134.70	65	156.85	187
90.80	301	110.85	155	136.75	146	158.75	146
91.10	121	112.90	82	137.10	68	160.80	154
92.05	2080	114.75	118	140.85	713	171.00	58
93.00	3323	115.80	333	141.90	67	171.95	902
94.00	8519	116.80	644	142.95	1085	172.80	516
95.00	61827	117.85	349	144.80	377	173.00	404
96.05	4410	118.90	548	147.75	174	173.90	47691

Average of 12.841 to 12.853 min.: VN081572.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
174.90	4055						
175.90	46656						
176.90	3178						

Instrument :

MSVOA_N

ClientSampleId :

BFB