


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032625\
Data File : VN086117.D
Acq On : 26 Mar 2025 10:50
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031825W.M
Title : SW846 8260
Last Update : Wed Mar 19 03:20:56 2025

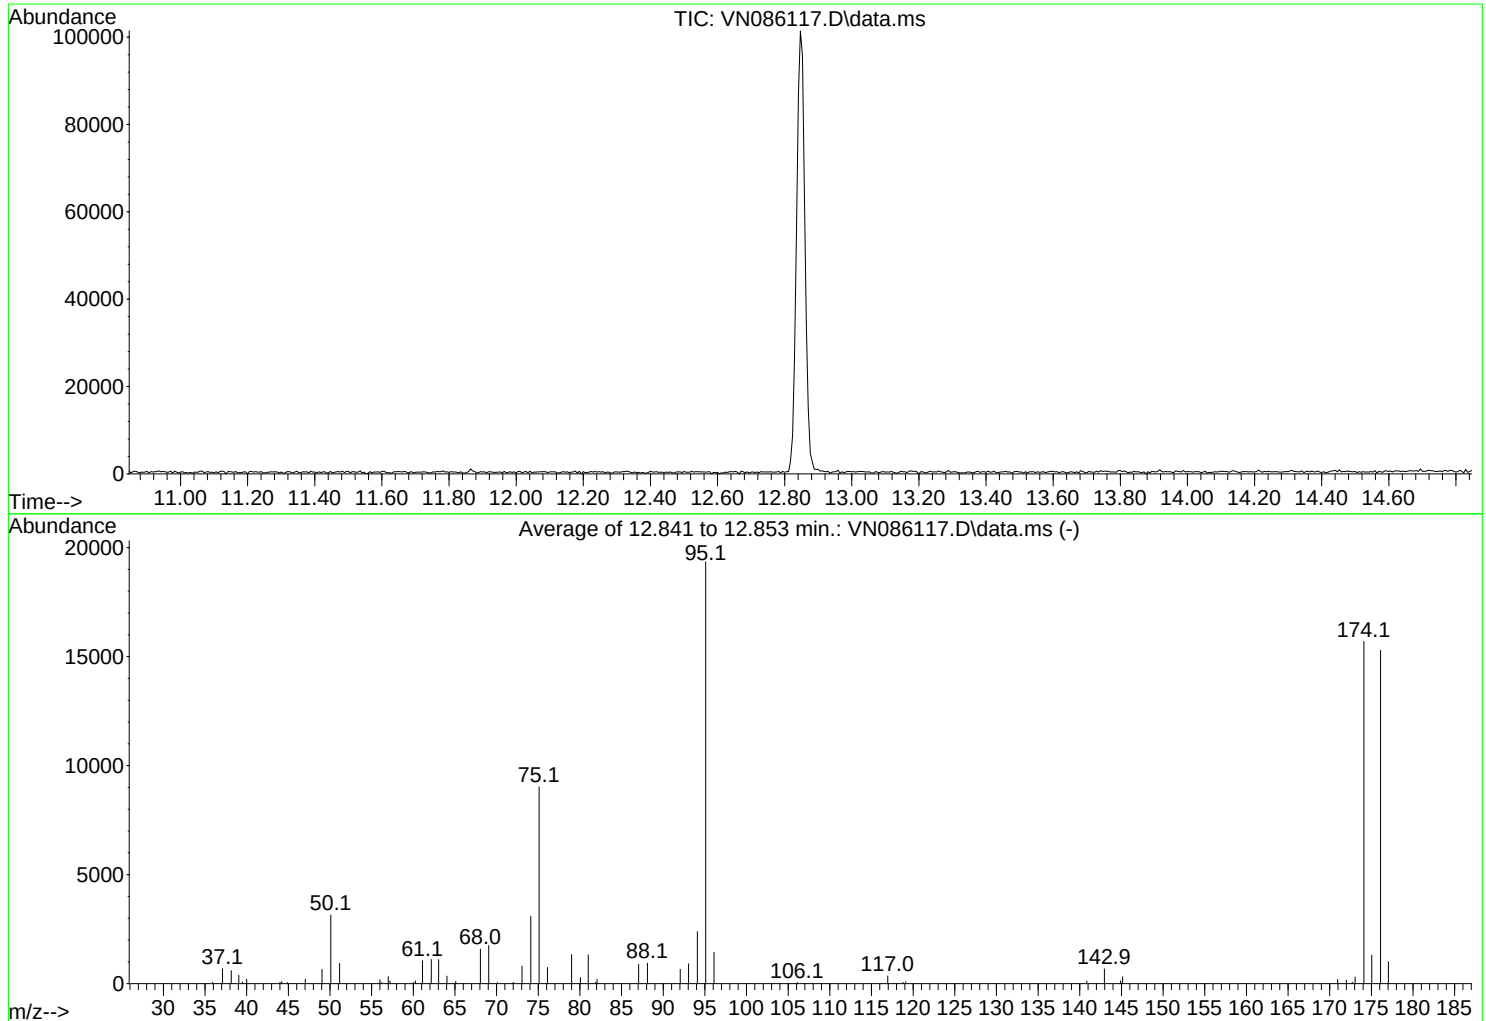

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.3	3149	PASS
75	95	30	60	46.7	9030	PASS
95	95	100	100	100.0	19347	PASS
96	95	5	9	7.4	1431	PASS
173	174	0.00	2	1.9	301	PASS
174	95	50	100	81.1	15695	PASS
175	174	5	9	8.3	1304	PASS
176	174	95	101	97.4	15289	PASS
177	176	5	9	6.6	1003	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	61	50.10	3149	64.05	346	80.05	261
37.10	682	51.15	934	65.10	106	81.00	132
38.15	597	56.00	175	68.05	1582	81.90	6
39.05	388	56.20	54	69.05	1749	82.05	19
39.50	75	57.00	321	70.10	51	87.05	879
40.00	209	57.20	114	72.00	59	88.10	940
44.00	59	60.00	63	73.05	811	92.05	651
44.20	92	60.25	128	74.10	3092	93.05	908
44.90	55	61.10	1050	75.10	9030	94.10	2386
47.05	209	62.15	1110	76.10	738	95.10	19347
49.05	656	63.05	1099	79.00	1331	96.10	1431

Average of 12.841 to 12.853 min.: VN086117.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
106.10	57	173.05	301				
116.95	353	174.10	15695				
118.80	58	175.05	1304				
119.10	86	176.10	15289				
140.85	126	177.05	1003				
142.95	678						
144.90	122						
145.15	314						
170.95	188						
172.00	159						
172.70	72						

Instrument :

MSVOA_N

ClientSampleId :

BFB