


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN032719\
 Data File : VN054707.D
 Acq On : 27 Mar 2019 8:34
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N032019W.M
 Title : SW846 8260
 Last Update : Fri Mar 22 02:09:07 2019

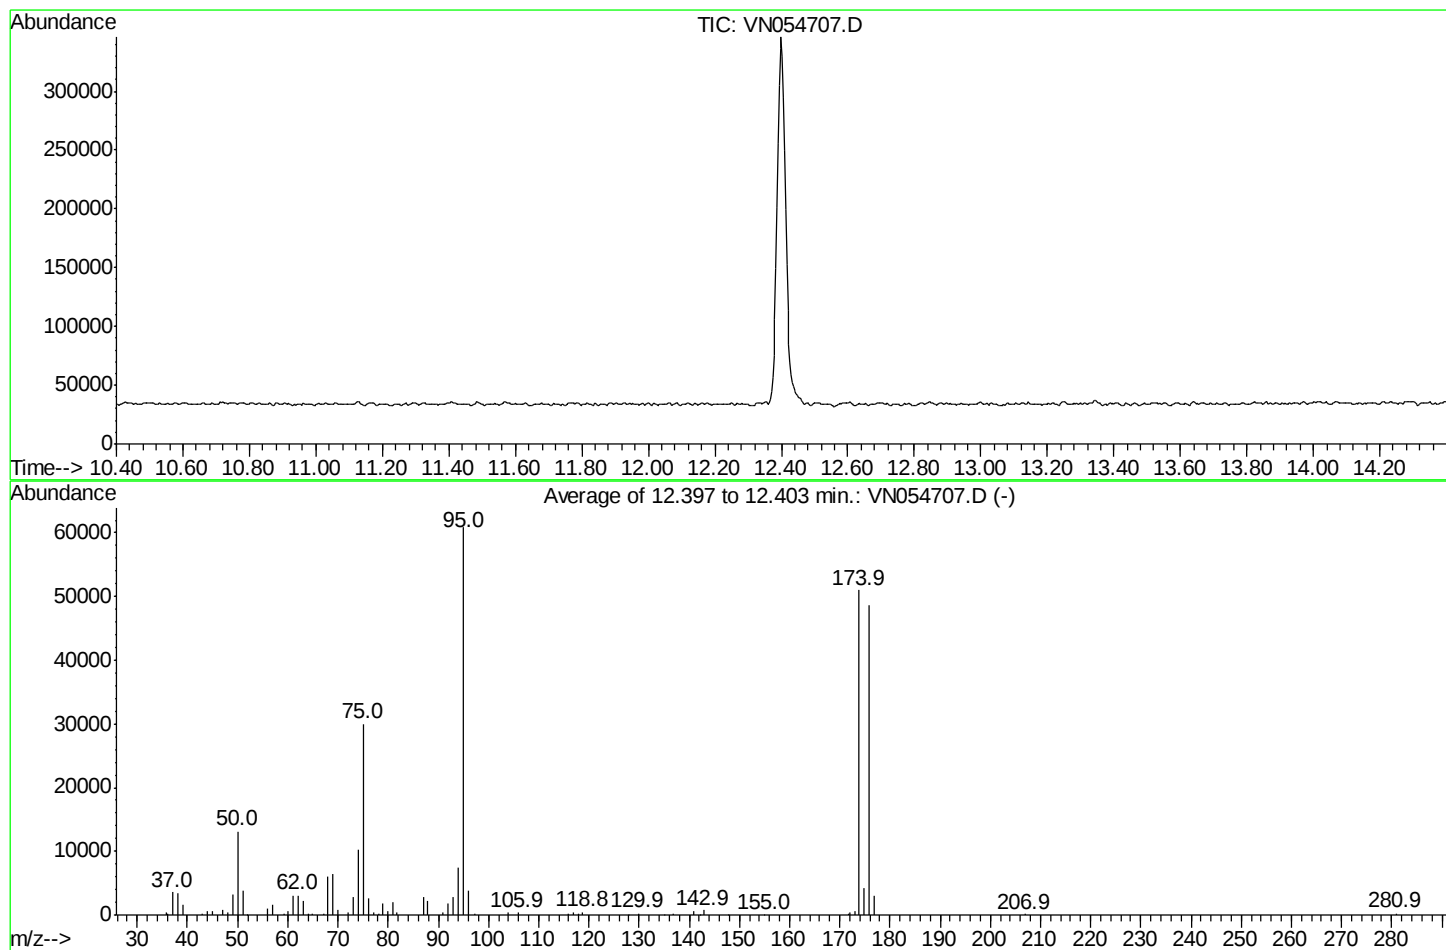

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	13168	PASS
75	95	30	60	49.2	29965	PASS
95	95	100	100	100.0	60869	PASS
96	95	5	9	6.3	3862	PASS
173	174	0.00	2	1.1	540	PASS
174	95	50	100	83.9	51045	PASS
175	174	5	9	8.2	4210	PASS
176	174	95	101	95.3	48629	PASS
177	176	5	9	6.3	3061	PASS