

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032723\
 Data File : VN077226.D
 Acq On : 28 Mar 2023 01:31
 Operator : JC\MD
 Sample : PB151677TB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB151677TB

Quant Time: Mar 28 07:50:11 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N032523W.M
 Quant Title : SW846 8260
 QLast Update : Mon Mar 27 02:47:06 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.231	168	427364	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.107	114	765326	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.866	117	665058	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.795	152	244780	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	323768	48.454	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	96.900%		
35) Dibromofluoromethane	8.172	113	238288	45.885	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	91.780%		
50) Toluene-d8	10.566	98	933059	47.951	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	95.900%		
62) 4-Bromofluorobenzene	12.854	95	302026	47.293	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	94.580%		
Target Compounds						Qvalue
3) Chloromethane	2.366	50	1744	0.279	ug/l #	40
11) Tert butyl alcohol	5.531	59	281	0.309	ug/l #	72
13) Acrolein	4.201	56	317	0.248	ug/l #	61
16) Acetone	4.448	43	57558	23.167	ug/l #	87
18) Methyl Acetate	5.048	43	9856	0.992	ug/l #	58
20) Methylene Chloride	5.290	84	15946	2.882	ug/l #	81
25) 2-Butanone	7.495	43	5443	1.401	ug/l #	63
29) Tetrahydrofuran	7.848	42	1799	0.699	ug/l #	65
36) 1,1-Dichloropropene	8.231	75	40429	5.594	ug/l #	49
37) Ethyl Acetate	7.566	43	93725	11.634	ug/l #	90
38) Carbon Tetrachloride	8.231	117	48624	6.635	ug/l #	16
43) Isopropyl Acetate	8.695	43	457283	35.184	ug/l #	75
45) 1,2-Dichloropropane	9.742	63	4442	0.754	ug/l #	45
48) Methyl methacrylate	9.672	41	12693	2.028	ug/l #	30
49) 1,4-Dioxane	9.672	88	58	0.544	ug/l #	1
51) 4-Methyl-2-Pentanone	10.448	43	15864	1.940	ug/l	98
53) t-1,3-Dichloropropene	10.724	75	2296	0.295	ug/l #	43
54) cis-1,3-Dichloropropene	10.360	75	131066	15.412	ug/l #	71
55) 1,1,2-Trichloroethane	11.042	97	1194	0.225	ug/l #	28
56) Ethyl methacrylate	10.872	69	5471	0.699	ug/l #	36
57) 1,3-Dichloropropane	11.207	76	15371	1.626	ug/l #	50
59) 2-Hexanone	11.172	43	359896	61.237	ug/l #	17
61) 1,2-Dibromoethane	11.454	107	1099	0.209	ug/l	100
74) N-amyl acetate	12.666	43	7870	0.938	ug/l #	43
75) 1,1,2,2-Tetrachloroethane	12.807	83	2455	0.382	ug/l #	26
76) 1,2,3-Trichloropropane	12.854	75	168928	34.020	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.854	75	168928	98.050	ug/l #	15
93) 1,2,4-Trichlorobenzene	15.395	180	129	4.406	ug/l #	12
95) Naphthalene	15.648	128	955	5.980	ug/l #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032723\
Data File : VN077226.D
Acq On : 28 Mar 2023 01:31
Operator : JC\MD
Sample : PB151677TB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB151677TB

Quant Time: Mar 28 07:50:11 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N032523W.M
Quant Title : SW846 8260
QLast Update : Mon Mar 27 02:47:06 2023
Response via : Initial Calibration

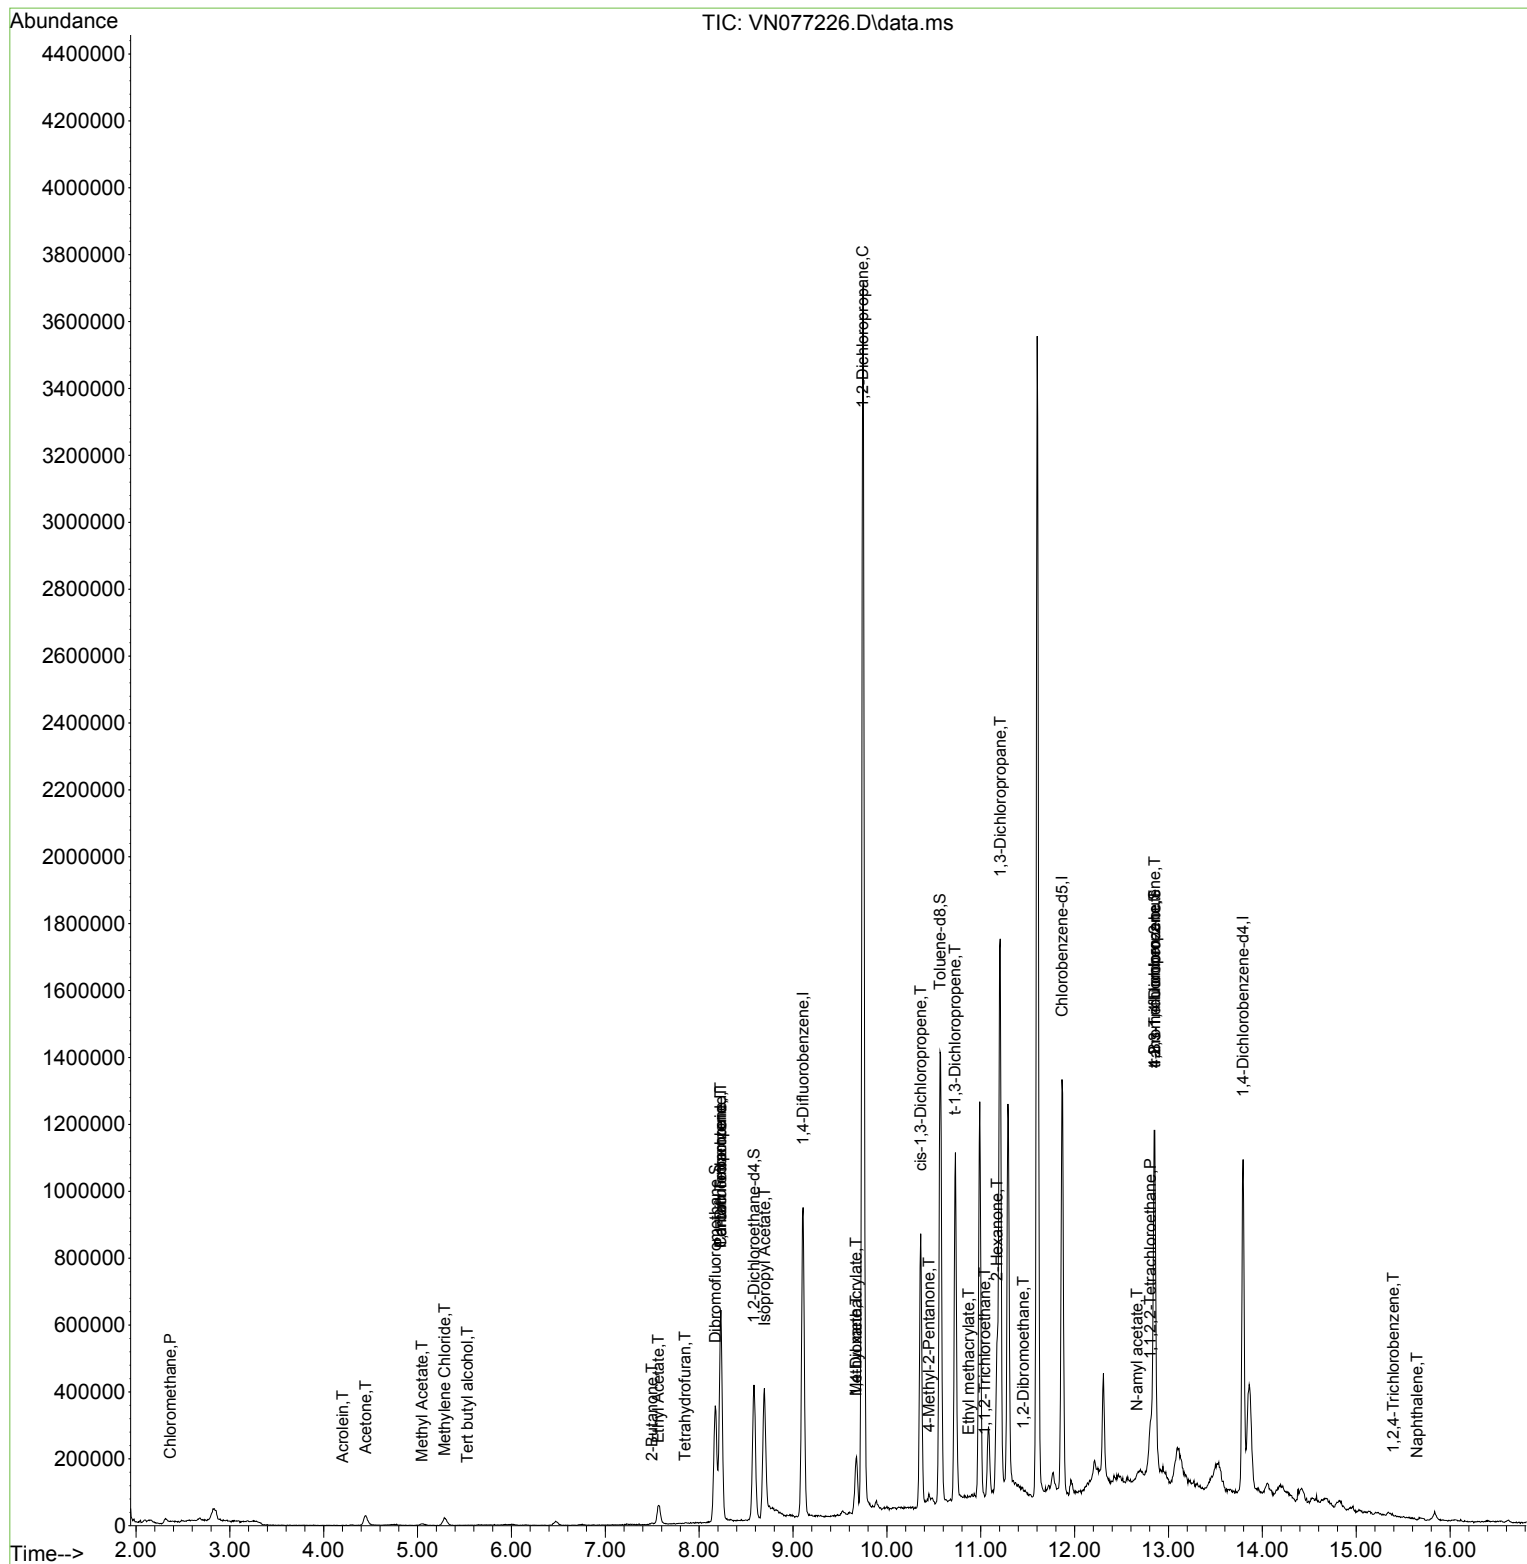



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.231 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN077226.D

Acq: 28 Mar 2023 01:31

Instrument :

MSVOA_N

ClientSampleId :





PB151677TB

Tgt Ion:168 Resp: 427364

Ion Ratio Lower Upper

168 100

99 63.1 48.6 73.0

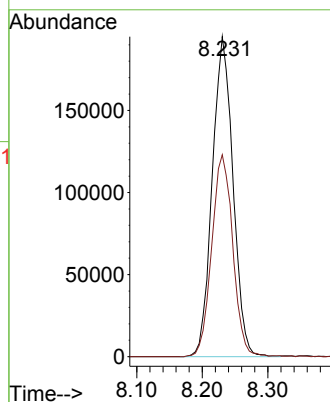

#3

Chloromethane

Concen: 0.279 ug/l

RT: 2.366 min Scan# 73

Delta R.T. -0.006 min

Lab File: VN077226.D




Acq: 28 Mar 2023 01:31


Tgt Ion: 50 Resp: 1744

Ion Ratio Lower Upper

50 100

52 0.0 27.9 41.9#









#11
Tert butyl alcohol
Concen: 0.309 ug/l
RT: 5.531 min Scan# 611
Delta R.T. -0.006 min
Lab File: VN077226.D
Acq: 28 Mar 2023 01:31




Instrument :
MSVOA_N
ClientSampleId :
PB151677TB


Tgt Ion: 59 Resp: 281
Ion Ratio Lower Upper
59 100
57 0.0 8.6 12.8#



#13
Acrolein
Concen: 0.248 ug/l
RT: 4.201 min Scan# 385
Delta R.T. 0.011 min
Lab File: VN077226.D
Acq: 28 Mar 2023 01:31

Tgt Ion: 56 Resp: 317
Ion Ratio Lower Upper
56 100
55 38.5 56.7 85.1#









#16
Acetone
Concen: 23.167 ug/l
RT: 4.448 min Scan# 41
Delta R.T. 0.011 min
Lab File: VN077226.D
Acq: 28 Mar 2023 01:31




Instrument :
MSVOA_N
ClientSampleId :
PB151677TB


Tgt Ion: 43 Resp: 57558
Ion Ratio Lower Upper
43 100
58 27.5 28.2 42.2#



#18
Methyl Acetate
Concen: 0.992 ug/l
RT: 5.048 min Scan# 529
Delta R.T. 0.011 min
Lab File: VN077226.D
Acq: 28 Mar 2023 01:31

Tgt Ion: 43 Resp: 9856
Ion Ratio Lower Upper
43 100
74 8.7 25.9 38.9#









#20
Methylene Chloride
Concen: 2.882 ug/l
RT: 5.290 min Scan# 51
Delta R.T. 0.006 min
Lab File: VN077226.D
Acq: 28 Mar 2023 01:31




Instrument :
MSVOA_N
ClientSampleId :
PB151677TB


Tgt Ion: 84	Resp: 15946
Ion Ratio	Lower Upper
84 100	
49 124.0	76.6 114.8#
51 36.2	25.4 38.2
86 70.4	51.1 76.7



#25
2-Butanone
Concen: 1.401 ug/l
RT: 7.495 min Scan# 945
Delta R.T. 0.005 min
Lab File: VN077226.D
Acq: 28 Mar 2023 01:31

Tgt Ion: 43	Resp: 5443
Ion Ratio	Lower Upper
43 100	
72 14.2	28.8 43.2#





#29

Tetrahydrofuran

Concen: 0.699 ug/l

RT: 7.848 min Scan# 1004

Delta R.T. 0.006 min

Lab File: VN077226.D

Acq: 28 Mar 2023 01:31

Instrument :

MSVOA_N

ClientSampleId :

PB151677TB





Tgt Ion: 42 Resp: 1799

Ion Ratio Lower Upper

42 100

72 28.3 48.6 73.0#

71 36.5 45.1 67.7#



#33

1,2-Dichloroethane-d4

Concen: 48.454 ug/l

RT: 8.583 min Scan# 1130

Delta R.T. -0.001 min

Lab File: VN077226.D




Acq: 28 Mar 2023 01:31


Tgt Ion: 65 Resp: 323768

Ion Ratio Lower Upper

65 100

67 52.2 0.0 107.2

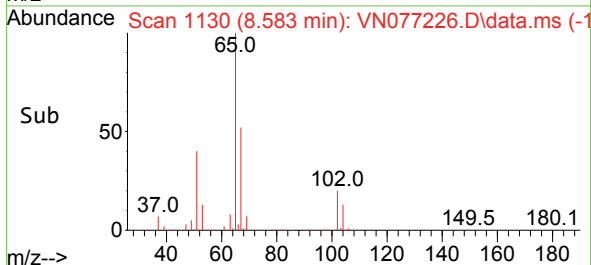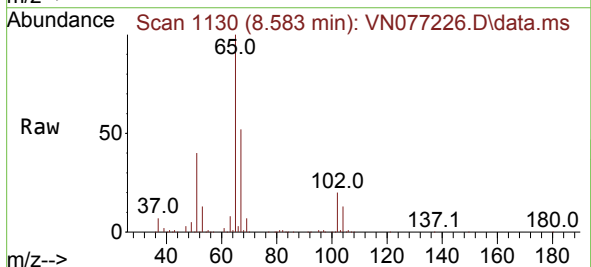



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.107 min Scan# 11

Delta R.T. -0.000 min

Lab File: VN077226.D

Acq: 28 Mar 2023 01:31

Instrument :

MSVOA_N

ClientSampleId :

PB151677TB





Tgt Ion:114 Resp: 765326

Ion Ratio Lower Upper

114 100

63 21.8 0.0 36.6

88 15.7 0.0 28.6



#35

Dibromofluoromethane

Concen: 45.885 ug/l

RT: 8.172 min Scan# 1060

Delta R.T. -0.000 min

Lab File: VN077226.D

Acq: 28 Mar 2023 01:31




Tgt Ion:113 Resp: 238288


Ion Ratio Lower Upper

113 100

111 108.1 81.8 122.8


192 17.9 13.9 20.9

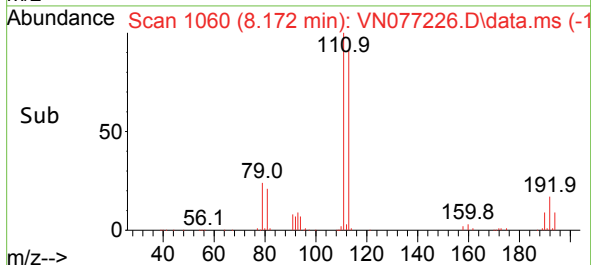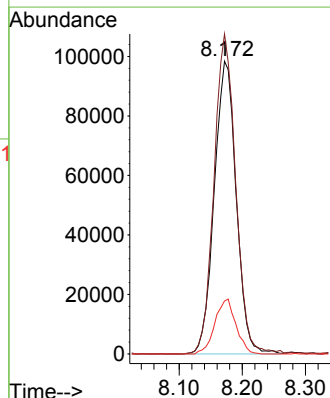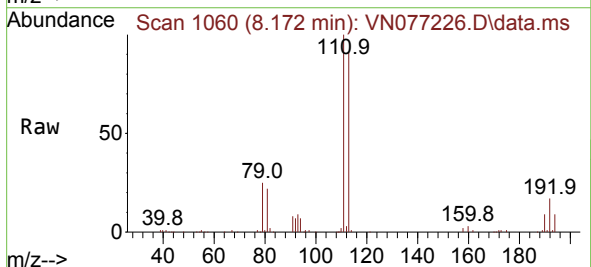






#36
1,1-Dichloropropene
Concen: 5.594 ug/l
RT: 8.231 min Scan# 1095
Delta R.T. -0.147 min
Lab File: VN077226.D
Acq: 28 Mar 2023 01:31

Instrument :
MSVOA_N
ClientSampleId :
PB151677TB







Tgt Ion: 75 Resp: 40429
Ion Ratio Lower Upper
75 100
110 9.4 18.9 56.9#
77 0.9 24.9 37.3#

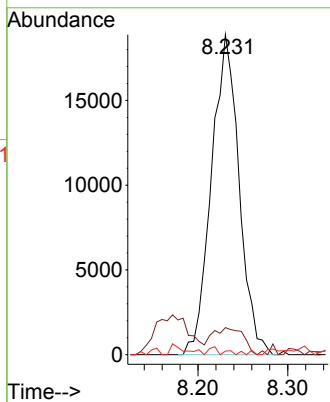

#37
Ethyl Acetate
Concen: 11.634 ug/l
RT: 7.566 min Scan# 957
Delta R.T. -0.000 min
Lab File: VN077226.D
Acq: 28 Mar 2023 01:31

Tgt Ion: 43 Resp: 93725
Ion Ratio Lower Upper
43 100
61 12.5 13.5 20.3#
70 9.7 11.0 16.6#

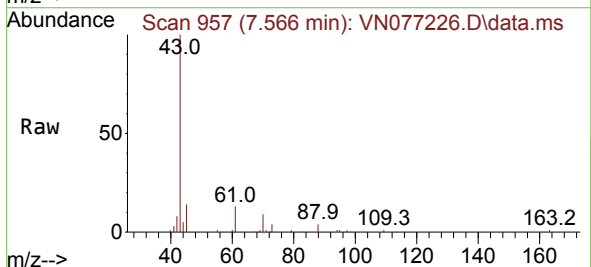



#38

Carbon Tetrachloride

Concen: 6.635 ug/l

RT: 8.231 min Scan# 1070

Delta R.T. -0.141 min

Lab File: VN077226.D


Acq: 28 Mar 2023 01:31

Instrument :

MSVOA_N

ClientSampleId :

PB151677TB






Tgt Ion:117 Resp: 48624

Ion Ratio Lower Upper

117 100

119 5.5 76.9 115.3#

121 0.0 23.2 34.8#

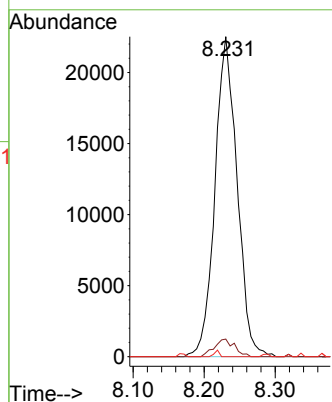

#43

Isopropyl Acetate

Concen: 35.184 ug/l

RT: 8.695 min Scan# 1149

Delta R.T. 0.000 min

Lab File: VN077226.D

Acq: 28 Mar 2023 01:31




Tgt Ion: 43 Resp: 457283


Ion Ratio Lower Upper

43 100

61 16.1 26.2 39.2#

87 10.5 14.8 22.2#





#45

1,2-Dichloropropane

Concen: 0.754 ug/l

RT: 9.742 min Scan# 1327

Delta R.T. 0.117 min

Lab File: VN077226.D

Acq: 28 Mar 2023 01:31

Instrument :

MSVOA_N

ClientSampleId :





PB151677TB

Tgt Ion: 63 Resp: 4442

Ion Ratio Lower Upper

63 100

65 0.9 25.0 37.6#

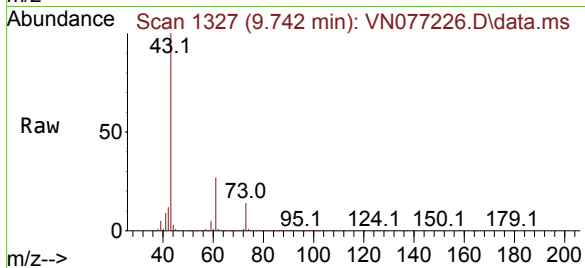

#48

Methyl methacrylate

Concen: 2.028 ug/l

RT: 9.672 min Scan# 1315

Delta R.T. -0.012 min

Lab File: VN077226.D

Acq: 28 Mar 2023 01:31




Tgt Ion: 41 Resp: 12693


Ion Ratio Lower Upper

41 100

69 0.0 92.6 139.0#

39 60.9 51.4 77.0

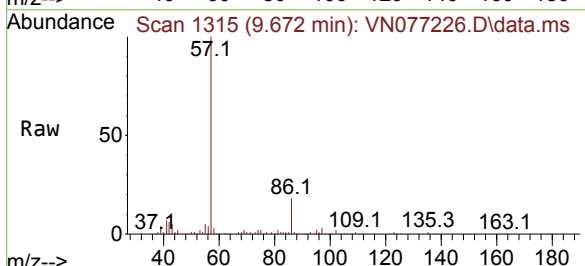



#49

1,4-Dioxane

Concen: 0.544 ug/l

RT: 9.672 min Scan# 11

Delta R.T. -0.023 min

Lab File: VN077226.D

Acq: 28 Mar 2023 01:31

Instrument :

MSVOA_N

ClientSampleId :

PB151677TB





Tgt Ion: 88 Resp: 58

Ion Ratio Lower Upper

88 100

43 0.0 15.3 22.9#

58 15020.7 47.6 71.4#

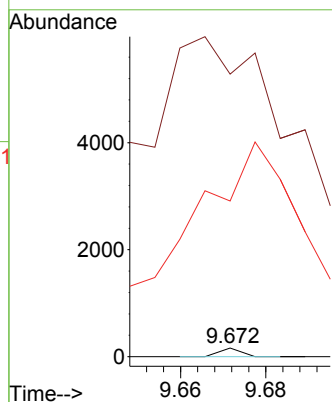

#50

Toluene-d8

Concen: 47.951 ug/l

RT: 10.566 min Scan# 1467

Delta R.T. -0.006 min

Lab File: VN077226.D




Acq: 28 Mar 2023 01:31


Tgt Ion: 98 Resp: 933059

Ion Ratio Lower Upper

98 100

100 63.8 52.8 79.2









#51
4-Methyl-2-Pentanone
Concen: 1.940 ug/l
RT: 10.448 min Scan# 1447
Delta R.T. 0.000 min
Lab File: VN077226.D
Acq: 28 Mar 2023 01:31




Instrument :
MSVOA_N
ClientSampleId :
PB151677TB


Tgt Ion: 43 Resp: 15864
Ion Ratio Lower Upper
43 100
58 45.2 37.4 56.0



#53
t-1,3-Dichloropropene
Concen: 0.295 ug/l
RT: 10.724 min Scan# 1494
Delta R.T. -0.112 min
Lab File: VN077226.D
Acq: 28 Mar 2023 01:31

Tgt Ion: 75 Resp: 2296
Ion Ratio Lower Upper
75 100
77 0.0 25.0 37.6#




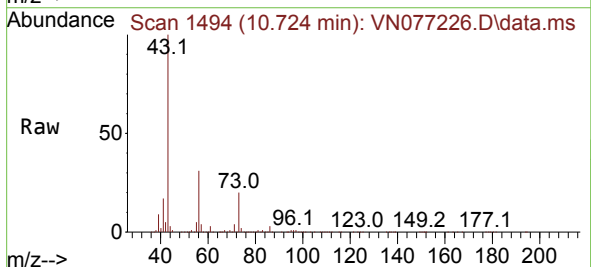


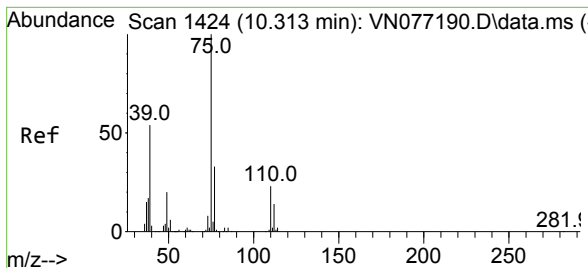

#54
cis-1,3-Dichloropropene
Concen: 15.412 ug/l
RT: 10.360 min Scan# 1424
Delta R.T. 0.047 min
Lab File: VN077226.D
Acq: 28 Mar 2023 01:31




Instrument :
MSVOA_N
ClientSampleId :
PB151677TB


Tgt Ion: 75 Resp: 131066
Ion Ratio Lower Upper
75 100
77 0.4 25.7 38.5#
39 39.8 29.7 44.5

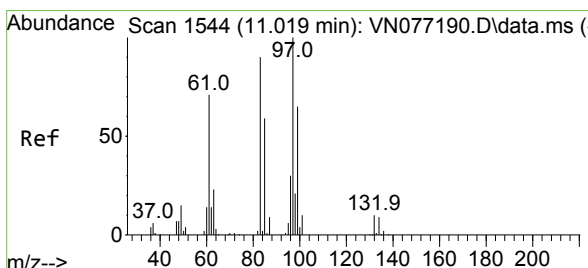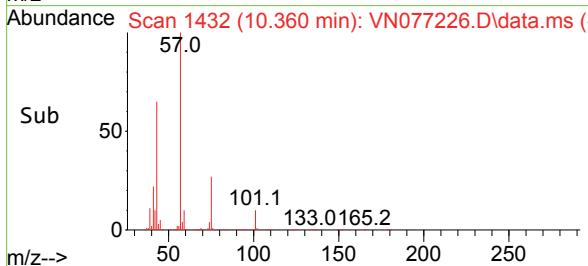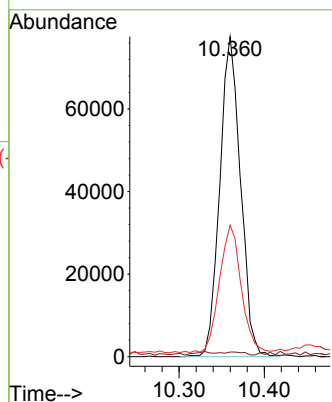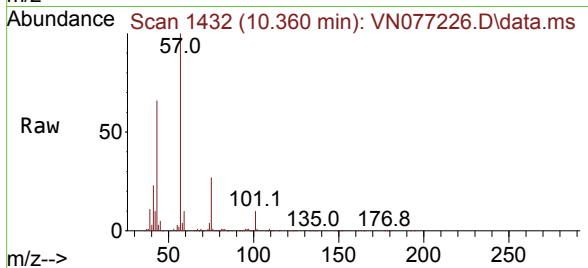

#55
1,1,2-Trichloroethane
Concen: 0.225 ug/l
RT: 11.042 min Scan# 1548
Delta R.T. 0.023 min
Lab File: VN077226.D
Acq: 28 Mar 2023 01:31

Tgt Ion: 97 Resp: 1194
Ion Ratio Lower Upper
97 100
83 0.0 67.1 100.7#
85 14.0 41.8 62.8#
99 17.9 50.4 75.6#


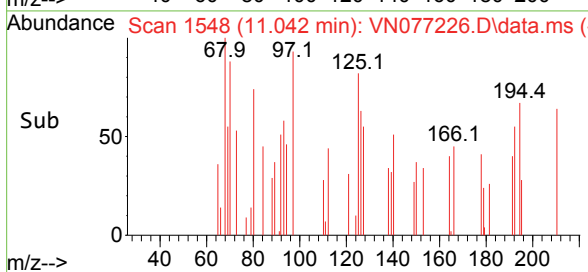

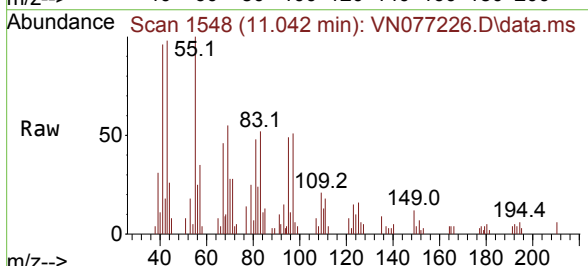


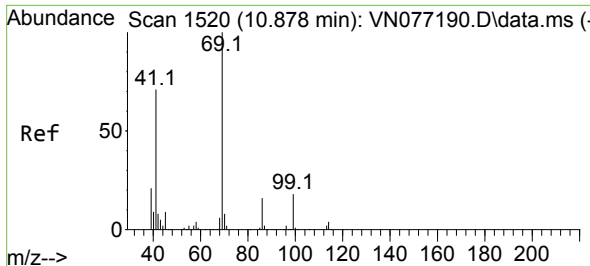

#56
Ethyl methacrylate
Concen: 0.699 ug/l
RT: 10.872 min Scan# 1519
Delta R.T. -0.006 min
Lab File: VN077226.D
Acq: 28 Mar 2023 01:31




Instrument :
MSVOA_N
ClientSampleId :
PB151677TB


Tgt Ion: 69 Resp: 5471
Ion Ratio Lower Upper
69 100
41 0.0 38.0 57.0#
39 0.0 22.4 33.6#

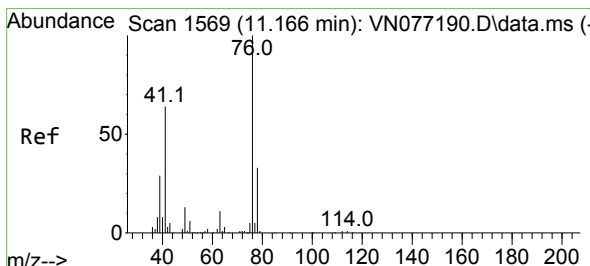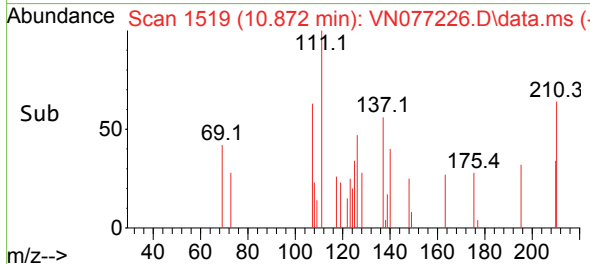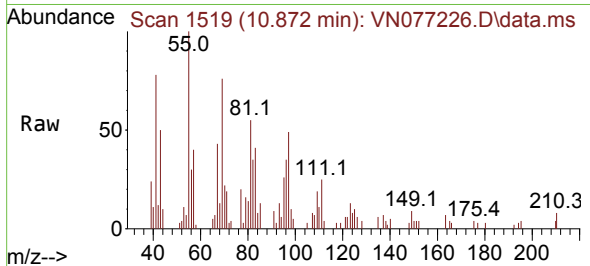

#57
1,3-Dichloropropane
Concen: 1.626 ug/l
RT: 11.207 min Scan# 1576
Delta R.T. 0.041 min
Lab File: VN077226.D
Acq: 28 Mar 2023 01:31

Tgt Ion: 76 Resp: 15371
Ion Ratio Lower Upper
76 100
78 4.7 26.1 39.1#


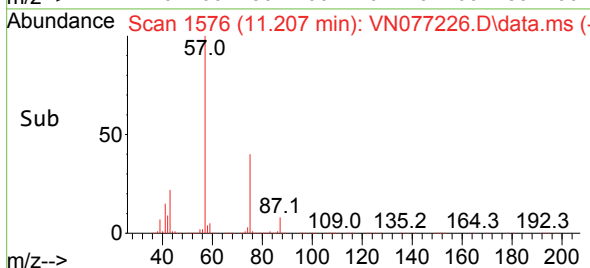
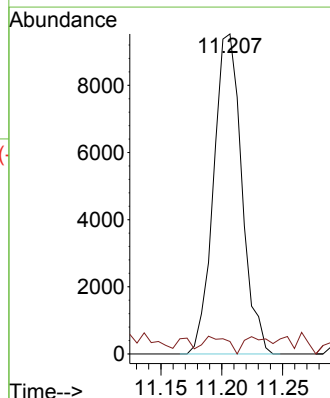
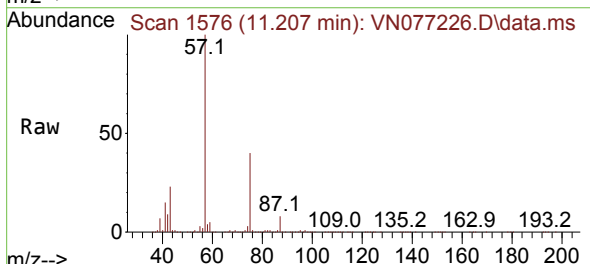




#59
2-Hexanone
Concen: 61.237 ug/l
RT: 11.172 min Scan# 11172
Delta R.T. -0.024 min
Lab File: VN077226.D
Acq: 28 Mar 2023 01:31




Instrument :
MSVOA_N
ClientSampleId :
PB151677TB


Tgt Ion: 43 Resp: 359896
Ion Ratio Lower Upper
43 100
58 0.0 32.6 98.0#

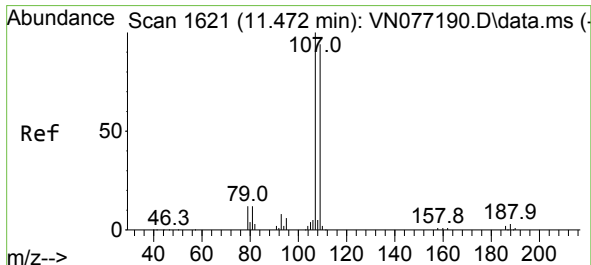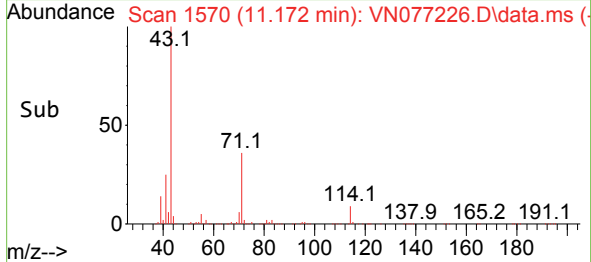

#61
1,2-Dibromoethane
Concen: 0.209 ug/l
RT: 11.454 min Scan# 1618
Delta R.T. -0.018 min
Lab File: VN077226.D
Acq: 28 Mar 2023 01:31

Tgt Ion: 107 Resp: 1099
Ion Ratio Lower Upper
107 100
109 94.4 75.9 113.9


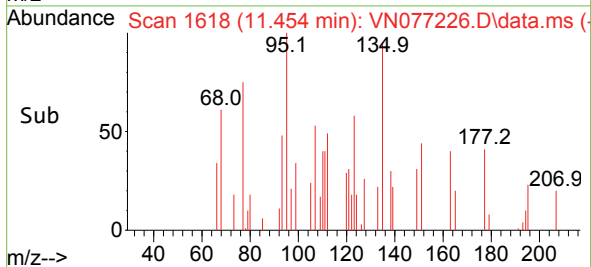

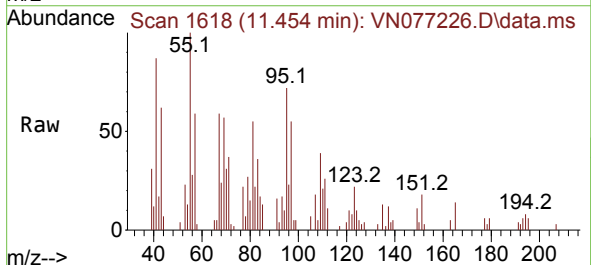


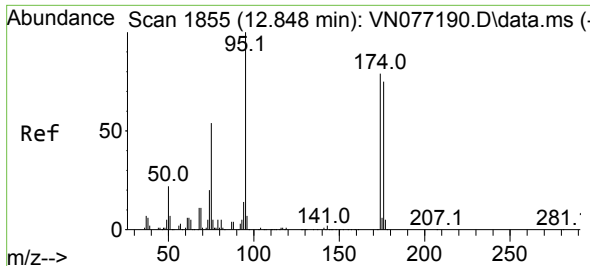

#62
4-Bromofluorobenzene
Concen: 47.293 ug/l
RT: 12.854 min Scan# 1856
Delta R.T. 0.006 min
Lab File: VN077226.D
Acq: 28 Mar 2023 01:31




Instrument :
MSVOA_N
ClientSampleId :
PB151677TB


Tgt Ion: 95 Resp: 302026
Ion Ratio Lower Upper
95 100
174 73.6 0.0 162.4
176 69.4 0.0 157.4

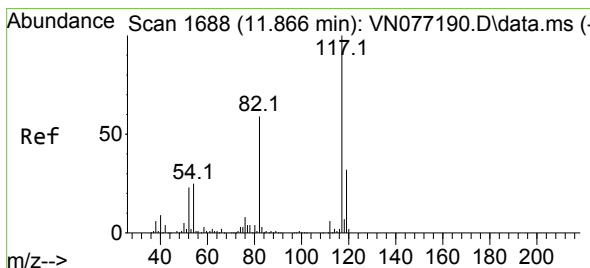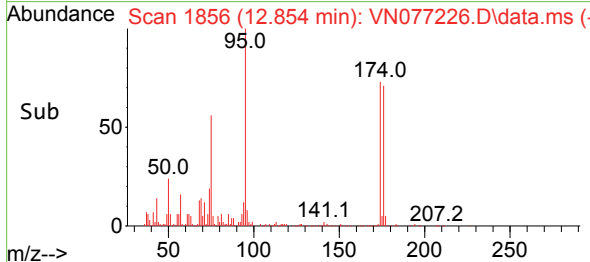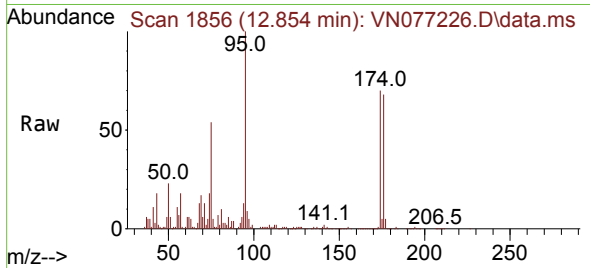

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.866 min Scan# 1688
Delta R.T. -0.000 min
Lab File: VN077226.D
Acq: 28 Mar 2023 01:31

Tgt Ion: 117 Resp: 665058
Ion Ratio Lower Upper
117 100
82 60.5 43.5 65.3
119 32.0 25.5 38.3


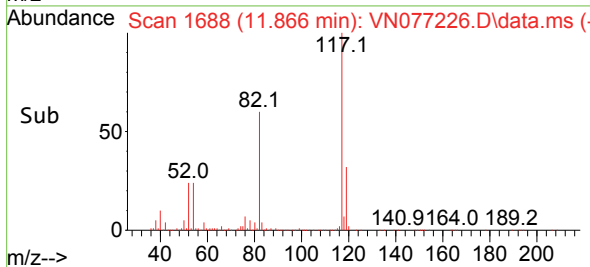

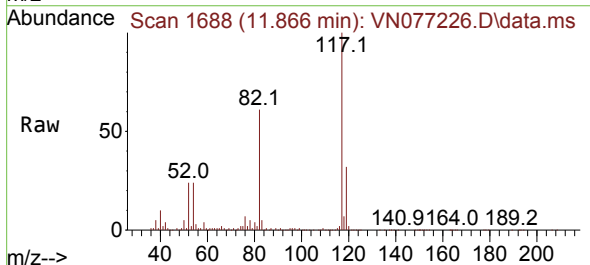


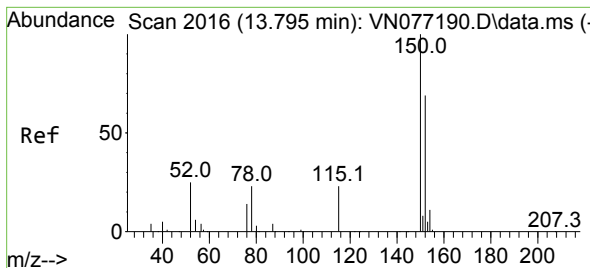

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.795 min Scan# 2016
Delta R.T. -0.000 min
Lab File: VN077226.D
Acq: 28 Mar 2023 01:31




Instrument :
MSVOA_N
ClientSampleId :
PB151677TB


Tgt Ion:152 Resp: 244780
Ion Ratio Lower Upper
152 100
115 62.8 30.3 90.9
150 160.3 0.0 353.6

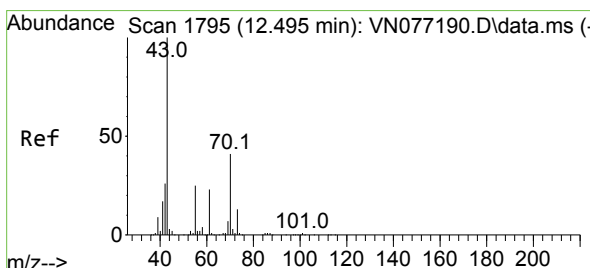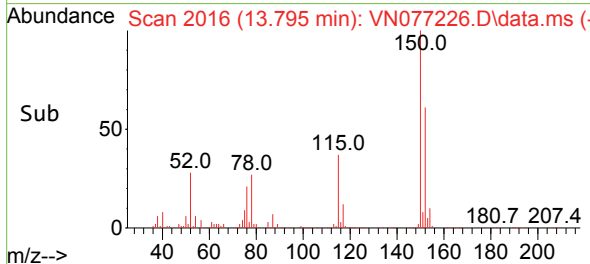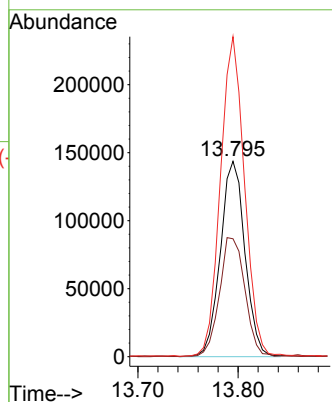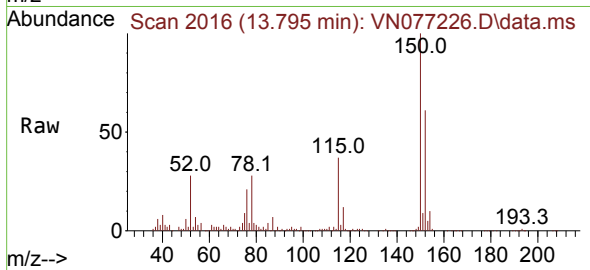

#74
N-ethyl acetate
Concen: 0.938 ug/l
RT: 12.666 min Scan# 1824
Delta R.T. 0.171 min
Lab File: VN077226.D
Acq: 28 Mar 2023 01:31

Tgt Ion: 43 Resp: 7870
Ion Ratio Lower Upper
43 100
70 0.0 46.8 70.2#
55 20.4 23.4 35.2#
61 0.0 23.8 35.8#


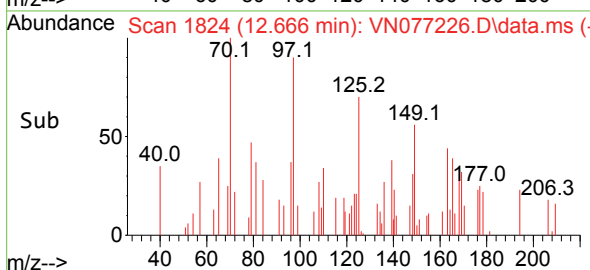

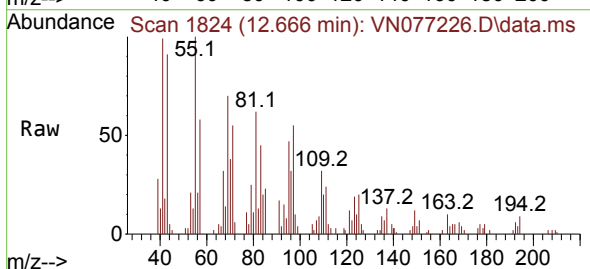


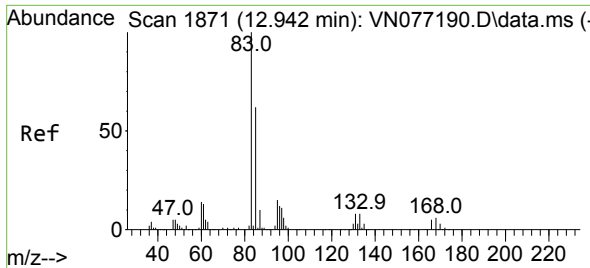

#75
1,1,2,2-Tetrachloroethane
Concen: 0.382 ug/l
RT: 12.807 min Scan# 1856
Delta R.T. -0.135 min
Lab File: VN077226.D
Acq: 28 Mar 2023 01:31




Instrument :
MSVOA_N
ClientSampleId :
PB151677TB


Tgt Ion: 83 Resp: 2455
Ion Ratio Lower Upper
83 100
131 0.0 5.3 16.1#
85 0.0 32.0 96.0#

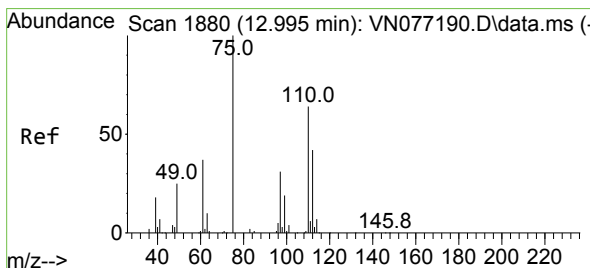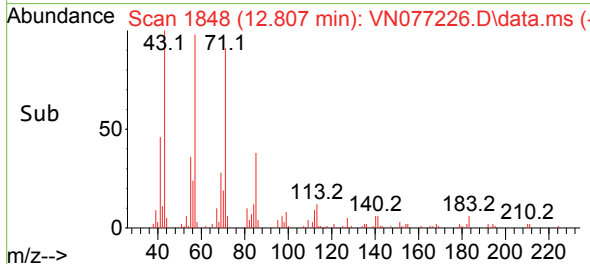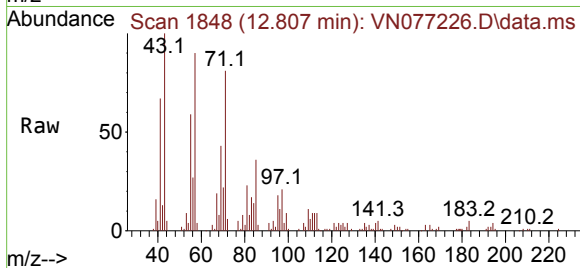

#76
1,2,3-Trichloropropane
Concen: 34.020 ug/l
RT: 12.854 min Scan# 1856
Delta R.T. -0.141 min
Lab File: VN077226.D
Acq: 28 Mar 2023 01:31

Tgt Ion: 75 Resp: 168928
Ion Ratio Lower Upper
75 100
77 2.2 93.8 281.4#


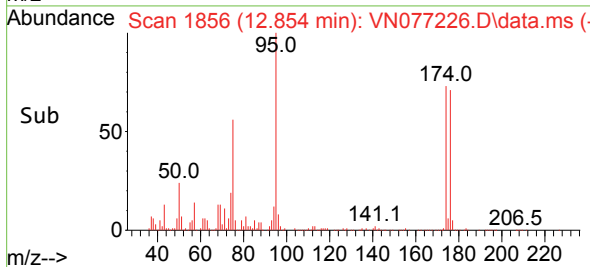

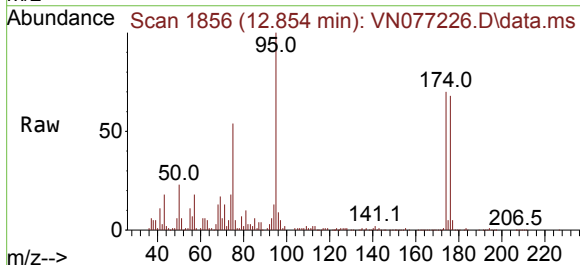




#81
trans-1,4-Dichloro-2-butene
Concen: 98.050 ug/l
RT: 12.854 min Scan# 1856
Delta R.T. 0.118 min
Lab File: VN077226.D
Acq: 28 Mar 2023 01:31




Instrument :
MSVOA_N
ClientSampleId :
PB151677TB


Tgt Ion: 75 Resp: 168928
Ion Ratio Lower Upper
75 100
53 0.0 67.4 101.0#
89 0.2 39.5 59.3#

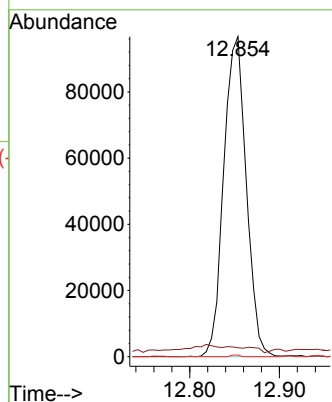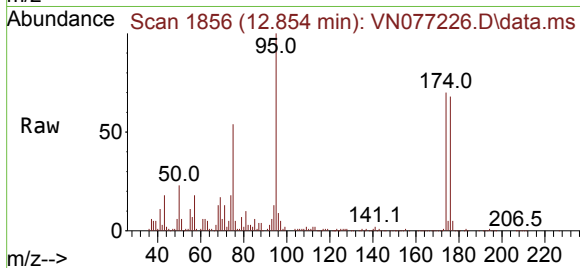

#93
1,2,4-Trichlorobenzene
Concen: 4.406 ug/l
RT: 15.395 min Scan# 2288
Delta R.T. -0.000 min
Lab File: VN077226.D
Acq: 28 Mar 2023 01:31

Tgt Ion:180 Resp: 129
Ion Ratio Lower Upper
180 100
182 0.0 47.4 142.2#
145 0.0 15.8 47.3#

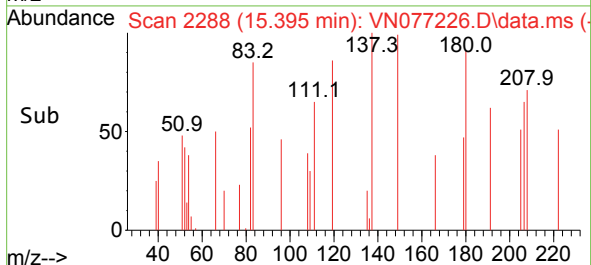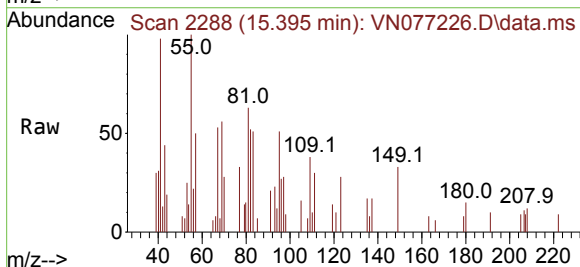



#95

Naphthalene

Concen: 5.980 ug/l

RT: 15.648 min Scan# 21

Delta R.T. 0.006 min

Lab File: VN077226.D


Acq: 28 Mar 2023 01:31

Instrument :

MSVOA_N

ClientSampleId :

PB151677TB



Tgt Ion:128 Resp: 955

Ion Ratio Lower Upper

128 100

127 0.0 10.2 15.4#

129 0.0 8.9 13.3#

