


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032723\
Data File : VN077196.D
Acq On : 27 Mar 2023 09:10
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N032423W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri Mar 24 05:55:38 2023

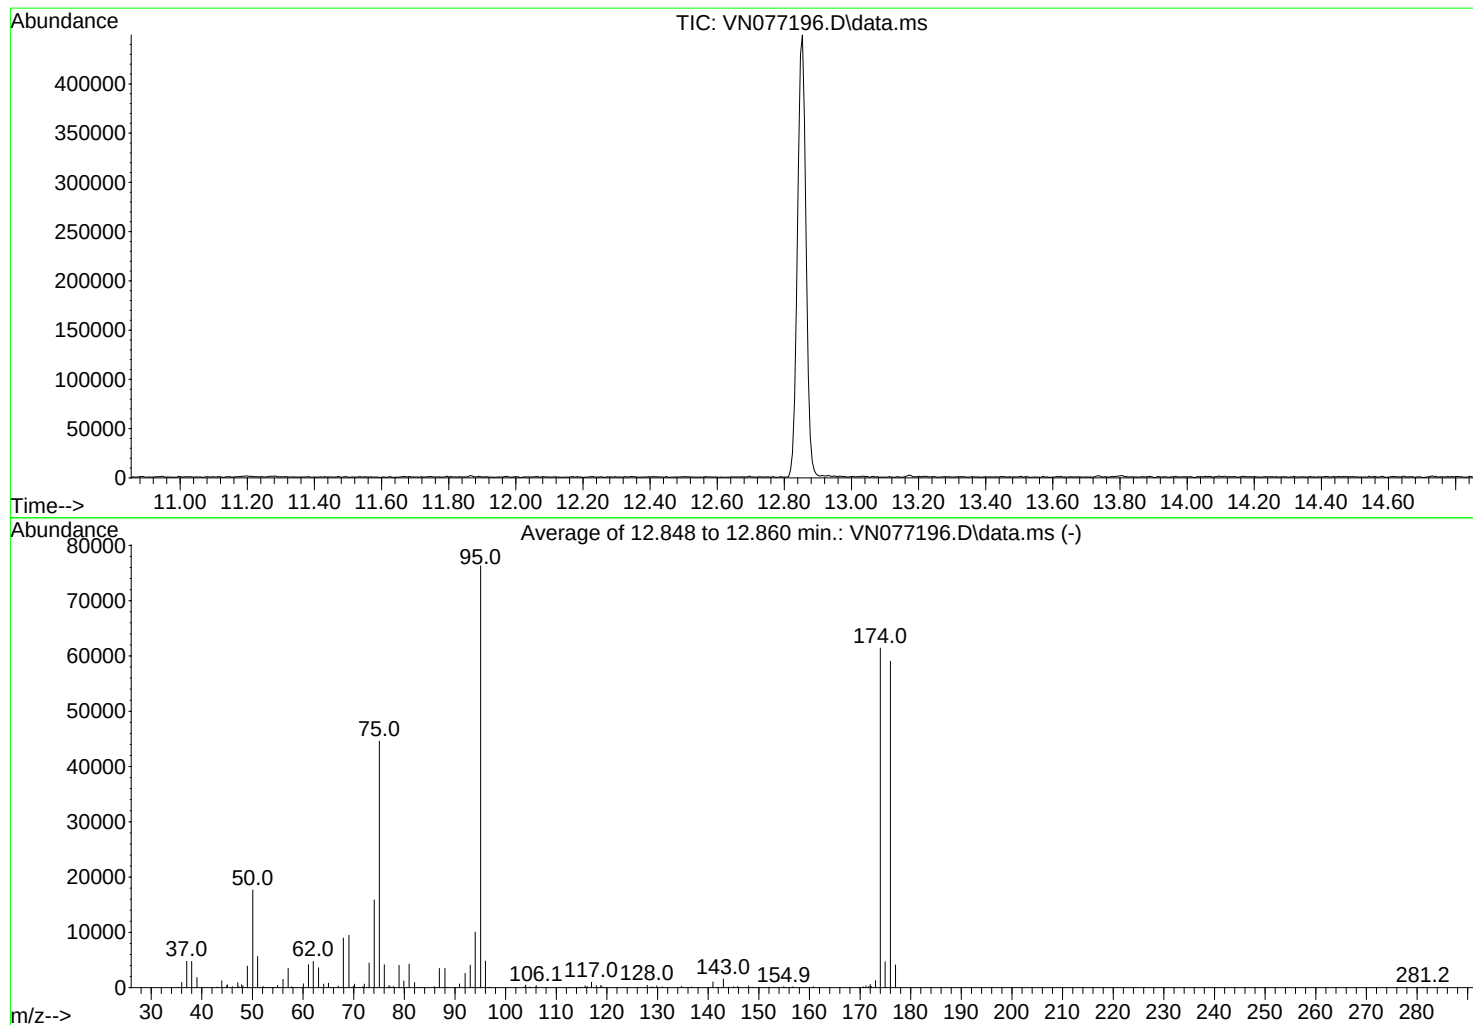

AutoFind: Scans 1855, 1856, 1857; Background Corrected with Scan 1847

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.2	17690	PASS
75	95	30	60	58.5	44611	PASS
95	95	100	100	100.0	76307	PASS
96	95	5	9	6.3	4823	PASS
173	174	0.00	2	2.0	1244	FAIL*
174	95	50	100	80.5	61424	PASS
175	174	5	9	7.6	4690	PASS
176	174	95	101	96.1	59040	PASS
177	176	5	9	7.0	4115	PASS