
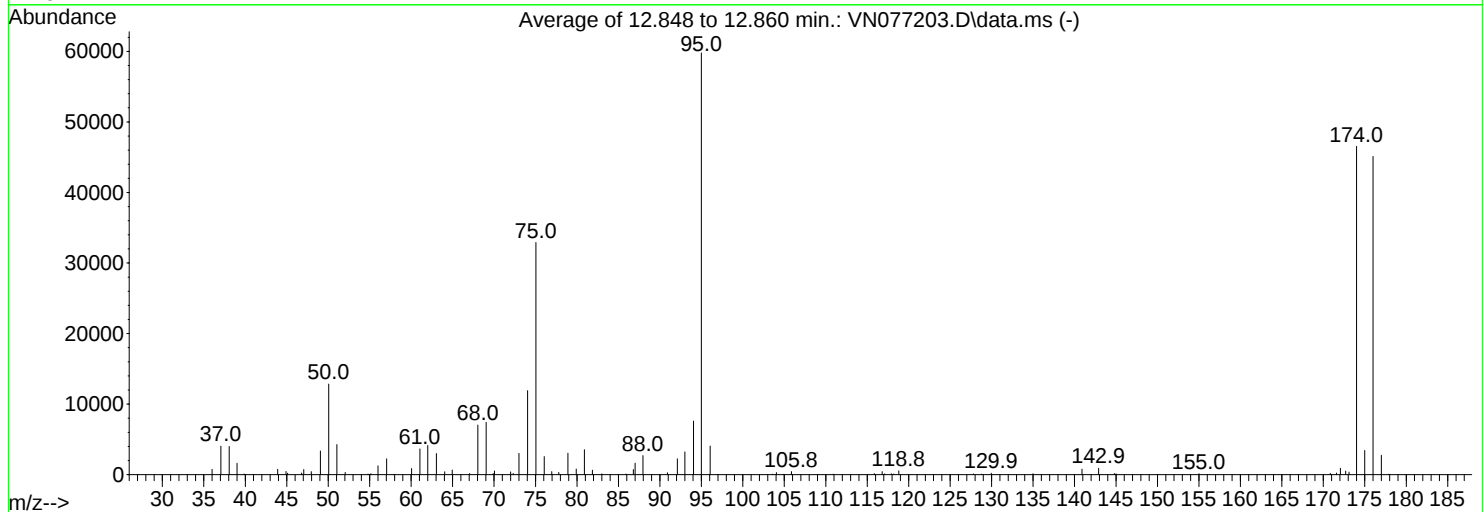


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032723\
Data File : VN077203.D
Acq On : 27 Mar 2023 15:34
Operator : JC\MD
Sample : BFB
Misc : 5.1mL/MSVOA_N/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N032423W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri Mar 24 05:55:38 2023

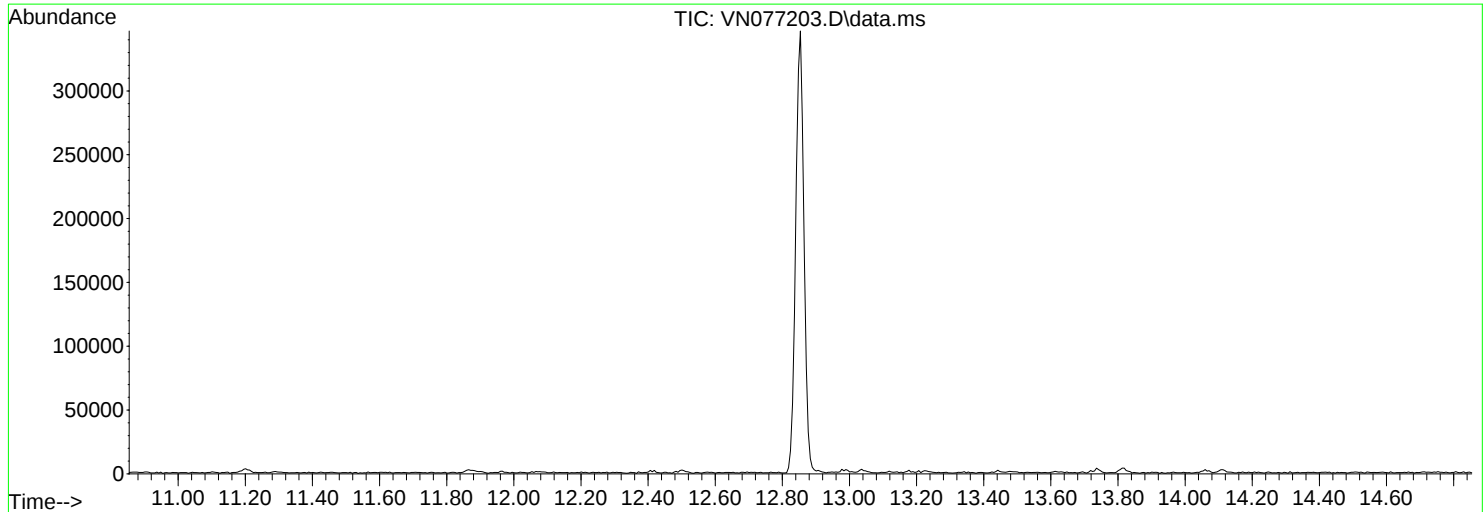

AutoFind: Scans 1855, 1856, 1857; Background Corrected with Scan 1847

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.5	12848	PASS
75	95	30	60	55.0	32907	PASS
95	95	100	100	100.0	59795	PASS
96	95	5	9	6.8	4061	PASS
173	174	0.00	2	1.1	492	PASS
174	95	50	100	77.8	46536	PASS
175	174	5	9	7.4	3424	PASS
176	174	95	101	97.0	45117	PASS
177	176	5	9	6.1	2747	PASS