
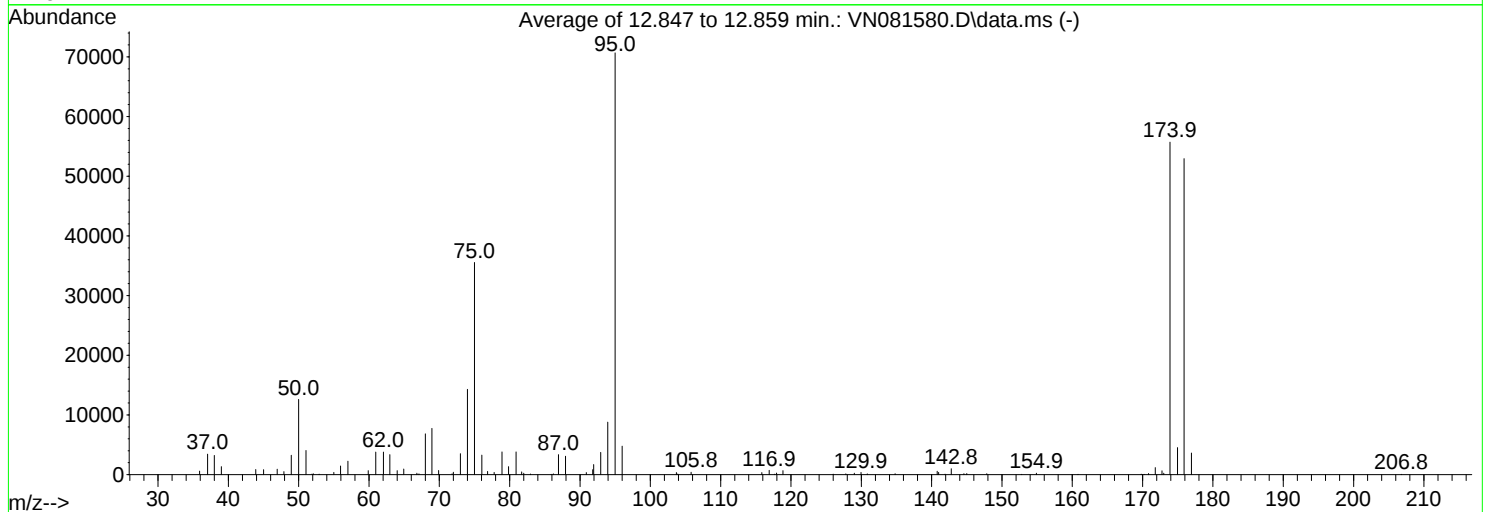


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032724\
Data File : VN081580.D
Acq On : 27 Mar 2024 11:22
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031824W.M
Title : SW846 8260
Last Update : Tue Mar 19 06:00:00 2024

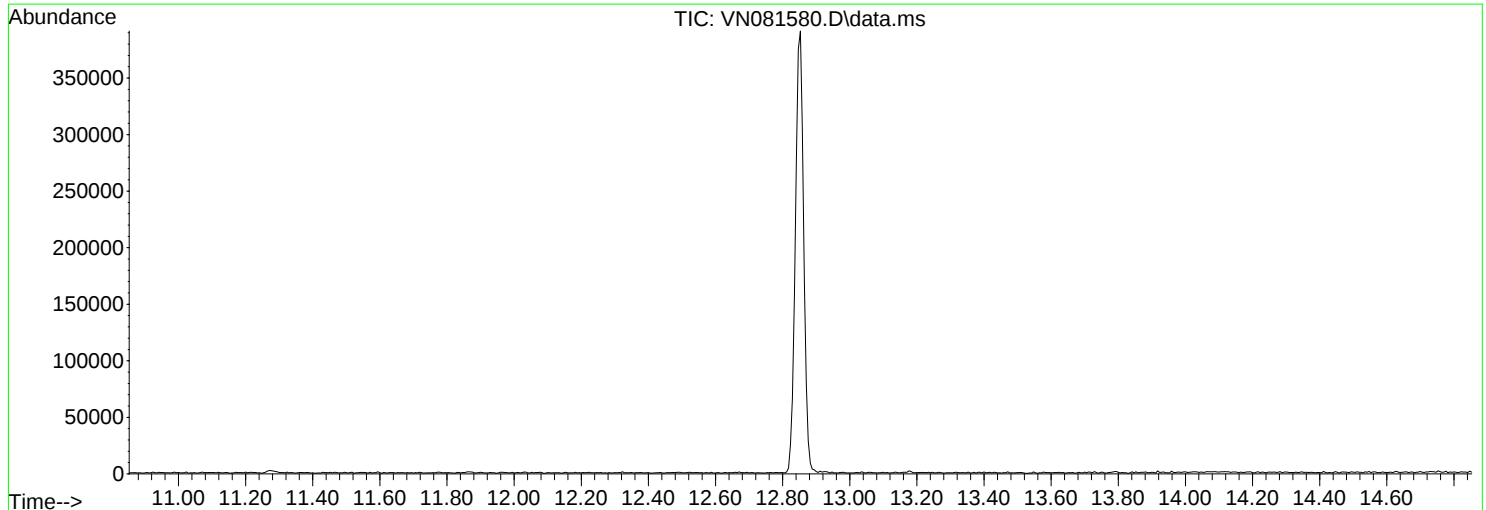

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	12597	PASS
75	95	30	60	50.3	35544	PASS
95	95	100	100	100.0	70677	PASS
96	95	5	9	6.7	4765	PASS
173	174	0.00	2	1.1	632	PASS
174	95	50	100	78.8	55712	PASS
175	174	5	9	8.1	4520	PASS
176	174	95	101	95.0	52952	PASS
177	176	5	9	6.8	3614	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	591	51.90	116	64.95	928	76.05	328
37.05	3447	52.10	131	66.80	252	76.85	55
38.00	3216	52.90	74	67.10	127	77.80	37
39.00	1351	55.00	378	68.00	6830	78.90	382
43.90	868	55.95	1462	68.95	7760	79.85	1349
45.00	825	57.00	2264	69.90	691	80.90	3818
46.95	903	59.90	667	71.80	150	81.70	460
47.90	501	60.95	3768	72.00	405	82.00	235
48.95	3238	62.05	3783	73.00	3519	82.95	111
50.00	12597	62.95	3354	74.00	14283	85.90	58
51.05	4054	64.00	684	75.00	35544	86.20	130

Average of 12.847 to 12.859 min.: VN081580.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
86.95	3342	105.80	394	134.80	165	169.80	78
87.95	3093	115.85	363	140.80	576	170.20	53
90.90	337	116.90	718	141.00	377	170.85	189
91.80	838	117.70	71	141.90	70	171.80	1180
91.95	1682	117.95	281	142.80	1006	172.75	632
92.95	3731	118.85	662	144.60	159	173.00	244
93.95	8787	126.00	72	145.00	198	173.90	55712
95.00	70677	127.80	137	147.85	169	174.95	4520
96.00	4765	129.00	245	152.80	52	175.90	52952
103.70	356	129.95	374	154.90	242	176.95	3614
103.90	104	130.85	135	160.80	57	206.80	67

Instrument :

MSVOA_N

ClientSampleId :

BFB