


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032822\
Data File : VN071604.D
Acq On : 28 Mar 2022 14:37
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N032822W.M
Title : SW846 8260
Last Update : Tue Mar 29 09:32:37 2022

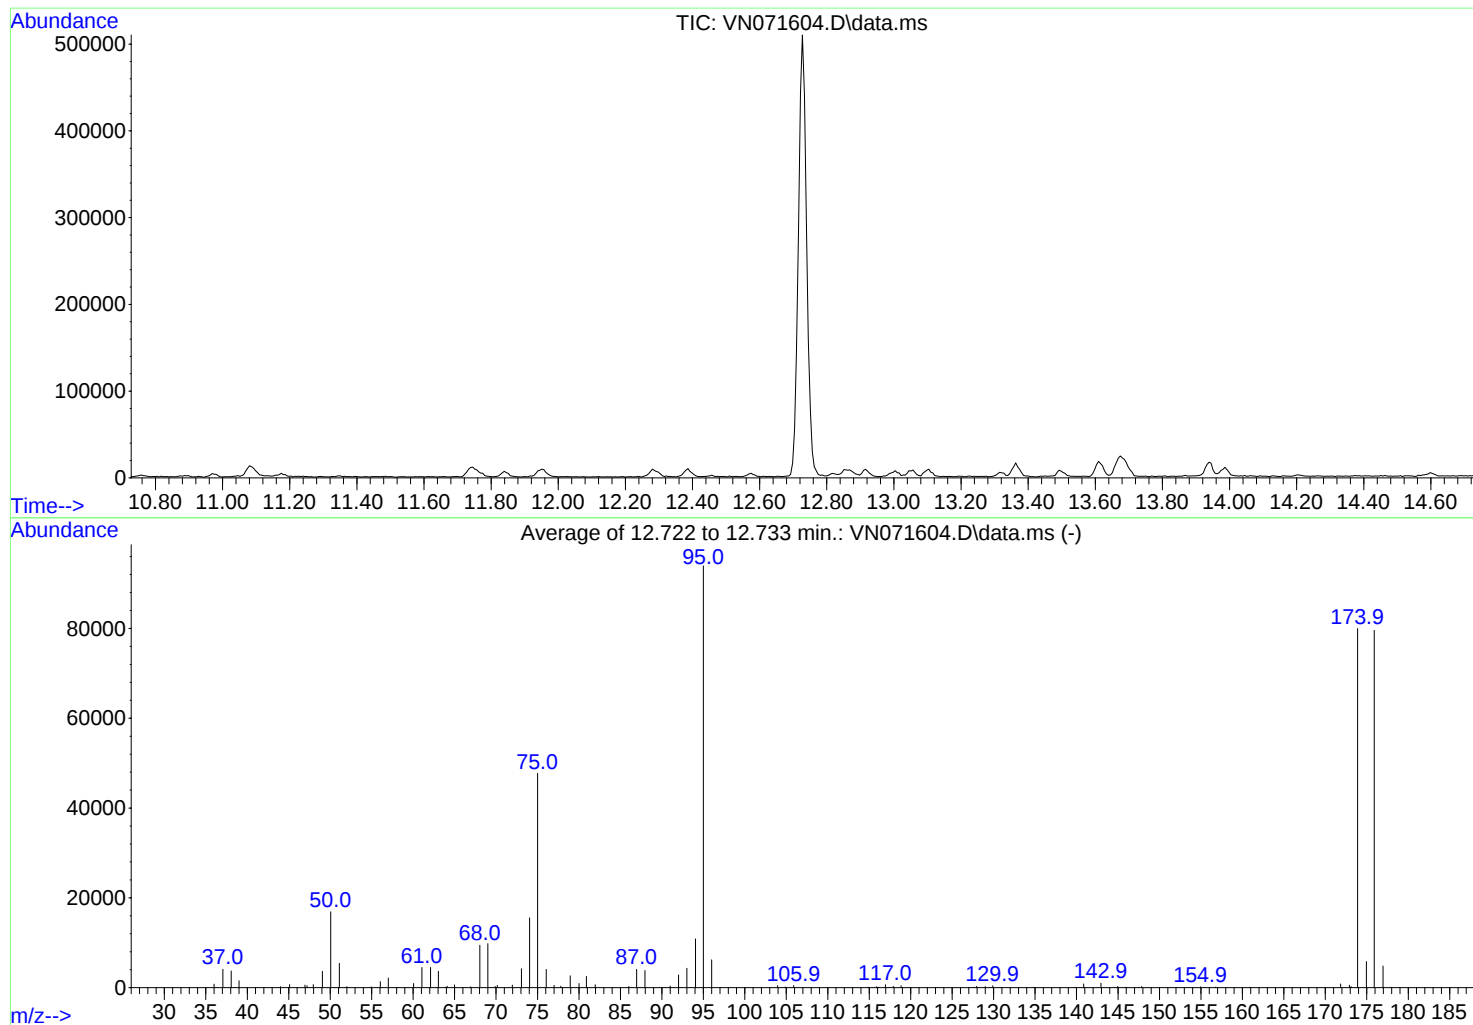

AutoFind: Scans 1825, 1826, 1827; Background Corrected with Scan 1817

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	16901	PASS
75	95	30	60	50.8	47715	PASS
95	95	100	100	100.0	93944	PASS
96	95	5	9	6.6	6211	PASS
173	174	0.00	2	0.7	535	PASS
174	95	50	100	85.1	79979	PASS
175	174	5	9	7.3	5824	PASS
176	174	95	101	99.5	79589	PASS
177	176	5	9	6.1	4821	PASS