

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032823\
 Data File : VN077231.D
 Acq On : 28 Mar 2023 12:30
 Operator : JC\MD
 Sample : VN0328WBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0328WBL01

Quant Time: Mar 29 01:11:39 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N032523W.M
 Quant Title : SW846 8260
 QLast Update : Mon Mar 27 02:47:06 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.230	168	219362	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.107	114	390030	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.866	117	341966	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.795	152	120839	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	171351	49.959	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	99.920%		
35) Dibromofluoromethane	8.172	113	124073	46.881	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	93.760%		
50) Toluene-d8	10.572	98	485404	48.948	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	97.900%		
62) 4-Bromofluorobenzene	12.854	95	128647	39.528	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	79.060%#		
Target Compounds						Qvalue
3) Chloromethane	2.384	50	923	0.288	ug/l #	40
5) Bromomethane	2.984	94	3659	1.264	ug/l	90
6) Chloroethane	3.219	64	2765	0.880	ug/l #	42
10) Methyl Iodide	4.601	142	583	0.217	ug/l #	79
13) Acrolein	4.190	56	294	0.448	ug/l #	14
15) Acrylonitrile	5.742	53	887	0.609	ug/l #	69
16) Acetone	4.442	43	506	0.397	ug/l #	40
17) Carbon Disulfide	4.731	76	2306	0.364	ug/l #	73
18) Methyl Acetate	5.037	43	1561	0.306	ug/l #	42
20) Methylene Chloride	5.272	84	655	0.231	ug/l #	51
31) Cyclohexane	8.230	56	7482	1.570	ug/l #	40
36) 1,1-Dichloropropene	8.225	75	21516	5.841	ug/l #	49
38) Carbon Tetrachloride	8.230	117	25788	6.905	ug/l #	18
51) 4-Methyl-2-Pentanone	10.442	43	1248	0.299	ug/l #	70
59) 2-Hexanone	11.195	43	2465	0.823	ug/l	81
68) m/p-Xylenes	12.077	106	1104	0.232	ug/l	93
71) Bromoform	12.854	173	2747	1.473	ug/l #	1
74) N-amyl acetate	12.501	43	1471	0.355	ug/l #	57
76) 1,2,3-Trichloropropane	12.854	75	80350	32.778	ug/l #	1
77) Bromobenzene	12.977	156	726	0.332	ug/l #	45
81) trans-1,4-Dichloro-2-b...	12.854	75	80350	94.471	ug/l #	15
82) 4-Chlorotoluene	13.218	91	1597	0.250	ug/l	93
87) 1,3-Dichlorobenzene	13.736	146	1456	0.369	ug/l	89
88) 1,4-Dichlorobenzene	13.736	146	1456	0.368	ug/l	90
89) n-Butylbenzene	14.065	91	2382	0.380	ug/l	90
91) 1,2-Dichlorobenzene	14.112	146	1250	0.317	ug/l	82
92) 1,2-Dibromo-3-Chloropr...	14.724	75	144	0.256	ug/l	92
93) 1,2,4-Trichlorobenzene	15.406	180	1607	5.140	ug/l	76
95) Naphthalene	15.636	128	4991	6.595	ug/l #	78
96) 1,2,3-Trichlorobenzene	15.842	180	2235	5.721	ug/l #	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032823\
Data File : VN077231.D
Acq On : 28 Mar 2023 12:30
Operator : JC\MD
Sample : VN0328WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0328WBL01

Quant Time: Mar 29 01:11:39 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N032523W.M
Quant Title : SW846 8260
QLast Update : Mon Mar 27 02:47:06 2023
Response via : Initial Calibration

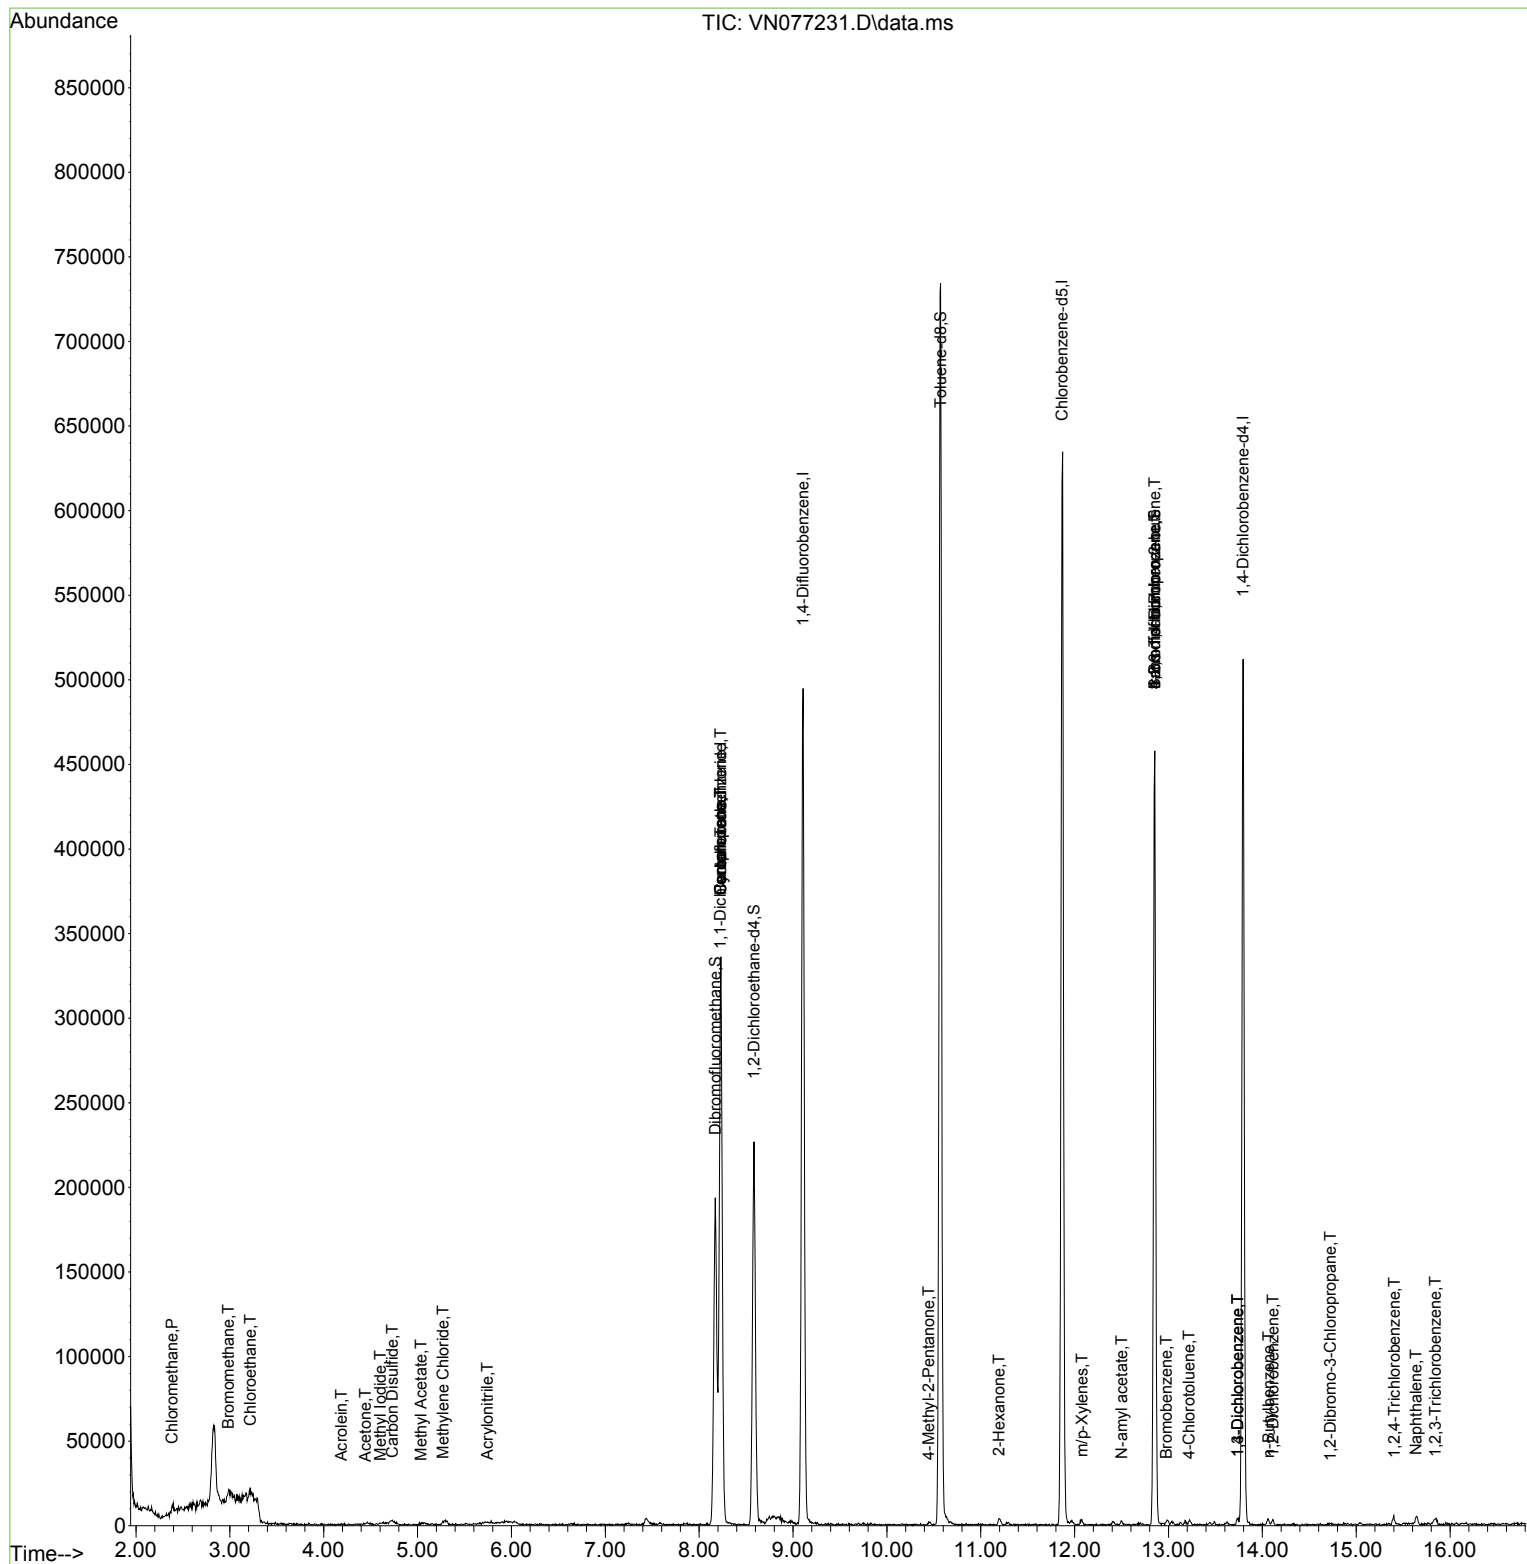



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.230 min Scan# 1

Delta R.T. -0.001 min

Lab File: VN077231.D

Acq: 28 Mar 2023 12:30

Instrument :

MSVOA_N

ClientSampleId :





VN0328WBL01

Tgt Ion:168 Resp: 219362

Ion Ratio Lower Upper

168 100

99 57.2 48.6 73.0

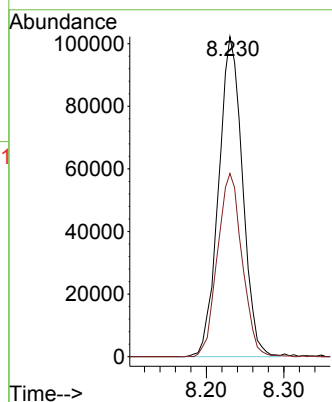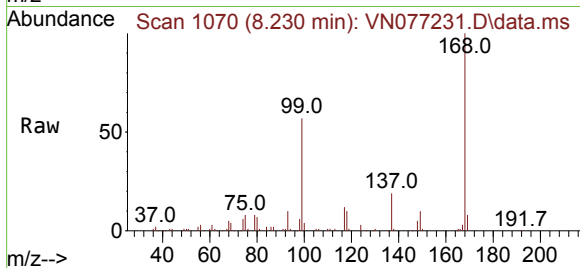

#3

Chloromethane

Concen: 0.288 ug/l

RT: 2.384 min Scan# 76

Delta R.T. 0.012 min

Lab File: VN077231.D




Acq: 28 Mar 2023 12:30


Tgt Ion: 50 Resp: 923

Ion Ratio Lower Upper

50 100

52 0.0 27.9 41.9#


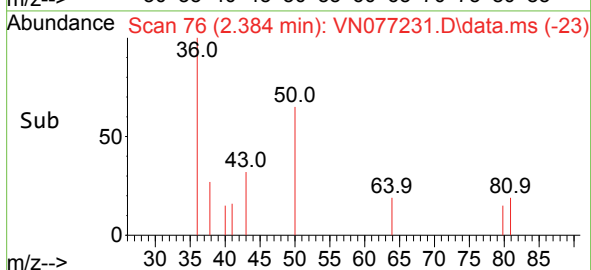

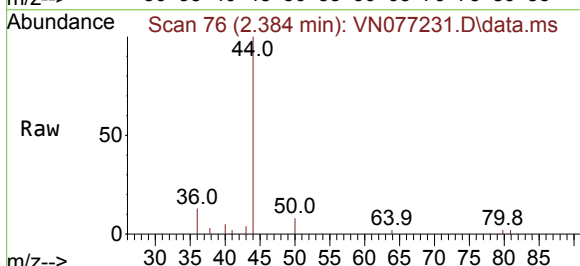




#5
Bromomethane
Concen: 1.264 ug/l
RT: 2.984 min Scan# 11
Delta R.T. 0.041 min
Lab File: VN077231.D
Acq: 28 Mar 2023 12:30




Instrument :
MSVOA_N
ClientSampleId :
VN0328WBL01


Tgt Ion: 94 Resp: 3659
Ion Ratio Lower Upper
94 100
96 89.0 79.0 118.6

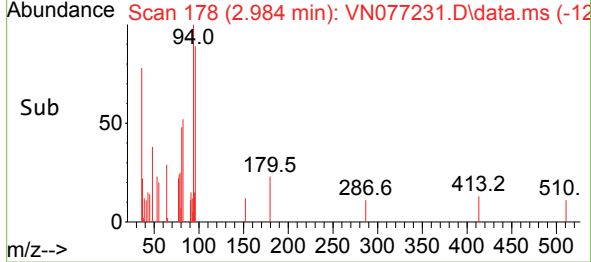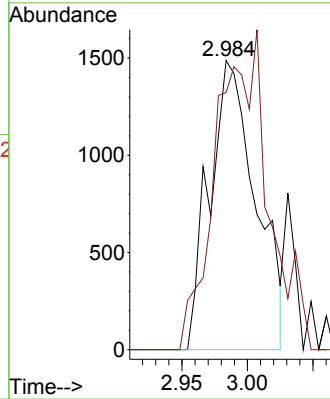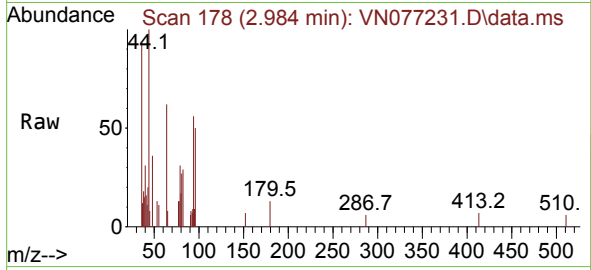

#6
Chloroethane
Concen: 0.880 ug/l
RT: 3.219 min Scan# 218
Delta R.T. 0.094 min
Lab File: VN077231.D
Acq: 28 Mar 2023 12:30


Tgt Ion: 64 Resp: 2765
Ion Ratio Lower Upper
64 100
66 0.0 26.2 39.4#

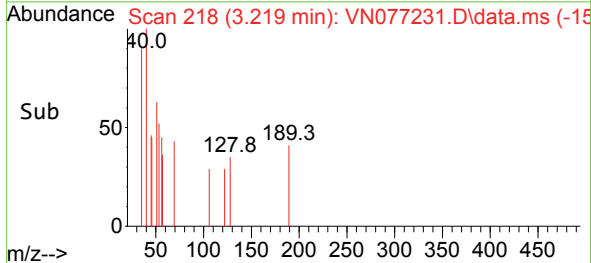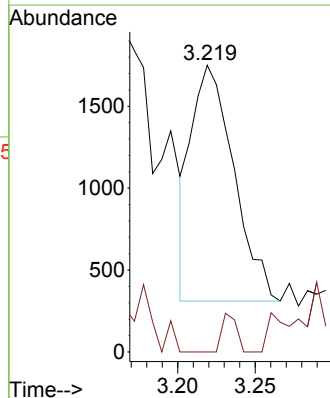






#10
Methyl Iodide
Concen: 0.217 ug/l
RT: 4.601 min Scan# 411
Delta R.T. -0.001 min
Lab File: VN077231.D
Acq: 28 Mar 2023 12:30


Instrument :
MSVOA_N
ClientSampleId :
VN0328WBL01





Tgt Ion:142 Resp: 583
Ion Ratio Lower Upper
142 100
127 32.9 35.2 52.8#
141 0.0 10.2 15.2#




#13
Acrolein
Concen: 0.448 ug/l
RT: 4.190 min Scan# 383
Delta R.T. -0.000 min
Lab File: VN077231.D
Acq: 28 Mar 2023 12:30



Tgt Ion: 56 Resp: 294
Ion Ratio Lower Upper
56 100
55 0.0 56.7 85.1#



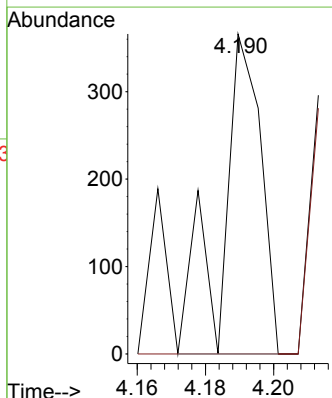





#15
Acrylonitrile
Concen: 0.609 ug/l
RT: 5.742 min Scan# 645
Delta R.T. 0.011 min
Lab File: VN077231.D
Acq: 28 Mar 2023 12:30




Instrument :
MSVOA_N
ClientSampleId :
VN0328WBL01


Tgt Ion: 53 Resp: 887
Ion Ratio Lower Upper
53 100
52 65.6 65.3 97.9
51 0.0 28.8 43.2#

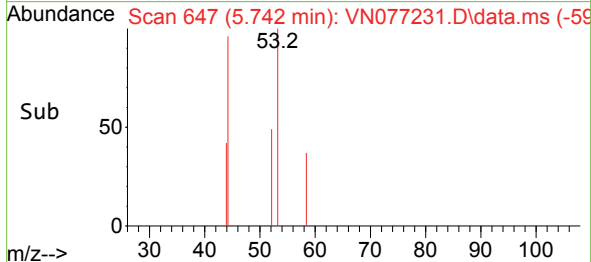

#16
Acetone
Concen: 0.397 ug/l
RT: 4.442 min Scan# 426
Delta R.T. 0.005 min
Lab File: VN077231.D
Acq: 28 Mar 2023 12:30

Tgt Ion: 43 Resp: 506
Ion Ratio Lower Upper
43 100
58 0.0 28.2 42.2#




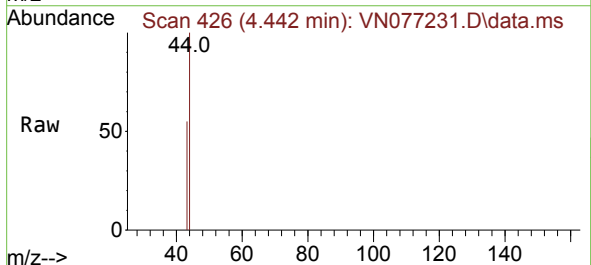




#17
Carbon Disulfide
Concen: 0.364 ug/l
RT: 4.731 min Scan# 41
Delta R.T. 0.006 min
Lab File: VN077231.D
Acq: 28 Mar 2023 12:30




Instrument :
MSVOA_N
ClientSampleId :
VN0328WBL01


Tgt Ion: 76 Resp: 2306
Ion Ratio Lower Upper
76 100
78 0.0 7.8 11.8#

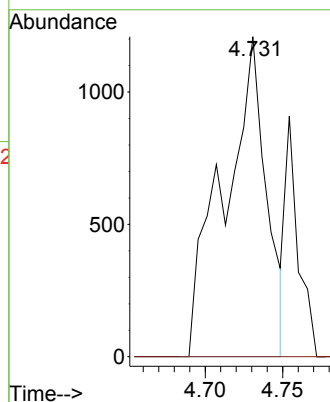

#18
Methyl Acetate
Concen: 0.306 ug/l
RT: 5.037 min Scan# 527
Delta R.T. -0.000 min
Lab File: VN077231.D
Acq: 28 Mar 2023 12:30

Tgt Ion: 43 Resp: 1561
Ion Ratio Lower Upper
43 100
74 0.0 25.9 38.9#

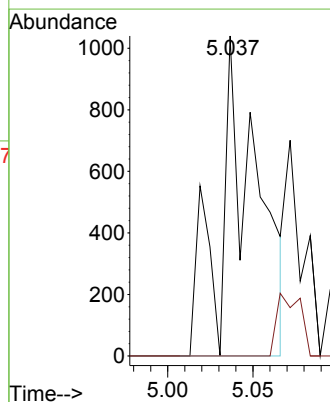







#20
Methylene Chloride
Concen: 0.231 ug/l
RT: 5.272 min Scan# 51
Delta R.T. -0.012 min
Lab File: VN077231.D
Acq: 28 Mar 2023 12:30

Instrument :
MSVOA_N
ClientSampleId :
VN0328WBL01

Tgt Ion: 84 Resp: 655




Ion	Ratio	Lower	Upper
84	100		
49	33.0	76.6	114.8#
51	30.3	25.4	38.2
86	26.4	51.1	76.7#

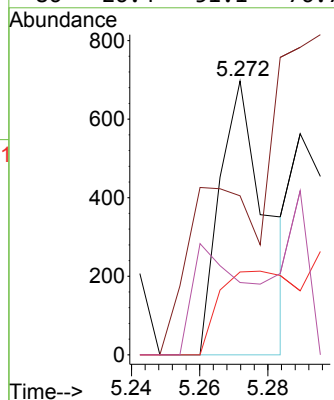


#31
Cyclohexane
Concen: 1.570 ug/l
RT: 8.230 min Scan# 1070
Delta R.T. -0.030 min
Lab File: VN077231.D
Acq: 28 Mar 2023 12:30

Tgt Ion: 56 Resp: 7482

Ion	Ratio	Lower	Upper
56	100		
69	117.3	27.0	40.6#
84	71.2	82.9	124.3#

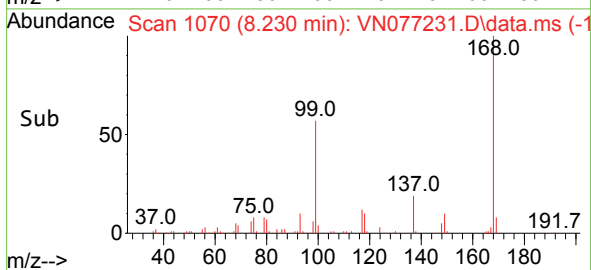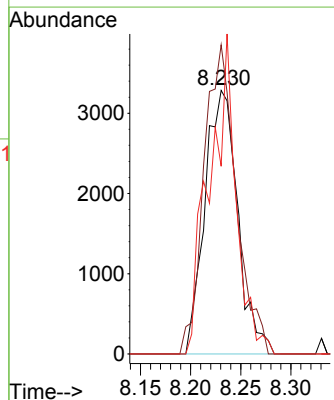



#33

1,2-Dichloroethane-d4

Concen: 49.959 ug/l

RT: 8.583 min Scan# 1130

Delta R.T. -0.001 min

Lab File: VN077231.D

Acq: 28 Mar 2023 12:30

Instrument :

MSVOA_N

ClientSampleId :





VN0328WBL01

Tgt Ion: 65 Resp: 171351

Ion Ratio Lower Upper

65 100

67 50.2 0.0 107.2



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.107 min Scan# 1219

Delta R.T. -0.000 min

Lab File: VN077231.D

Acq: 28 Mar 2023 12:30




Tgt Ion: 114 Resp: 390030


Ion Ratio Lower Upper

114 100

63 21.7 0.0 36.6

88 15.5 0.0 28.6



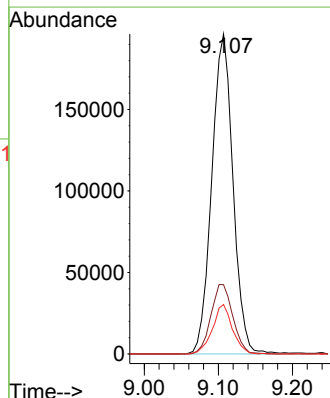





#35
Dibromofluoromethane
Concen: 46.881 ug/l
RT: 8.172 min Scan# 1060
Delta R.T. -0.000 min
Lab File: VN077231.D
Acq: 28 Mar 2023 12:30




Instrument :
MSVOA_N
ClientSampleId :
VN0328WBL01


Tgt Ion:113 Resp: 124073
Ion Ratio Lower Upper
113 100
111 103.9 81.8 122.8
192 18.4 13.9 20.9

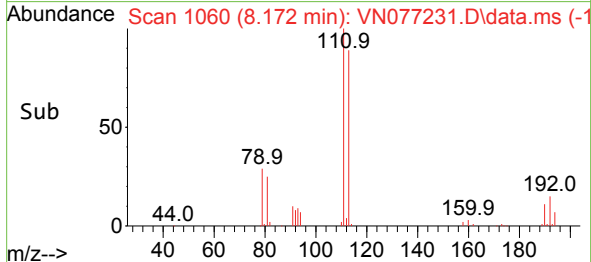

#36
1,1-Dichloropropene
Concen: 5.841 ug/l
RT: 8.225 min Scan# 1069
Delta R.T. -0.153 min
Lab File: VN077231.D
Acq: 28 Mar 2023 12:30

Tgt Ion: 75 Resp: 21516
Ion Ratio Lower Upper
75 100
110 9.4 18.9 56.9#
77 0.0 24.9 37.3#

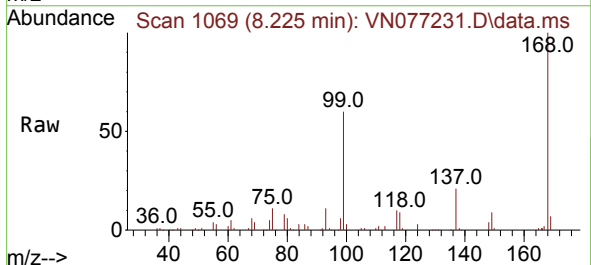



#38

Carbon Tetrachloride

Concen: 6.905 ug/l

RT: 8.230 min Scan# 1

Delta R.T. -0.142 min

Lab File: VN077231.D

Acq: 28 Mar 2023 12:30

Instrument :

MSVOA_N

ClientSampleId :

VN0328WBL01





Tgt Ion:117 Resp: 25788

Ion Ratio Lower Upper

117 100

119 7.2 76.9 115.3#

121 0.0 23.2 34.8#



#50

Toluene-d8

Concen: 48.948 ug/l

RT: 10.572 min Scan# 1468

Delta R.T. -0.000 min

Lab File: VN077231.D




Acq: 28 Mar 2023 12:30


Tgt Ion: 98 Resp: 485404

Ion Ratio Lower Upper

98 100

100 62.0 52.8 79.2


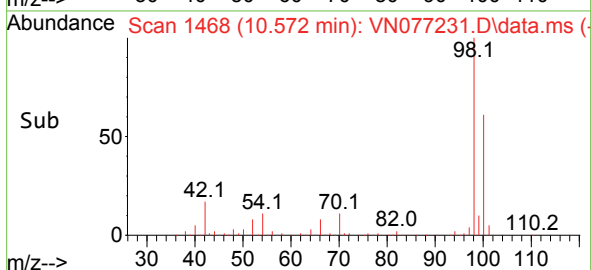




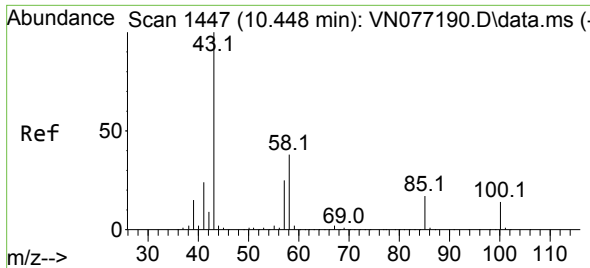

#51
4-Methyl-2-Pentanone
Concen: 0.299 ug/l
RT: 10.442 min Scan# 1446
Delta R.T. -0.006 min
Lab File: VN077231.D
Acq: 28 Mar 2023 12:30




Instrument :
MSVOA_N
ClientSampleId :
VN0328WBL01


Tgt Ion: 43 Resp: 1248
Ion Ratio Lower Upper
43 100
58 26.6 37.4 56.0#

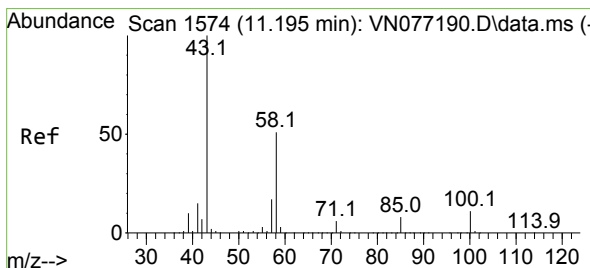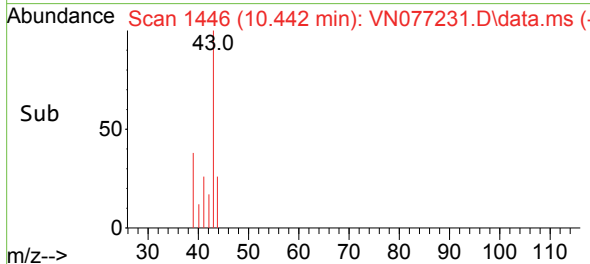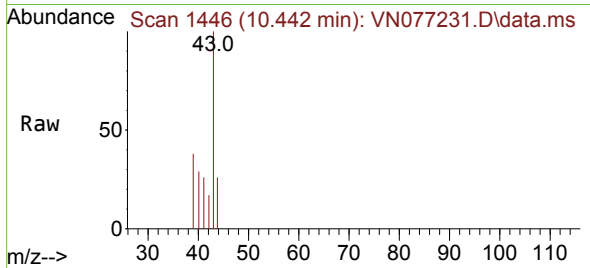

#59
2-Hexanone
Concen: 0.823 ug/l
RT: 11.195 min Scan# 1574
Delta R.T. -0.000 min
Lab File: VN077231.D
Acq: 28 Mar 2023 12:30

Tgt Ion: 43 Resp: 2465
Ion Ratio Lower Upper
43 100
58 50.0 32.6 98.0


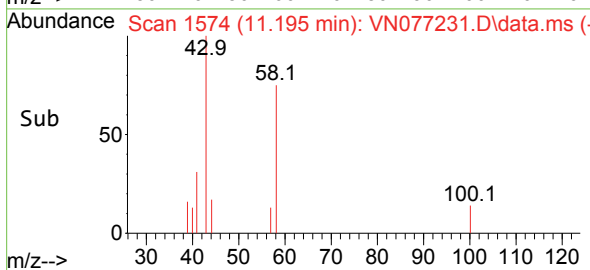

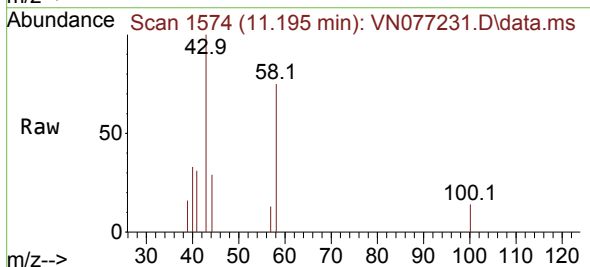




#62
4-Bromofluorobenzene
Concen: 39.528 ug/l
RT: 12.854 min Scan# 1856
Delta R.T. 0.006 min
Lab File: VN077231.D
Acq: 28 Mar 2023 12:30




Instrument :
MSVOA_N
ClientSampleId :
VN0328WBL01


Tgt Ion: 95 Resp: 128647
Ion Ratio Lower Upper
95 100
174 86.1 0.0 162.4
176 81.1 0.0 157.4

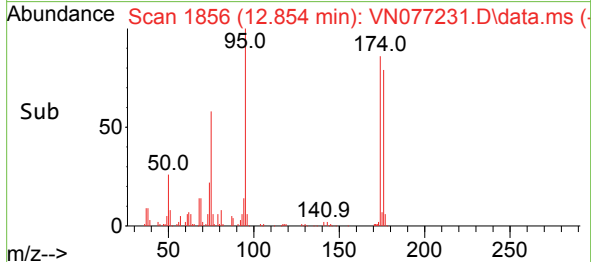

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.866 min Scan# 1688
Delta R.T. -0.000 min
Lab File: VN077231.D
Acq: 28 Mar 2023 12:30

Tgt Ion: 117 Resp: 341966
Ion Ratio Lower Upper
117 100
82 54.4 43.5 65.3
119 27.7 25.5 38.3




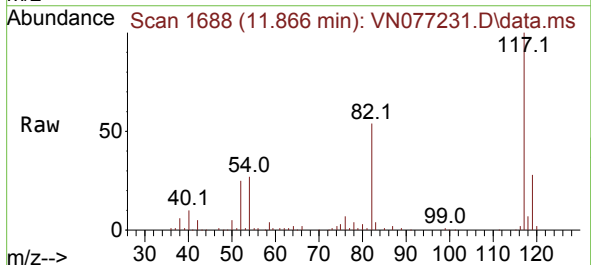




#68
m/p-Xylenes
Concen: 0.232 ug/l
RT: 12.077 min Scan# 11
Delta R.T. 0.005 min
Lab File: VN077231.D
Acq: 28 Mar 2023 12:30




Instrument :
MSVOA_N
ClientSampleId :
VN0328WBL01


Tgt Ion:106 Resp: 1104
Ion Ratio Lower Upper
106 100
91 186.9 158.0 237.0

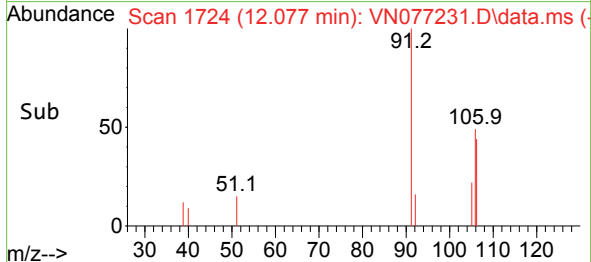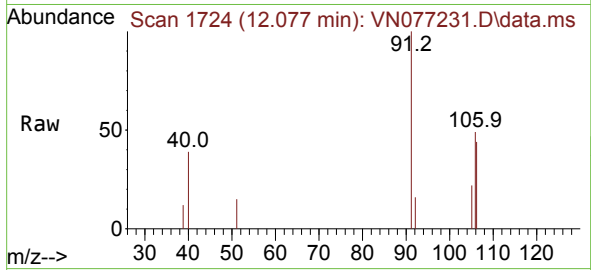

#71
Bromoform
Concen: 1.473 ug/l
RT: 12.854 min Scan# 1856
Delta R.T. 0.271 min
Lab File: VN077231.D
Acq: 28 Mar 2023 12:30

Tgt Ion:173 Resp: 2747
Ion Ratio Lower Upper
173 100
175 310.2 24.9 74.6#
254 0.0 0.0 0.0





#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.795 min Scan# 2016

Delta R.T. -0.000 min

Lab File: VN077231.D

Acq: 28 Mar 2023 12:30

Instrument :

MSVOA_N

ClientSampleId :

VN0328WBL01





Tgt Ion:152 Resp: 120839

Ion Ratio Lower Upper

152 100

115 58.9 30.3 90.9

150 160.2 0.0 353.6

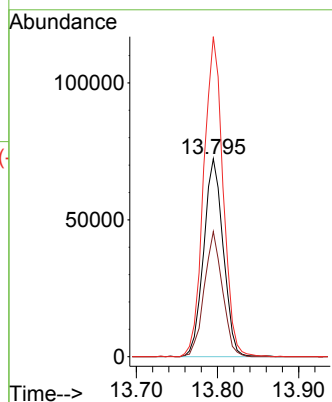

#74

N-ethyl acetate

Concen: 0.355 ug/l

RT: 12.501 min Scan# 1796

Delta R.T. 0.006 min

Lab File: VN077231.D

Acq: 28 Mar 2023 12:30

Tgt Ion: 43 Resp: 1471




Ion Ratio Lower Upper


43 100

70 10.3 46.8 70.2#

55 6.9 23.4 35.2#

61 30.5 23.8 35.8

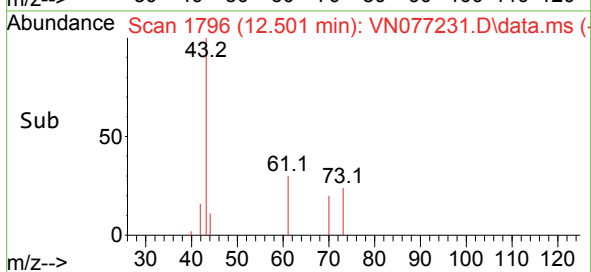



#76

1,2,3-Trichloropropane

Concen: 32.778 ug/l

RT: 12.854 min Scan# 1856

Delta R.T. -0.141 min

Lab File: VN077231.D

Acq: 28 Mar 2023 12:30

Instrument :

MSVOA_N

ClientSampleId :





VN0328WBL01

Tgt Ion: 75 Resp: 80350

Ion Ratio Lower Upper

75 100

77 1.1 93.8 281.4#

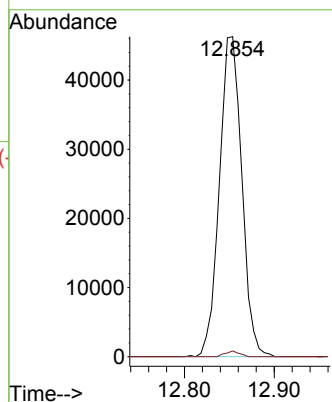

#77

Bromobenzene

Concen: 0.332 ug/l

RT: 12.977 min Scan# 1877

Delta R.T. -0.006 min

Lab File: VN077231.D

Acq: 28 Mar 2023 12:30




Tgt Ion: 156 Resp: 726


Ion Ratio Lower Upper

156 100

77 137.5 101.3 303.7

158 16.8 48.9 146.7#


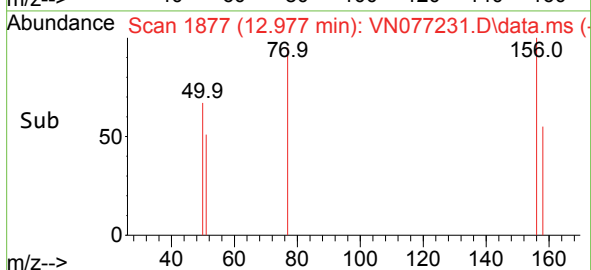






#81
trans-1,4-Dichloro-2-butene
Concen: 94.471 ug/l
RT: 12.854 min Scan# 1856
Delta R.T. 0.118 min
Lab File: VN077231.D
Acq: 28 Mar 2023 12:30




Instrument :
MSVOA_N
ClientSampleId :
VN0328WBL01


Tgt Ion: 75 Resp: 80350
Ion Ratio Lower Upper
75 100
53 0.1 67.4 101.0#
89 0.0 39.5 59.3#



#82
4-Chlorotoluene
Concen: 0.250 ug/l
RT: 13.218 min Scan# 1918
Delta R.T. -0.006 min
Lab File: VN077231.D
Acq: 28 Mar 2023 12:30

Tgt Ion: 91 Resp: 1597
Ion Ratio Lower Upper
91 100
126 40.4 18.0 54.0









#87
 1,3-Dichlorobenzene
 Concen: 0.369 ug/l
 RT: 13.736 min Scan# 2006
 Delta R.T. 0.000 min
 Lab File: VN077231.D
 Acq: 28 Mar 2023 12:30




Instrument :
 MSVOA_N
 ClientSampleId :
 VN0328WBL01


Tgt Ion:146 Resp: 1456
 Ion Ratio Lower Upper
 146 100
 111 35.9 20.4 61.2
 148 73.4 31.5 94.5

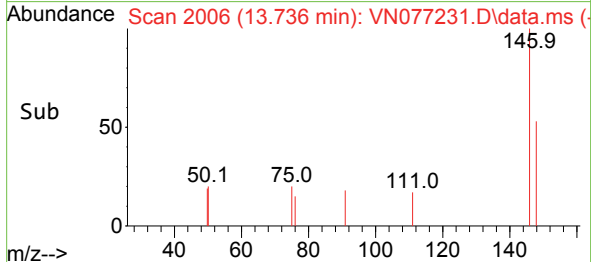

#88
 1,4-Dichlorobenzene
 Concen: 0.368 ug/l
 RT: 13.736 min Scan# 2006
 Delta R.T. -0.077 min
 Lab File: VN077231.D
 Acq: 28 Mar 2023 12:30

Tgt Ion:146 Resp: 1456
 Ion Ratio Lower Upper
 146 100
 111 35.9 20.0 60.0
 148 73.4 31.8 95.4




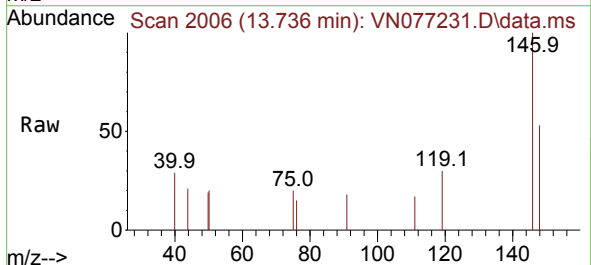


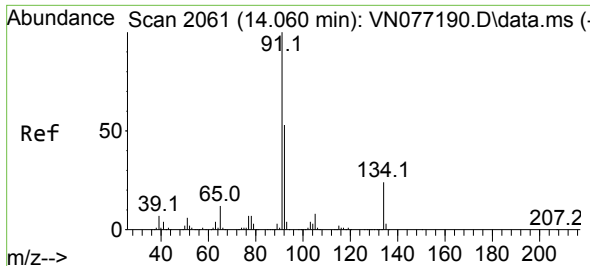

#89
n-Butylbenzene
Concen: 0.380 ug/l
RT: 14.065 min Scan# 2061
Delta R.T. 0.005 min
Lab File: VN077231.D
Acq: 28 Mar 2023 12:30




Instrument :
MSVOA_N
ClientSampleId :
VN0328WBL01


Tgt Ion: 91 Resp: 2382
Ion Ratio Lower Upper
91 100
92 54.4 26.6 79.7
134 13.8 13.6 40.7

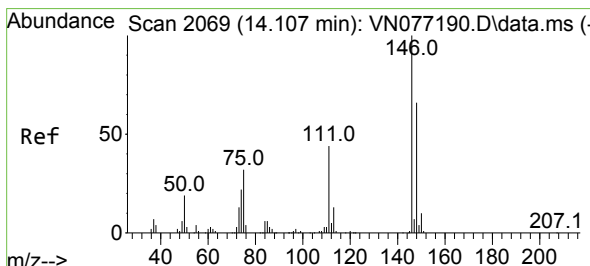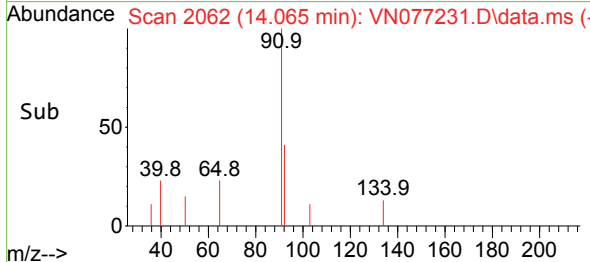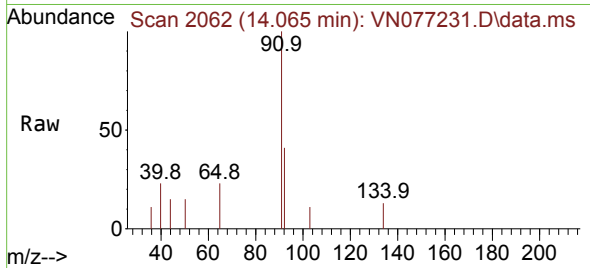

#91
1,2-Dichlorobenzene
Concen: 0.317 ug/l
RT: 14.112 min Scan# 2070
Delta R.T. 0.005 min
Lab File: VN077231.D
Acq: 28 Mar 2023 12:30

Tgt Ion: 146 Resp: 1250
Ion Ratio Lower Upper
146 100
111 48.0 21.4 64.2
148 83.8 32.0 96.0


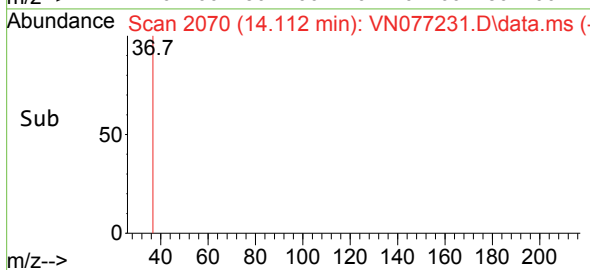

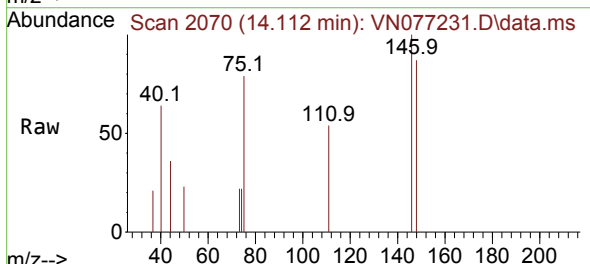


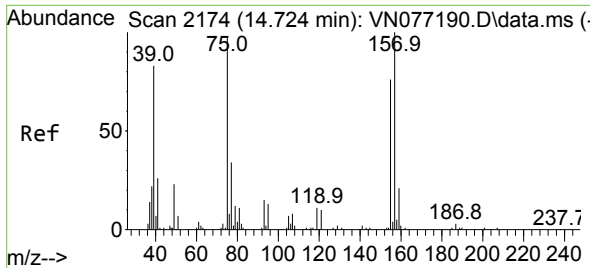

#92
 1,2-Dibromo-3-Chloropropane
 Concen: 0.256 ug/l
 RT: 14.724 min Scan# 2174
 Delta R.T. 0.000 min
 Lab File: VN077231.D
 Acq: 28 Mar 2023 12:30




Instrument :
 MSVOA_N
 ClientSampleId :
 VN0328WBL01


Tgt Ion: 75 Resp: 144
 Ion Ratio Lower Upper
 75 100
 155 91.7 44.3 132.8
 157 129.9 58.3 174.8

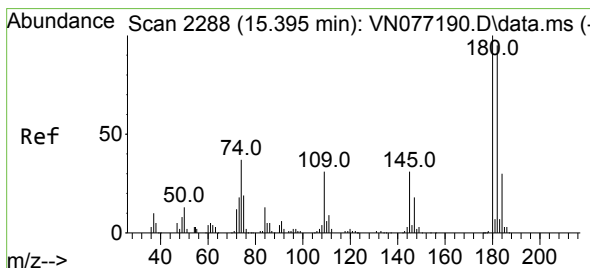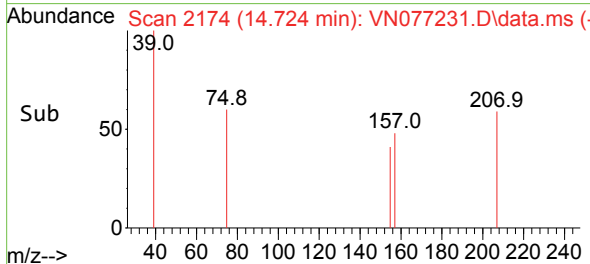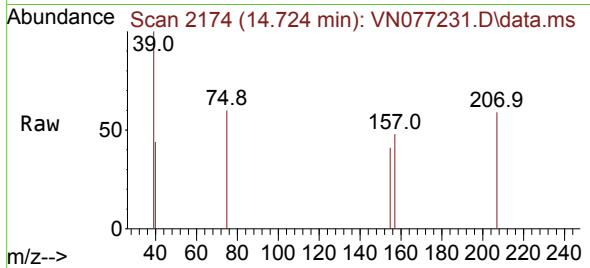

#93
 1,2,4-Trichlorobenzene
 Concen: 5.140 ug/l
 RT: 15.406 min Scan# 2290
 Delta R.T. 0.011 min
 Lab File: VN077231.D
 Acq: 28 Mar 2023 12:30

Tgt Ion: 180 Resp: 1607
 Ion Ratio Lower Upper
 180 100
 182 123.8 47.4 142.2
 145 27.7 15.8 47.3


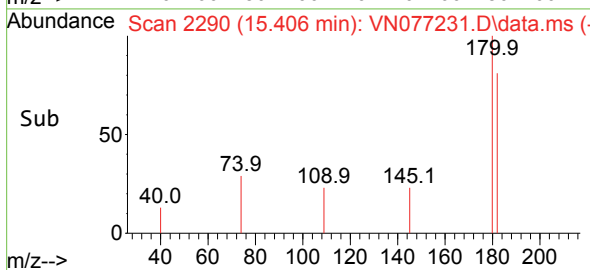

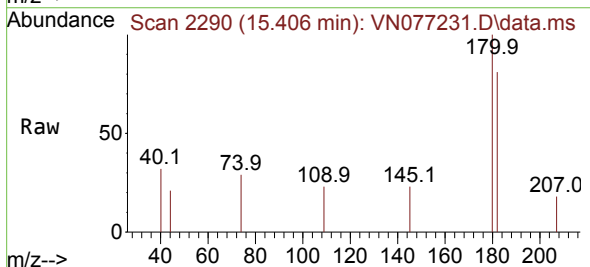


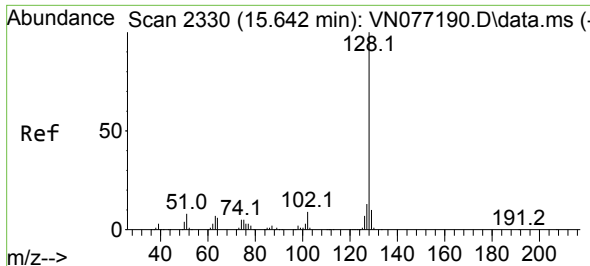

#95
Naphthalene
Concen: 6.595 ug/l
RT: 15.636 min Scan# 2329
Delta R.T. -0.006 min
Lab File: VN077231.D
Acq: 28 Mar 2023 12:30

Instrument :
MSVOA_N
ClientSampleId :
VN0328WBL01

Tgt Ion:128 Resp: 4991
Ion Ratio Lower Upper
128 100
127 4.8 10.2 15.4#
129 2.2 8.9 13.3#

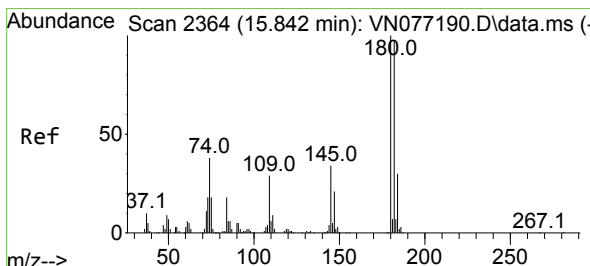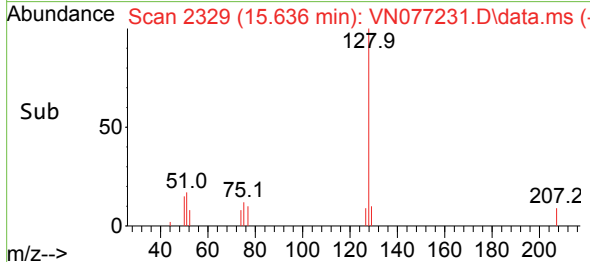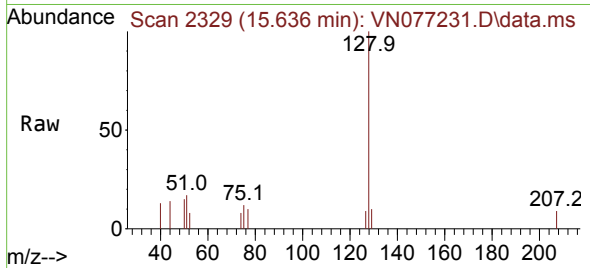

#96
1,2,3-Trichlorobenzene
Concen: 5.721 ug/l
RT: 15.842 min Scan# 2364
Delta R.T. -0.000 min
Lab File: VN077231.D
Acq: 28 Mar 2023 12:30

Tgt Ion:180 Resp: 2235
Ion Ratio Lower Upper
180 100
182 86.4 47.7 143.1
145 8.0 17.0 51.0#

