
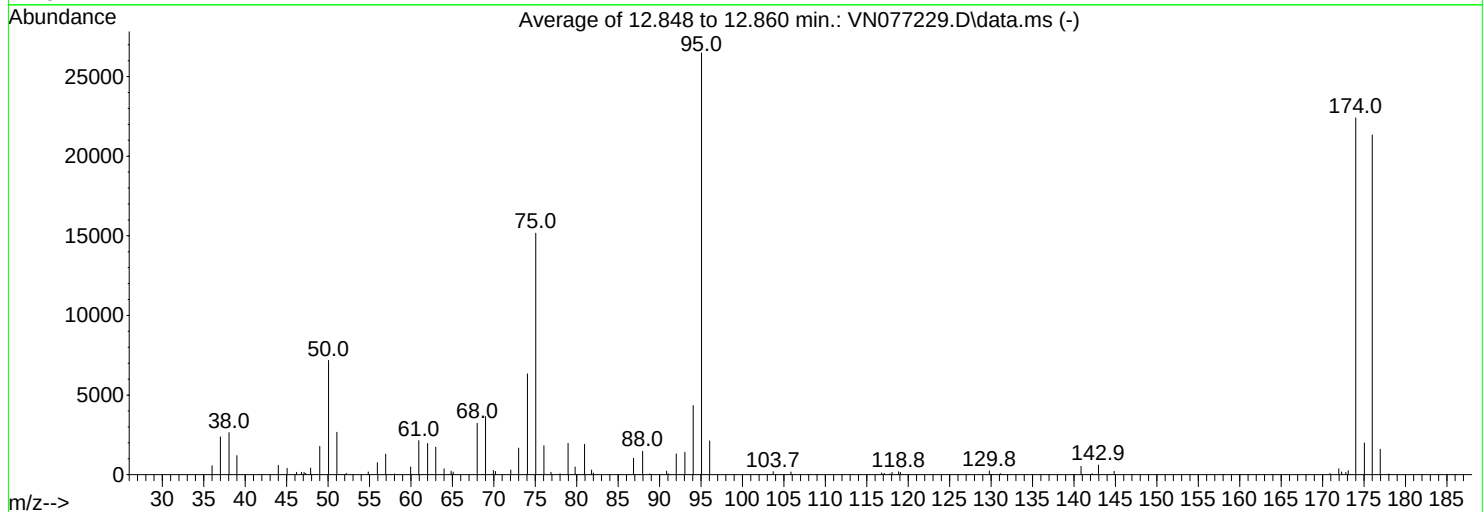


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032823\
Data File : VN077229.D
Acq On : 28 Mar 2023 10:39
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N032523W.M
Title : SW846 8260
Last Update : Mon Mar 27 02:47:06 2023

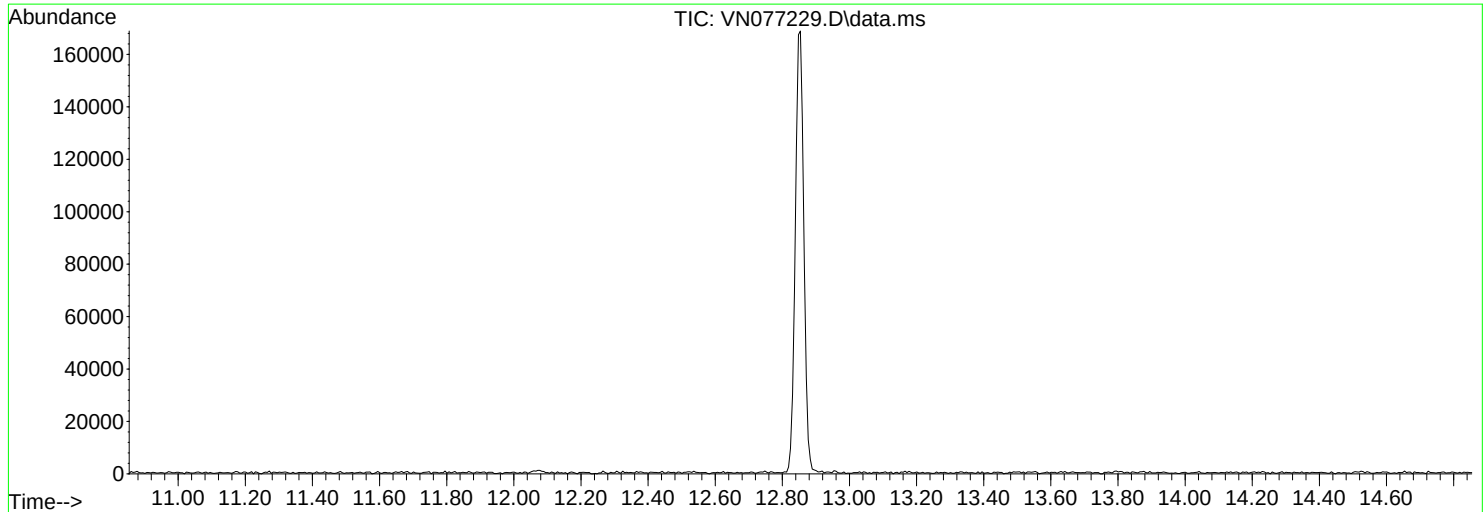

AutoFind: Scans 1855, 1856, 1857; Background Corrected with Scan 1846

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	27.1	7171	PASS
75	95	30	60	57.2	15165	PASS
95	95	100	100	100.0	26493	PASS
96	95	5	9	8.0	2116	PASS
173	174	0.00	2	1.1	248	PASS
174	95	50	100	84.6	22408	PASS
175	174	5	9	8.9	1990	PASS
176	174	95	101	95.2	21339	PASS
177	176	5	9	7.5	1597	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	568	49.00	1782	63.00	1730	75.05	1516
37.00	2369	50.05	7171	64.00	371	76.05	1811
38.05	2645	51.05	2665	64.85	226	76.90	1515
39.00	1200	52.20	83	65.10	158	78.00	58
44.00	582	54.85	175	68.00	3227	78.95	1968
45.05	407	55.95	754	69.00	3648	79.80	480
46.20	145	56.95	1284	69.95	259	80.95	1914
46.80	152	58.00	50	70.20	206	81.80	293
47.10	146	59.95	478	72.05	293	82.00	102
47.30	78	60.95	2143	73.00	1666	86.85	1029
47.90	415	62.00	1959	74.05	6329	87.95	1472

Average of 12.848 to 12.860 min.: VN077229.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
88.80	51	117.10	81	170.90	67		
90.85	219	117.80	50	171.95	369		
91.10	53	118.05	137	172.30	171		
92.00	1304	118.85	179	172.80	145		
93.05	1406	119.05	146	173.10	248		
94.05	4342	129.80	232	174.00	22408		
95.05	26493	131.10	68	175.05	1990		
96.05	2116	140.85	525	176.00	21339		
103.70	194	142.20	60	176.95	1597		
105.85	168	142.95	608	178.00	50		
116.80	106	144.85	215				

Instrument :

MSVOA_N

ClientSampleId :

BFB