
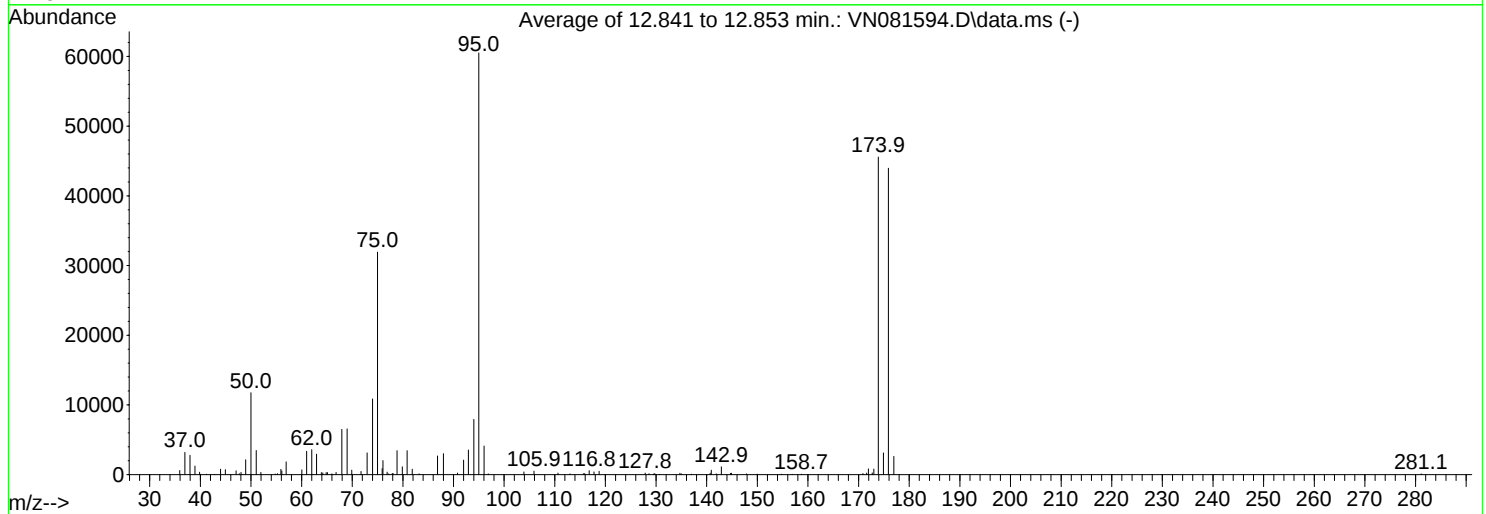


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032824\
Data File : VN081594.D
Acq On : 28 Mar 2024 09:37
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031824W.M
Title : SW846 8260
Last Update : Tue Mar 19 06:00:00 2024

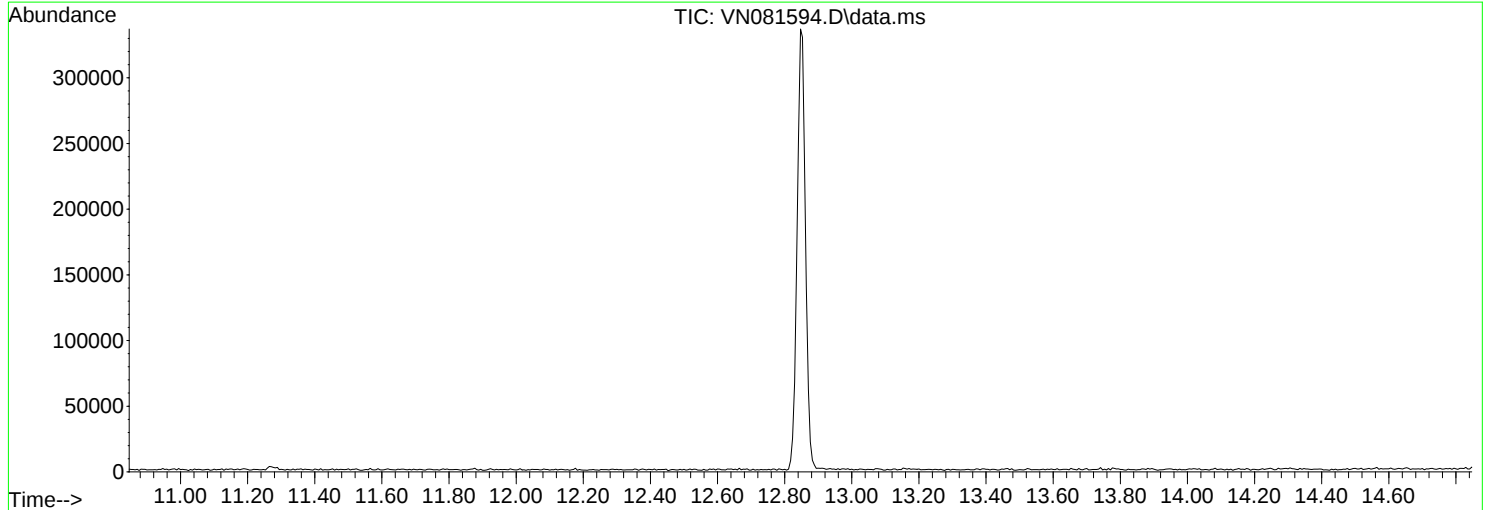

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	11750	PASS
75	95	30	60	52.8	31936	PASS
95	95	100	100	100.0	60520	PASS
96	95	5	9	6.8	4119	PASS
173	174	0.00	2	1.8	813	PASS
174	95	50	100	75.3	45560	PASS
175	174	5	9	6.9	3128	PASS
176	174	95	101	96.5	43973	PASS
177	176	5	9	6.0	2620	PASS

Average of 12.841 to 12.853 min.: VN081594.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	601	48.05	327	61.00	3348	69.90	641
36.95	3192	48.95	2145	62.00	3583	71.75	451
37.95	2780	50.00	11750	62.95	2949	72.95	313
38.95	1237	51.05	3463	63.90	288	74.00	1086
39.85	351	51.95	314	64.20	254	75.00	31936
41.20	72	54.80	92	64.85	301	75.90	873
42.80	51	55.25	149	65.10	296	76.05	2016
44.00	793	55.90	760	66.00	126	76.90	369
44.95	721	56.10	550	66.80	315	77.20	123
47.05	551	56.95	1831	67.95	6498	77.90	150
47.70	143	60.05	679	69.00	6577	78.05	178

Average of 12.841 to 12.853 min.: VN081594.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.85	3454	95.00	60520	118.75	476	141.90	119
79.90	1131	96.05	4119	127.85	228	142.90	1122
80.85	3438	96.85	120	128.60	132	144.70	180
81.85	790	103.90	397	129.50	88	144.90	212
83.20	121	105.90	516	129.75	157	147.85	125
86.85	2694	110.65	226	130.70	55	150.00	61
88.00	3012	113.00	107	134.70	204	154.80	68
90.80	241	115.65	139	135.00	112	156.90	53
92.00	2083	115.90	166	137.00	74	158.70	69
92.95	3527	116.80	573	140.70	200	170.85	158
94.00	7916	117.75	383	140.90	643	171.60	228

Average of 12.841 to 12.853 min.: VN081594.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
171.95	836						
172.70	255						
173.00	813						
173.90	45560						
174.90	3128						
175.90	43973						
176.95	2620						
281.10	116						

Instrument :

MSVOA_N

ClientSampleId :

BFB