


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032825\
Data File : VN086139.D
Acq On : 28 Mar 2025 10:11
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031825W.M
Title : SW846 8260
Last Update : Wed Mar 19 03:20:56 2025

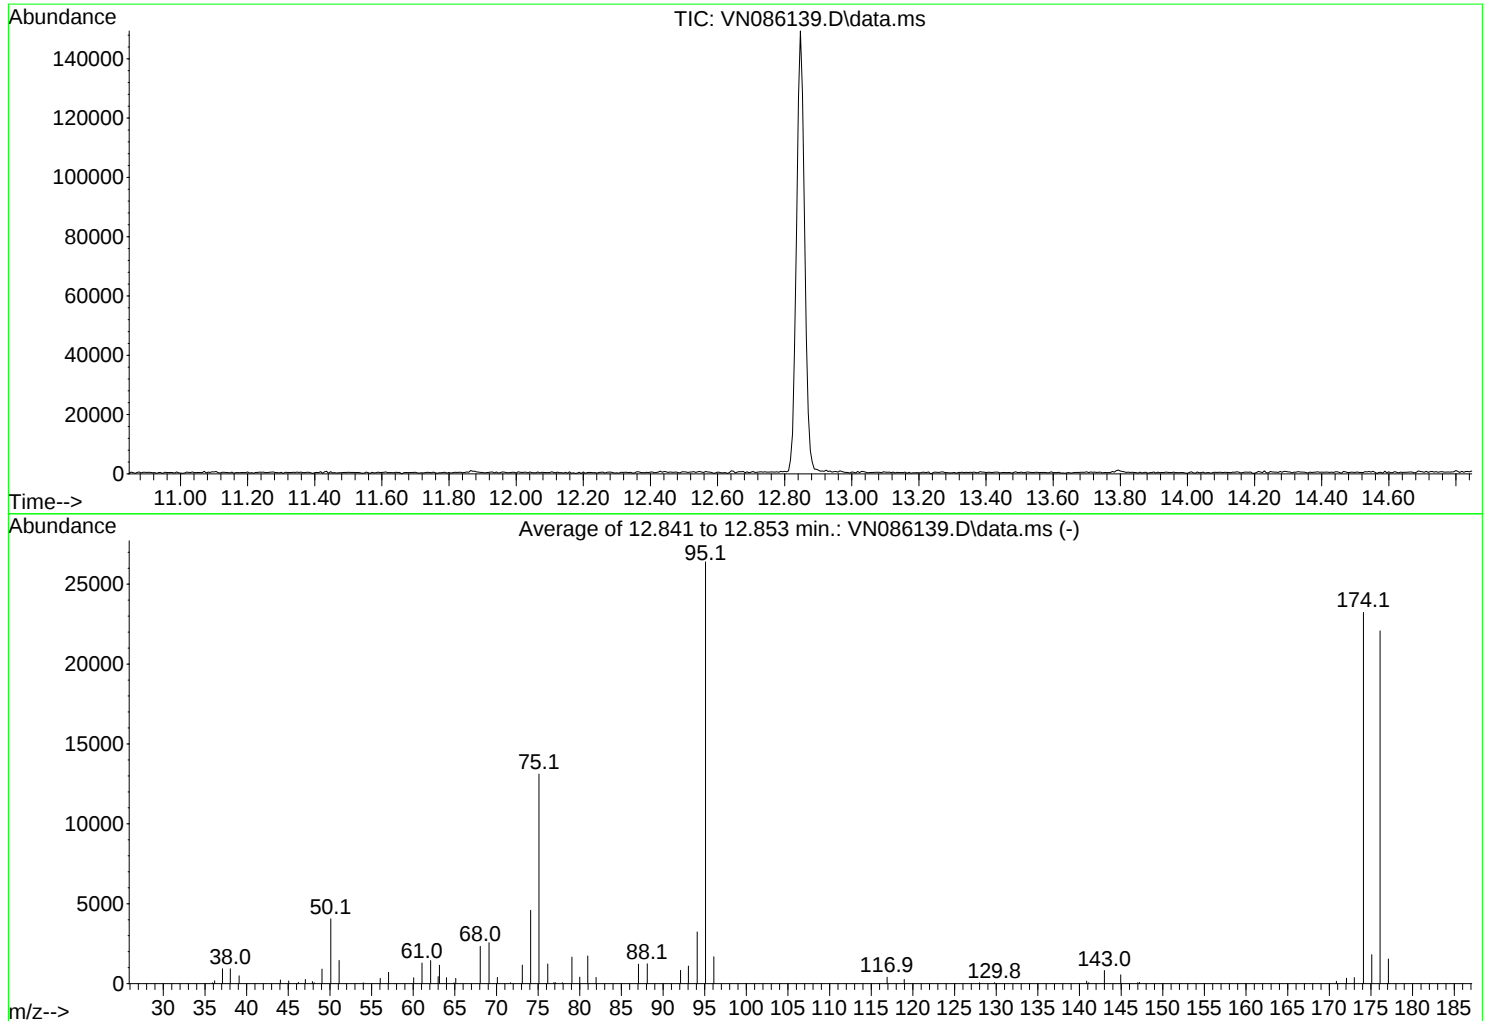

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.4	4056	PASS
75	95	30	60	49.7	13115	PASS
95	95	100	100	100.0	26397	PASS
96	95	5	9	6.4	1678	PASS
173	174	0.00	2	1.6	377	PASS
174	95	50	100	88.0	23235	PASS
175	174	5	9	7.8	1814	PASS
176	174	95	101	95.0	22077	PASS
177	176	5	9	7.0	1546	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	54	49.05	912	64.00	370	76.90	61
36.15	181	50.10	4056	64.90	51	77.10	61
37.10	928	51.10	1449	65.10	333	77.90	51
38.05	934	54.00	55	68.05	2336	79.05	166
39.10	490	56.05	335	69.10	2566	80.00	409
44.05	228	57.05	713	70.10	386	80.95	1736
45.05	167	60.05	370	71.70	61	81.95	386
46.20	84	61.05	1295	73.10	1160	87.05	1220
47.05	264	62.10	1444	74.10	4584	88.10	1244
47.90	135	63.00	440	75.10	13115	92.10	834
48.10	65	63.15	1149	76.15	1232	93.05	1102

Average of 12.841 to 12.853 min.: VN086139.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
94.10	3231	147.00	64				
95.10	26397	147.20	77				
96.10	1678	170.85	149				
116.90	397	172.05	344				
118.95	269	173.00	377				
128.00	57	174.10	23235				
129.80	59	175.10	1814				
140.85	163	176.10	22077				
141.10	58	177.10	1546				
143.00	819						
144.95	554						

Instrument :

MSVOA_N

ClientSampleId :

BFB