

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN032919\
 Data File : VN054787.D
 Acq On : 29 Mar 2019 22:50
 Operator : JC/SP
 Sample : K1698-04
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 TR-05-032819

Quant Time: Mar 30 22:12:48 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N032919W.M
 Quant Title : SW846 8260
 QLast Update : Sat Mar 30 00:48:18 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	533597	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	856038	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	738413	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.35	152	277029	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.03	65	352504	49.01	ug/l	0.00
Spiked Amount 50.000			Recovery	=	98.02%	
35) Dibromofluoromethane	7.59	113	273414	47.91	ug/l	0.00
Spiked Amount 50.000			Recovery	=	95.82%	
50) Toluene-d8	10.09	98	1034850	48.77	ug/l	0.00
Spiked Amount 50.000			Recovery	=	97.54%	
62) 4-Bromofluorobenzene	12.40	95	321988	45.63	ug/l	0.00
Spiked Amount 50.000			Recovery	=	91.26%	
Target Compounds						
16) Acetone	3.82	43	11414	6.654	ug/l #	83
20) Methylene Chloride	4.54	84	23489	3.882	ug/l #	84
43) Isopropyl Acetate	8.17	43	15360	1.616	ug/l #	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN032919\
Data File : VN054787.D
Acq On : 29 Mar 2019 22:50
Operator : JC/SP
Sample : K1698-04
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
TR-05-032819

Quant Time: Mar 30 22:12:48 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N032919W.M
Quant Title : SW846 8260
QLast Update : Sat Mar 30 00:48:18 2019
Response via : Initial Calibration

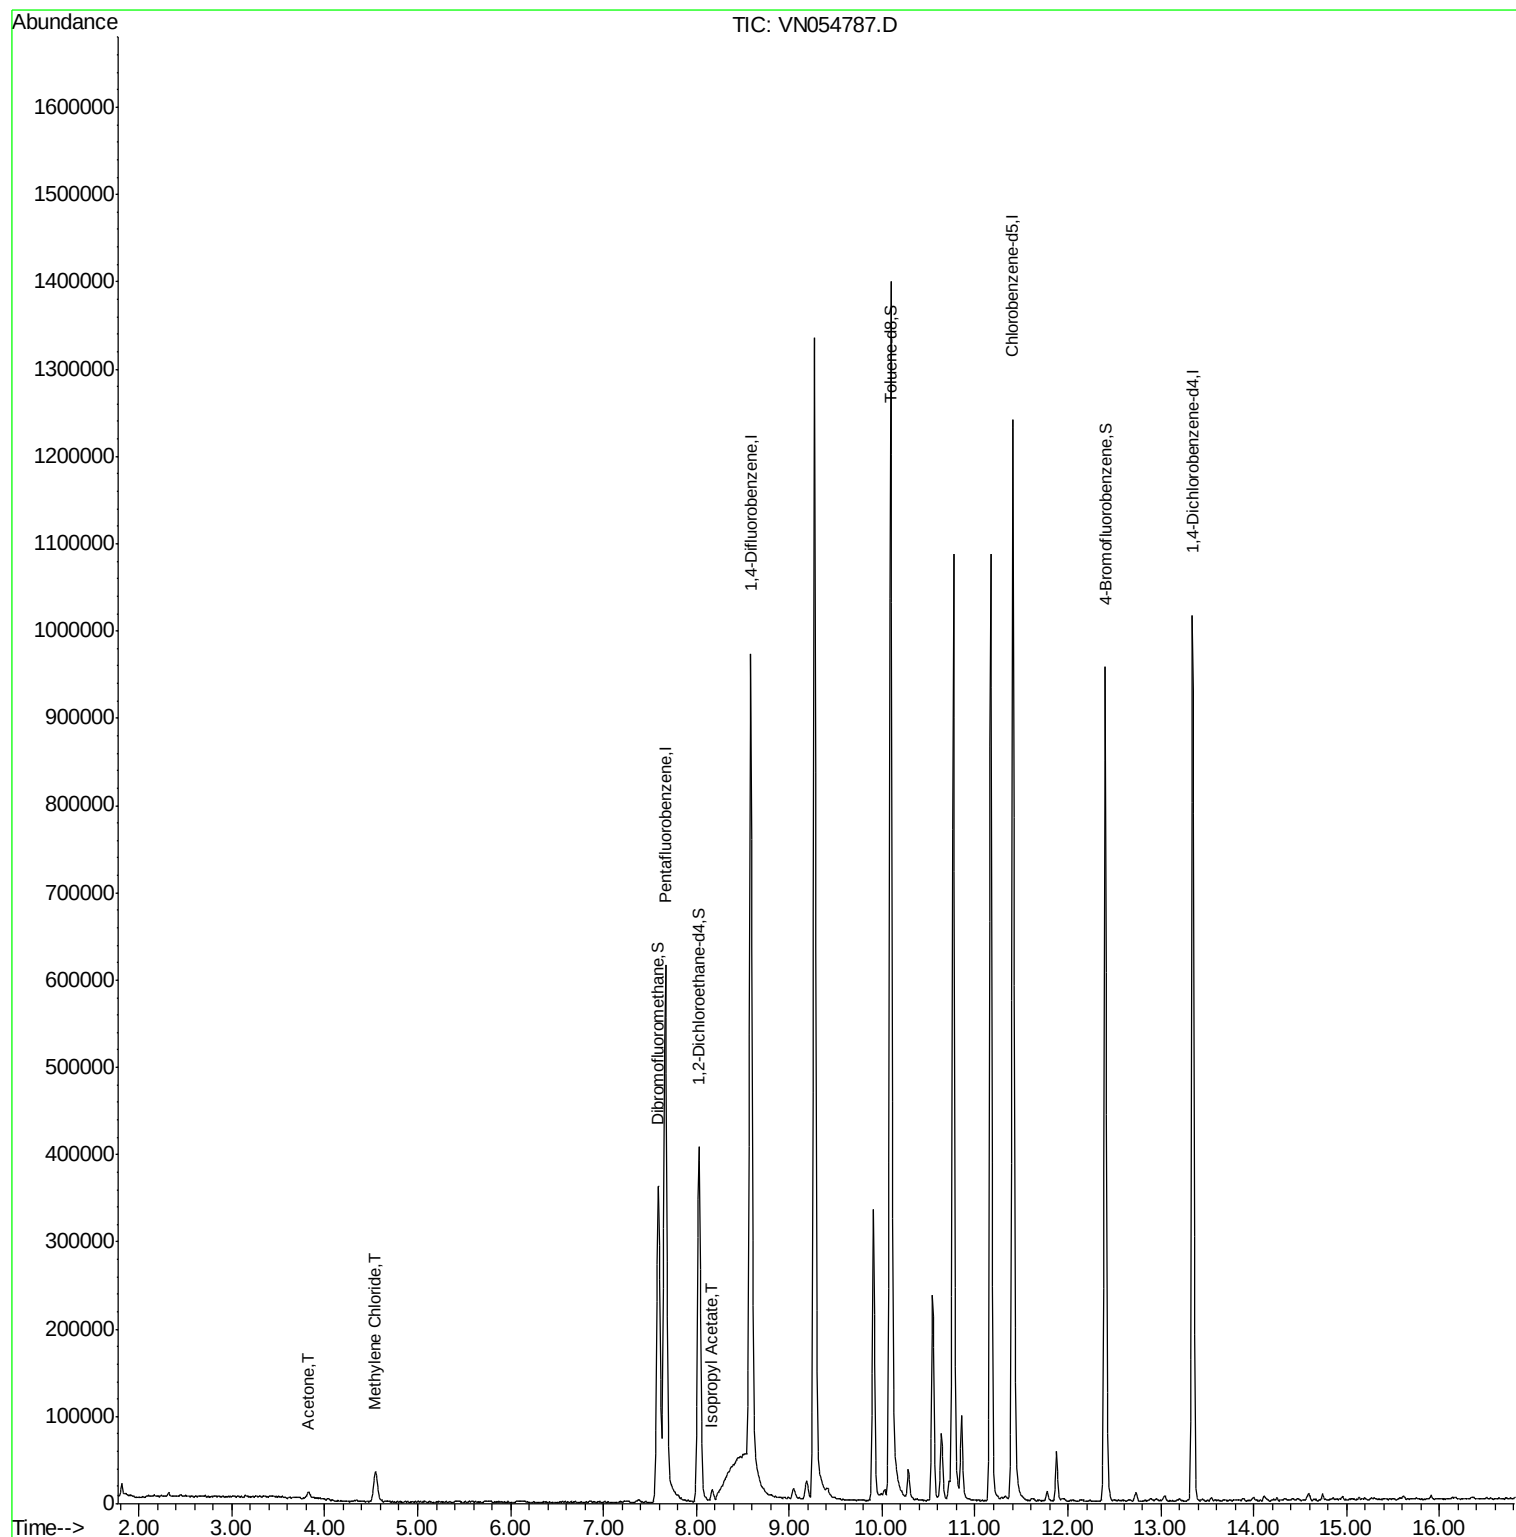

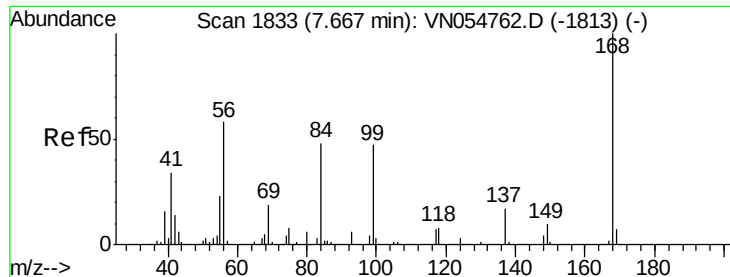

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.67 min Scan# 1833

Delta R.T. -0.00 min

Lab File: VN054787.D

Acq: 29 Mar 2019 22:50

Instrument :

MSVOA_N

ClientSampleId :


TR-05-032819

Tot Ion:168 Resp: 533597

Ion Ratio Lower Upper

168 100

99 55.1 37.1 55.7

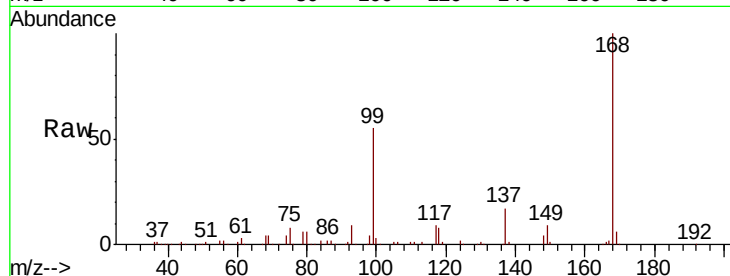

Abundance Ion 167.90 (167.60 to 168.60): VN054787.D (-1740) (-)

Ion 98.90 (98.60 to 99.60): VN054787.D (-1740) (-)

7.67

250000

200000



150000

100000

50000

0

Time--> 7.50 7.60 7.70 7.80

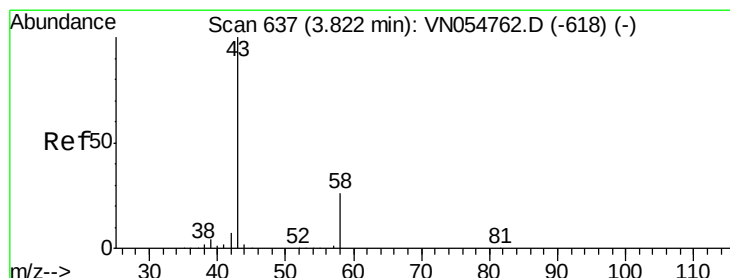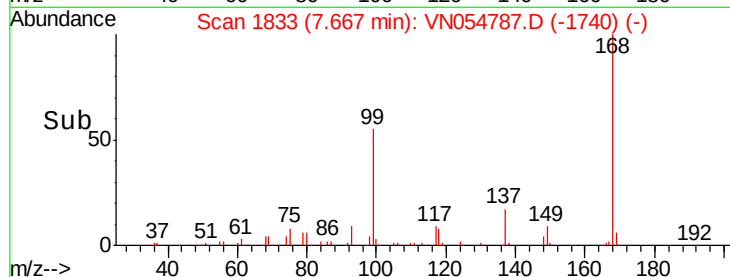

#16

Acetone

Concen: 6.654 ug/l

RT: 3.82 min Scan# 637

Delta R.T. -0.00 min

Lab File: VN054787.D


Acq: 29 Mar 2019 22:50

Tgt Ion: 43 Resp: 11414

Ion Ratio Lower Upper

43 100

58 27.5 29.9 44.9#

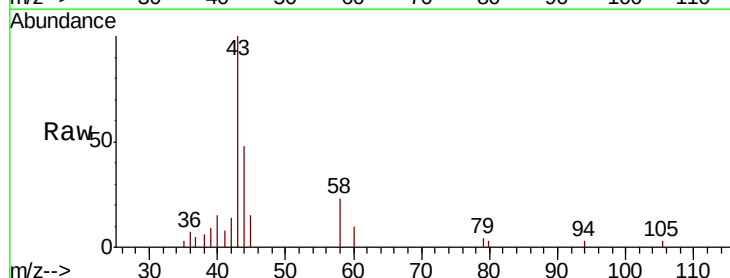

Abundance Ion 43.00 (42.70 to 43.70): VN054787.D (-544) (-)

Ion 58.00 (57.70 to 58.70): VN054787.D (-544) (-)

3.82

5000

4000


3000


2000

1000

0

Time--> 3.75 3.80 3.85 3.90




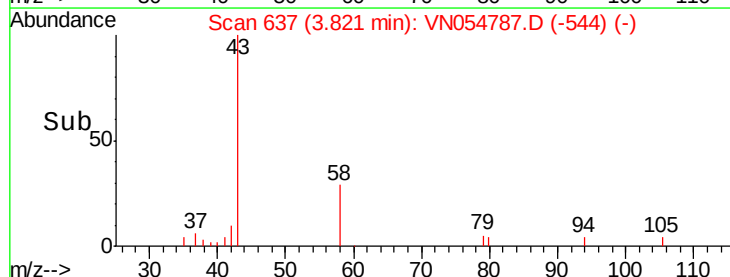


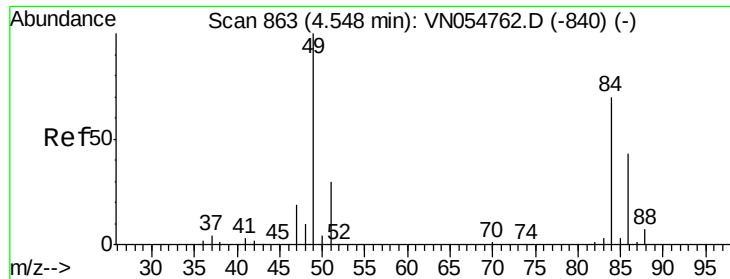

#20
Methylene Chloride
Concen: 3.882 ug/l
RT: 4.54 min Scan# 862
Delta R.T. -0.00 min
Lab File: VN054787.D
Acq: 29 Mar 2019 22:50




Instrument :
MSVOA_N
ClientSampled :
TR-05-032819


Tot Ion: 84 Resp: 23489
Ion Ratio Lower Upper
84 100
49 140.4 89.7 134.5#
51 39.4 28.2 42.4
86 62.3 50.8 76.2

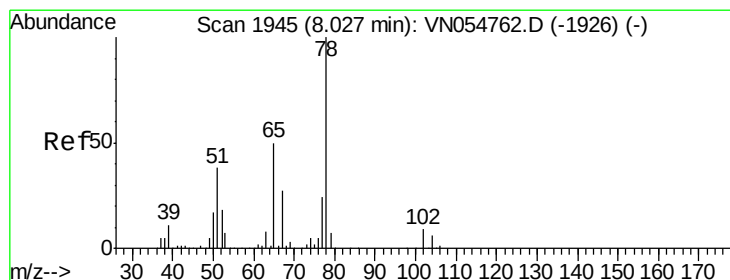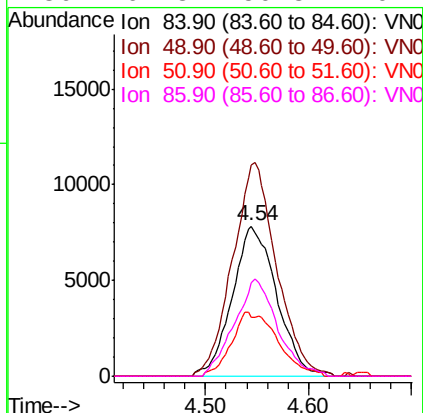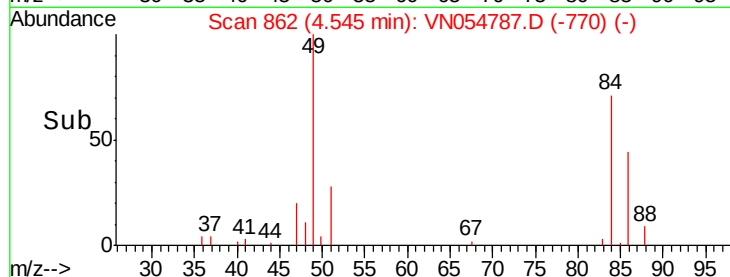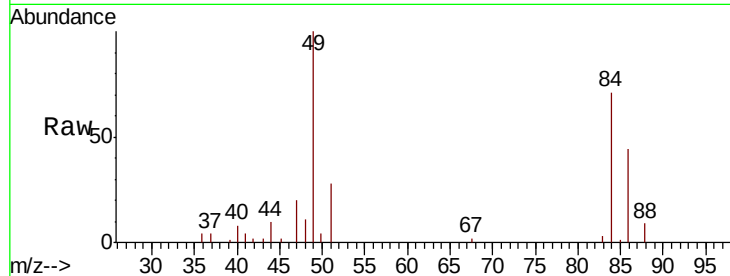

#33
1,2-Dichloroethane-d4
Concen: 49.006 ug/l
RT: 8.03 min Scan# 1946
Delta R.T. 0.00 min
Lab File: VN054787.D
Acq: 29 Mar 2019 22:50

Tgt Ion: 65 Resp: 352504
Ion Ratio Lower Upper
65 100
67 51.7 0.0 104.6

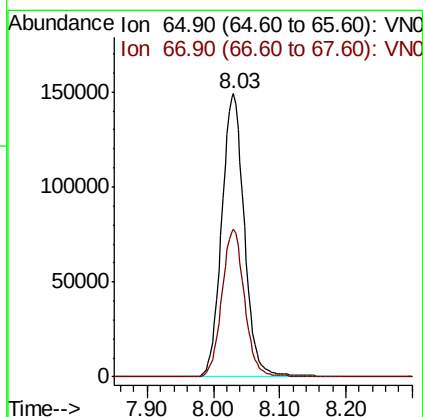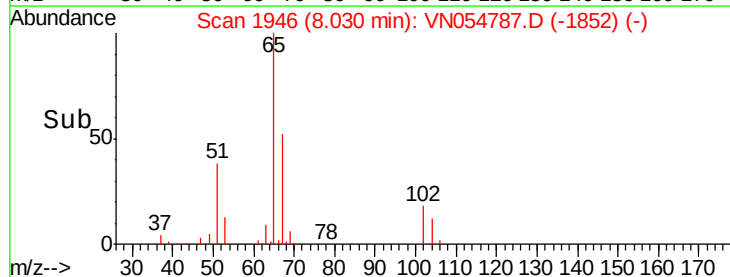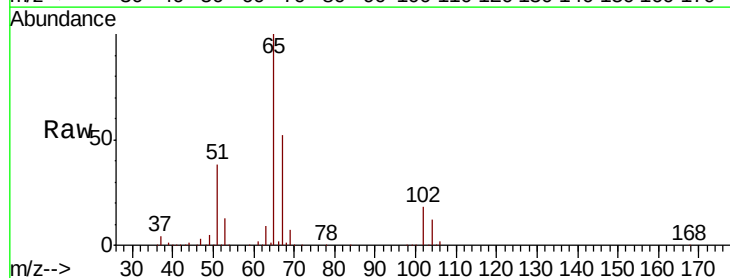

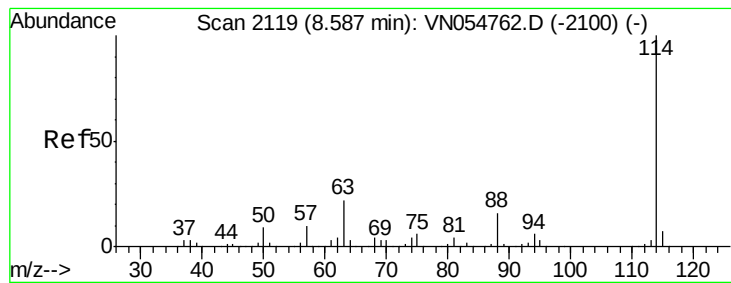

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.59 min Scan# 2119

Delta R.T. -0.00 min

Lab File: VN054787.D

Acq: 29 Mar 2019 22:50

Instrument :

MSVOA_N

ClientSampleId :

TR-05-032819


Tot Ion:114 Resp: 856038

Ion Ratio Lower Upper

114 100

63 22.2 0.0 35.2




88 15.7 0.0 30.2

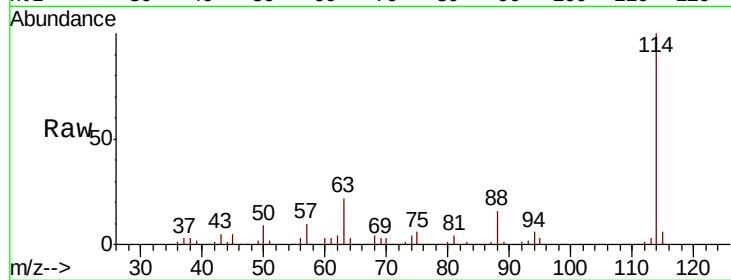

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VN

Ion 87.90 (87.60 to 88.60): VN

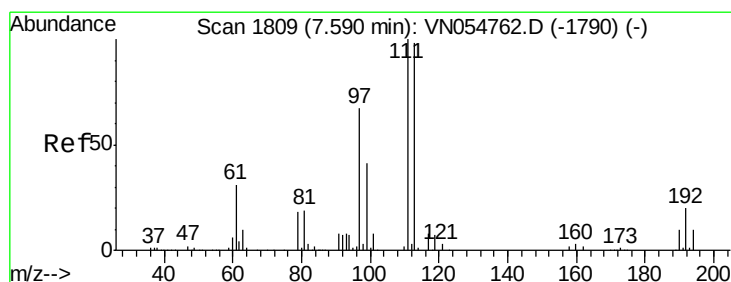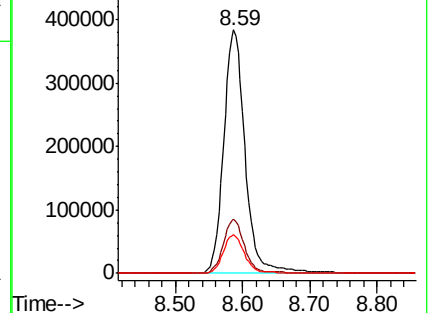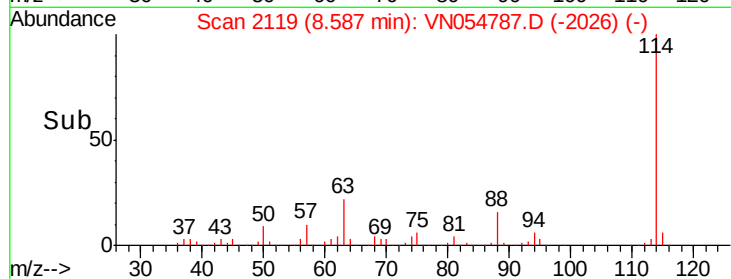

#35

Dibromofluoromethane

Concen: 47.907 ug/l

RT: 7.59 min Scan# 1809

Delta R.T. -0.00 min

Lab File: VN054787.D

Acq: 29 Mar 2019 22:50


Tgt Ion:113 Resp: 273414

Ion Ratio Lower Upper

113 100

111 103.3 82.2 123.4



192 20.6 19.2 28.8

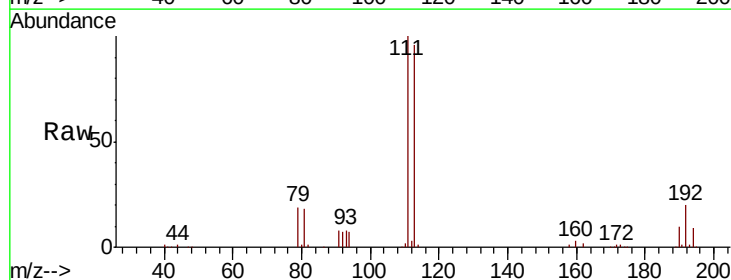


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

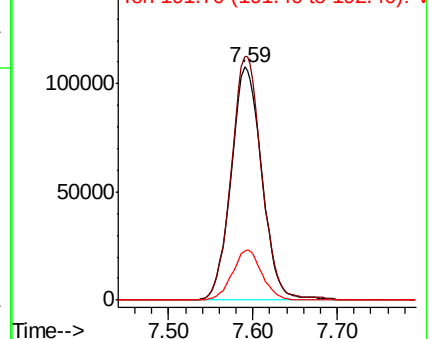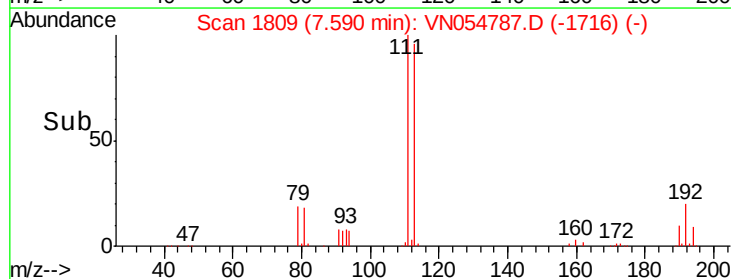

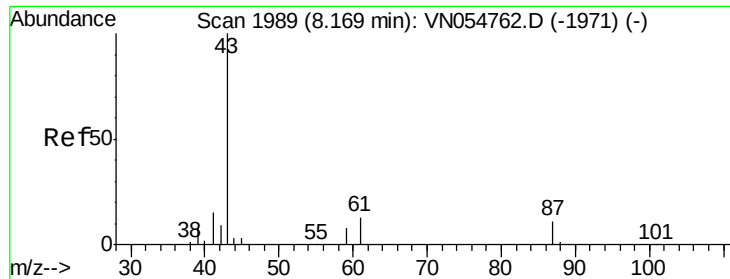

#43

Isopropyl Acetate

Concen: 1.616 ug/l

RT: 8.17 min Scan# 1989

Delta R.T. -0.00 min

Lab File: VN054787.D

Acq: 29 Mar 2019 22:50

Instrument :

MSVOA_N

ClientSampleId :

TR-05-032819


Tot Ion: 43 Resp: 15360

Ion Ratio Lower Upper

43 100

61 18.2 15.8 23.8




87 5.8 12.0 18.0#

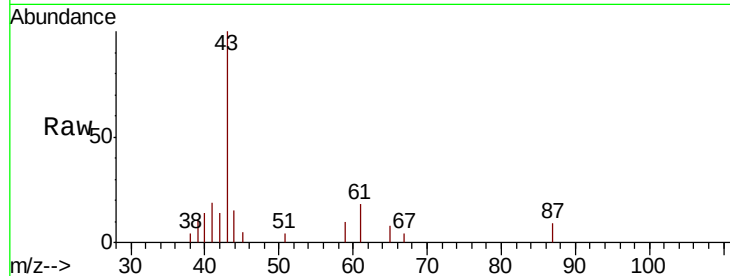

Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 61.00 (60.70 to 61.70): VN0

Ion 87.00 (86.70 to 87.70): VN0

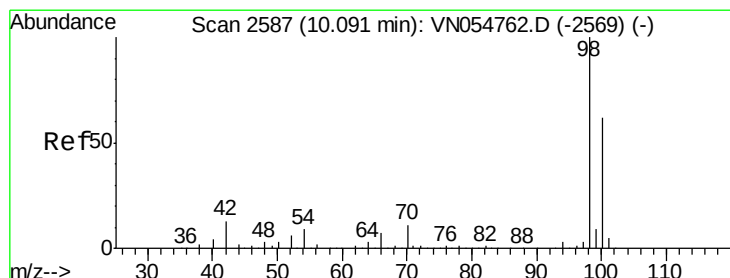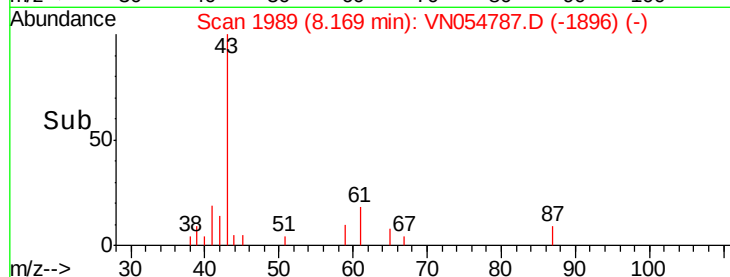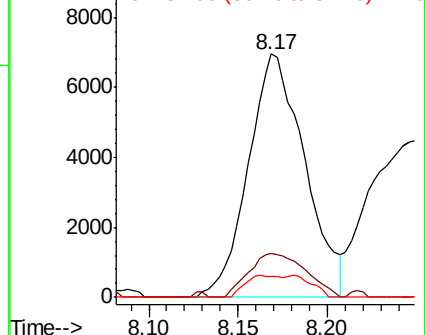

#50

Toluene-d8

Concen: 48.773 ug/l

RT: 10.09 min Scan# 2587

Delta R.T. -0.00 min

Lab File: VN054787.D


Acq: 29 Mar 2019 22:50

Tgt Ion: 98 Resp: 1034850

Ion Ratio Lower Upper



98 100


100 64.0 51.2 76.8

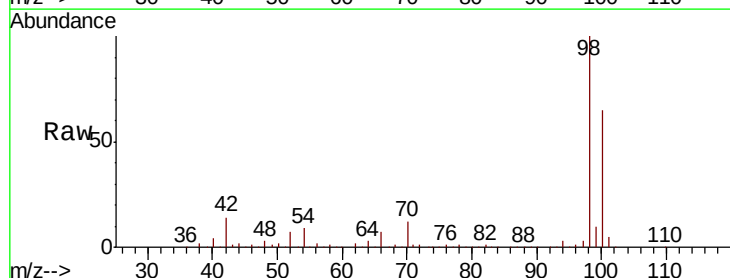

Abundance Ion 98.00 (97.70 to 98.70): VN0

Ion 100.00 (99.70 to 100.70): VN0

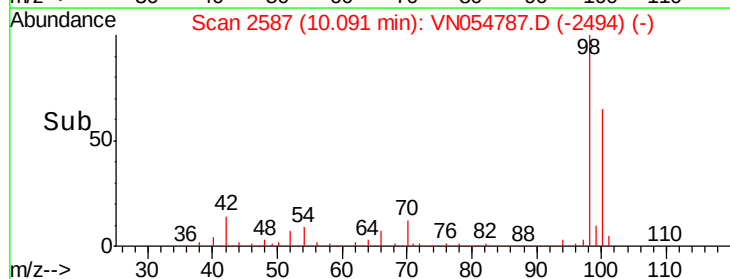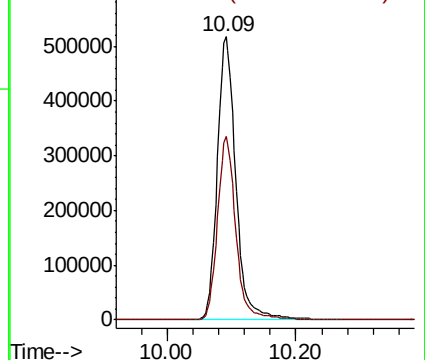

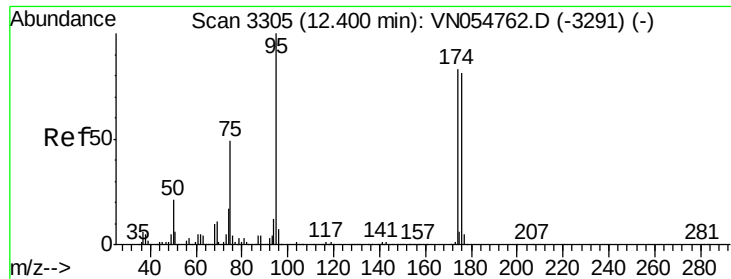

#62

4-Bromofluorobenzene

Concen: 45.630 ug/l

RT: 12.40 min Scan# 3306

Delta R.T. 0.00 min

Lab File: VN054787.D

Acq: 29 Mar 2019 22:50

Instrument :

MSVOA_N

ClientSampleId :

TR-05-032819





Tot Ion: 95 Resp: 321988

Ion Ratio Lower Upper

95 100

174 84.1 0.0 191.0

176 82.5 0.0 187.4

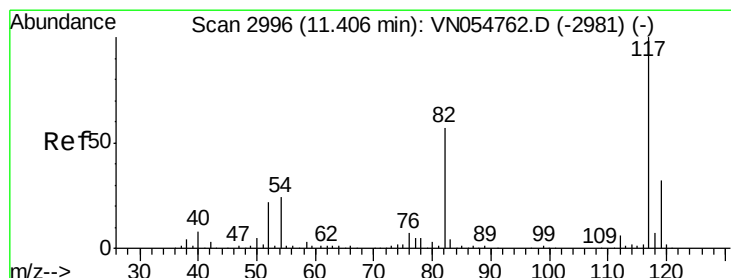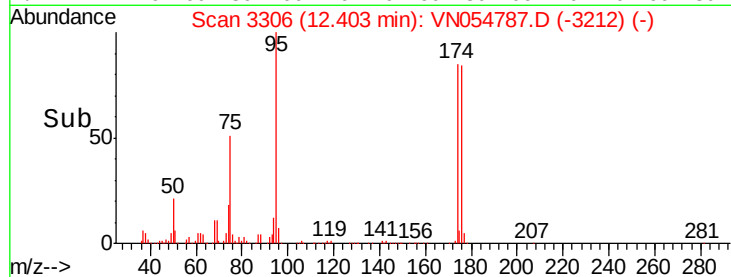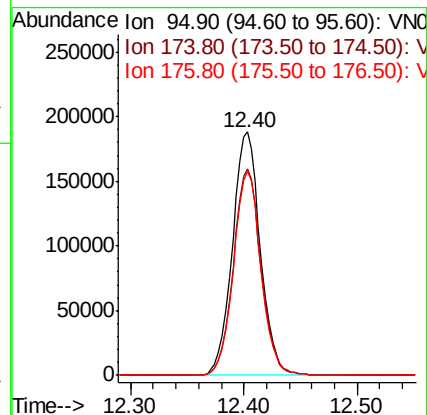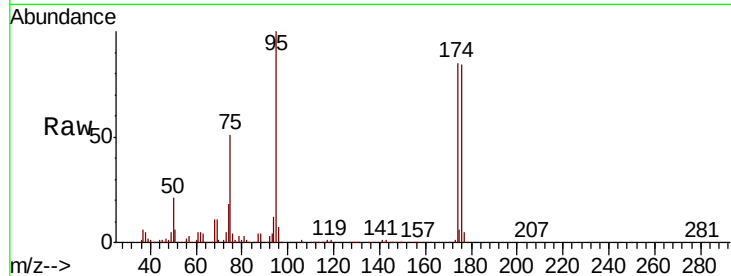

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.41 min Scan# 2996

Delta R.T. -0.00 min

Lab File: VN054787.D

Acq: 29 Mar 2019 22:50




Tgt Ion: 117 Resp: 738413


Ion Ratio Lower Upper

117 100

82 57.0 40.0 60.0

119 32.1 25.8 38.6

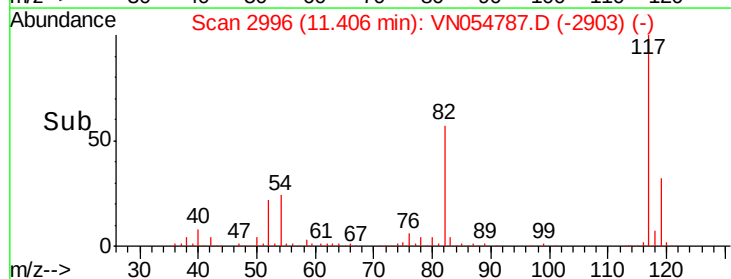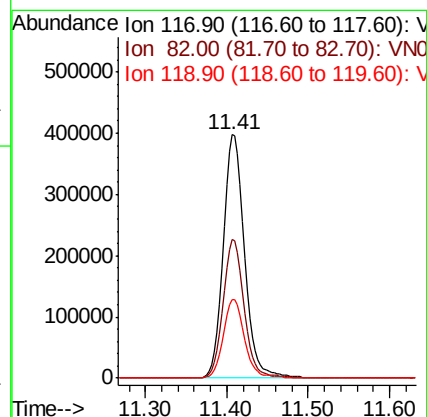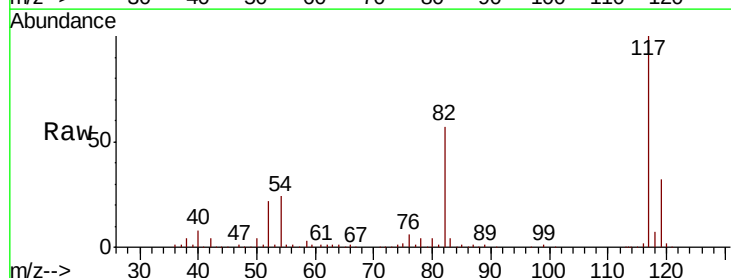

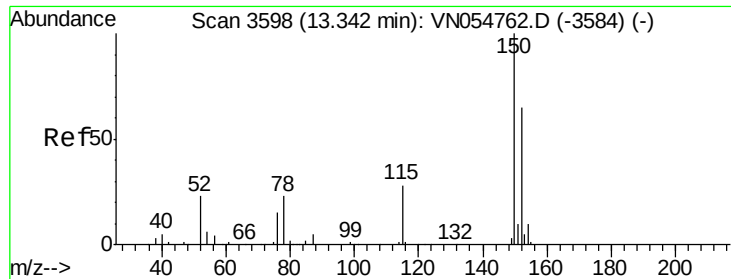

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.35 min Scan# 3599

Delta R.T. 0.00 min

Lab File: VN054787.D

Acq: 29 Mar 2019 22:50

Instrument :

MSVOA_N

ClientSampleId :

TR-05-032819


Tot Ion:152 Resp: 277029

Ion Ratio Lower Upper

152 100

115 57.3 27.2 81.6

150 156.0 0.0 349.2

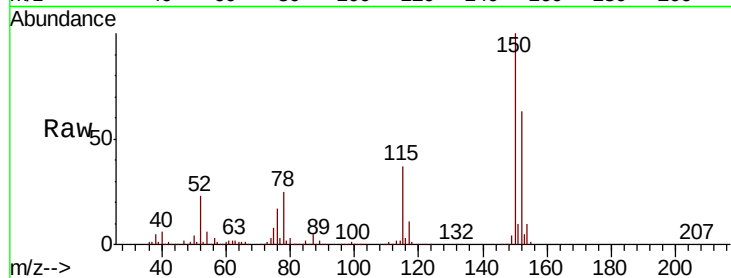

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

