


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN032919\
Data File : VN054758.D
Acq On : 29 Mar 2019 8:24
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N032919W.M
Title : SW846 8260
Last Update : Sat Mar 30 00:48:18 2019

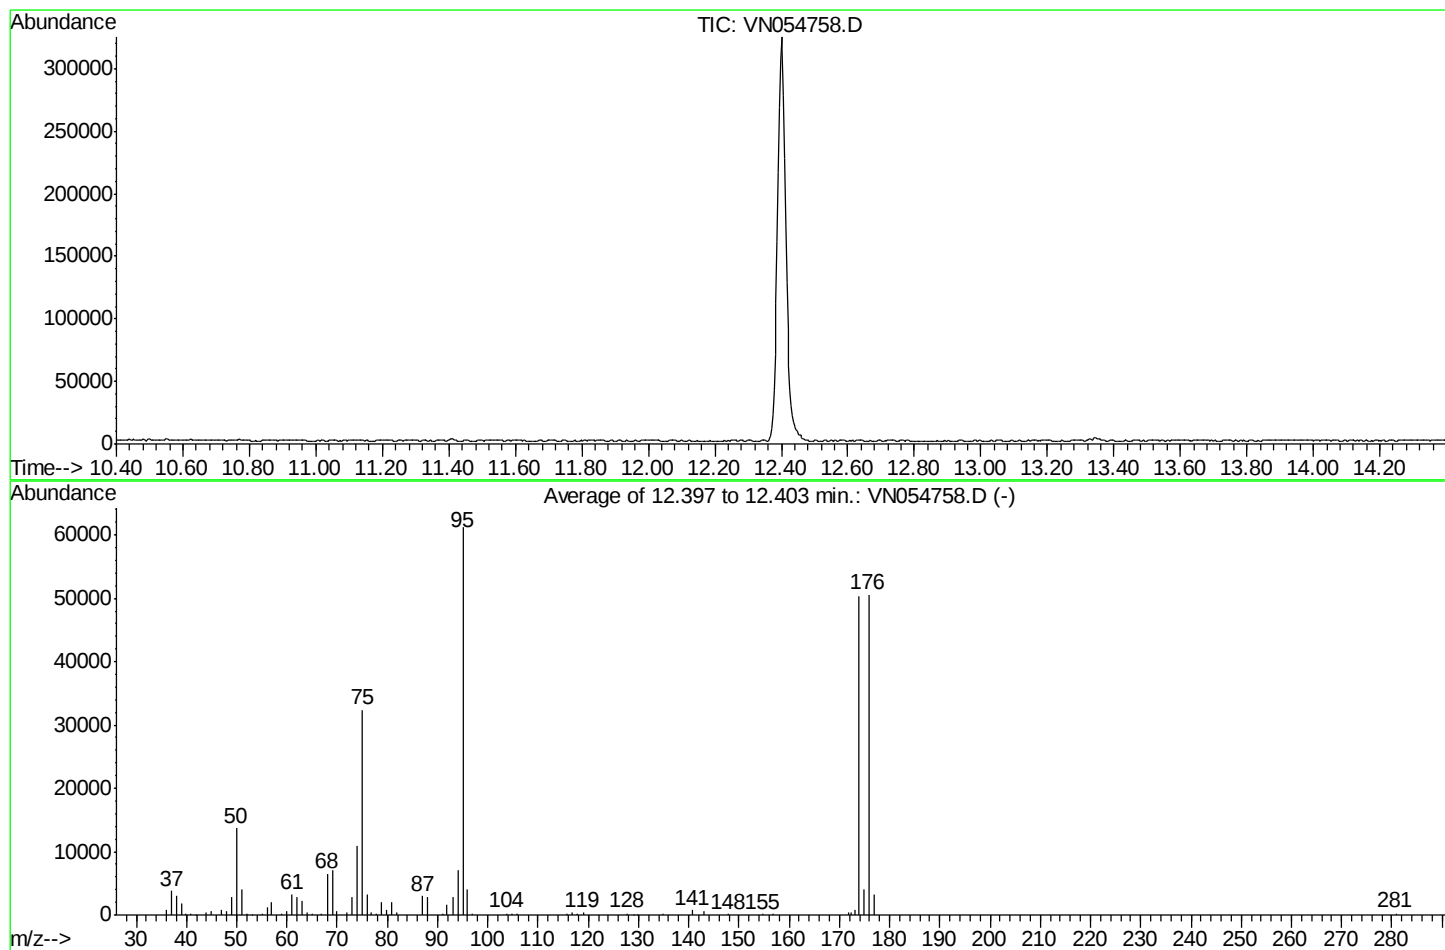

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.4	13721	PASS
75	95	30	60	52.9	32368	PASS
95	95	100	100	100.0	61210	PASS
96	95	5	9	6.8	4149	PASS
173	174	0.00	2	1.4	714	PASS
174	95	50	100	82.2	50330	PASS
175	174	5	9	8.1	4082	PASS
176	174	95	101	100.6	50629	PASS
177	176	5	9	6.4	3229	PASS