


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN032919\
 Data File : VN054768.D
 Acq On : 29 Mar 2019 14:15
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N032919W.M
 Title : SW846 8260
 Last Update : Sat Mar 30 00:48:18 2019

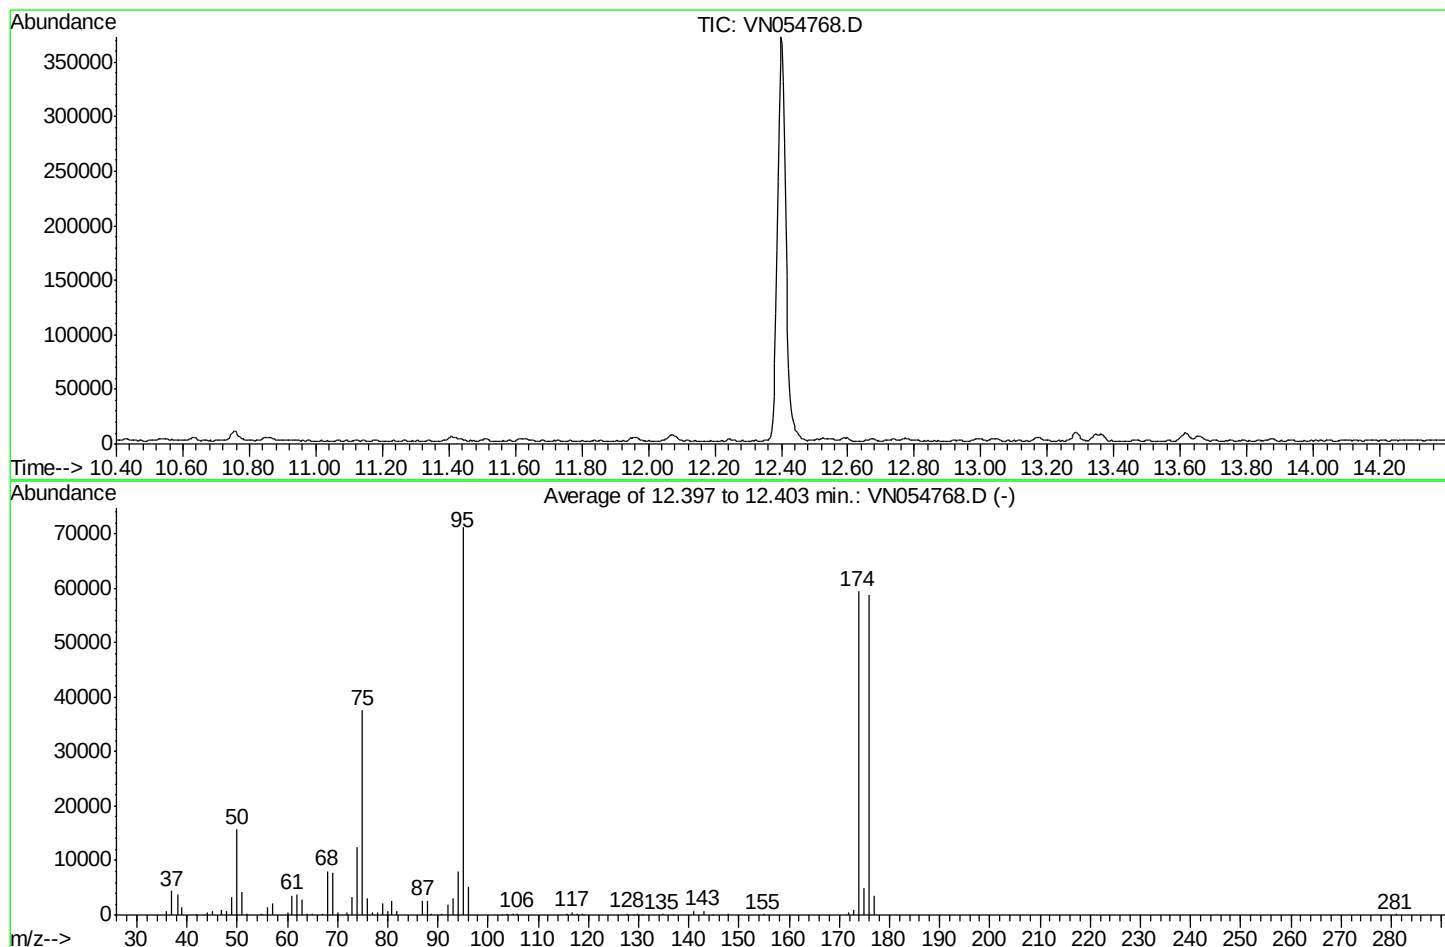

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.1	15729	PASS
75	95	30	60	52.8	37578	PASS
95	95	100	100	100.0	71189	PASS
96	95	5	9	7.4	5271	PASS
173	174	0.00	2	1.5	919	PASS
174	95	50	100	83.5	59424	PASS
175	174	5	9	8.5	5049	PASS
176	174	95	101	98.9	58784	PASS
177	176	5	9	6.2	3639	PASS