

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032921\
 Data File : VN066382.D
 Acq On : 29 Mar 2021 17:21
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 IBLK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N032521W.M
 Title : SW846 8260

Signal : TIC: VN066382.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.411	249	269	277	rBV6	34450	93530	3.53%	0.636%
2	7.507	2148	2169	2183	rBV2	349804	871996	32.95%	5.929%
3	7.582	2183	2197	2223	rVB	598311	1432195	54.12%	9.738%
4	7.949	2309	2334	2362	rBV2	426360	1022869	38.65%	6.955%
5	8.512	2524	2544	2573	rBV	854177	1780413	67.28%	12.105%
6	10.028	3089	3109	3124	rBV	1462034	2646333	100.00%	17.993%
7	10.089	3125	3132	3150	rVB	74299	136868	5.17%	0.931%
8	11.347	3584	3601	3627	rBV	1106685	1937058	73.20%	13.170%
9	11.454	3627	3641	3658	rVV	89748	159348	6.02%	1.083%
10	11.562	3666	3681	3706	rBV	248144	497000	18.78%	3.379%
11	11.892	3787	3804	3822	rBV	68184	115349	4.36%	0.784%
12	12.345	3959	3973	3998	rBV	853949	1438122	54.34%	9.778%
13	12.600	4059	4068	4077	rBV	32035	56073	2.12%	0.381%
14	12.680	4091	4098	4113	rVB	32086	53519	2.02%	0.364%
15	12.841	4148	4158	4171	rVB4	17460	28970	1.09%	0.197%
16	12.986	4200	4212	4234	rBV	108372	204000	7.71%	1.387%
17	13.289	4310	4325	4372	rBV	723018	1510062	57.06%	10.267%
18	15.072	4979	4990	5017	rVB	206471	404664	15.29%	2.751%
19	16.081	5355	5366	5385	rVB	155465	319534	12.07%	2.173%




Sum of corrected areas: 14707903

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032921\
Data File : VN066382.D
Acq On : 29 Mar 2021 17:21
Operator : JC/MD
Sample : IBLK
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N032521W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

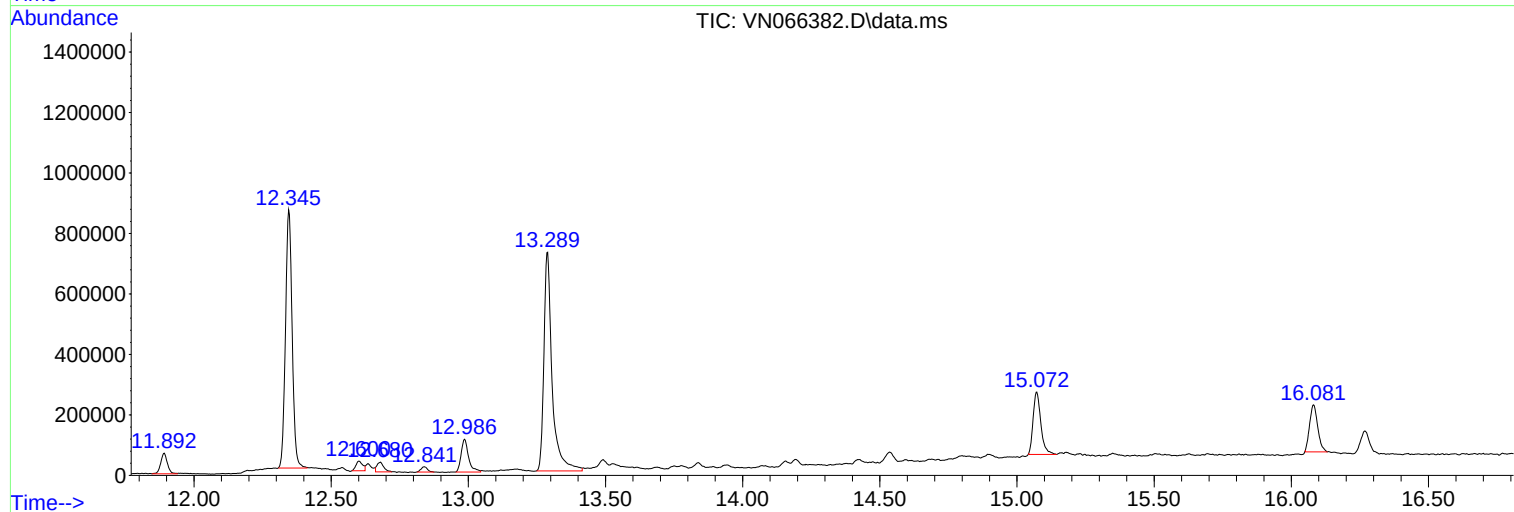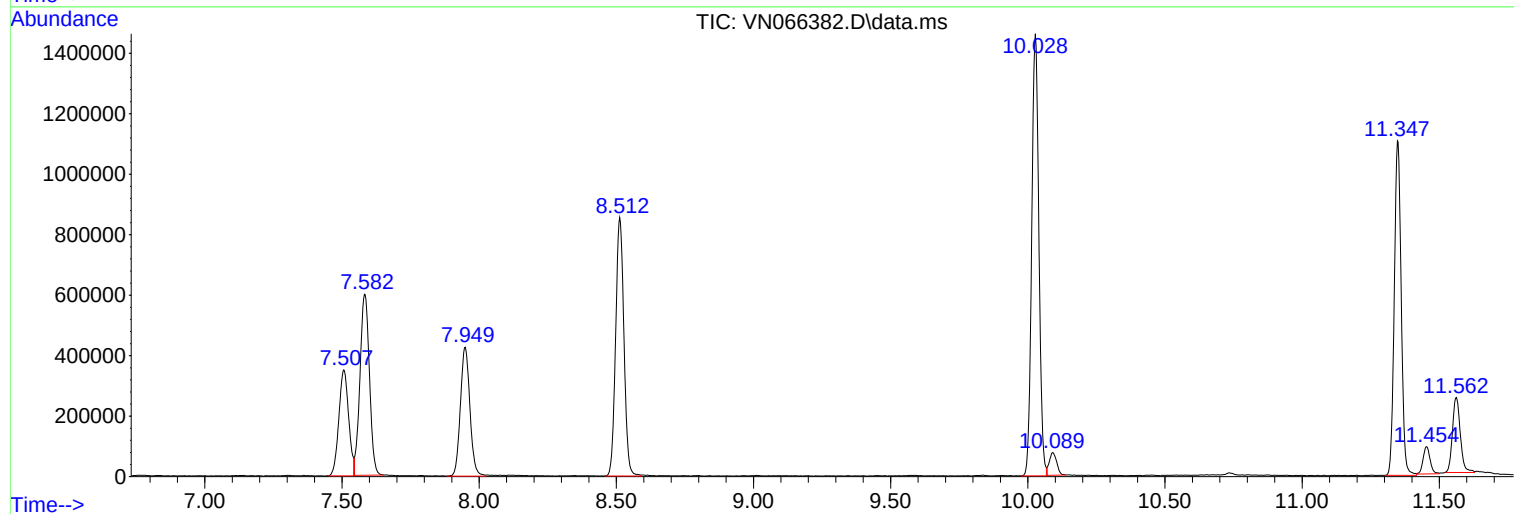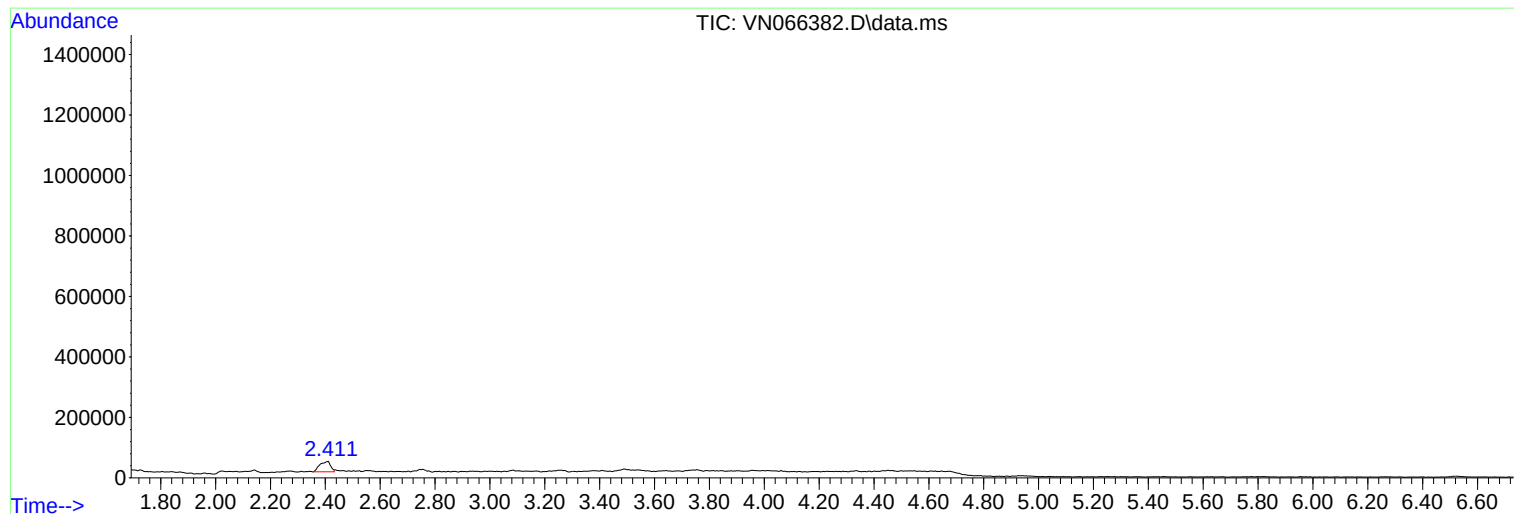

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032921\
Data File : VN066382.D
Acq On : 29 Mar 2021 17:21
Operator : JC/MD
Sample : IBLK
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
IBLK










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N032521W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Naphthalene, 2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
16.081	10.58 ug/l	319534	1,4-Dichlorobenzene-d4	13.289

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		Naphthalene, 1-methyl-	142	C11H10	000090-12-0	96
2		Naphthalene, 2-methyl-	142	C11H10	000091-57-6	96
3		Benzocycloheptatriene	142	C11H10	000264-09-5	91
4		1,4-Methanonaphthalene, 1,4-dihy...	142	C11H10	004453-90-1	90
5		1H-Indene, 1-ethylidene-	142	C11H10	002471-83-2	59

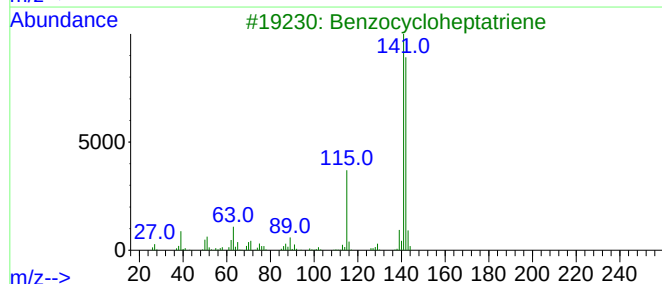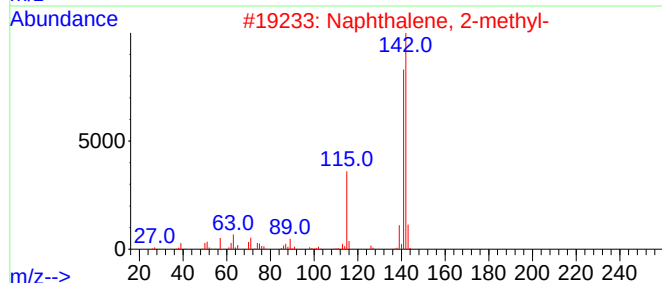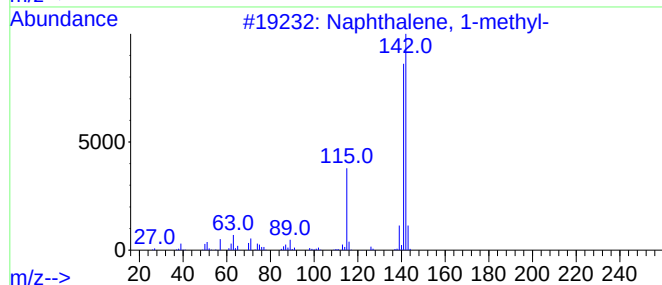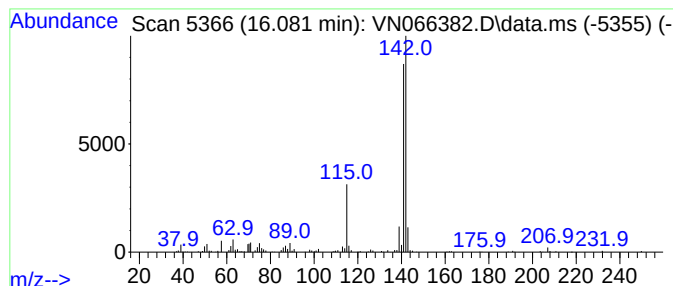

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032921\
Data File : VN066382.D
Acq On : 29 Mar 2021 17:21
Operator : JC/MD
Sample : IBLK
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N032521W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Naphthalene, 2-...	16.081	10.6	ug/l	319534	4	13.289	1510060	50.0