


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032921\
 Data File : VN066363.D
 Acq On : 29 Mar 2021 8:40
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N032521W.M
 Title : SW846 8260
 Last Update : Fri Mar 26 16:26:01 2021

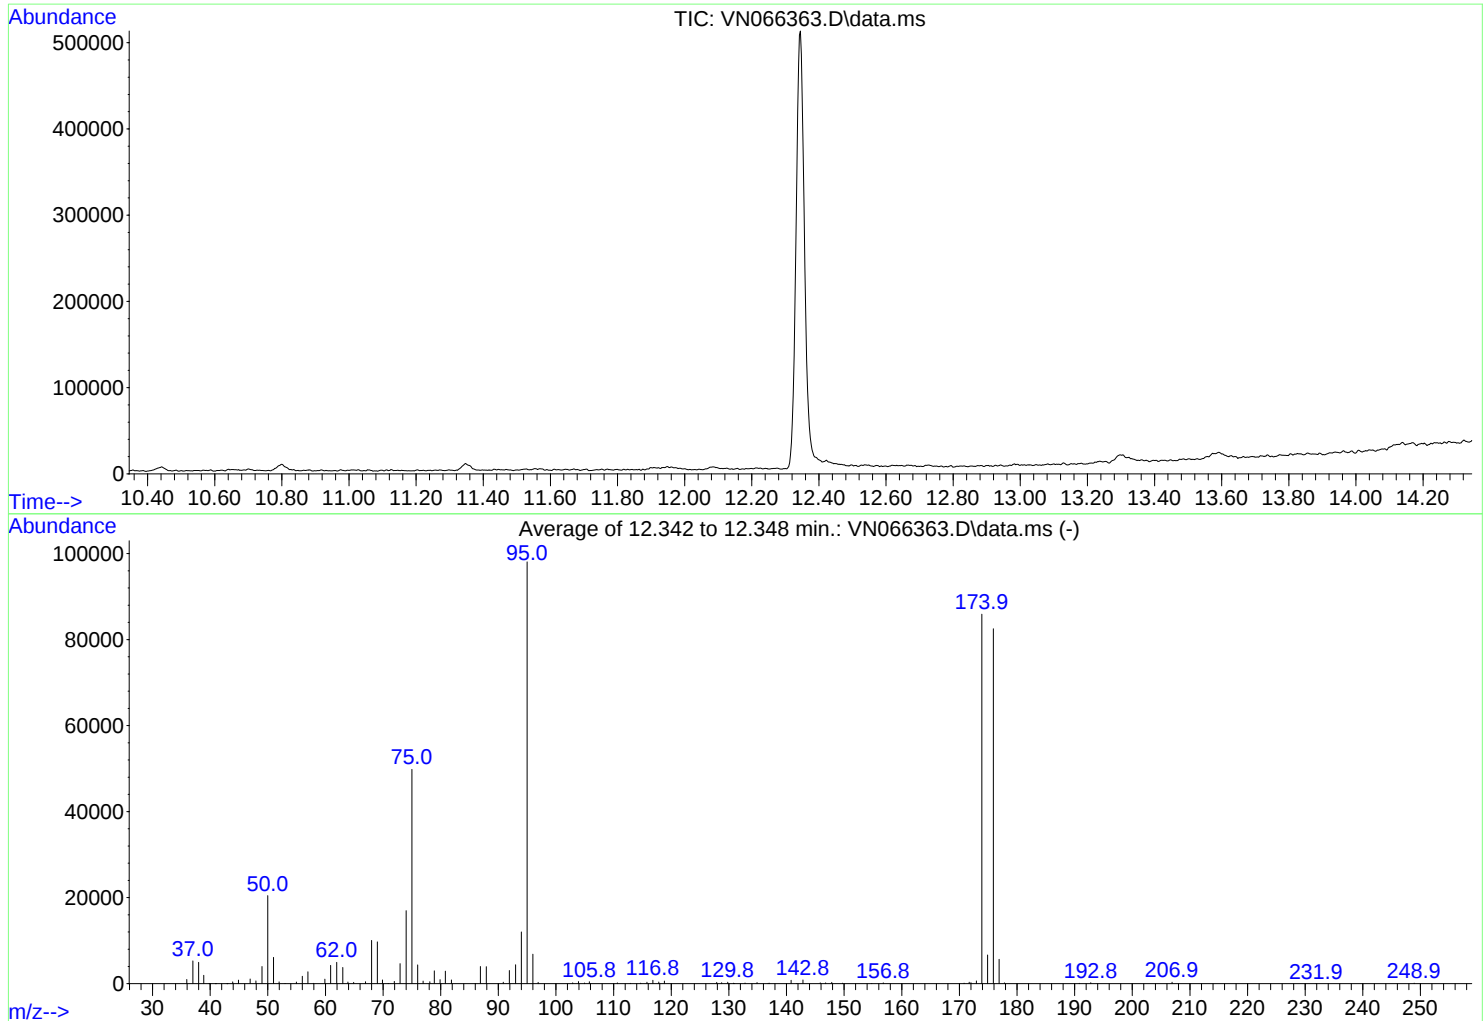

AutoFind: Scans 3972, 3973, 3974; Background Corrected with Scan 3955

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.9	20477	PASS
75	95	30	60	50.8	49821	PASS
95	95	100	100	100.0	98075	PASS
96	95	5	9	7.0	6853	PASS
173	174	0.00	2	0.8	650	PASS
174	95	50	100	87.6	85909	PASS
175	174	5	9	7.8	6668	PASS
176	174	95	101	96.0	82507	PASS
177	176	5	9	6.8	5648	PASS