


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032922\
Data File : VN071625.D
Acq On : 29 Mar 2022 09:55
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N032822W.M
Title : SW846 8260
Last Update : Tue Mar 29 09:32:37 2022

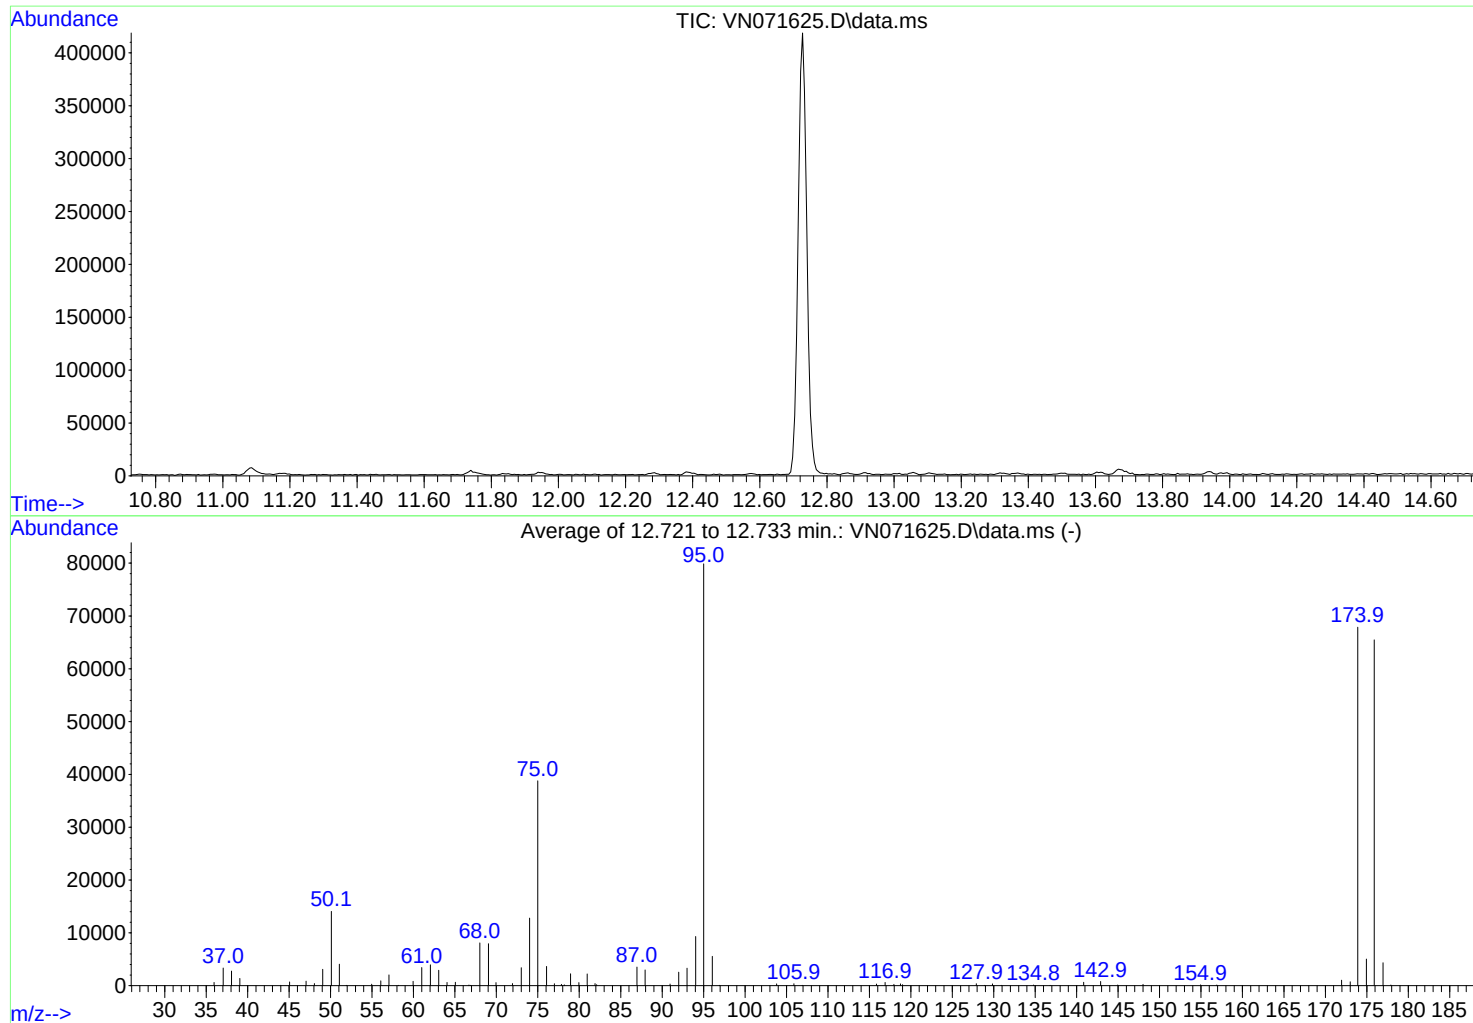

AutoFind: Scans 1825, 1826, 1827; Background Corrected with Scan 1816

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	14066	PASS
75	95	30	60	48.6	38792	PASS
95	95	100	100	100.0	79869	PASS
96	95	5	9	7.0	5552	PASS
173	174	0.00	2	1.1	732	PASS
174	95	50	100	85.0	67859	PASS
175	174	5	9	7.4	5018	PASS
176	174	95	101	96.5	65477	PASS
177	176	5	9	6.6	4335	PASS