

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032924\
 Data File : VN081608.D
 Acq On : 29 Mar 2024 12:08
 Operator : JC\MD
 Sample : VN0329MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0329MBL01

Quant Time: Mar 30 00:26:25 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031824W.M
 Quant Title : SW846 8260
 QLast Update : Tue Mar 19 06:00:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	337747	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	612477	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	559488	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	230790	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	234586	54.464	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 108.920%	
35) Dibromofluoromethane	8.165	113	206476	53.417	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 106.840%	
50) Toluene-d8	10.565	98	743617	53.219	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 106.440%	
62) 4-Bromofluorobenzene	12.853	95	227237	46.154	ug/l	0.00
Spiked Amount	50.000	Range	64 - 133	Recovery	= 92.300%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032924\
Data File : VN081608.D
Acq On : 29 Mar 2024 12:08
Operator : JC\MD
Sample : VN0329MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0329MBL01

Quant Time: Mar 30 00:26:25 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031824W.M
Quant Title : SW846 8260
QLast Update : Tue Mar 19 06:00:00 2024
Response via : Initial Calibration




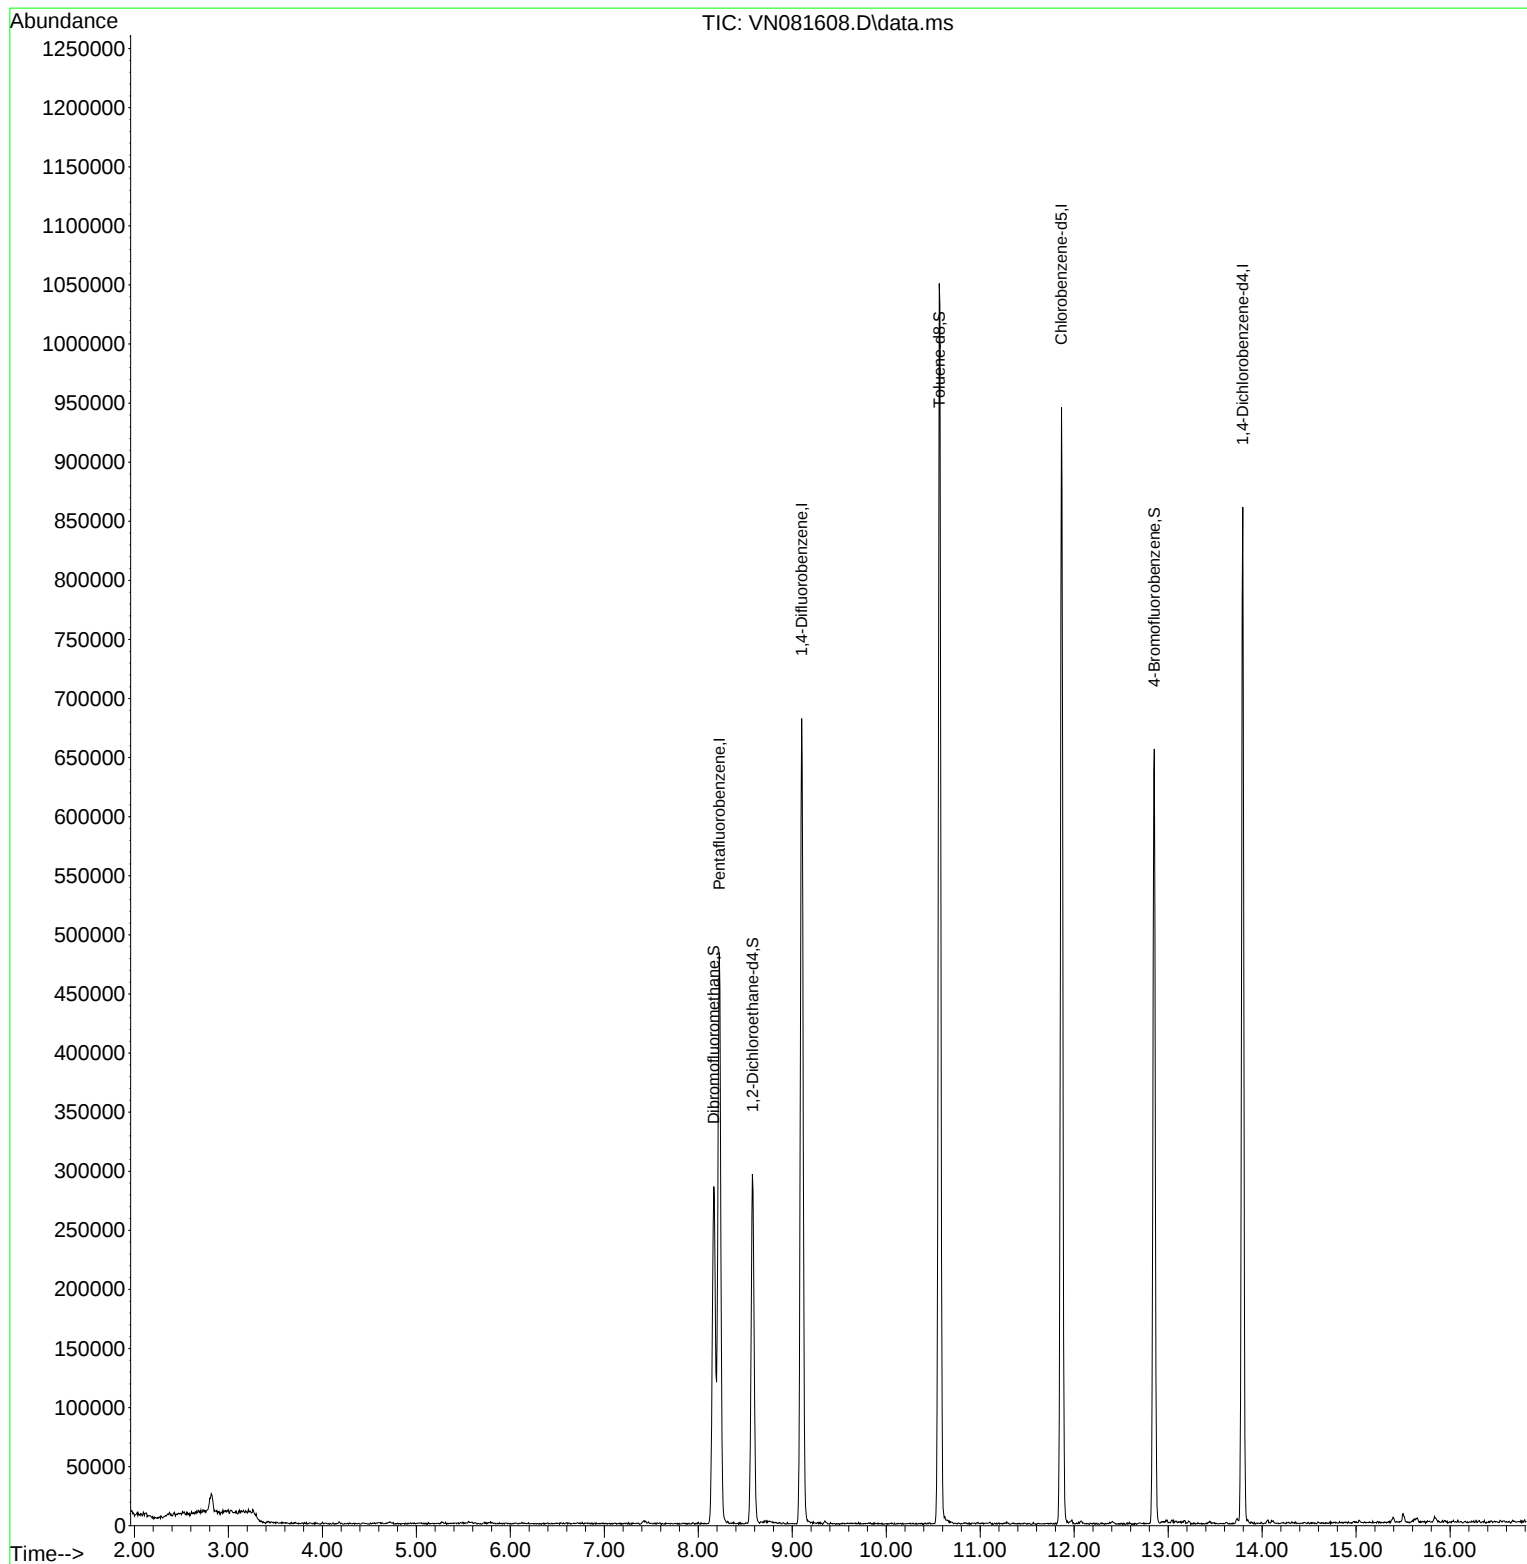


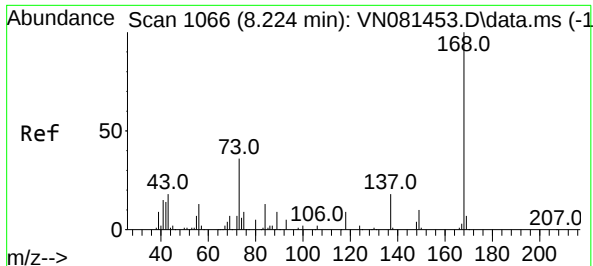

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.000 min
Lab File: VN081608.D
Acq: 29 Mar 2024 12:08




Instrument :
MSVOA_N
ClientSampleId :
VN0329MBL01


Tgt Ion:168 Resp: 337747
Ion Ratio Lower Upper
168 100
99 61.5 59.9 89.9

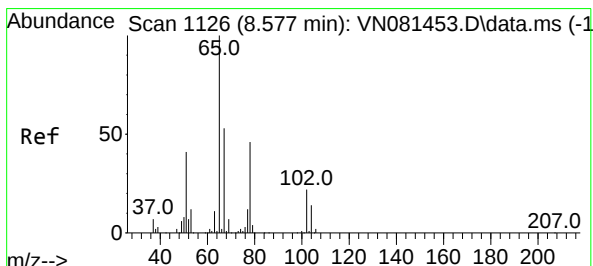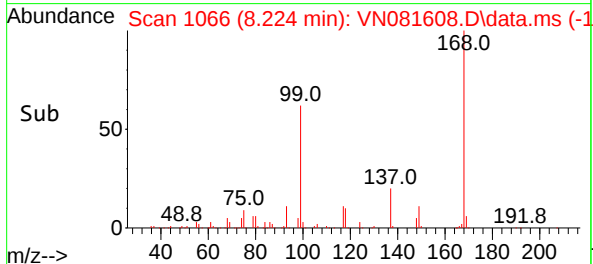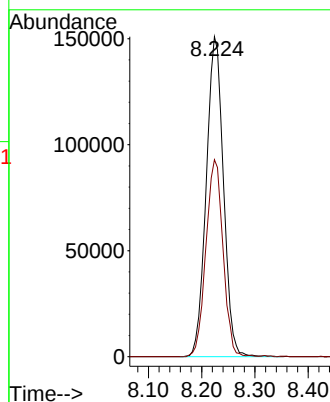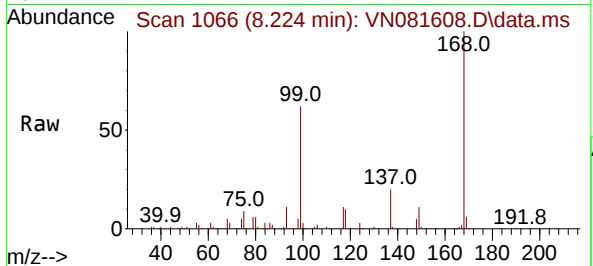

#33
1,2-Dichloroethane-d4
Concen: 54.464 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. 0.000 min
Lab File: VN081608.D
Acq: 29 Mar 2024 12:08

Tgt Ion: 65 Resp: 234586
Ion Ratio Lower Upper
65 100
67 52.3 0.0 102.4

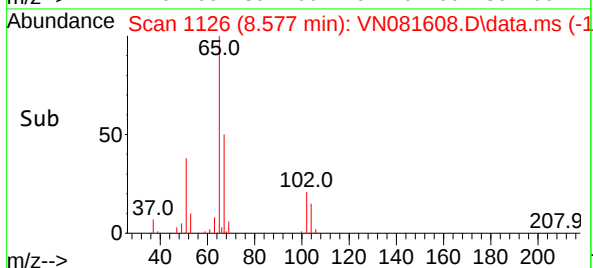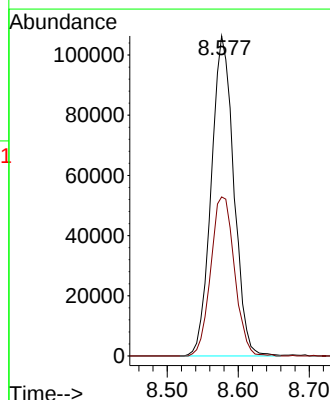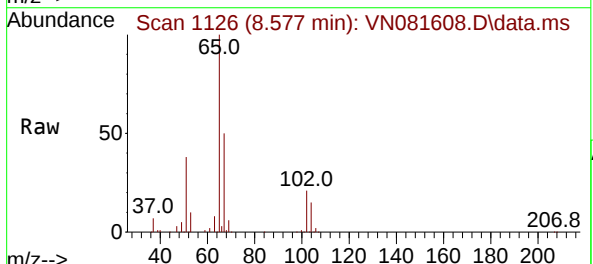

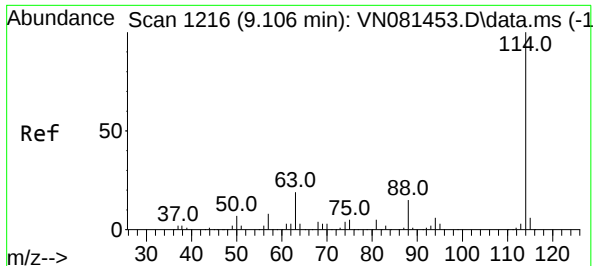

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1

Delta R.T. -0.006 min

Lab File: VN081608.D

Acq: 29 Mar 2024 12:08

Instrument :

MSVOA_N

ClientSampleId :

VN0329MBL01





Tgt Ion:114 Resp: 612477

Ion Ratio Lower Upper

114 100

63 19.8 0.0 48.0

88 14.7 0.0 34.8

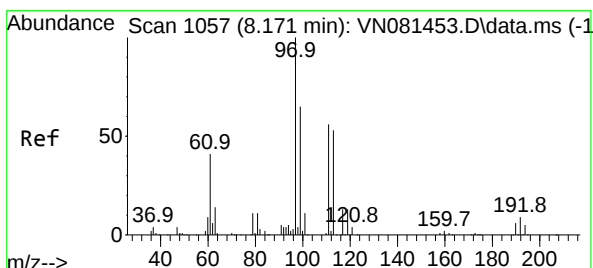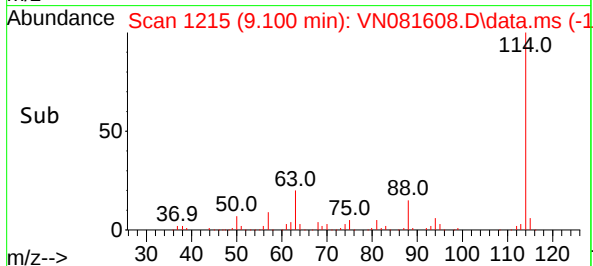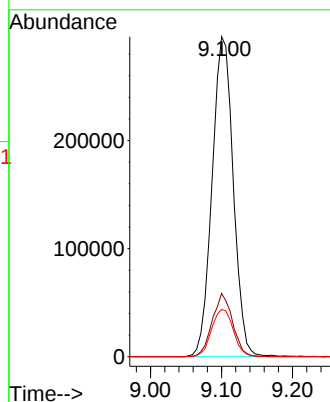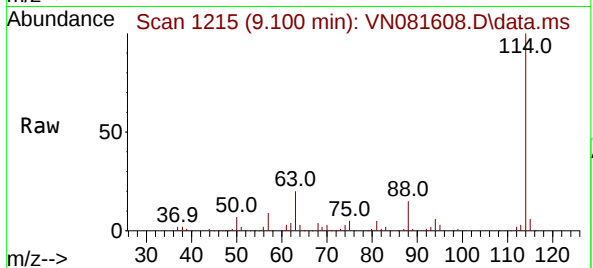

#35

Dibromofluoromethane

Concen: 53.417 ug/l

RT: 8.165 min Scan# 1056

Delta R.T. -0.006 min

Lab File: VN081608.D

Acq: 29 Mar 2024 12:08




Tgt Ion:113 Resp: 206476


Ion Ratio Lower Upper

113 100

111 101.7 82.2 123.4

192 16.3 12.5 18.7


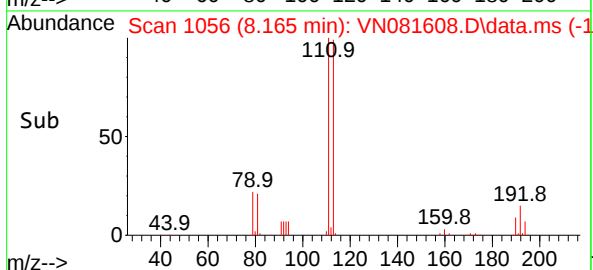
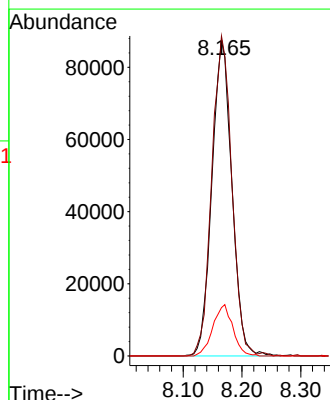
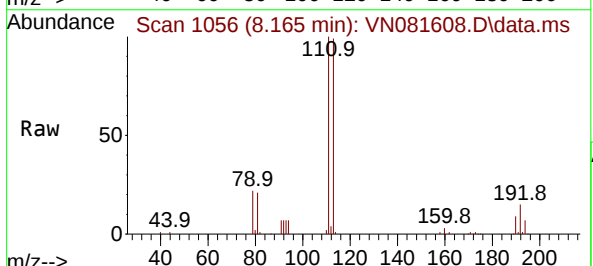


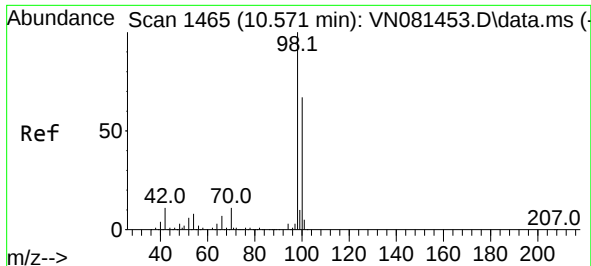

#50
Toluene-d8
Concen: 53.219 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. -0.006 min
Lab File: VN081608.D
Acq: 29 Mar 2024 12:08




Instrument :
MSVOA_N
ClientSampleId :
VN0329MBL01


Tgt Ion: 98 Resp: 743617
Ion Ratio Lower Upper
98 100
100 64.0 51.4 77.0

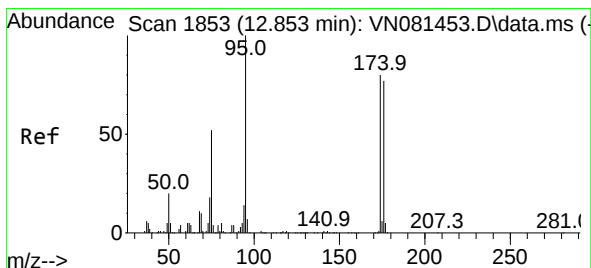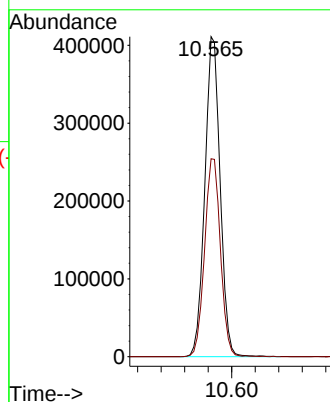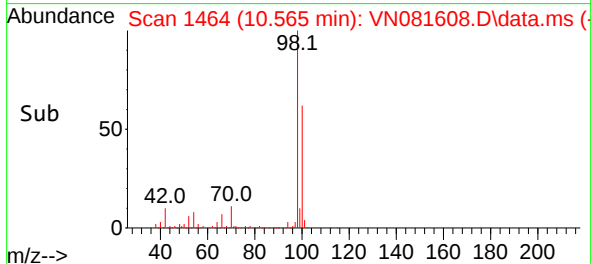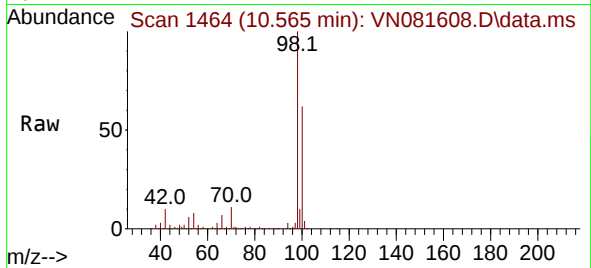

#62
4-Bromofluorobenzene
Concen: 46.154 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.000 min
Lab File: VN081608.D
Acq: 29 Mar 2024 12:08

Tgt Ion: 95 Resp: 227237
Ion Ratio Lower Upper
95 100
174 76.3 0.0 120.4
176 71.5 0.0 121.0


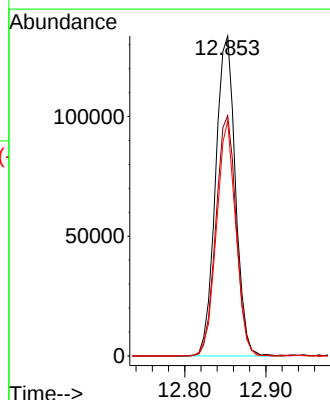
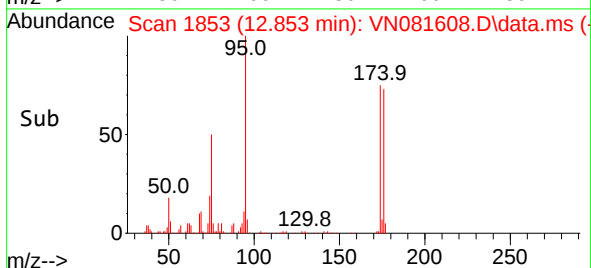
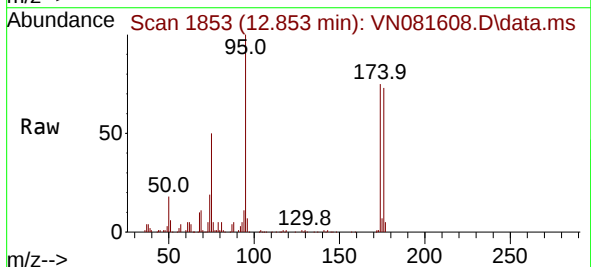


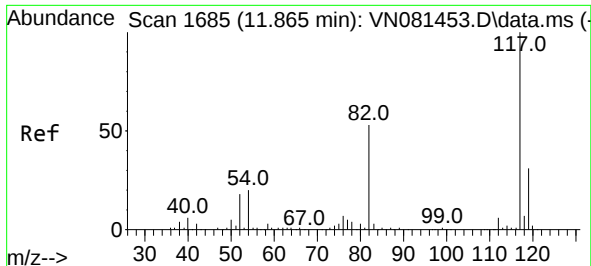

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 117
Delta R.T. 0.000 min
Lab File: VN081608.D
Acq: 29 Mar 2024 12:08

Instrument :
MSVOA_N
ClientSampleId :
VN0329MBL01

Tgt Ion:117 Resp: 559488
Ion Ratio Lower Upper
117 100
82 53.5 52.7 79.1
119 31.9 25.3 37.9

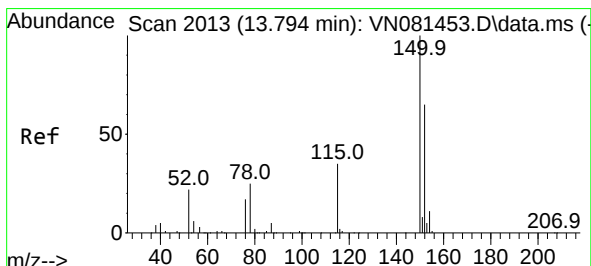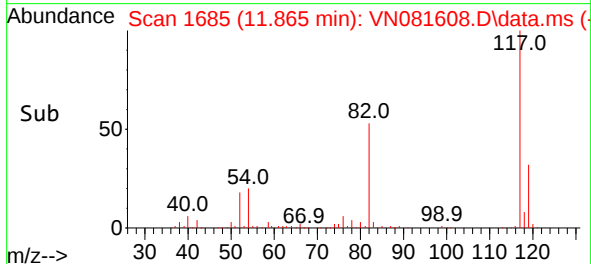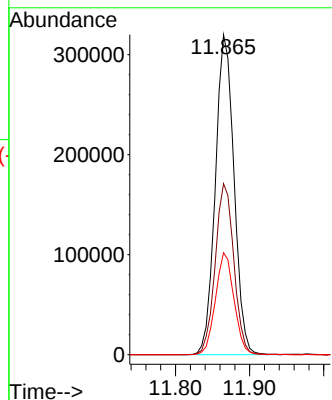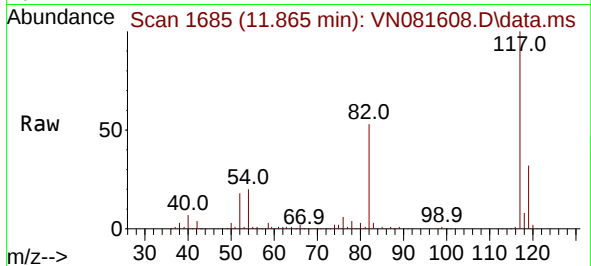

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. 0.000 min
Lab File: VN081608.D
Acq: 29 Mar 2024 12:08

Tgt Ion:152 Resp: 230790
Ion Ratio Lower Upper
152 100
115 60.6 32.3 96.8
150 150.7 0.0 339.8

