
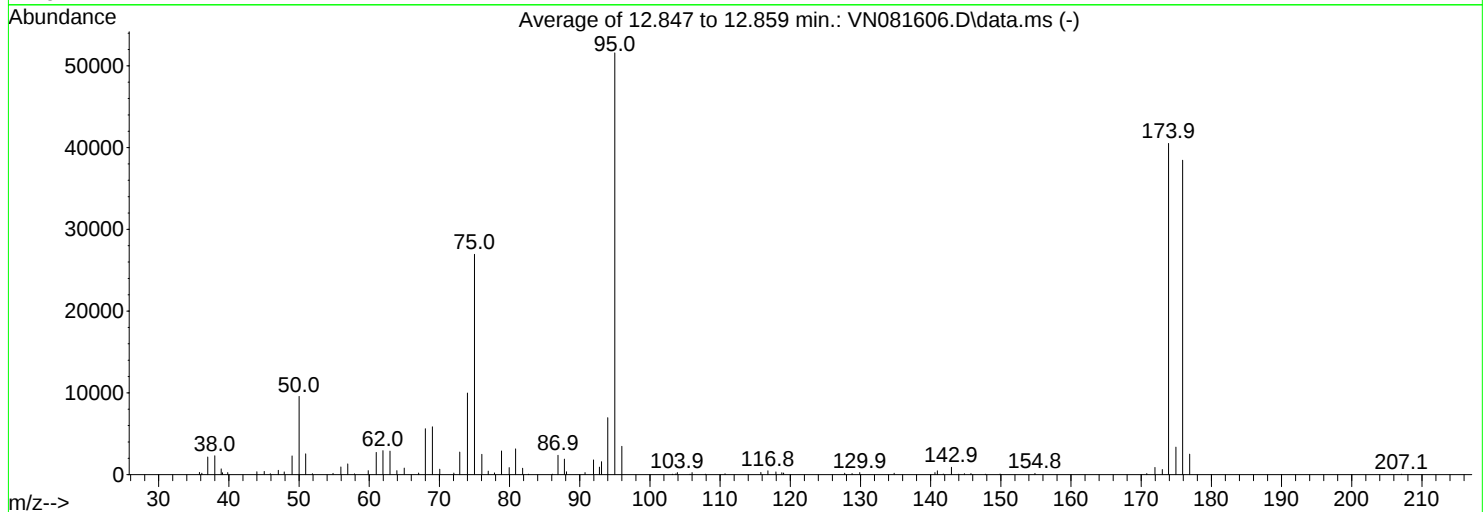


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032924\
Data File : VN081606.D
Acq On : 29 Mar 2024 10:47
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031824W.M
Title : SW846 8260
Last Update : Tue Mar 19 06:00:00 2024

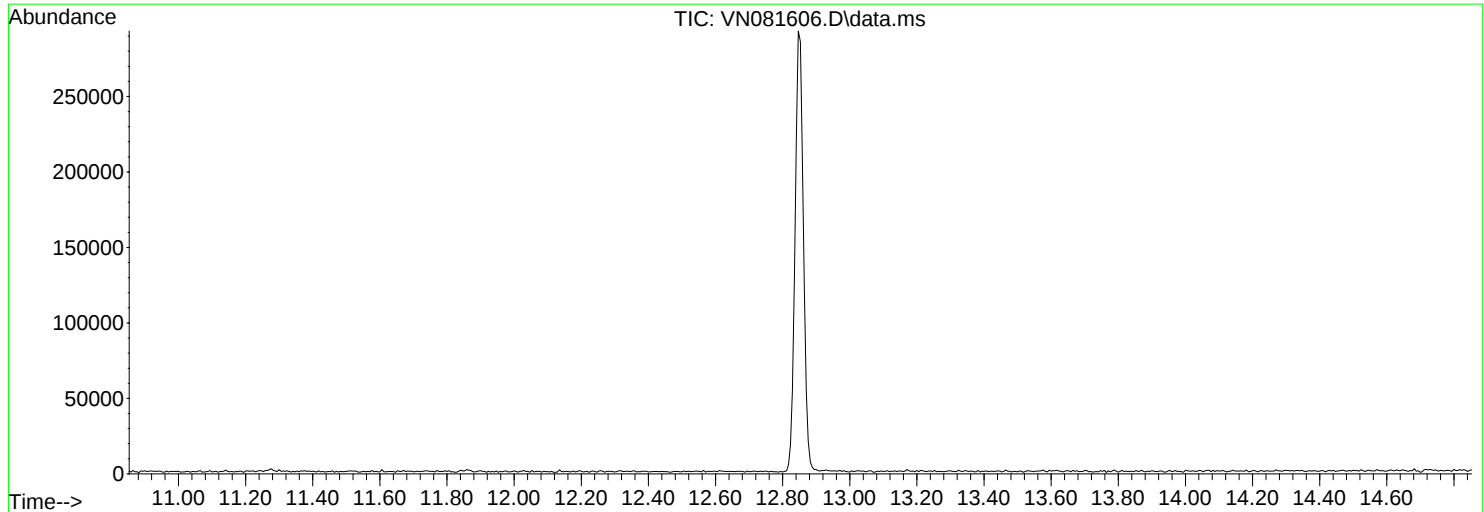

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	9564	PASS
75	95	30	60	52.2	26949	PASS
95	95	100	100	100.0	51589	PASS
96	95	5	9	6.7	3472	PASS
173	174	0.00	2	1.6	631	PASS
174	95	50	100	78.5	40512	PASS
175	174	5	9	8.3	3376	PASS
176	174	95	101	94.9	38464	PASS
177	176	5	9	6.5	2498	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.80	276	47.90	334	61.95	2942	75.00	2694
36.15	176	49.00	2293	62.95	2869	76.05	248
37.00	2152	50.00	9564	63.95	496	76.95	43
38.00	2312	50.95	2536	65.00	808	77.85	22
38.90	697	51.90	114	67.05	204	78.85	2904
39.10	226	54.85	160	68.00	5612	79.95	865
39.85	249	55.95	932	69.00	5848	80.85	3157
44.00	353	56.95	1307	70.05	666	81.85	788
45.05	388	57.90	101	72.05	193	82.70	69
45.90	112	59.85	490	72.90	2762	86.10	65
47.05	534	61.00	2722	74.00	9984	86.90	2366

Average of 12.847 to 12.859 min.: VN081606.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
87.80	1891	103.90	263	128.80	128	149.90	70
88.10	359	105.70	69	129.90	260	154.85	161
90.75	263	106.00	260	134.80	187	170.80	137
91.95	1797	107.90	66	140.60	255	171.95	885
92.80	920	110.70	119	140.95	473	173.00	631
93.10	1588	115.80	275	141.80	79	173.90	40512
94.00	6965	116.80	468	142.95	908	174.95	3376
95.00	51589	117.95	324	144.00	64	175.90	38464
96.00	3472	118.80	235	144.80	121	176.90	2498
103.20	54	119.05	202	145.75	133	207.10	64
103.70	90	127.75	170	147.80	56		

Instrument :

MSVOA_N

ClientSampleId :

BFB