


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN033020\
 Data File : VN060759.D
 Acq On : 30 Mar 2020 10:02
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N031820W.M
 Title : SW846 8260
 Last Update : Wed Mar 18 08:49:09 2020

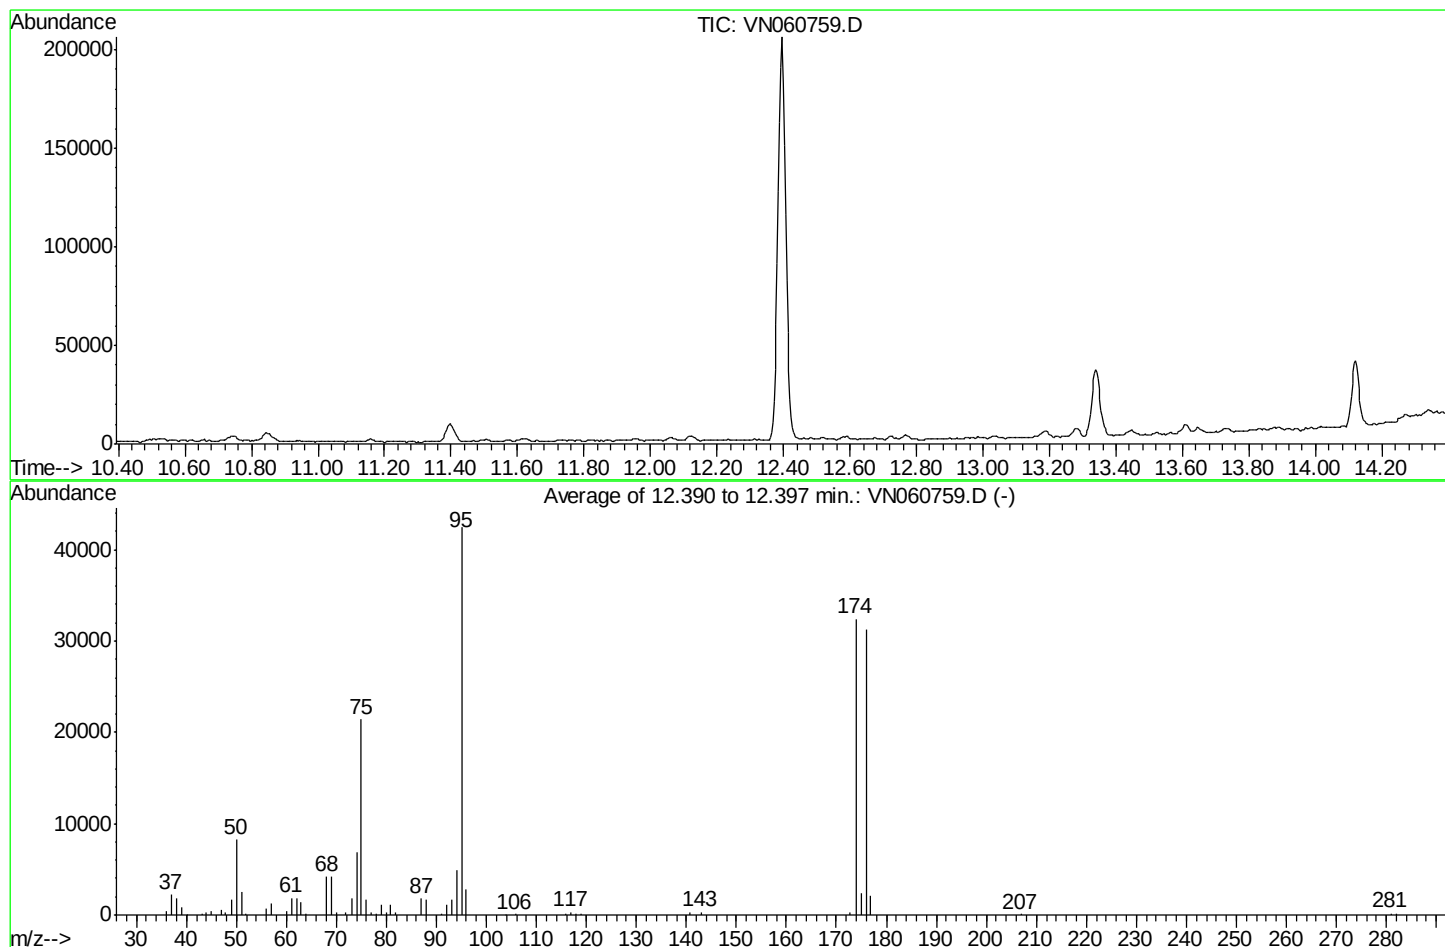

AutoFind: Scans 3302, 3303, 3304; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	8227	PASS
75	95	30	60	50.5	21421	PASS
95	95	100	100	100.0	42453	PASS
96	95	5	9	6.7	2845	PASS
173	174	0.00	2	0.7	238	PASS
174	95	50	100	76.4	32442	PASS
175	174	5	9	7.6	2455	PASS
176	174	95	101	96.5	31293	PASS
177	176	5	9	6.9	2153	PASS