
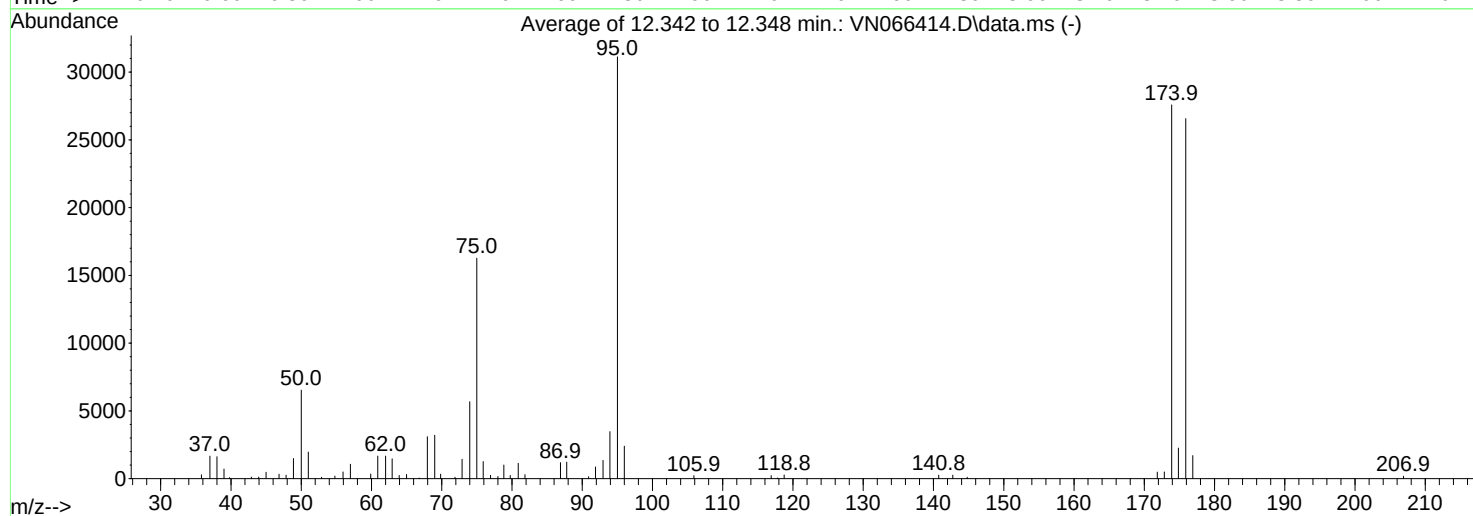


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN033021\
 Data File : VN066414.D
 Acq On : 30 Mar 2021 8:48
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N032421W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Thu Mar 25 05:52:50 2021

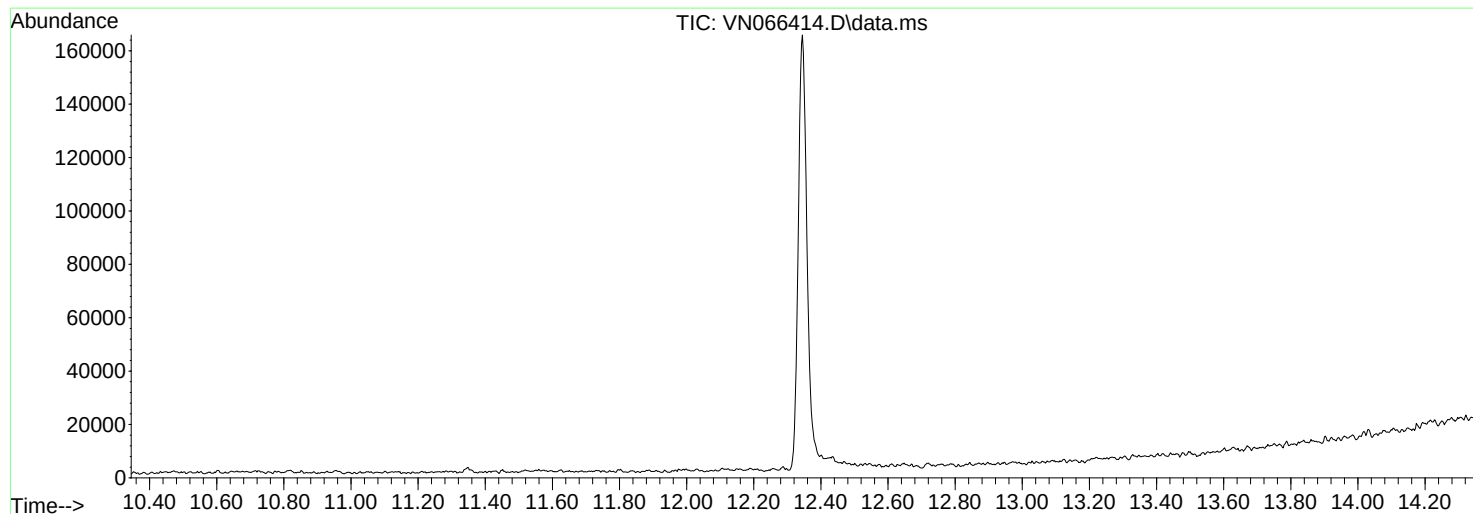

AutoFind: Scans 3972, 3973, 3974; Background Corrected with Scan 3957

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.0	6531	PASS
75	95	30	60	52.3	16270	PASS
95	95	100	100	100.0	31125	PASS
96	95	5	9	7.7	2392	PASS
173	174	0.00	2	1.8	497	PASS
174	95	50	100	88.6	27579	PASS
175	174	5	9	8.2	2261	PASS
176	174	95	101	96.3	26568	PASS
177	176	5	9	6.4	1706	PASS