
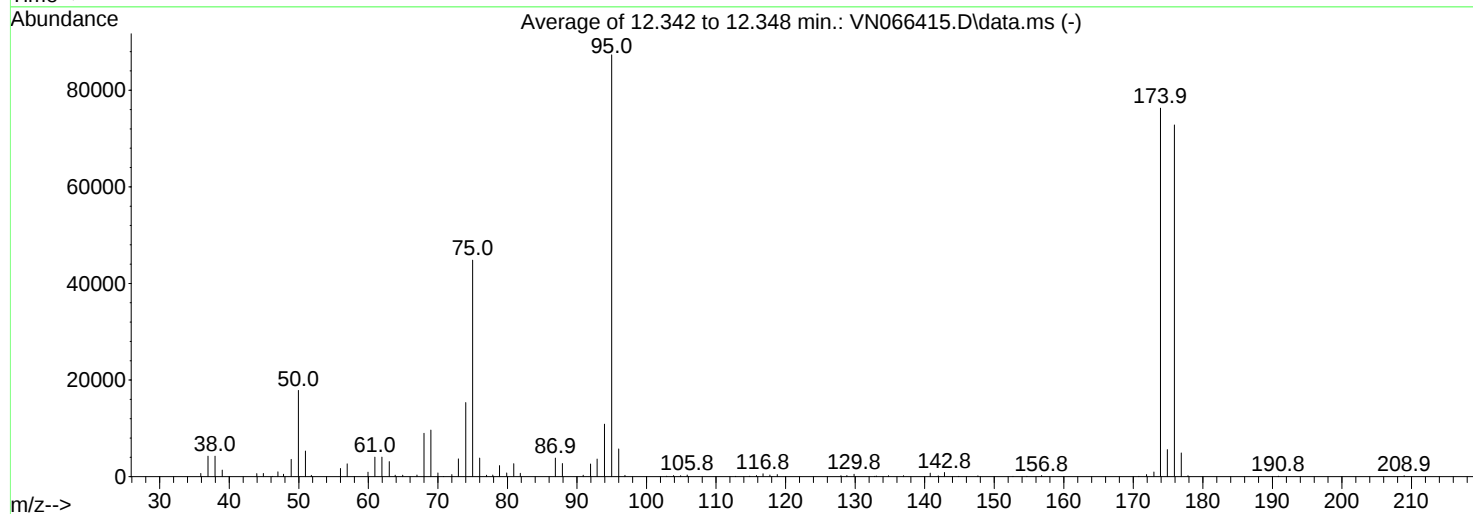


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN033021\
 Data File : VN066415.D
 Acq On : 30 Mar 2021 10:52
 Operator : JC/MD
 Sample : VSTDCCC020
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N032421W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Thu Mar 25 05:52:50 2021

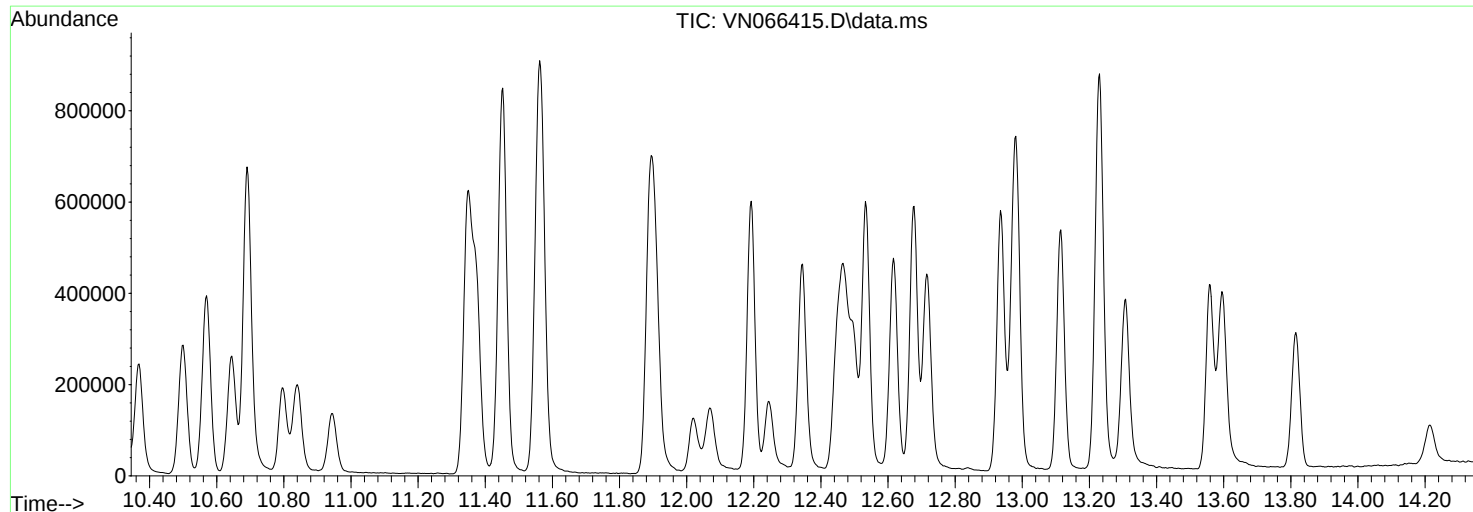

AutoFind: Scans 3972, 3973, 3974; Background Corrected with Scan 3956

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	17844	PASS
75	95	30	60	51.3	44818	PASS
95	95	100	100	100.0	87333	PASS
96	95	5	9	6.6	5735	PASS
173	174	0.00	2	1.3	967	PASS
174	95	50	100	87.4	76307	PASS
175	174	5	9	7.4	5612	PASS
176	174	95	101	95.4	72811	PASS
177	176	5	9	6.8	4918	PASS