


Methyl Acetate

Response Ratio

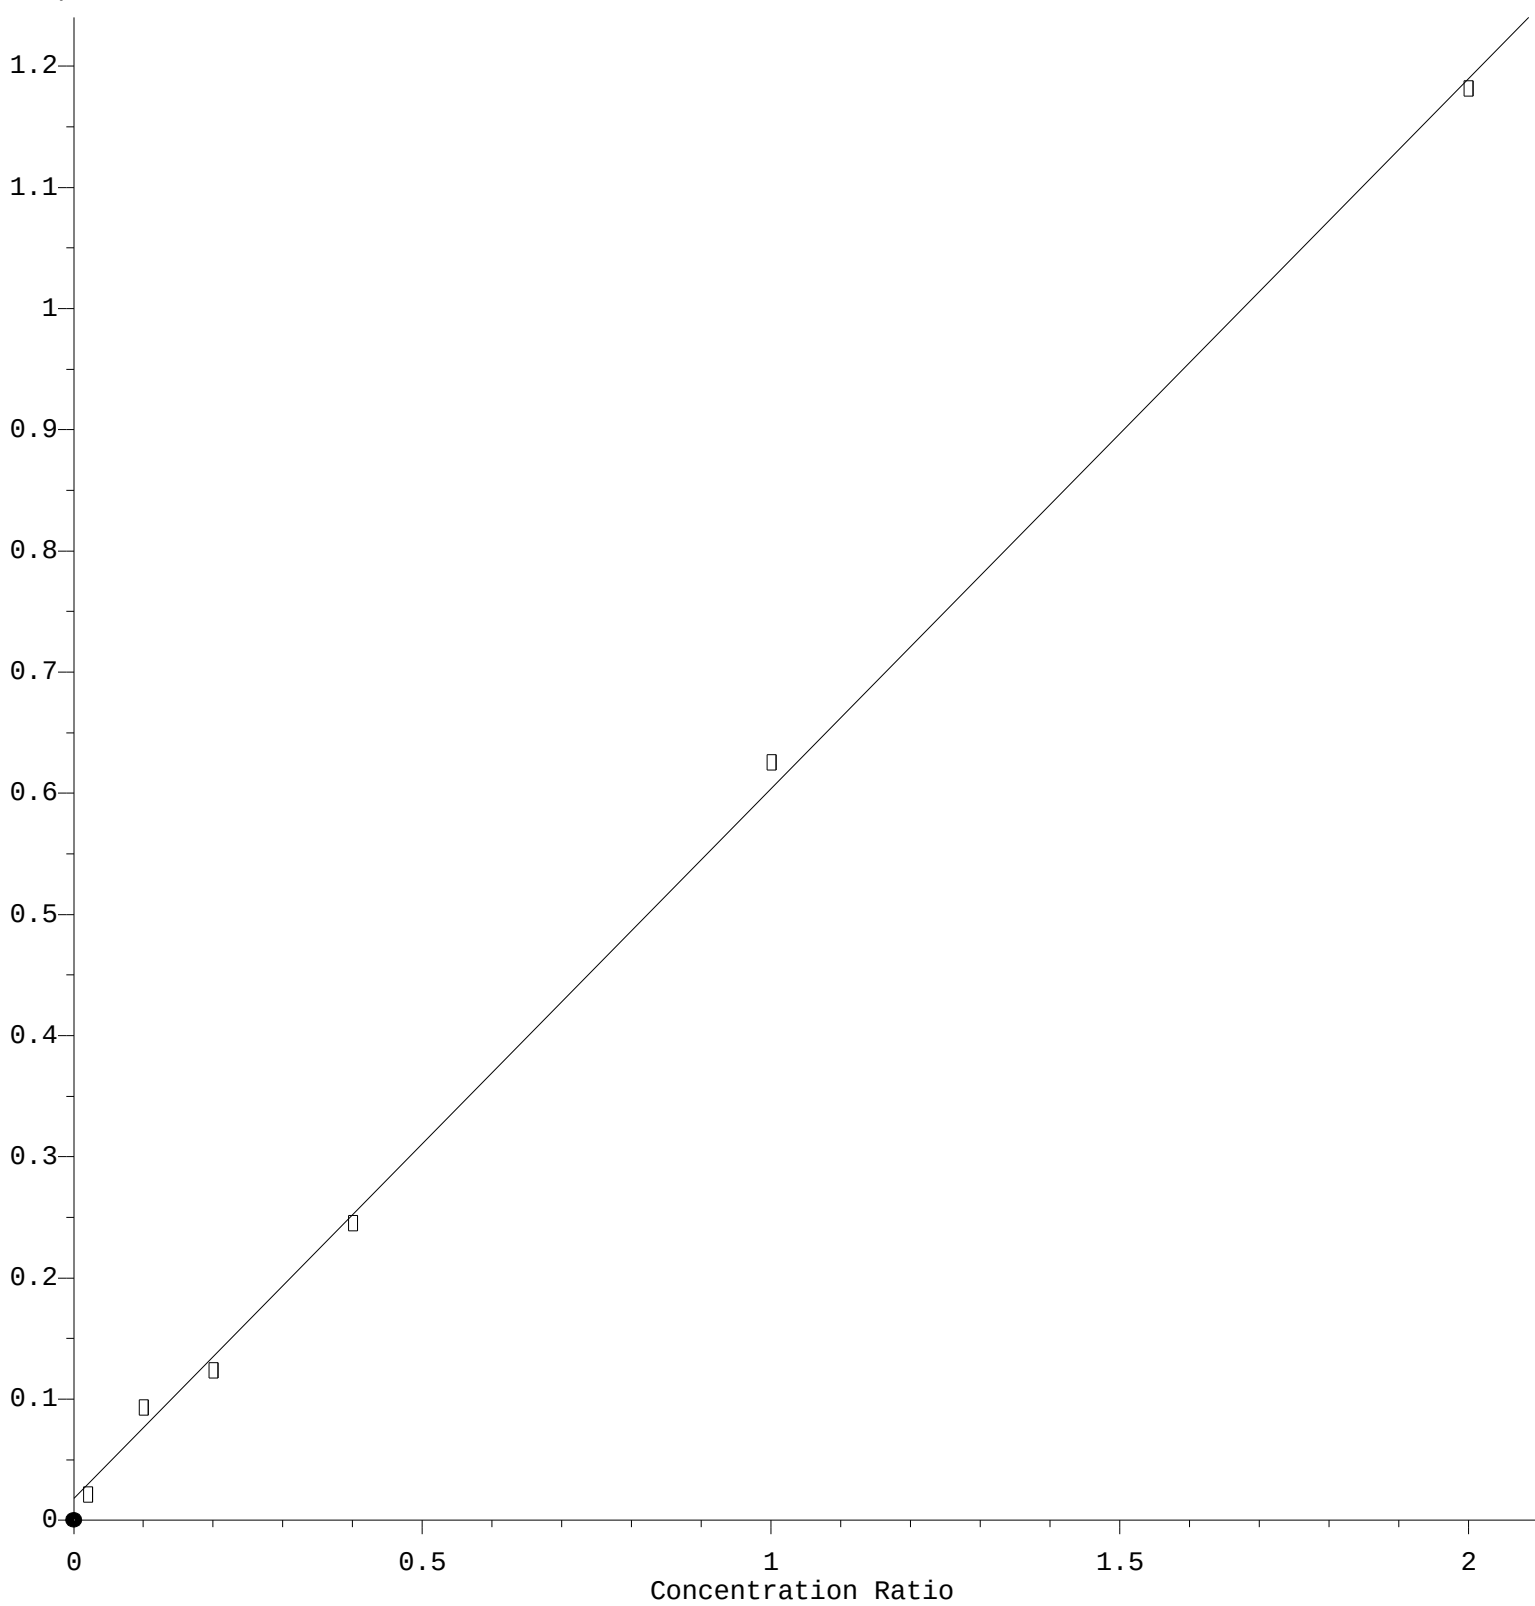


$$\text{Response} = 5.858\text{e-}001 * \text{Amt} + 1.829\text{e-}002$$

Coef of Det (r^2) = 0.998925 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M

Calibration Table Last Updated: Thu Mar 31 01:57:54 2022


1,4-Dioxane

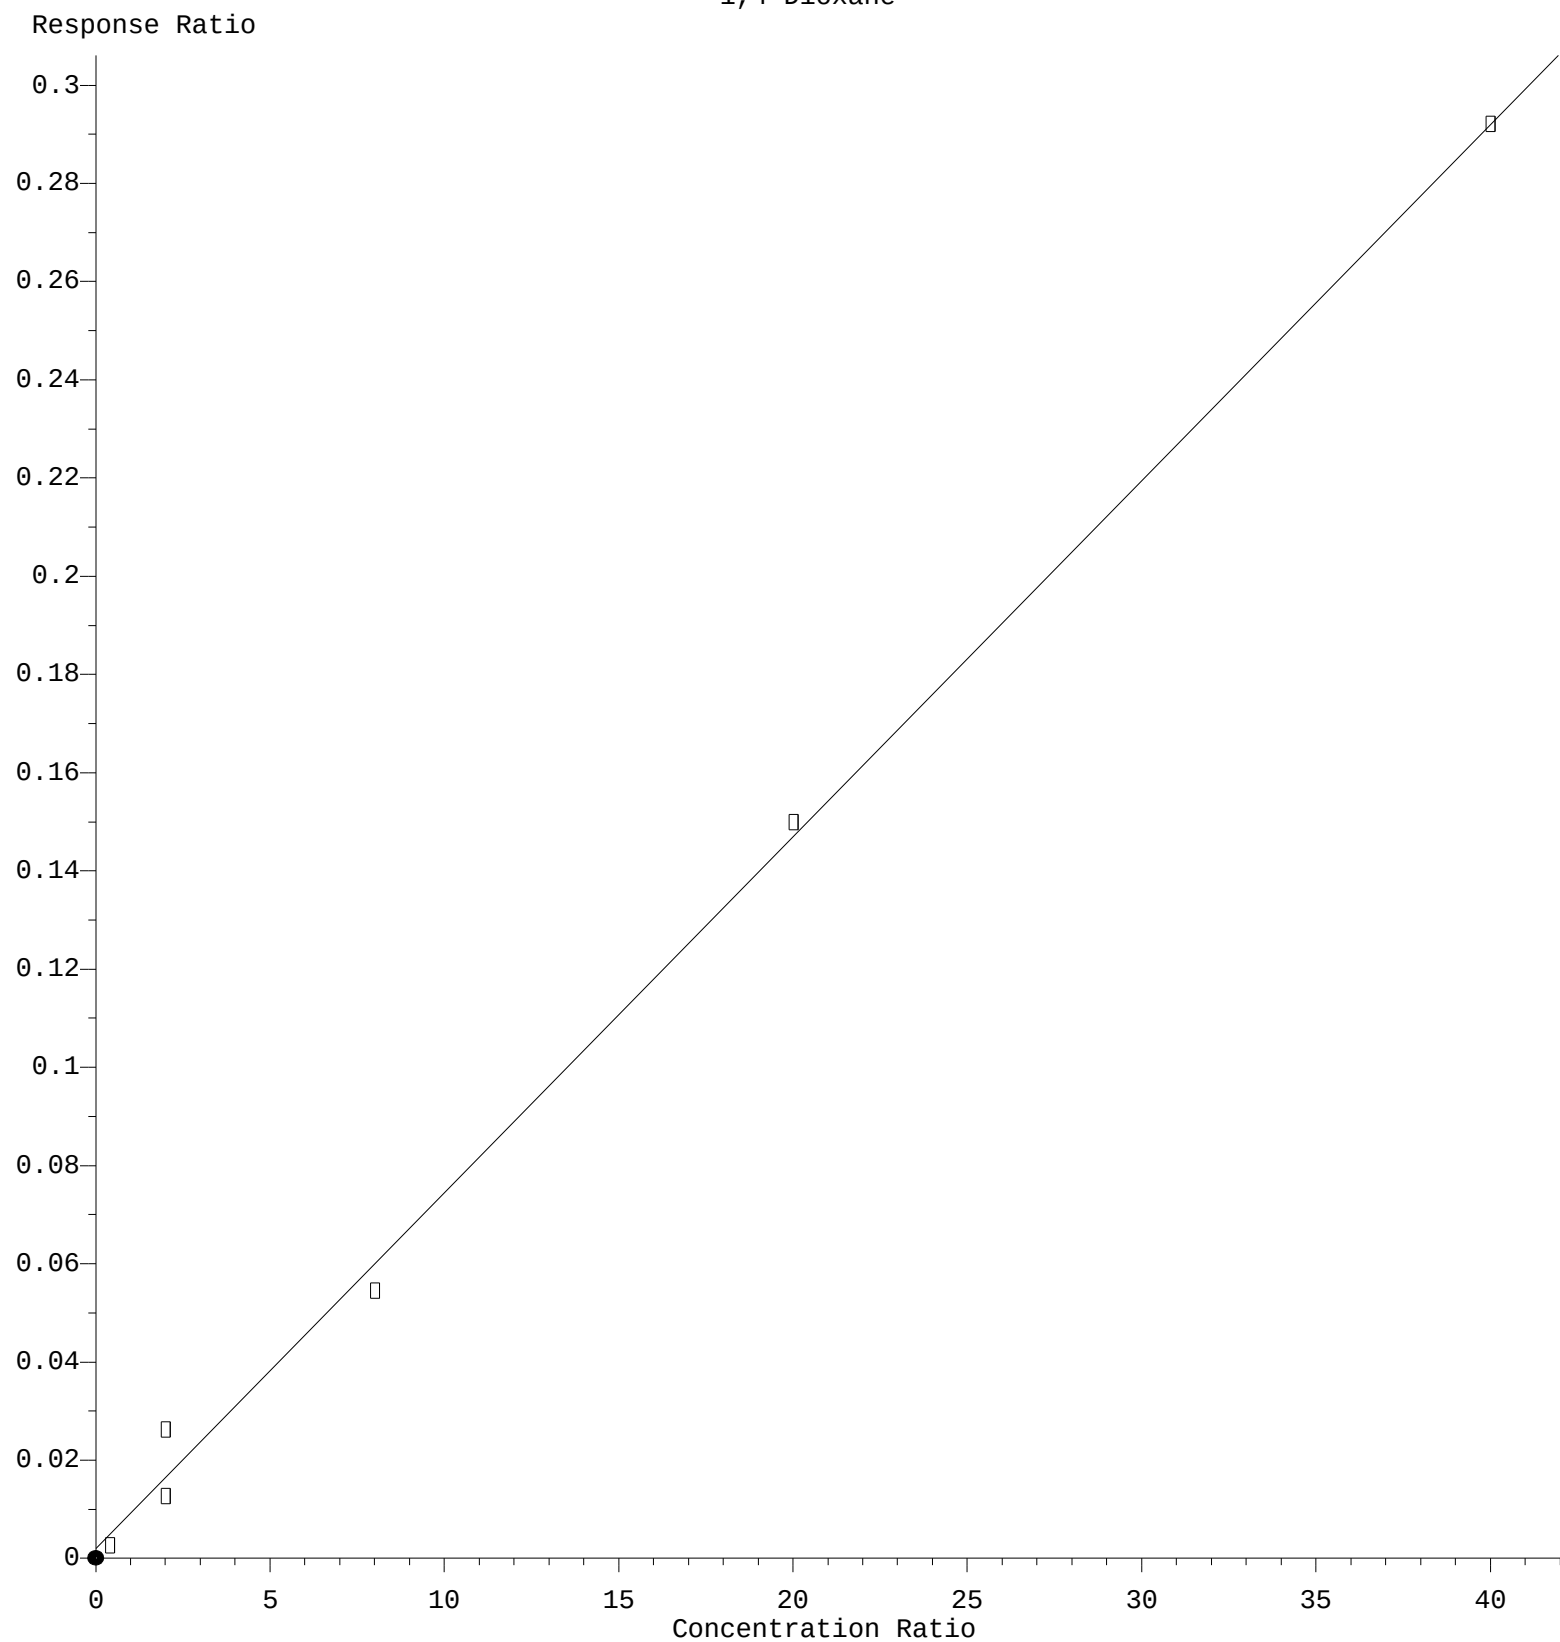

Response = $7.261 \times 10^{-3} \times \text{Amt} + 2.034 \times 10^{-3}$
 Coef of Det (r^2) = 0.997558 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
 Calibration Table Last Updated: Thu Mar 31 01:57:54 2022

2-Chloroethyl Vinyl ether

Response Ratio

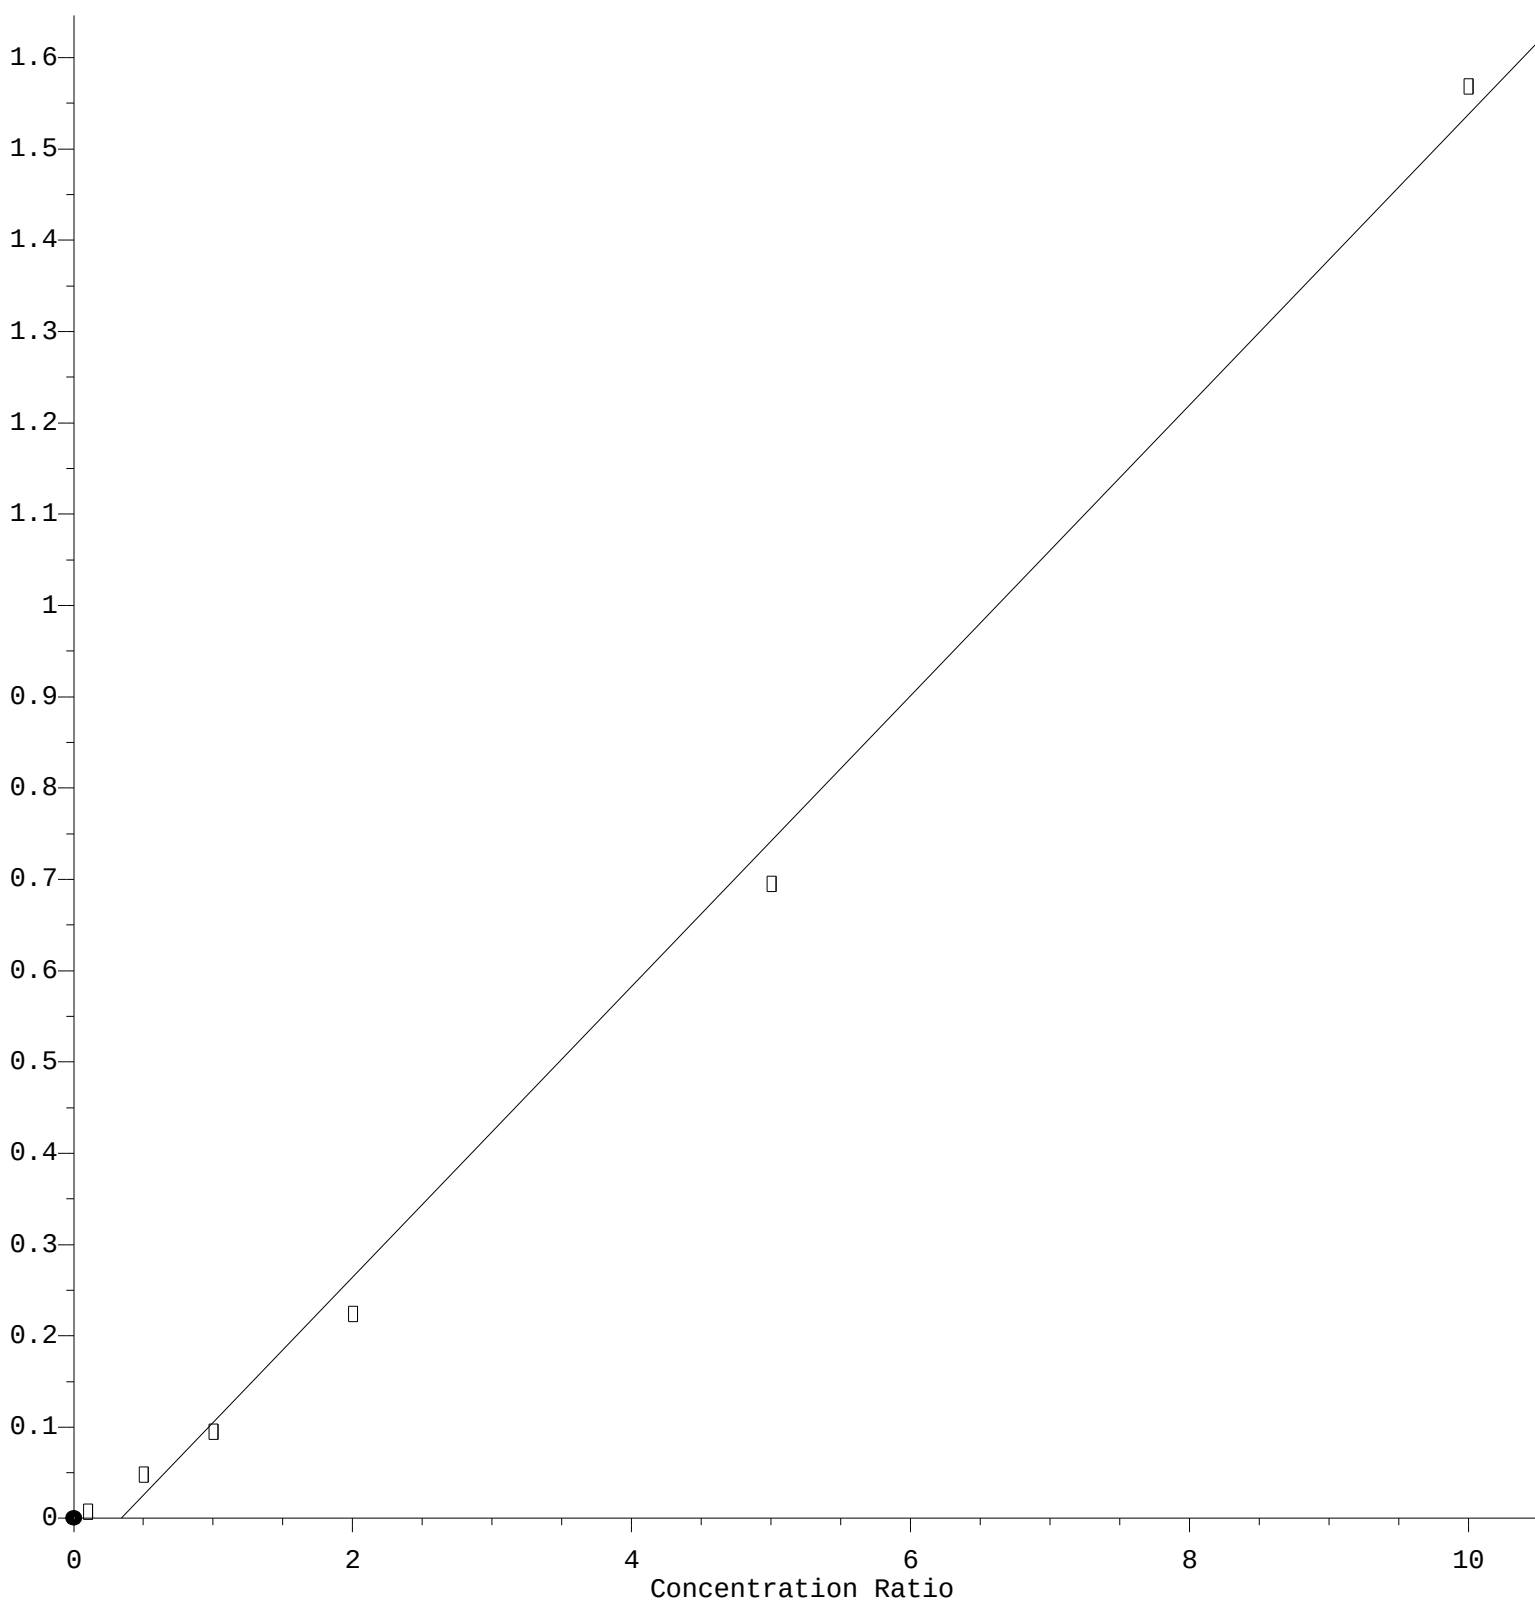

$$\text{Response} = 1.591\text{e-}001 * \text{Amt} - 5.399\text{e-}002$$


Coef of Det (r^2) = 0.996010 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M

Calibration Table Last Updated: Thu Mar 31 01:57:54 2022

1,2,4-Trichlorobenzene

Response Ratio

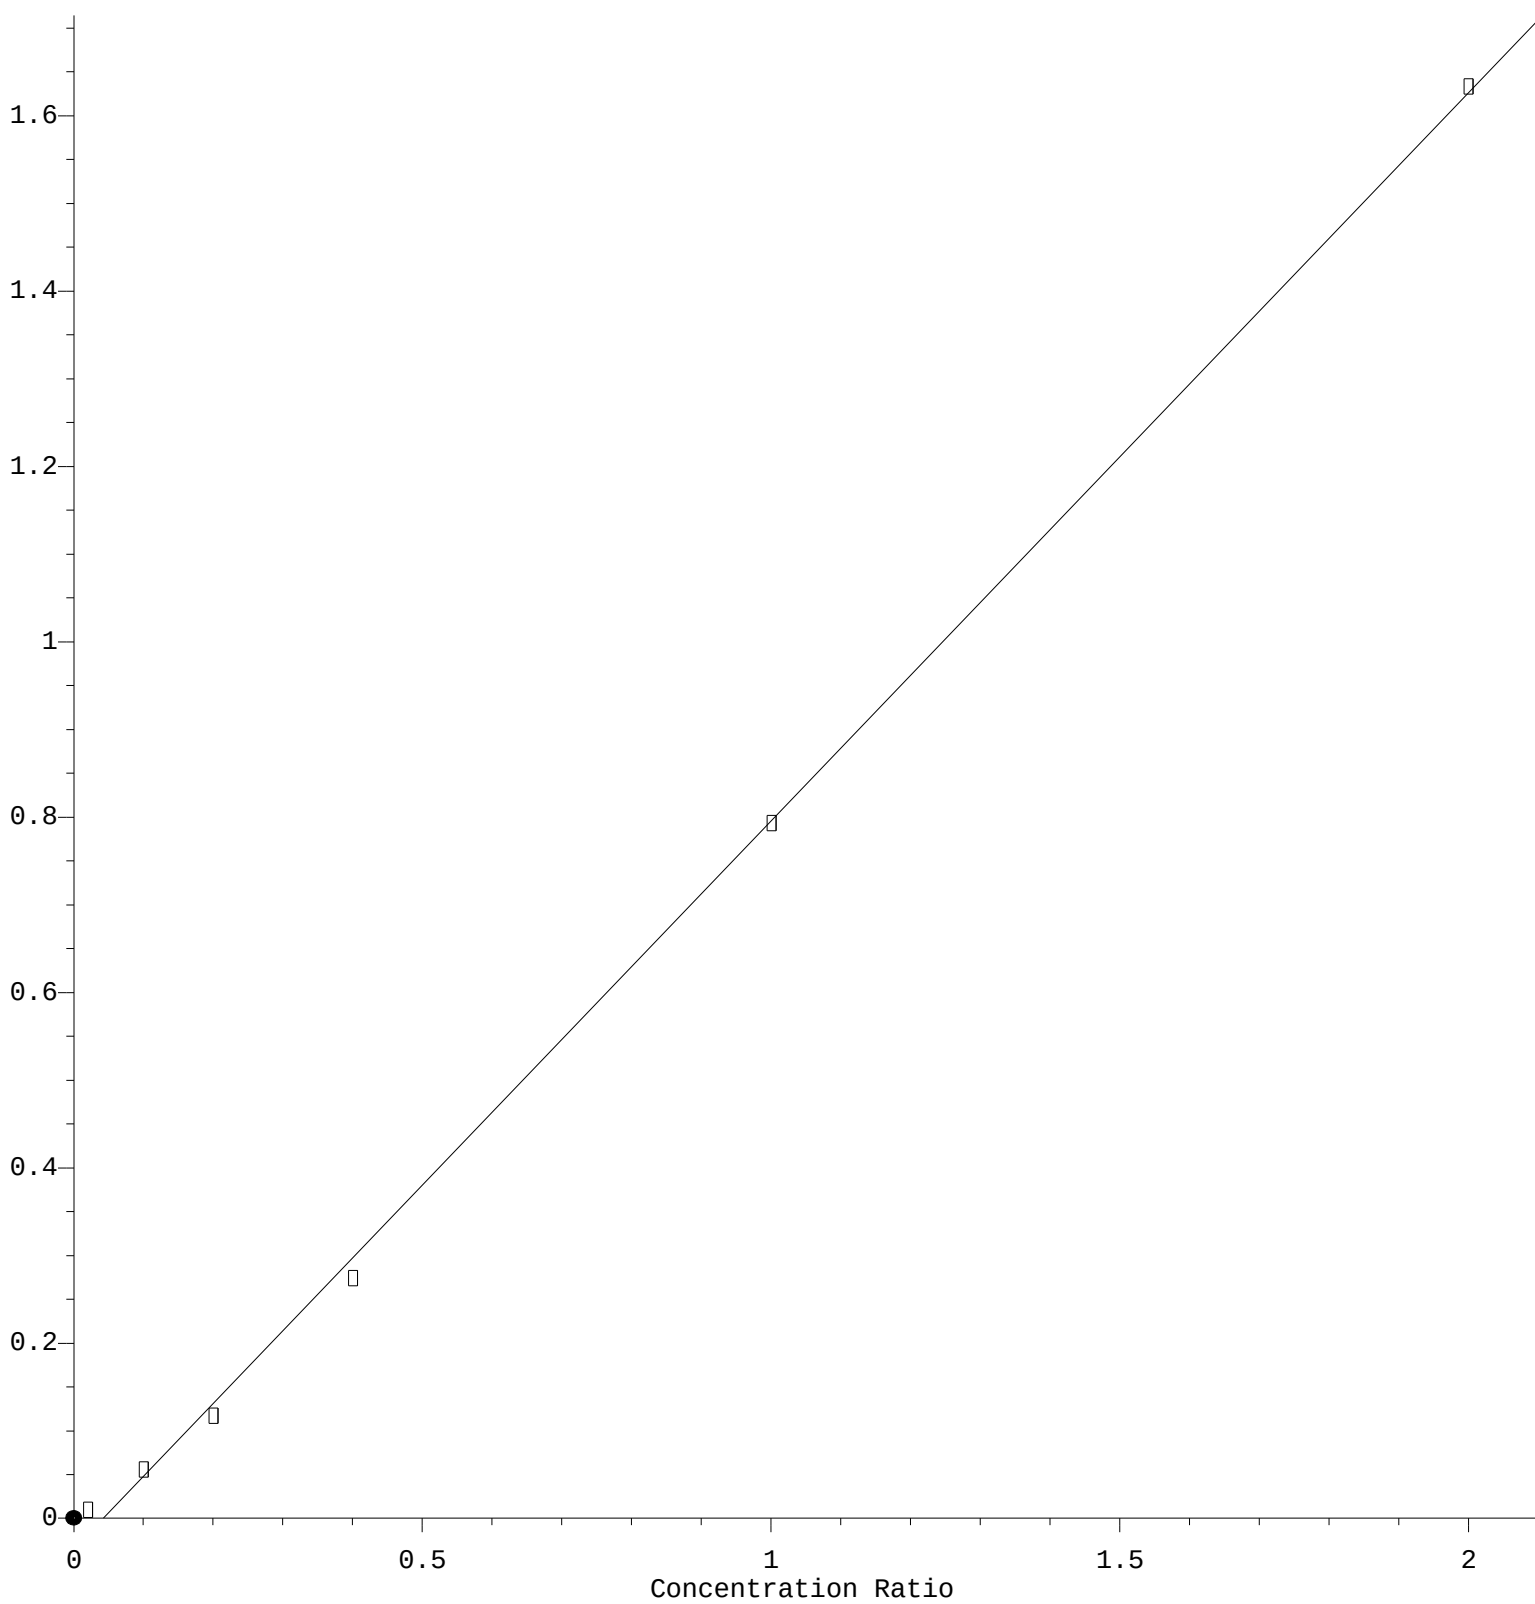

$$\text{Response} = 8.304\text{e-}001 * \text{Amt} - 3.464\text{e-}002$$


Coef of Det (r^2) = 0.999188 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M

Calibration Table Last Updated: Thu Mar 31 01:57:54 2022

Naphthalene

Response Ratio

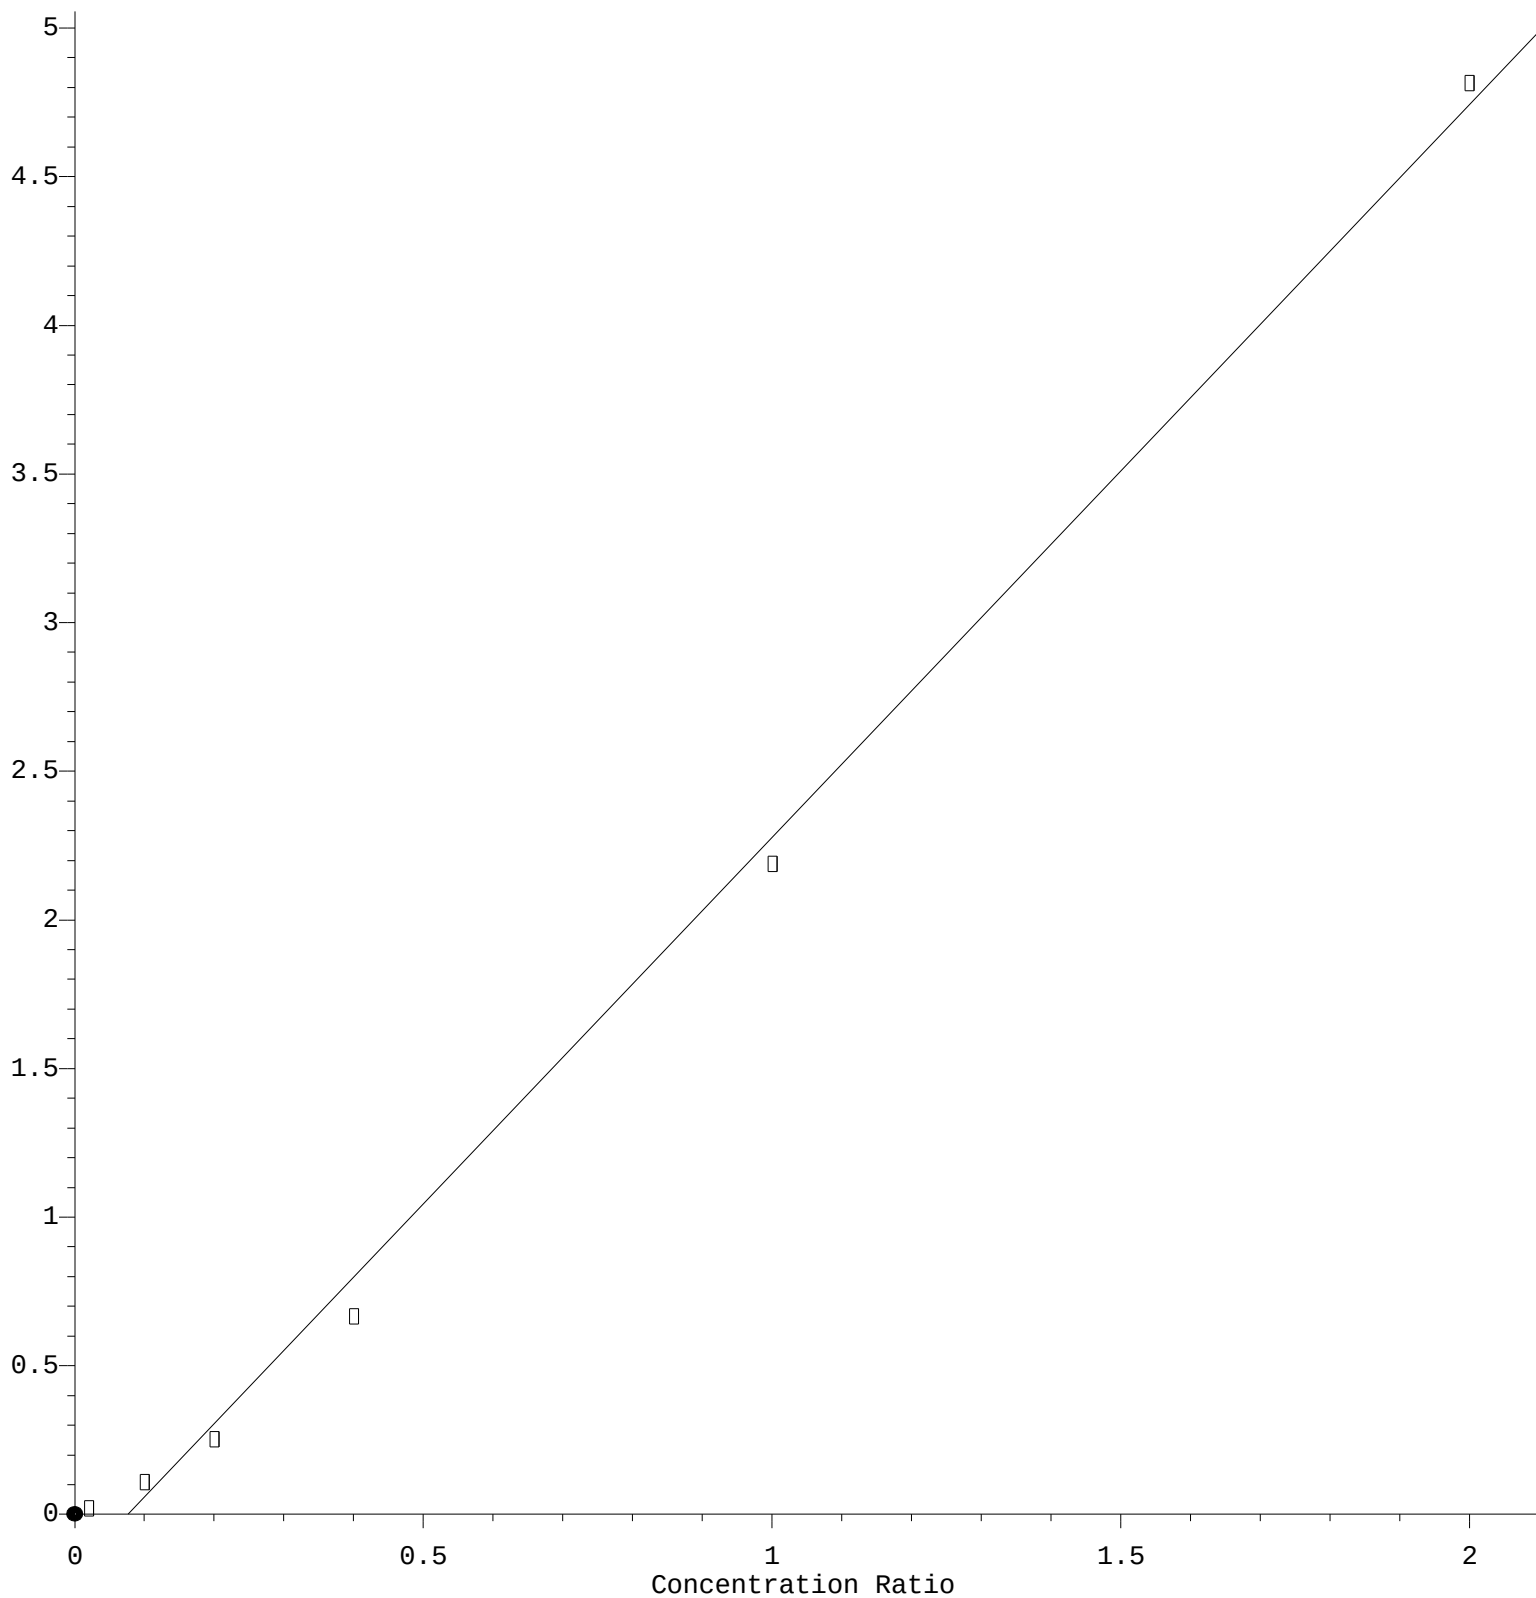

$$\text{Response} = 2.464\text{e}+000 * \text{Amt} - 1.874\text{e}-001$$


Coef of Det (r^2) = 0.996535 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M

Calibration Table Last Updated: Thu Mar 31 01:57:54 2022

1,2,3-Trichlorobenzene

Response Ratio

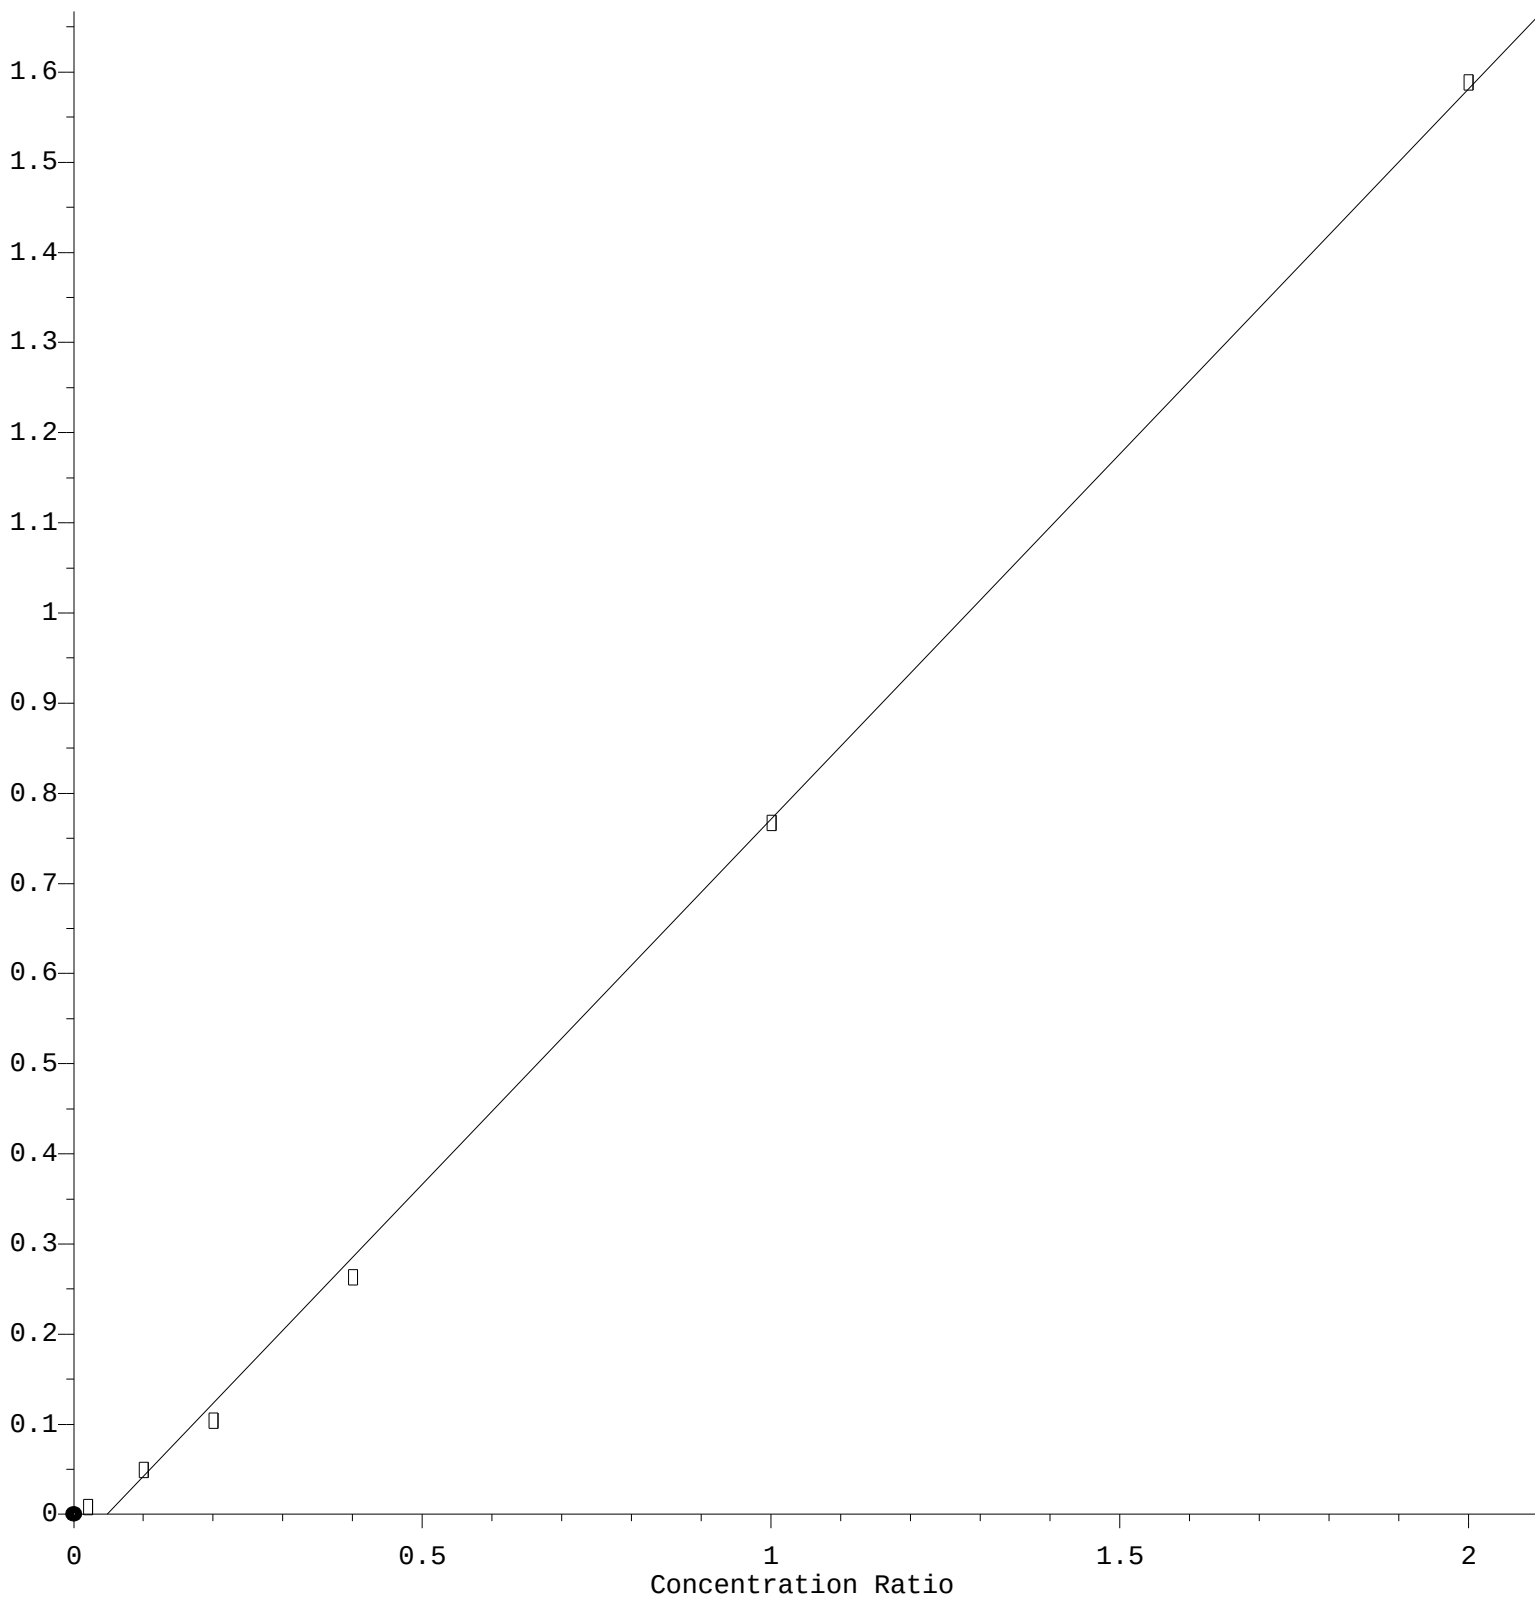

$$\text{Response} = 8.100\text{e-}001 * \text{Amt} - 3.911\text{e-}002$$

Coef of Det (r^2) = 0.998972 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M

Calibration Table Last Updated: Thu Mar 31 01:57:54 2022